

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042523\
 Data File : VV030857.D
 Acq On : 25 Apr 2023 23:55
 Operator : SY/MD
 Sample : 02474-07
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 36 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0AS9

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM041723WMA.M
 Title : VOC Analysis

Signal : TIC: VV030857.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.281	68	75	89	rBV	99396	114409	13.80%	1.787%
2	1.535	148	154	166	rVB	88381	103779	12.52%	1.621%
3	2.066	310	319	333	rBV	195441	285932	34.49%	4.467%
4	2.204	360	362	365	rBV4	1376	523	0.06%	0.008%
5	2.445	434	437	438	rBV3	1284	835	0.10%	0.013%
6	2.487	447	450	454	rBV6	1067	754	0.09%	0.012%
7	2.532	462	464	465	rBV2	1487	684	0.08%	0.011%
8	2.616	487	490	492	rBV3	1196	606	0.07%	0.009%
9	2.828	553	556	557	rBV2	1394	843	0.10%	0.013%
10	2.992	602	607	609	rBV5	1487	1437	0.17%	0.022%
11	3.043	621	623	625	rVV3	1214	459	0.06%	0.007%
12	3.063	627	629	632	rVV4	1996	1055	0.13%	0.016%
13	3.121	644	647	651	rBV6	1180	1216	0.15%	0.019%
14	3.259	687	690	694	rVB4	1487	891	0.11%	0.014%
15	3.593	789	794	797	rBV7	1647	1604	0.19%	0.025%
16	3.699	824	827	830	rBV4	1530	1026	0.12%	0.016%
17	3.715	830	832	835	rBV5	1007	648	0.08%	0.010%
18	3.757	841	845	847	rBV4	1248	775	0.09%	0.012%
19	3.799	847	858	883	rBV	53624	160320	19.34%	2.505%
20	4.259	988	1001	1026	rVB2	135513	339929	41.01%	5.310%
21	4.670	1124	1129	1132	rBV6	2153	1748	0.21%	0.027%
22	4.789	1163	1166	1169	rBV4	1110	636	0.08%	0.010%
23	4.966	1205	1221	1246	rVV2	309668	828950	100.00%	12.950%
24	5.365	1341	1345	1350	rBV7	1308	1278	0.15%	0.020%
25	5.413	1357	1360	1363	rBV4	1220	915	0.11%	0.014%
26	5.542	1388	1400	1421	rBV	256033	533072	64.31%	8.328%
27	5.998	1528	1542	1566	rBV	184508	386854	46.67%	6.044%
28	6.288	1631	1632	1634	rBV3	1071	431	0.05%	0.007%
29	6.381	1656	1661	1665	rBV8	1936	1742	0.21%	0.027%
30	6.429	1673	1676	1677	rBV3	1428	726	0.09%	0.011%
31	6.452	1681	1683	1685	rBV4	1158	526	0.06%	0.008%
32	6.519	1702	1704	1707	rBV3	1100	631	0.08%	0.010%
33	6.632	1736	1739	1741	rBV3	1500	1079	0.13%	0.017%
34	6.664	1748	1749	1753	rVB4	1202	453	0.05%	0.007%
35	6.789	1785	1788	1792	rVB5	1442	1082	0.13%	0.017%
36	6.809	1792	1794	1796	rBV2	1376	839	0.10%	0.013%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW042523\
 Data File : VW030857.D
 Acq On : 25 Apr 2023 23:55
 Operator : SY/MD
 Sample : 02474-07
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 36 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0AS9

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM041723WMA.M
 Title : VOC Analysis

37	6.921	1819	1829	1851	rBV2	94875	179680	21.68%	2.807%
38	7.252	1920	1932	1952	rBV	350117	628835	75.86%	9.824%
39	7.481	1999	2003	2009	rBV9	1838	2426	0.29%	0.038%
40	7.561	2019	2028	2048	rBV2	68375	124137	14.98%	1.939%
41	7.773	2092	2094	2097	rBV3	1209	556	0.07%	0.009%
42	7.805	2101	2104	2106	rBV3	1122	819	0.10%	0.013%
43	7.876	2121	2126	2128	rBV6	3929	4366	0.53%	0.068%
44	8.034	2166	2175	2207	rBV	161846	328717	39.65%	5.135%
45	8.435	2298	2300	2304	rBV3	1141	962	0.12%	0.015%
46	8.522	2324	2327	2328	rBV3	1003	606	0.07%	0.009%
47	8.641	2361	2364	2368	rBV6	1539	1304	0.16%	0.020%
48	8.686	2376	2378	2379	rBV2	1037	444	0.05%	0.007%
49	8.792	2400	2411	2434	rBV	389695	656281	79.17%	10.253%
50	9.075	2496	2499	2500	rBV3	1541	806	0.10%	0.013%
51	9.217	2541	2543	2546	rBV4	1117	791	0.10%	0.012%
52	9.336	2577	2580	2583	rVB4	1208	717	0.09%	0.011%
53	9.355	2583	2586	2589	rBV5	1403	1168	0.14%	0.018%
54	9.603	2660	2663	2665	rBV4	1538	927	0.11%	0.014%
55	9.706	2694	2695	2698	rBV2	1084	612	0.07%	0.010%
56	9.805	2724	2726	2730	rBV5	1223	911	0.11%	0.014%
57	9.898	2753	2755	2758	rVB2	2015	831	0.10%	0.013%
58	9.915	2758	2760	2761	rBV2	1167	471	0.06%	0.007%
59	10.085	2811	2813	2816	rBV4	793	453	0.05%	0.007%
60	10.162	2825	2837	2852	rBV	255596	408522	49.28%	6.382%
61	10.397	2908	2910	2912	rBV3	1090	576	0.07%	0.009%
62	10.570	2962	2964	2968	rBV4	1422	801	0.10%	0.013%
63	10.799	3032	3035	3040	rVB4	1539	1112	0.13%	0.017%
64	10.857	3051	3053	3058	rBV5	952	582	0.07%	0.009%
65	10.950	3080	3082	3084	rBV3	1171	610	0.07%	0.010%
66	11.033	3104	3108	3110	rBV4	1021	950	0.11%	0.015%
67	11.114	3129	3133	3135	rBV4	1218	958	0.12%	0.015%
68	11.194	3147	3158	3176	rBV	400235	629957	75.99%	9.841%
69	11.419	3226	3228	3231	rVB4	1876	1118	0.13%	0.017%
70	11.570	3263	3275	3291	rBV	382155	616605	74.38%	9.633%
71	11.892	3372	3375	3376	rBV3	856	585	0.07%	0.009%
72	11.995	3403	3407	3409	rBV4	1045	788	0.10%	0.012%
73	12.139	3449	3452	3454	rVB3	1009	614	0.07%	0.010%
74	12.156	3454	3457	3461	rBV5	1845	1729	0.21%	0.027%
75	12.188	3465	3467	3470	rBV4	1566	970	0.12%	0.015%
76	12.249	3483	3486	3487	rBV2	995	524	0.06%	0.008%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042523\
 Data File : VV030857.D
 Acq On : 25 Apr 2023 23:55
 Operator : SY/MD
 Sample : 02474-07
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 36 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0AS9

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM041723WMA.M
 Title : VOC Analysis

77	12.278	3492	3495	3498	rBV3	1219	803	0.10%	0.013%
78	12.419	3536	3539	3540	rBV3	1133	511	0.06%	0.008%
79	12.471	3553	3555	3560	rBV5	846	603	0.07%	0.009%
80	12.554	3579	3581	3586	rBV6	955	670	0.08%	0.010%
81	12.615	3598	3600	3602	rBV4	847	444	0.05%	0.007%
82	12.741	3635	3639	3641	rBV4	830	694	0.08%	0.011%
83	12.792	3653	3655	3658	rBV3	1063	575	0.07%	0.009%
84	12.898	3684	3688	3689	rBV4	1130	733	0.09%	0.011%
85	13.204	3781	3783	3784	rBV2	1481	699	0.08%	0.011%
86	13.406	3843	3846	3847	rBV3	1113	675	0.08%	0.011%
87	13.445	3856	3858	3862	rBV5	1618	1289	0.16%	0.020%
88	13.541	3887	3888	3891	rBV3	1039	621	0.07%	0.010%
89	13.615	3909	3911	3913	rBV3	1223	648	0.08%	0.010%
90	13.699	3933	3937	3941	rBV6	1604	1218	0.15%	0.019%
91	13.776	3958	3961	3963	rBV5	1740	1302	0.16%	0.020%
92	13.815	3971	3973	3974	rBV2	1112	471	0.06%	0.007%
93	13.901	3998	4000	4004	rBV4	1578	1073	0.13%	0.017%
94	14.037	4038	4042	4043	rBV4	1016	722	0.09%	0.011%
95	14.114	4065	4066	4070	rBV4	990	549	0.07%	0.009%
96	14.249	4104	4108	4111	rBV5	1267	1315	0.16%	0.021%
97	14.316	4127	4129	4131	rBV3	1124	445	0.05%	0.007%
98	14.483	4179	4181	4185	rBV5	1357	1097	0.13%	0.017%
99	14.731	4256	4258	4260	rBV3	1876	879	0.11%	0.014%
100	14.853	4294	4296	4298	rBV4	1093	532	0.06%	0.008%




Sum of corrected areas: 6401076

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042523\
Data File : VV030857.D
Acq On : 25 Apr 2023 23:55
Operator : SY/MD
Sample : 02474-07
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 36 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0AS9

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM041723WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

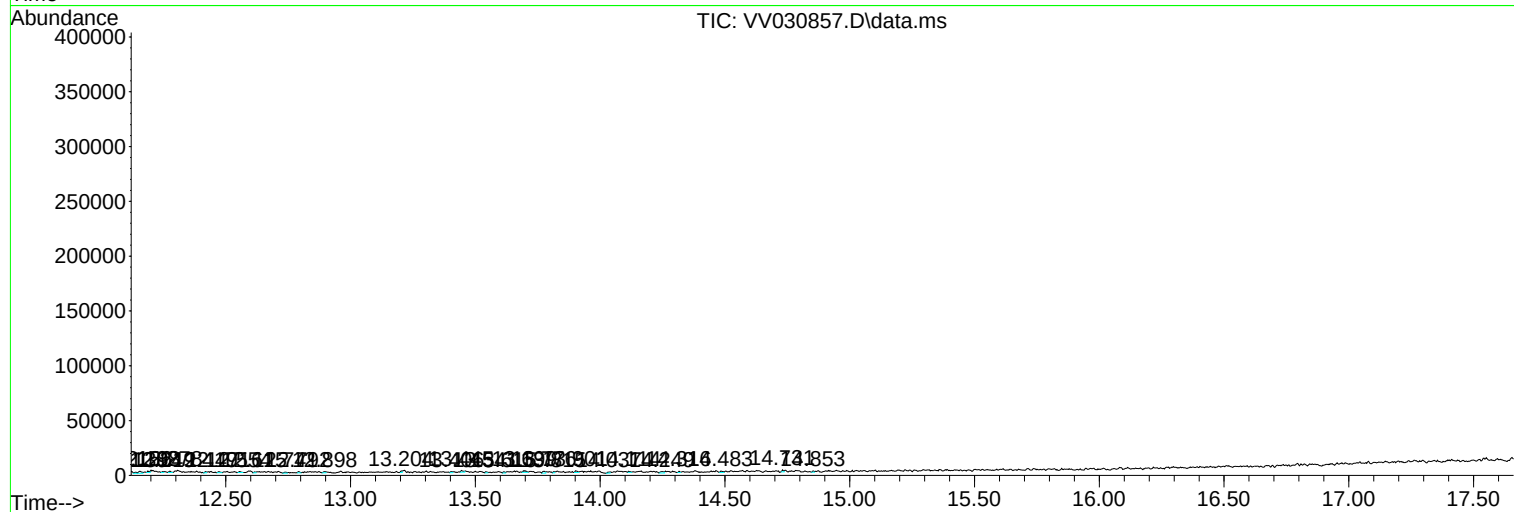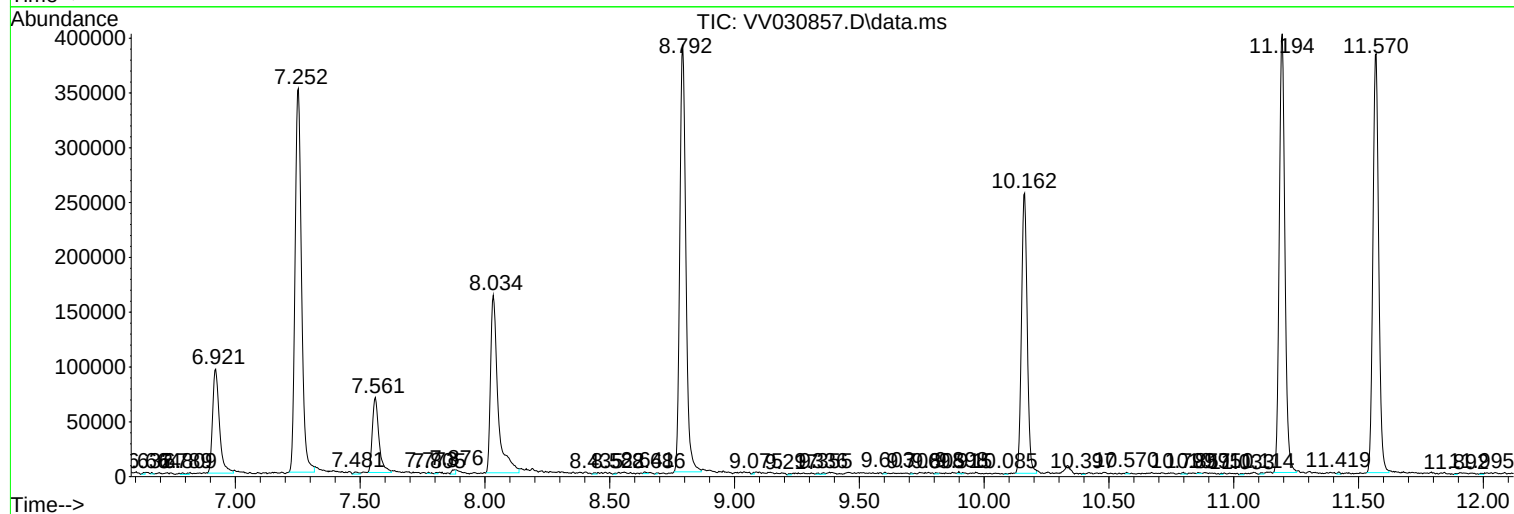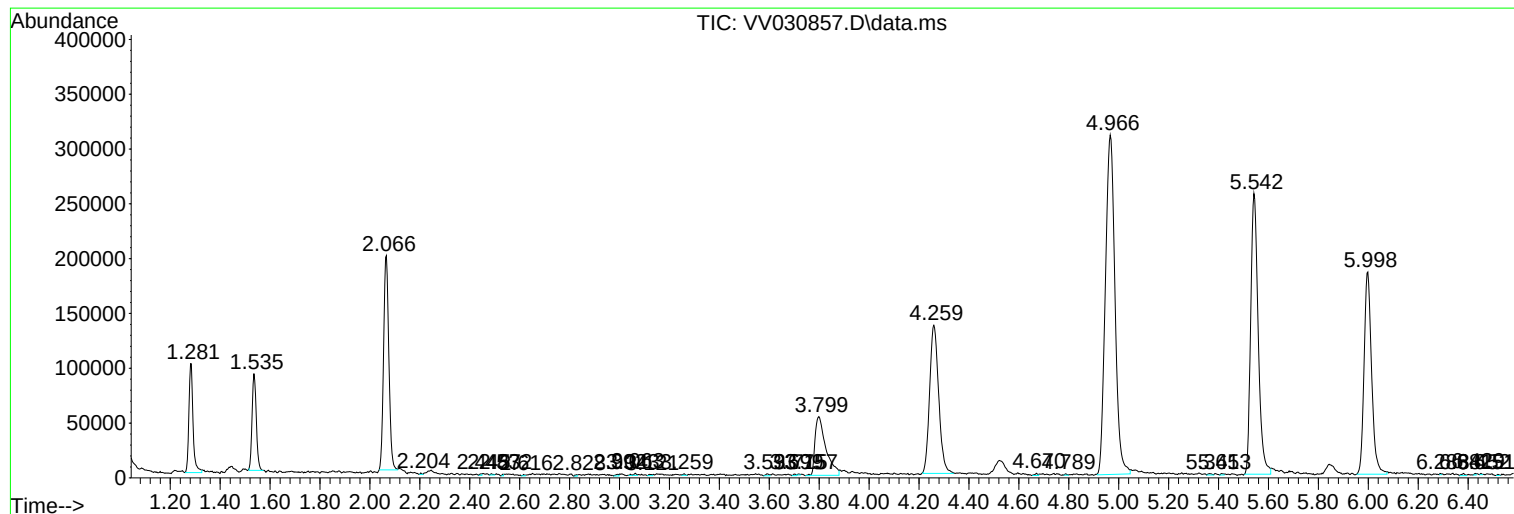

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042523\
Data File : VV030857.D
Acq On : 25 Apr 2023 23:55
Operator : SY/MD
Sample : 02474-07
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 36 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0AS9

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM041723WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042523\
Data File : VV030857.D
Acq On : 25 Apr 2023 23:55
Operator : SY/MD
Sample : 02474-07
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 36 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0AS9

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM041723WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------