

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042523\
 Data File : VV030858.D
 Acq On : 26 Apr 2023 00:19
 Operator : SY/MD
 Sample : 02474-09
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 37 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0AT1

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM041723WMA.M
 Title : VOC Analysis

Signal : TIC: VV030858.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.285	69	76	89	rVB	97811	105446	13.04%	1.666%
2	1.535	147	154	166	rVB	91759	107787	13.33%	1.703%
3	2.066	310	319	331	rBV	193156	281953	34.86%	4.455%
4	2.423	428	430	433	rBV4	1435	976	0.12%	0.015%
5	2.519	457	460	463	rBV4	1494	863	0.11%	0.014%
6	2.574	475	477	482	rVB4	1673	1054	0.13%	0.017%
7	2.667	502	506	508	rBV5	1018	674	0.08%	0.011%
8	2.696	511	515	516	rBV3	1057	698	0.09%	0.011%
9	2.706	516	518	525	rVB7	1928	1726	0.21%	0.027%
10	2.738	525	528	531	rBV4	1057	712	0.09%	0.011%
11	2.825	553	555	558	rVB4	1281	749	0.09%	0.012%
12	2.841	558	560	565	rBV5	1018	879	0.11%	0.014%
13	2.879	569	572	573	rBV3	1110	607	0.08%	0.010%
14	2.924	583	586	591	rVB9	1309	792	0.10%	0.013%
15	3.008	609	612	616	rVB6	1544	1119	0.14%	0.018%
16	3.037	618	621	624	rVB5	1706	815	0.10%	0.013%
17	3.240	682	684	688	rBV4	1191	796	0.10%	0.013%
18	3.320	707	709	711	rBV2	1496	574	0.07%	0.009%
19	3.471	754	756	759	rBV3	794	657	0.08%	0.010%
20	3.510	766	768	773	rVB7	1177	588	0.07%	0.009%
21	3.577	785	789	791	rBV5	1167	940	0.12%	0.015%
22	3.709	826	830	834	rBV5	1621	1226	0.15%	0.019%
23	3.799	848	858	883	rBV	52918	152136	18.81%	2.404%
24	4.195	978	981	982	rBV4	1300	720	0.09%	0.011%
25	4.259	987	1001	1024	rVB	133281	339714	42.01%	5.368%
26	4.683	1131	1133	1137	rBV3	1674	1273	0.16%	0.020%
27	4.760	1154	1157	1159	rBV3	1420	831	0.10%	0.013%
28	4.786	1162	1165	1168	rBV4	1235	609	0.08%	0.010%
29	4.838	1179	1181	1183	rVB3	1415	576	0.07%	0.009%
30	4.850	1183	1185	1187	rBV2	1194	647	0.08%	0.010%
31	4.966	1204	1221	1244	rBV2	303736	808740	100.00%	12.780%
32	5.394	1352	1354	1359	rVB6	1743	1287	0.16%	0.020%
33	5.420	1359	1362	1365	rBV5	1479	1222	0.15%	0.019%
34	5.542	1388	1400	1422	rBV	237088	498993	61.70%	7.885%
35	5.844	1484	1494	1508	rBV	58104	113372	14.02%	1.792%
36	5.998	1531	1542	1563	rVB	176508	359500	44.45%	5.681%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW042523\
 Data File : VW030858.D
 Acq On : 26 Apr 2023 00:19
 Operator : SY/MD
 Sample : 02474-09
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 37 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 COAT1

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM041723WMA.M
 Title : VOC Analysis

37	6.307	1636	1638	1642	rBV4	1514	1193	0.15%	0.019%
38	6.477	1689	1691	1694	rBV5	1438	871	0.11%	0.014%
39	6.522	1703	1705	1706	rBV2	1408	652	0.08%	0.010%
40	6.857	1806	1809	1810	rBV3	1243	699	0.09%	0.011%
41	6.921	1819	1829	1849	rBV	88067	167232	20.68%	2.643%
42	7.143	1893	1898	1902	rBV6	1858	2065	0.26%	0.033%
43	7.252	1920	1932	1955	rBV	345580	620216	76.69%	9.801%
44	7.471	1998	2000	2005	rVB4	1467	891	0.11%	0.014%
45	7.516	2010	2014	2016	rVB6	1104	593	0.07%	0.009%
46	7.561	2016	2028	2049	rBV2	68774	127634	15.78%	2.017%
47	7.809	2103	2105	2108	rVB4	1184	607	0.08%	0.010%
48	7.944	2141	2147	2149	rBV5	1603	1347	0.17%	0.021%
49	8.034	2166	2175	2213	rBV	160618	333143	41.19%	5.264%
50	8.571	2338	2342	2345	rBV4	1821	1499	0.19%	0.024%
51	8.792	2400	2411	2434	rBV	377523	628429	77.70%	9.931%
52	9.362	2582	2588	2591	rVV7	1115	1266	0.16%	0.020%
53	9.461	2616	2619	2620	rBV3	996	617	0.08%	0.010%
54	9.677	2684	2686	2689	rVB3	1157	759	0.09%	0.012%
55	9.841	2735	2737	2741	rVB5	1658	838	0.10%	0.013%
56	10.050	2800	2802	2804	rBV2	1394	715	0.09%	0.011%
57	10.159	2824	2836	2851	rBV	244652	397208	49.11%	6.277%
58	10.329	2885	2889	2899	rVB4	5333	7658	0.95%	0.121%
59	10.538	2952	2954	2957	rBV3	1053	691	0.09%	0.011%
60	10.577	2962	2966	2968	rVV4	1282	847	0.10%	0.013%
61	10.599	2971	2973	2976	rBV4	1551	871	0.11%	0.014%
62	10.654	2988	2990	2992	rVB3	1703	699	0.09%	0.011%
63	10.670	2992	2995	3000	rBV7	1823	1658	0.21%	0.026%
64	10.718	3006	3010	3011	rBV2	929	787	0.10%	0.012%
65	10.837	3045	3047	3053	rVB7	1095	835	0.10%	0.013%
66	10.876	3053	3059	3063	rBV9	1692	1702	0.21%	0.027%
67	10.960	3083	3085	3088	rVB3	1211	614	0.08%	0.010%
68	10.992	3088	3095	3096	rBV8	1721	1282	0.16%	0.020%
69	11.050	3110	3113	3116	rBV4	1313	904	0.11%	0.014%
70	11.194	3147	3158	3173	rBV	371019	584531	72.28%	9.237%
71	11.339	3201	3203	3205	rBV3	1783	996	0.12%	0.016%
72	11.477	3241	3246	3250	rBV7	1767	1571	0.19%	0.025%
73	11.567	3263	3274	3296	rBV	373883	595986	73.69%	9.418%
74	11.802	3342	3347	3349	rBV5	1418	1081	0.13%	0.017%
75	12.246	3482	3485	3488	rVB4	1368	852	0.11%	0.013%
76	12.297	3493	3501	3510	rBV10	10898	17322	2.14%	0.274%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042523\
 Data File : VV030858.D
 Acq On : 26 Apr 2023 00:19
 Operator : SY/MD
 Sample : 02474-09
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 37 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0AT1

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM041723WMA.M
 Title : VOC Analysis

77	12.583	3585	3590	3592	rBV6	1376	1111	0.14%	0.018%
78	12.664	3612	3615	3618	rBV5	746	600	0.07%	0.009%
79	12.715	3628	3631	3633	rBV3	1319	648	0.08%	0.010%
80	12.805	3657	3659	3663	rVB4	1657	1050	0.13%	0.017%
81	12.831	3663	3667	3668	rBV4	1447	914	0.11%	0.014%
82	13.030	3725	3729	3730	rBV3	1359	992	0.12%	0.016%
83	13.062	3736	3739	3742	rVB6	1150	763	0.09%	0.012%
84	13.082	3742	3745	3746	rBV3	991	613	0.08%	0.010%
85	13.120	3754	3757	3760	rBV3	1691	1554	0.19%	0.025%
86	13.175	3771	3774	3777	rBV4	1178	708	0.09%	0.011%
87	13.210	3781	3785	3787	rBV5	2020	1474	0.18%	0.023%
88	13.361	3829	3832	3834	rVB3	1659	778	0.10%	0.012%
89	13.387	3834	3840	3844	rBV8	2952	3659	0.45%	0.058%
90	13.429	3849	3853	3854	rBV4	2075	1331	0.16%	0.021%
91	13.490	3869	3872	3875	rBV4	864	752	0.09%	0.012%
92	13.551	3888	3891	3894	rBV5	1488	1251	0.15%	0.020%
93	13.590	3900	3903	3906	rBV4	1108	700	0.09%	0.011%
94	13.683	3928	3932	3934	rBV5	1211	938	0.12%	0.015%
95	13.757	3953	3955	3959	rBV5	1142	785	0.10%	0.012%
96	14.078	4052	4055	4060	rBV7	1413	878	0.11%	0.014%
97	14.184	4086	4088	4091	rBV4	1306	823	0.10%	0.013%
98	14.451	4166	4171	4172	rBV5	1309	1139	0.14%	0.018%
99	14.512	4187	4190	4193	rBV4	1344	1008	0.12%	0.016%
100	14.599	4208	4217	4220	rBV4	2164	3124	0.39%	0.049%


Sum of corrected areas: 6328205

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042523\
Data File : VV030858.D
Acq On : 26 Apr 2023 00:19
Operator : SY/MD
Sample : 02474-09
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 37 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0AT1

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM041723WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

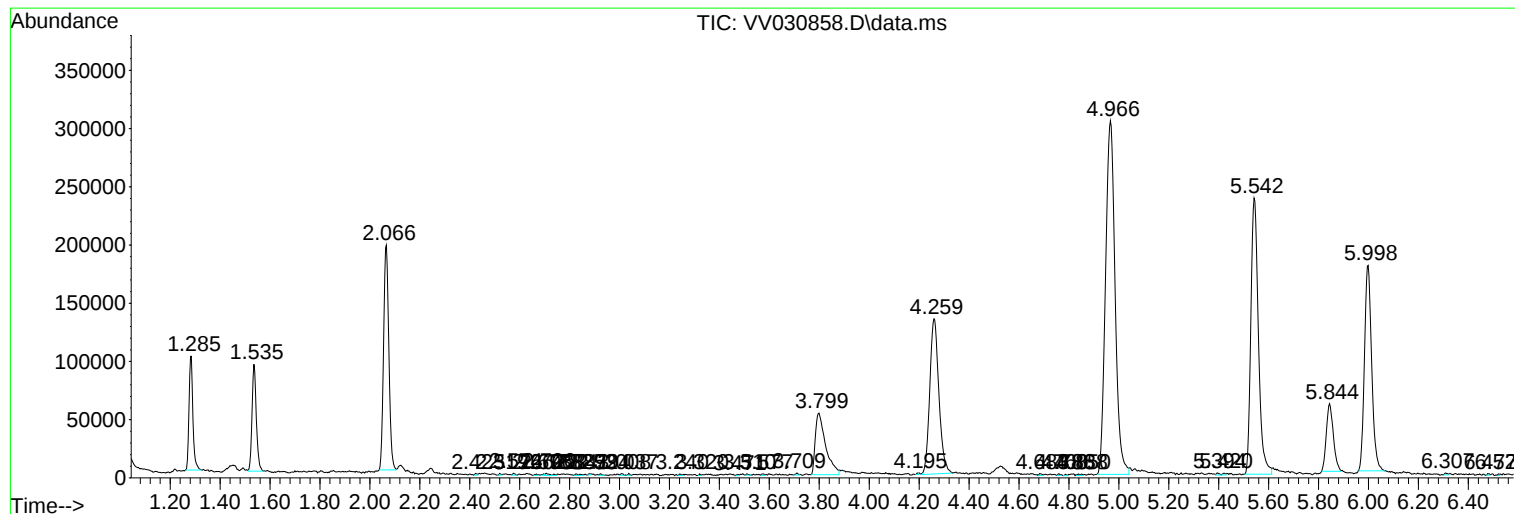

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042523\
Data File : VV030858.D
Acq On : 26 Apr 2023 00:19
Operator : SY/MD
Sample : 02474-09
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 37 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0AT1

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM041723WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042523\
Data File : VV030858.D
Acq On : 26 Apr 2023 00:19
Operator : SY/MD
Sample : 02474-09
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 37 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0AT1

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM041723WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------