

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042523\
 Data File : VV030860.D
 Acq On : 26 Apr 2023 01:07
 Operator : SY/MD
 Sample : 02474-11
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 39 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0AT3

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM041723WMA.M
 Title : VOC Analysis

Signal : TIC: VV030860.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.282	68	75	86	rBV	94106	103431	12.97%	1.666%
2	1.536	148	154	167	rVB	90867	103766	13.01%	1.672%
3	2.066	309	319	333	rBV	189397	277839	34.83%	4.476%
4	2.458	438	441	444	rVV4	1673	1176	0.15%	0.019%
5	2.491	449	451	453	rBV3	1003	514	0.06%	0.008%
6	2.684	509	511	513	rVV2	1177	549	0.07%	0.009%
7	2.761	533	535	538	rBV3	1241	587	0.07%	0.009%
8	2.847	560	562	563	rBV2	1022	521	0.07%	0.008%
9	2.902	576	579	583	rBV5	1512	1381	0.17%	0.022%
10	3.079	631	634	635	rBV	1194	657	0.08%	0.011%
11	3.102	639	641	646	rVB4	1482	932	0.12%	0.015%
12	3.198	668	671	673	rBV3	1315	730	0.09%	0.012%
13	3.253	685	688	689	rBV3	738	496	0.06%	0.008%
14	3.388	728	730	732	rVB3	1254	596	0.07%	0.010%
15	3.420	737	740	743	rBV4	1090	1019	0.13%	0.016%
16	3.658	807	814	815	rBV6	1208	1105	0.14%	0.018%
17	3.709	828	830	831	rBV2	1329	456	0.06%	0.007%
18	3.761	844	846	847	rBV2	878	399	0.05%	0.006%
19	3.799	849	858	880	rVV	52941	144928	18.17%	2.335%
20	4.259	988	1001	1023	rBV	129480	324830	40.72%	5.233%
21	4.465	1063	1065	1068	rBV5	1633	1081	0.14%	0.017%
22	4.632	1114	1117	1120	rBV4	1151	755	0.09%	0.012%
23	4.654	1120	1124	1125	rVV3	1013	635	0.08%	0.010%
24	4.767	1157	1159	1161	rBV3	1067	658	0.08%	0.011%
25	4.847	1182	1184	1188	rBV4	741	650	0.08%	0.010%
26	4.873	1190	1192	1194	rBV3	1001	501	0.06%	0.008%
27	4.966	1204	1221	1248	rBV3	299528	797635	100.00%	12.849%
28	5.413	1357	1360	1364	rBV5	1294	785	0.10%	0.013%
29	5.487	1379	1383	1386	rBV4	1510	1290	0.16%	0.021%
30	5.542	1388	1400	1423	rVV	256739	538537	67.52%	8.675%
31	5.896	1509	1510	1513	rBV3	1022	482	0.06%	0.008%
32	5.995	1530	1541	1565	rBV	175031	361997	45.38%	5.832%
33	6.240	1615	1617	1621	rBV5	1097	441	0.06%	0.007%
34	6.301	1633	1636	1637	rBV3	1113	543	0.07%	0.009%
35	6.397	1663	1666	1668	rBV5	1191	859	0.11%	0.014%
36	6.507	1696	1700	1703	rBV6	1254	939	0.12%	0.015%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW042523\
 Data File : VW030860.D
 Acq On : 26 Apr 2023 01:07
 Operator : SY/MD
 Sample : 02474-11
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 39 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0AT3

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM041723WMA.M
 Title : VOC Analysis

37	6.667	1746	1750	1756	rVB8	1230	1473	0.18%	0.024%
38	6.748	1771	1775	1777	rBV5	1282	898	0.11%	0.014%
39	6.780	1783	1785	1788	rBV2	732	564	0.07%	0.009%
40	6.825	1797	1799	1803	rBV5	1264	1140	0.14%	0.018%
41	6.921	1816	1829	1849	rBV	88738	174534	21.88%	2.812%
42	7.252	1920	1932	1956	rBV	337298	607890	76.21%	9.793%
43	7.561	2019	2028	2045	rBV	64452	115032	14.42%	1.853%
44	7.851	2116	2118	2123	rBV6	1366	1166	0.15%	0.019%
45	7.960	2147	2152	2153	rBV5	1628	1469	0.18%	0.024%
46	8.034	2166	2175	2204	rBV	149178	304946	38.23%	4.912%
47	8.555	2335	2337	2338	rBV	1373	550	0.07%	0.009%
48	8.703	2381	2383	2387	rBV4	1592	1154	0.14%	0.019%
49	8.793	2399	2411	2431	rBV	397969	667431	83.68%	10.752%
50	9.076	2494	2499	2501	rBV4	2098	2192	0.27%	0.035%
51	9.728	2696	2702	2703	rBV6	1742	1731	0.22%	0.028%
52	9.809	2724	2727	2728	rBV3	972	602	0.08%	0.010%
53	9.863	2738	2744	2745	rBV5	1236	1017	0.13%	0.016%
54	9.940	2766	2768	2770	rBV3	986	435	0.05%	0.007%
55	10.037	2793	2798	2801	rBV5	1825	1900	0.24%	0.031%
56	10.117	2821	2823	2825	rBV2	1985	867	0.11%	0.014%
57	10.159	2825	2836	2855	rVV	240688	389424	48.82%	6.273%
58	10.333	2885	2890	2901	rVB4	5883	10566	1.32%	0.170%
59	10.426	2916	2919	2923	rBV5	1006	842	0.11%	0.014%
60	10.461	2928	2930	2931	rBV2	1122	475	0.06%	0.008%
61	10.506	2942	2944	2946	rBV3	674	422	0.05%	0.007%
62	10.548	2954	2957	2959	rBV4	1689	1166	0.15%	0.019%
63	10.683	2997	2999	3000	rBV2	1188	575	0.07%	0.009%
64	10.783	3025	3030	3031	rBV3	1287	889	0.11%	0.014%
65	11.194	3146	3158	3176	rBV	396531	632618	79.31%	10.191%
66	11.313	3191	3195	3197	rBV4	1754	1417	0.18%	0.023%
67	11.567	3263	3274	3292	rBV	364331	582822	73.07%	9.389%
68	11.908	3378	3380	3383	rBV4	1040	474	0.06%	0.008%
69	11.947	3389	3392	3393	rVB2	1304	520	0.07%	0.008%
70	11.979	3400	3402	3404	rBV3	1388	581	0.07%	0.009%
71	12.111	3440	3443	3444	rBV3	1209	736	0.09%	0.012%
72	12.165	3457	3460	3461	rBV4	1020	672	0.08%	0.011%
73	12.281	3494	3496	3497	rBV2	997	490	0.06%	0.008%
74	12.477	3555	3557	3561	rBV3	1186	645	0.08%	0.010%
75	12.503	3561	3565	3568	rBV4	1102	1112	0.14%	0.018%
76	12.587	3588	3591	3592	rBV3	1258	726	0.09%	0.012%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042523\
 Data File : VV030860.D
 Acq On : 26 Apr 2023 01:07
 Operator : SY/MD
 Sample : 02474-11
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 39 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0AT3

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM041723WMA.M
 Title : VOC Analysis

77	12.670	3615	3617	3621	rVB2	990	629	0.08%	0.010%
78	12.715	3630	3631	3633	rBV2	1002	418	0.05%	0.007%
79	12.744	3637	3640	3641	rBV3	984	638	0.08%	0.010%
80	12.905	3688	3690	3691	rBV2	1087	418	0.05%	0.007%
81	12.966	3702	3709	3712	rBV6	1738	2077	0.26%	0.033%
82	13.014	3722	3724	3726	rBV3	1025	593	0.07%	0.010%
83	13.088	3744	3747	3748	rBV2	1374	757	0.09%	0.012%
84	13.143	3761	3764	3766	rBV4	1336	812	0.10%	0.013%
85	13.243	3793	3795	3797	rBV2	939	503	0.06%	0.008%
86	13.400	3841	3844	3845	rBV2	1422	704	0.09%	0.011%
87	13.410	3845	3847	3851	rVB4	1509	991	0.12%	0.016%
88	13.587	3900	3902	3904	rBV2	1151	654	0.08%	0.011%
89	13.609	3907	3909	3912	rBV3	817	599	0.08%	0.010%
90	13.818	3972	3974	3978	rBV5	869	507	0.06%	0.008%
91	13.879	3991	3993	3996	rBV4	1307	915	0.11%	0.015%
92	13.927	4006	4008	4011	rBV4	1142	672	0.08%	0.011%
93	14.021	4035	4037	4038	rBV2	1420	604	0.08%	0.010%
94	14.075	4049	4054	4057	rBV6	1809	1708	0.21%	0.028%
95	14.243	4104	4106	4110	rBV5	962	796	0.10%	0.013%
96	14.474	4174	4178	4179	rBV3	1232	783	0.10%	0.013%
97	14.686	4242	4244	4250	rBV6	1110	734	0.09%	0.012%
98	14.815	4281	4284	4285	rBV2	1491	922	0.12%	0.015%
99	14.850	4293	4295	4298	rBV3	1530	910	0.11%	0.015%
100	14.985	4336	4337	4343	rVB6	2174	1385	0.17%	0.022%

Sum of corrected areas: 6207592




Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042523\
Data File : VV030860.D
Acq On : 26 Apr 2023 01:07
Operator : SY/MD
Sample : 02474-11
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 39 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0AT3

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM041723WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L

TIC Integration Parameters: LSCINT.P

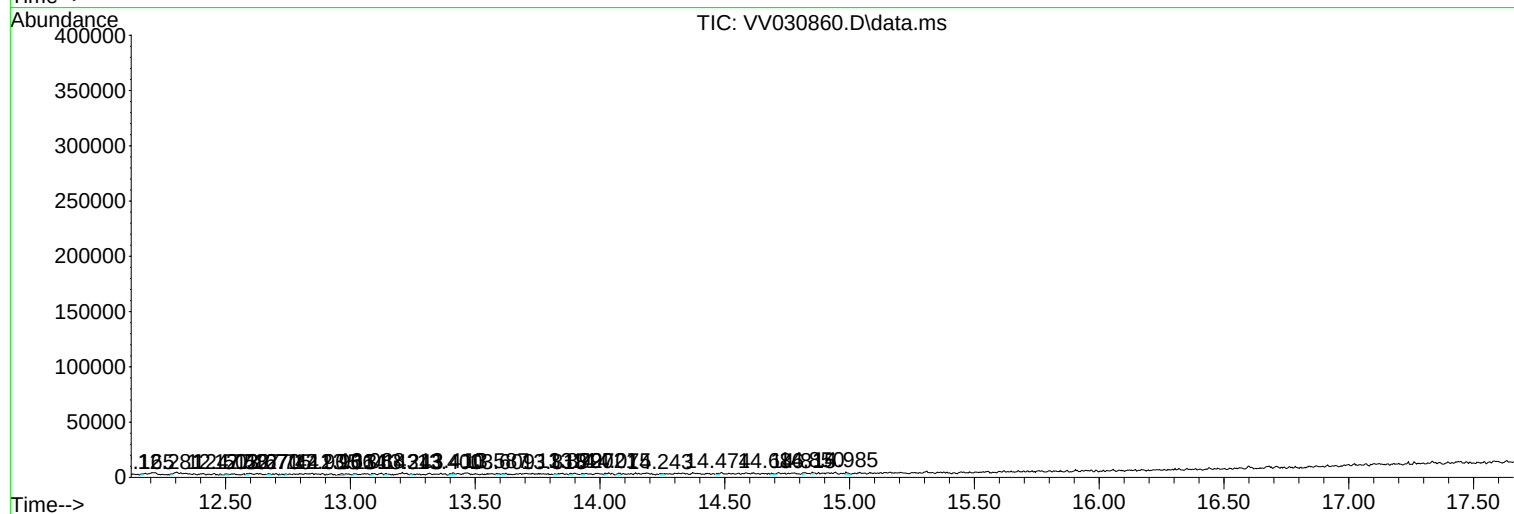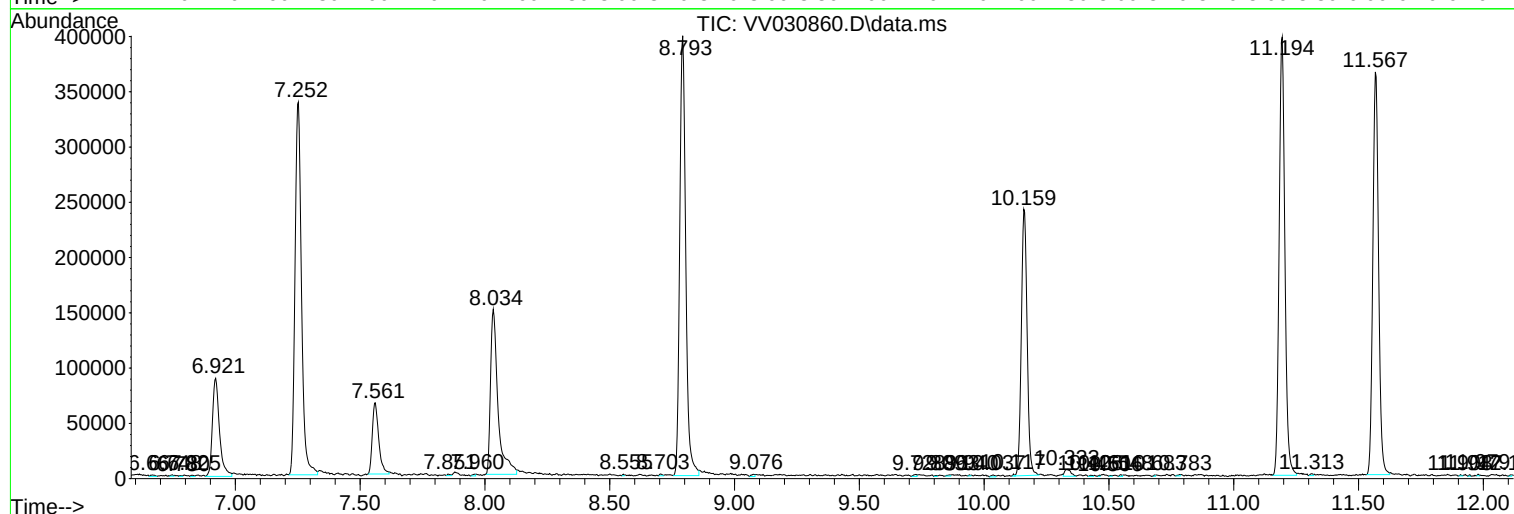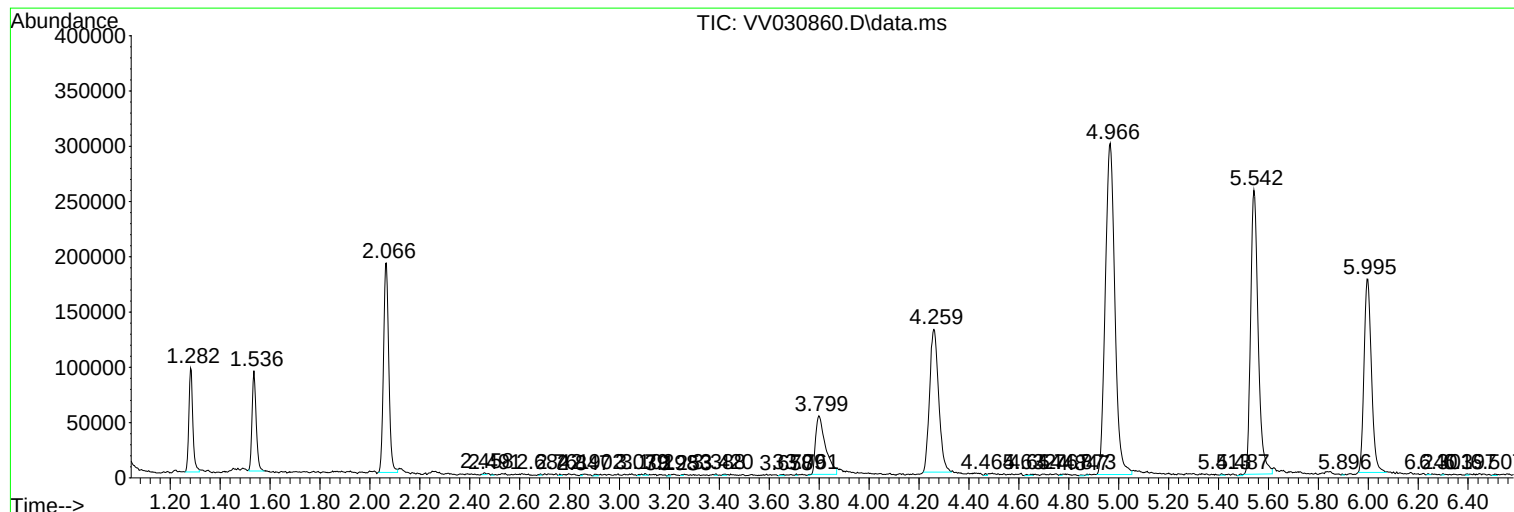

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042523\
Data File : VV030860.D
Acq On : 26 Apr 2023 01:07
Operator : SY/MD
Sample : 02474-11
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 39 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0AT3

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM041723WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042523\
Data File : VV030860.D
Acq On : 26 Apr 2023 01:07
Operator : SY/MD
Sample : 02474-11
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 39 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0AT3

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM041723WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------