

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042523\
 Data File : VV030862.D
 Acq On : 26 Apr 2023 01:55
 Operator : SY/MD
 Sample : 02474-13
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 41 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0AT5

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM041723WMA.M
 Title : VOC Analysis

Signal : TIC: VV030862.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.282	69	75	87	rBV	76278	82133	11.43%	1.459%
2	1.536	147	154	167	rVB	77843	93842	13.05%	1.667%
3	2.063	309	318	331	rBV	155950	227506	31.65%	4.040%
4	2.355	407	409	411	rBV3	957	572	0.08%	0.010%
5	2.658	499	503	506	rBV5	1354	1008	0.14%	0.018%
6	2.703	515	517	520	rBV4	1050	745	0.10%	0.013%
7	3.092	634	638	643	rVB7	1464	1621	0.23%	0.029%
8	3.118	643	646	651	rBV7	1256	1191	0.17%	0.021%
9	3.166	656	661	662	rBV5	1107	860	0.12%	0.015%
10	3.249	685	687	691	rBV3	1324	709	0.10%	0.013%
11	3.278	693	696	699	rVV4	1413	864	0.12%	0.015%
12	3.532	774	775	779	rVB3	1009	534	0.07%	0.009%
13	3.577	785	789	793	rBV7	1219	1046	0.15%	0.019%
14	3.619	799	802	804	rBV3	1162	825	0.11%	0.015%
15	3.661	813	815	821	rVB7	898	881	0.12%	0.016%
16	3.709	827	830	833	rBV5	680	485	0.07%	0.009%
17	3.799	846	858	881	rBV2	52774	156871	21.82%	2.786%
18	4.259	988	1001	1027	rVB	117018	296119	41.19%	5.259%
19	4.516	1078	1081	1084	rVB6	1690	1211	0.17%	0.022%
20	4.667	1125	1128	1131	rVB5	1623	950	0.13%	0.017%
21	4.683	1131	1133	1136	rBV4	1123	779	0.11%	0.014%
22	4.847	1183	1184	1187	rBV3	1165	806	0.11%	0.014%
23	4.966	1202	1221	1245	rBV3	265984	718884	100.00%	12.767%
24	5.394	1351	1354	1355	rBV3	966	562	0.08%	0.010%
25	5.542	1389	1400	1429	rBV	226205	475758	66.18%	8.449%
26	5.998	1529	1542	1563	rBV	162816	335808	46.71%	5.964%
27	6.352	1648	1652	1654	rBV5	1147	1081	0.15%	0.019%
28	6.455	1680	1684	1686	rBV4	1299	897	0.12%	0.016%
29	6.478	1689	1691	1694	rBV4	875	712	0.10%	0.013%
30	6.558	1713	1716	1717	rBV3	1354	795	0.11%	0.014%
31	6.658	1744	1747	1748	rBV3	1095	657	0.09%	0.012%
32	6.725	1766	1768	1772	rBV5	1164	592	0.08%	0.011%
33	6.863	1808	1811	1816	rBV7	2164	1733	0.24%	0.031%
34	6.921	1819	1829	1844	rBV	79609	150223	20.90%	2.668%
35	7.043	1865	1867	1869	rBV2	1349	545	0.08%	0.010%
36	7.146	1894	1899	1901	rBV6	1564	1436	0.20%	0.026%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW042523\
 Data File : VW030862.D
 Acq On : 26 Apr 2023 01:55
 Operator : SY/MD
 Sample : 02474-13
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 41 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0AT5

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM041723WMA.M
 Title : VOC Analysis

37	7.252	1920	1932	1959	rBV	295646	540679	75.21%	9.602%
38	7.561	2020	2028	2044	rBV	59164	99920	13.90%	1.775%
39	7.809	2103	2105	2108	rVB3	1369	677	0.09%	0.012%
40	7.873	2121	2125	2131	rBV6	2049	2529	0.35%	0.045%
41	7.931	2141	2143	2144	rBV2	1406	592	0.08%	0.011%
42	8.034	2165	2175	2206	rBV	155639	317625	44.18%	5.641%
43	8.542	2327	2333	2334	rBV4	1553	1239	0.17%	0.022%
44	8.793	2400	2411	2433	rBV	352812	598507	83.26%	10.629%
45	9.088	2501	2503	2506	rVB4	1388	506	0.07%	0.009%
46	9.233	2543	2548	2550	rBV6	1286	1223	0.17%	0.022%
47	9.423	2603	2607	2614	rVV9	1842	2478	0.34%	0.044%
48	9.513	2633	2635	2637	rBV4	1054	550	0.08%	0.010%
49	9.715	2695	2698	2700	rBV3	1585	998	0.14%	0.018%
50	9.728	2700	2702	2705	rBV3	600	498	0.07%	0.009%
51	9.953	2769	2772	2774	rBV4	1152	525	0.07%	0.009%
52	10.005	2786	2788	2792	rVB4	935	678	0.09%	0.012%
53	10.043	2796	2800	2802	rVB4	910	666	0.09%	0.012%
54	10.159	2825	2836	2853	rBV	229925	372901	51.87%	6.623%
55	10.326	2882	2888	2890	rBV5	3972	3992	0.56%	0.071%
56	10.445	2923	2925	2929	rVB5	1076	786	0.11%	0.014%
57	10.625	2978	2981	2984	rBV5	1432	1255	0.17%	0.022%
58	10.690	2998	3001	3007	rVB7	2068	1743	0.24%	0.031%
59	10.767	3022	3025	3027	rBV4	1344	592	0.08%	0.011%
60	10.854	3050	3052	3055	rBV4	1405	692	0.10%	0.012%
61	10.911	3066	3070	3072	rVB4	1614	874	0.12%	0.016%
62	10.927	3072	3075	3077	rBV4	2016	1149	0.16%	0.020%
63	11.072	3115	3120	3123	rBV7	1233	1222	0.17%	0.022%
64	11.194	3146	3158	3175	rBV	354313	561630	78.13%	9.974%
65	11.493	3249	3251	3254	rVB3	1400	615	0.09%	0.011%
66	11.509	3254	3256	3258	rBV4	1123	673	0.09%	0.012%
67	11.567	3263	3274	3290	rVV	322681	522331	72.66%	9.276%
68	11.763	3333	3335	3340	rVB5	1348	951	0.13%	0.017%
69	11.792	3340	3344	3348	rBV6	1831	1546	0.22%	0.027%
70	11.866	3364	3367	3371	rBV6	1243	1099	0.15%	0.020%
71	11.924	3381	3385	3387	rBV4	1020	699	0.10%	0.012%
72	11.985	3401	3404	3407	rBV4	2089	1239	0.17%	0.022%
73	12.001	3407	3409	3411	rBV3	1137	731	0.10%	0.013%
74	12.037	3417	3420	3422	rBV5	916	537	0.07%	0.010%
75	12.198	3467	3470	3472	rBV3	1167	718	0.10%	0.013%
76	12.297	3499	3501	3502	rBV2	1977	875	0.12%	0.016%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042523\
 Data File : VV030862.D
 Acq On : 26 Apr 2023 01:55
 Operator : SY/MD
 Sample : 02474-13
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 41 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0AT5

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM041723WMA.M
 Title : VOC Analysis

77	12.349	3514	3517	3520	rBV3	771	569	0.08%	0.010%
78	12.503	3563	3565	3568	rBV3	1162	701	0.10%	0.012%
79	12.567	3583	3585	3588	rBV4	1083	605	0.08%	0.011%
80	12.599	3592	3595	3599	rVB4	1801	1082	0.15%	0.019%
81	12.670	3614	3617	3618	rBV2	1291	685	0.10%	0.012%
82	12.792	3652	3655	3658	rBV4	1193	942	0.13%	0.017%
83	12.960	3705	3707	3709	rVB3	1909	679	0.09%	0.012%
84	13.072	3739	3742	3745	rVB4	1540	922	0.13%	0.016%
85	13.088	3745	3747	3752	rBV6	1022	941	0.13%	0.017%
86	13.275	3803	3805	3806	rBV2	1153	545	0.08%	0.010%
87	13.419	3847	3850	3852	rVB3	1526	778	0.11%	0.014%
88	13.487	3868	3871	3872	rBV3	1589	811	0.11%	0.014%
89	13.525	3881	3883	3886	rBV3	1106	474	0.07%	0.008%
90	13.609	3907	3909	3913	rVB3	1644	985	0.14%	0.017%
91	13.628	3913	3915	3916	rBV2	909	492	0.07%	0.009%
92	13.763	3955	3957	3961	rBV4	1375	814	0.11%	0.014%
93	13.853	3982	3985	3990	rBV8	1657	1512	0.21%	0.027%
94	13.924	4005	4007	4011	rVB5	947	605	0.08%	0.011%
95	13.947	4011	4014	4018	rBV4	1402	1167	0.16%	0.021%
96	13.998	4028	4030	4033	rVB2	1145	571	0.08%	0.010%
97	14.143	4071	4075	4081	rBV8	1319	1295	0.18%	0.023%
98	14.442	4164	4168	4169	rBV4	1522	917	0.13%	0.016%
99	14.898	4306	4310	4315	rBV8	1688	1834	0.26%	0.033%
100	15.291	4430	4432	4435	rBV3	1321	810	0.11%	0.014%

Sum of corrected areas: 5630717




Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042523\
Data File : VV030862.D
Acq On : 26 Apr 2023 01:55
Operator : SY/MD
Sample : 02474-13
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 41 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0AT5

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM041723WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L

TIC Integration Parameters: LSCINT.P

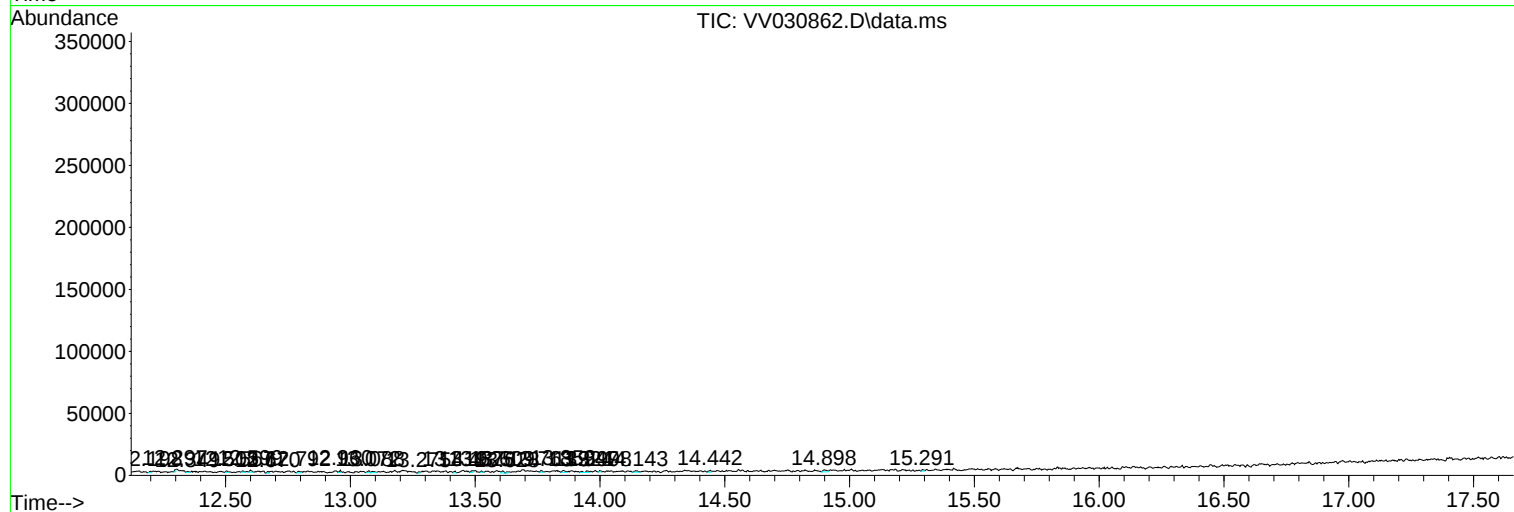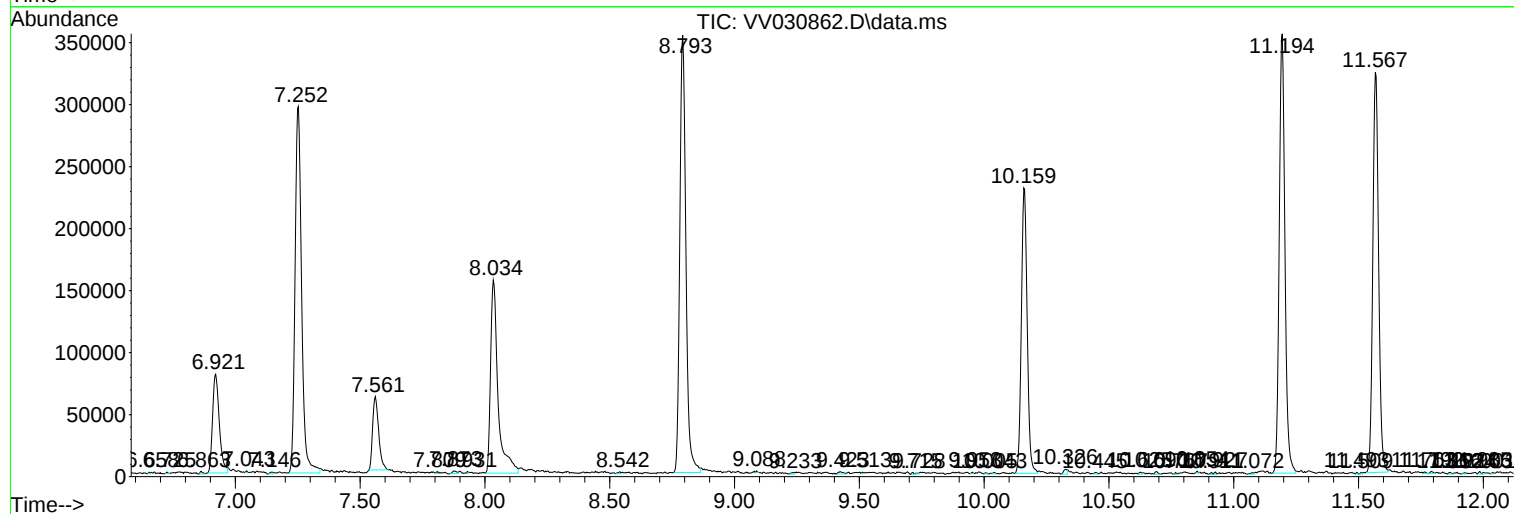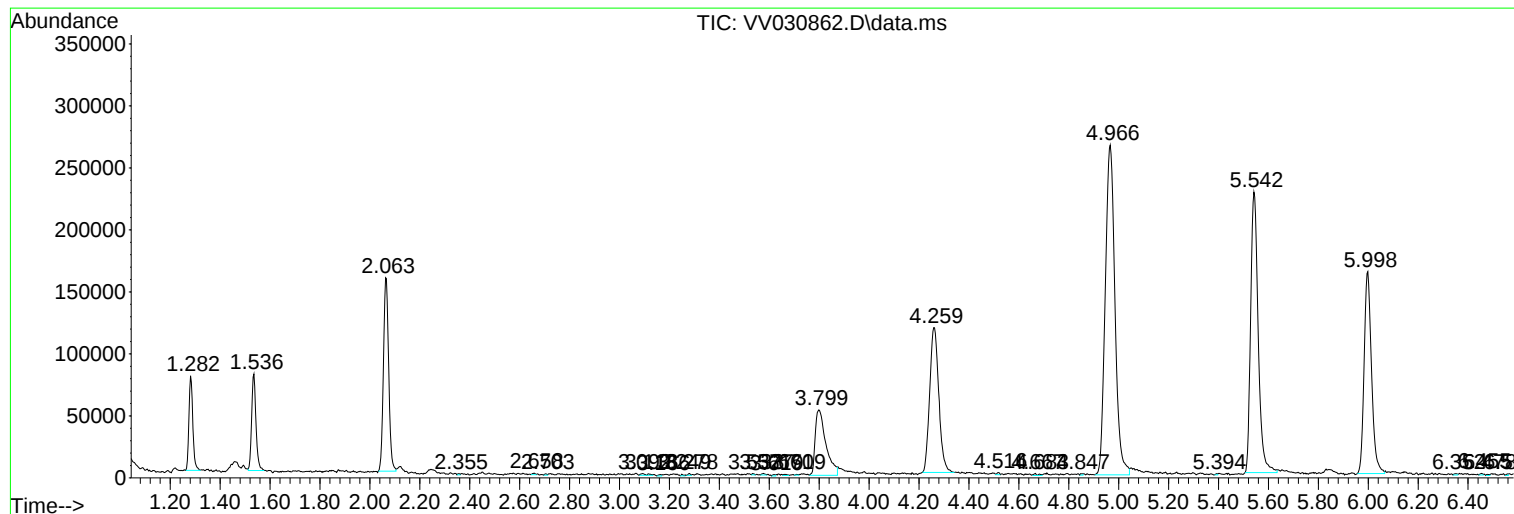

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042523\
Data File : VV030862.D
Acq On : 26 Apr 2023 01:55
Operator : SY/MD
Sample : 02474-13
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 41 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0AT5

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM041723WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042523\
Data File : VV030862.D
Acq On : 26 Apr 2023 01:55
Operator : SY/MD
Sample : 02474-13
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 41 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0AT5

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM041723WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc