

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042523\
 Data File : VV030864.D
 Acq On : 26 Apr 2023 02:43
 Operator : SY/MD
 Sample : 02474-18
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 43 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0AW0

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM041723WMA.M
 Title : VOC Analysis

Signal : TIC: VV030864.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.281	69	75	87	rBV	107959	117873	14.74%	1.889%
2	1.535	147	154	167	rVB	85290	102751	12.85%	1.646%
3	2.066	310	319	330	rBV	185359	266935	33.39%	4.277%
4	2.243	364	374	379	rBV9	3973	7626	0.95%	0.122%
5	2.635	494	496	498	rBV2	1074	565	0.07%	0.009%
6	2.690	510	513	515	rBV3	1566	1109	0.14%	0.018%
7	2.751	529	532	536	rBV6	706	497	0.06%	0.008%
8	2.947	590	593	595	rBV3	772	483	0.06%	0.008%
9	3.130	646	650	653	rBV5	1645	1561	0.20%	0.025%
10	3.252	687	688	692	rVB4	951	393	0.05%	0.006%
11	3.355	717	720	723	rBV4	1448	1108	0.14%	0.018%
12	3.458	750	752	753	rBV2	1138	475	0.06%	0.008%
13	3.632	804	806	809	rVB4	1283	729	0.09%	0.012%
14	3.690	822	824	828	rBV5	960	608	0.08%	0.010%
15	3.731	834	837	838	rBV3	1338	873	0.11%	0.014%
16	3.799	847	858	884	rBV2	49671	149076	18.65%	2.389%
17	3.973	908	912	915	rBV6	1924	1756	0.22%	0.028%
18	4.259	985	1001	1022	rBV2	129968	332668	41.61%	5.331%
19	4.519	1079	1082	1087	rBV6	1257	1304	0.16%	0.021%
20	4.725	1141	1146	1148	rBV4	1293	1165	0.15%	0.019%
21	4.966	1203	1221	1250	rBV2	296266	799456	100.00%	12.810%
22	5.323	1330	1332	1336	rVB5	1437	1018	0.13%	0.016%
23	5.461	1371	1375	1377	rBV4	1349	840	0.11%	0.013%
24	5.542	1388	1400	1422	rBV	258527	541457	67.73%	8.676%
25	5.998	1530	1542	1568	rBV2	176167	364241	45.56%	5.836%
26	6.252	1617	1621	1624	rBV5	1280	1019	0.13%	0.016%
27	6.272	1624	1627	1629	rBV3	1197	868	0.11%	0.014%
28	6.394	1663	1665	1668	rBV4	979	455	0.06%	0.007%
29	6.638	1737	1741	1743	rBV4	1500	1241	0.16%	0.020%
30	6.921	1817	1829	1844	rBV	89854	169339	21.18%	2.713%
31	7.101	1882	1885	1890	rVB7	1906	1550	0.19%	0.025%
32	7.127	1890	1893	1896	rBV5	1399	1203	0.15%	0.019%
33	7.252	1920	1932	1952	rBV	340837	601721	75.27%	9.642%
34	7.558	2019	2027	2044	rBV	63981	114584	14.33%	1.836%
35	7.841	2113	2115	2117	rBV3	918	528	0.07%	0.008%
36	8.034	2165	2175	2207	rBV	151668	318033	39.78%	5.096%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW042523\
 Data File : VW030864.D
 Acq On : 26 Apr 2023 02:43
 Operator : SY/MD
 Sample : 02474-18
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 43 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0AW0

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM041723WMA.M
 Title : VOC Analysis

37	8.587	2345	2347	2348	rBV3	1219	576	0.07%	0.009%
38	8.648	2363	2366	2370	rBV5	997	974	0.12%	0.016%
39	8.680	2374	2376	2380	rVB5	941	544	0.07%	0.009%
40	8.712	2380	2386	2387	rBV6	1645	1179	0.15%	0.019%
41	8.792	2400	2411	2430	rBV	404286	666795	83.41%	10.684%
42	9.310	2570	2572	2578	rBV7	879	732	0.09%	0.012%
43	9.342	2578	2582	2584	rBV5	1162	950	0.12%	0.015%
44	9.432	2608	2610	2612	rBV3	1625	776	0.10%	0.012%
45	9.455	2615	2617	2620	rVB4	896	452	0.06%	0.007%
46	9.490	2625	2628	2629	rBV2	1265	628	0.08%	0.010%
47	9.693	2688	2691	2695	rBV5	1182	929	0.12%	0.015%
48	9.982	2777	2781	2783	rVV5	954	777	0.10%	0.012%
49	10.079	2808	2811	2813	rVB4	1182	648	0.08%	0.010%
50	10.095	2813	2816	2818	rBV4	846	399	0.05%	0.006%
51	10.159	2824	2836	2855	rBV	239497	391916	49.02%	6.280%
52	10.468	2928	2932	2933	rBV4	1014	627	0.08%	0.010%
53	10.577	2963	2966	2967	rBV3	1693	801	0.10%	0.013%
54	10.667	2989	2994	2998	rBV8	1768	1728	0.22%	0.028%
55	10.686	2998	3000	3003	rVB5	1120	587	0.07%	0.009%
56	10.722	3009	3011	3013	rVB2	1262	479	0.06%	0.008%
57	10.799	3033	3035	3037	rBV3	948	463	0.06%	0.007%
58	10.959	3083	3085	3088	rVB3	755	387	0.05%	0.006%
59	10.992	3092	3095	3099	rBV5	780	588	0.07%	0.009%
60	11.043	3108	3111	3112	rBV3	936	501	0.06%	0.008%
61	11.078	3119	3122	3125	rBV5	1790	1381	0.17%	0.022%
62	11.111	3125	3132	3135	rBV7	2673	3694	0.46%	0.059%
63	11.194	3144	3158	3177	rBV	403801	645005	80.68%	10.335%
64	11.397	3216	3221	3222	rBV4	1669	1207	0.15%	0.019%
65	11.477	3242	3246	3247	rBV3	1406	828	0.10%	0.013%
66	11.525	3257	3261	3262	rBV5	1126	839	0.10%	0.013%
67	11.567	3264	3274	3292	rVV	365506	582230	72.83%	9.329%
68	11.815	3348	3351	3352	rBV3	774	544	0.07%	0.009%
69	11.976	3399	3401	3404	rBV3	1142	702	0.09%	0.011%
70	11.992	3404	3406	3408	rVV3	1278	391	0.05%	0.006%
71	12.008	3408	3411	3413	rVB3	1207	643	0.08%	0.010%
72	12.156	3454	3457	3461	rVB5	1384	992	0.12%	0.016%
73	12.178	3461	3464	3465	rBV4	907	617	0.08%	0.010%
74	12.197	3466	3470	3472	rBV4	1639	1177	0.15%	0.019%
75	12.230	3477	3480	3485	rVB7	1626	979	0.12%	0.016%
76	12.271	3488	3493	3494	rBV5	1629	1139	0.14%	0.018%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042523\
 Data File : VV030864.D
 Acq On : 26 Apr 2023 02:43
 Operator : SY/MD
 Sample : 02474-18
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 43 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0AW0

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM041723WMA.M
 Title : VOC Analysis

77	12.397	3529	3532	3534	rBV4	1130	586	0.07%	0.009%
78	12.509	3565	3567	3569	rVB3	994	400	0.05%	0.006%
79	12.551	3578	3580	3583	rVB4	1232	652	0.08%	0.010%
80	12.609	3596	3598	3600	rBV3	1186	499	0.06%	0.008%
81	12.783	3650	3652	3655	rBV3	900	571	0.07%	0.009%
82	12.850	3671	3673	3676	rVB3	1260	609	0.08%	0.010%
83	12.876	3678	3681	3686	rBV4	1180	1297	0.16%	0.021%
84	12.924	3694	3696	3698	rBV4	1116	649	0.08%	0.010%
85	12.953	3702	3705	3708	rBV3	1726	921	0.12%	0.015%
86	13.030	3727	3729	3731	rVB2	1150	440	0.06%	0.007%
87	13.239	3792	3794	3796	rBV2	1156	467	0.06%	0.007%
88	13.291	3806	3810	3811	rBV3	1874	987	0.12%	0.016%
89	13.320	3815	3819	3820	rVV3	958	616	0.08%	0.010%
90	13.345	3824	3827	3829	rBV3	1168	584	0.07%	0.009%
91	13.397	3841	3843	3848	rBV5	1132	1049	0.13%	0.017%
92	13.426	3848	3852	3853	rBV4	801	616	0.08%	0.010%
93	13.484	3868	3870	3873	rBV3	942	600	0.08%	0.010%
94	13.551	3889	3891	3893	rVB3	1113	397	0.05%	0.006%
95	13.567	3893	3896	3899	rBV5	938	591	0.07%	0.009%
96	13.705	3938	3939	3942	rVB3	1555	544	0.07%	0.009%
97	14.110	4064	4065	4067	rBV2	1267	565	0.07%	0.009%
98	14.168	4080	4083	4084	rBV4	1854	932	0.12%	0.015%
99	14.323	4129	4131	4133	rBV3	1499	797	0.10%	0.013%
100	14.554	4199	4203	4206	rBV6	1806	1548	0.19%	0.025%




Sum of corrected areas: 6240829

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042523\
Data File : VV030864.D
Acq On : 26 Apr 2023 02:43
Operator : SY/MD
Sample : 02474-18
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 43 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0AW0

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM041723WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

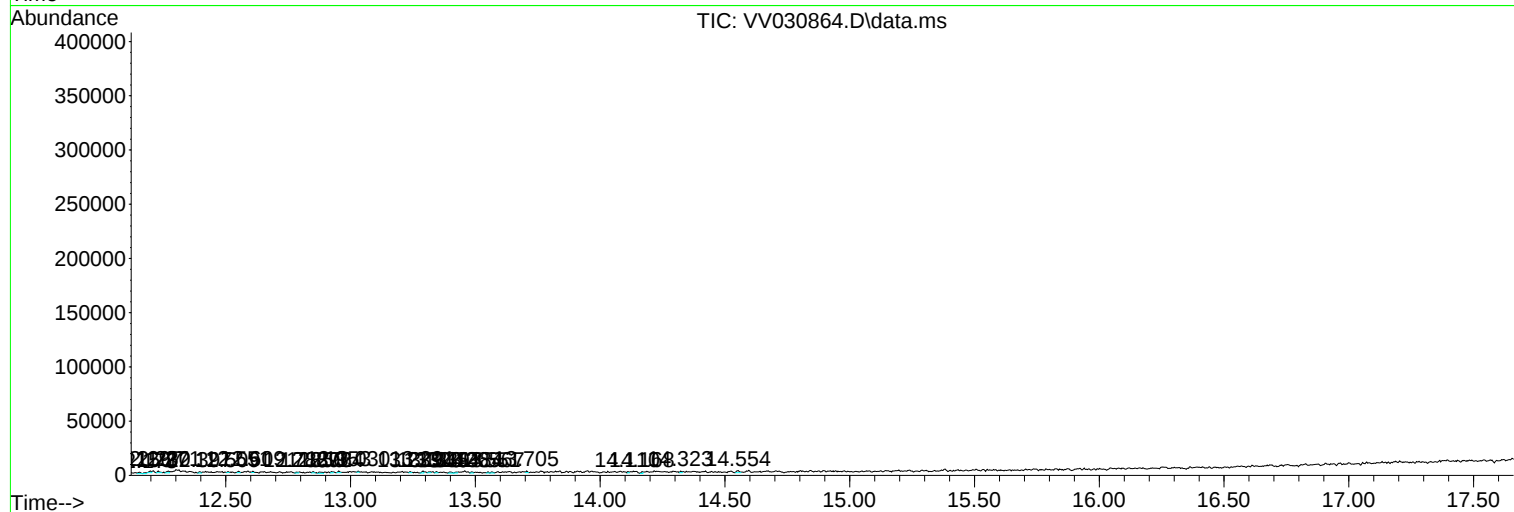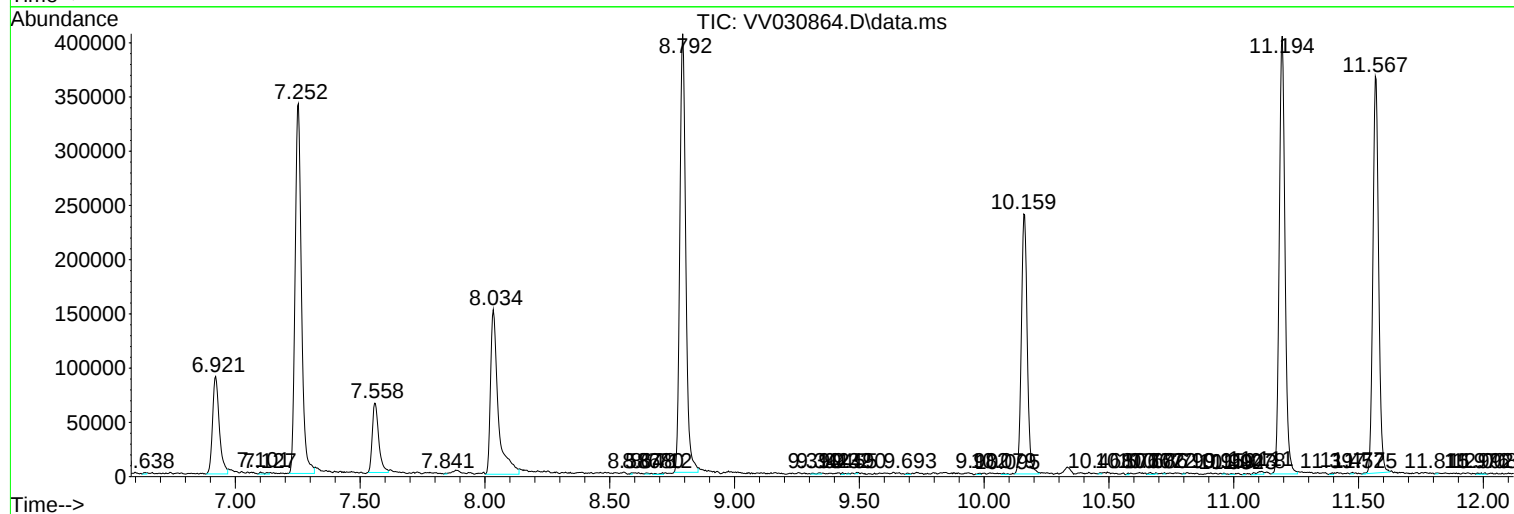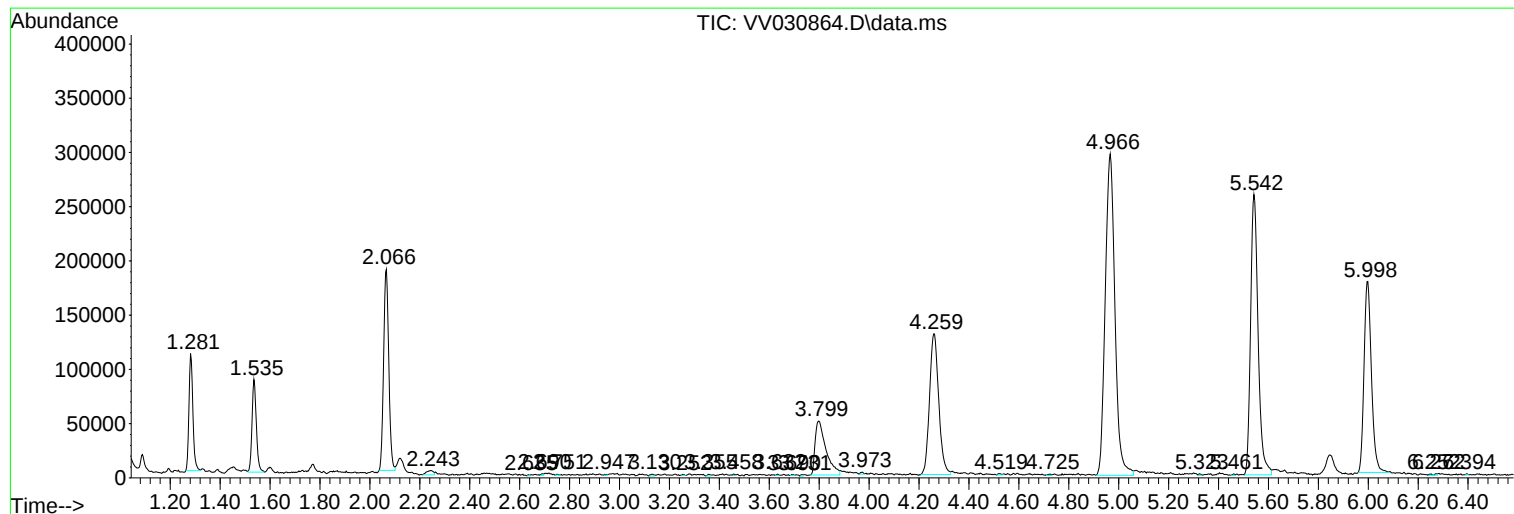

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042523\
Data File : VV030864.D
Acq On : 26 Apr 2023 02:43
Operator : SY/MD
Sample : 02474-18
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 43 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0AW0

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM041723WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042523\
Data File : VV030864.D
Acq On : 26 Apr 2023 02:43
Operator : SY/MD
Sample : 02474-18
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 43 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0AW0

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM041723WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------