

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042523\
 Data File : VV030865.D
 Acq On : 26 Apr 2023 03:07
 Operator : SY/MD
 Sample : 02474-19
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 44 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0AW1

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM041723WMA.M
 Title : VOC Analysis

Signal : TIC: VV030865.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.281	69	75	87	rBV	95189	101996	12.79%	1.605%
2	1.535	148	154	167	rVB	83788	103177	12.94%	1.624%
3	2.066	309	319	331	rBV	186720	276560	34.69%	4.352%
4	2.542	463	467	469	rBV4	1307	1037	0.13%	0.016%
5	2.722	521	523	525	rVB3	1487	572	0.07%	0.009%
6	2.738	525	528	532	rBV5	1283	1035	0.13%	0.016%
7	3.005	607	611	613	rBV4	1088	685	0.09%	0.011%
8	3.063	625	629	635	rBV8	1432	1674	0.21%	0.026%
9	3.088	635	637	640	rBV4	923	641	0.08%	0.010%
10	3.304	700	704	705	rBV3	1201	557	0.07%	0.009%
11	3.400	731	734	736	rBV4	1295	725	0.09%	0.011%
12	3.468	753	755	758	rBV4	1186	608	0.08%	0.010%
13	3.542	774	778	781	rVB6	1267	782	0.10%	0.012%
14	3.632	803	806	809	rBV4	1513	1125	0.14%	0.018%
15	3.709	828	830	833	rBV5	1057	615	0.08%	0.010%
16	3.799	848	858	882	rBV	51996	145537	18.25%	2.290%
17	4.185	975	978	981	rBV4	1333	955	0.12%	0.015%
18	4.259	987	1001	1023	rBV	131193	331240	41.54%	5.212%
19	4.619	1109	1113	1116	rVB6	1677	1057	0.13%	0.017%
20	4.658	1122	1125	1129	rBV6	1399	1025	0.13%	0.016%
21	4.683	1132	1133	1137	rBV3	956	541	0.07%	0.009%
22	4.815	1172	1174	1178	rBV6	1182	741	0.09%	0.012%
23	4.841	1178	1182	1185	rBV6	982	771	0.10%	0.012%
24	4.966	1204	1221	1248	rBV2	296451	797344	100.00%	12.547%
25	5.227	1298	1302	1304	rBV5	1410	977	0.12%	0.015%
26	5.304	1324	1326	1328	rVB3	1350	712	0.09%	0.011%
27	5.317	1328	1330	1331	rBV2	1407	572	0.07%	0.009%
28	5.426	1360	1364	1367	rBV6	1975	1574	0.20%	0.025%
29	5.542	1386	1400	1419	rBV	261265	545973	68.47%	8.591%
30	5.844	1482	1494	1509	rBV2	66987	137886	17.29%	2.170%
31	5.998	1530	1542	1565	rBV	176542	366049	45.91%	5.760%
32	6.252	1619	1621	1625	rVB5	1413	625	0.08%	0.010%
33	6.307	1636	1638	1641	rBV3	1282	902	0.11%	0.014%
34	6.442	1675	1680	1682	rBV6	1453	1183	0.15%	0.019%
35	6.783	1784	1786	1789	rVB4	1321	737	0.09%	0.012%
36	6.857	1804	1809	1811	rVB5	1426	1100	0.14%	0.017%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW042523\
 Data File : VW030865.D
 Acq On : 26 Apr 2023 03:07
 Operator : SY/MD
 Sample : 02474-19
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 44 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0AW1

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM041723WMA.M
 Title : VOC Analysis

37	6.870	1811	1813	1817	rBV5	1035	576	0.07%	0.009%
38	6.921	1817	1829	1843	rBV	89564	167740	21.04%	2.640%
39	7.252	1921	1932	1962	rBV	339179	603655	75.71%	9.499%
40	7.464	1993	1998	2000	rBV6	1274	1228	0.15%	0.019%
41	7.561	2019	2028	2044	rBV	65137	115171	14.44%	1.812%
42	7.780	2094	2096	2100	rBV4	1284	809	0.10%	0.013%
43	7.831	2110	2112	2114	rBV3	1141	631	0.08%	0.010%
44	7.995	2157	2163	2165	rBV6	1205	1122	0.14%	0.018%
45	8.034	2165	2175	2192	rBV	152966	296018	37.13%	4.658%
46	8.307	2257	2260	2262	rBV4	911	594	0.07%	0.009%
47	8.323	2262	2265	2266	rBV3	1436	666	0.08%	0.010%
48	8.442	2299	2302	2307	rVB7	2083	1534	0.19%	0.024%
49	8.468	2307	2310	2312	rBV4	932	681	0.09%	0.011%
50	8.571	2340	2342	2344	rBV3	1300	691	0.09%	0.011%
51	8.792	2397	2411	2431	rBV	396831	673131	84.42%	10.592%
52	9.062	2492	2495	2499	rBV5	1369	1012	0.13%	0.016%
53	9.271	2555	2560	2564	rBV6	1611	1900	0.24%	0.030%
54	9.307	2569	2571	2572	rBV2	1605	636	0.08%	0.010%
55	9.384	2591	2595	2596	rBV3	745	647	0.08%	0.010%
56	9.471	2620	2622	2626	rVB5	1205	673	0.08%	0.011%
57	9.583	2655	2657	2660	rBV4	1020	733	0.09%	0.012%
58	9.683	2685	2688	2691	rBV4	1174	540	0.07%	0.008%
59	9.789	2718	2721	2723	rBV2	1299	725	0.09%	0.011%
60	9.870	2741	2746	2748	rBV5	1185	1158	0.15%	0.018%
61	9.902	2752	2756	2759	rVB5	1466	985	0.12%	0.015%
62	10.159	2826	2836	2853	rBV	243434	385635	48.36%	6.068%
63	10.333	2884	2890	2901	rVB5	5022	7255	0.91%	0.114%
64	10.426	2917	2919	2921	rVB3	1900	950	0.12%	0.015%
65	10.442	2921	2924	2926	rBV4	1622	1101	0.14%	0.017%
66	10.461	2928	2930	2933	rVB4	1201	595	0.07%	0.009%
67	10.519	2946	2948	2949	rBV2	1441	562	0.07%	0.009%
68	10.577	2963	2966	2968	rBV4	894	561	0.07%	0.009%
69	10.622	2973	2980	2981	rBV6	1460	1180	0.15%	0.019%
70	10.648	2985	2988	2989	rBV2	1325	865	0.11%	0.014%
71	10.673	2993	2996	2997	rBV3	1163	691	0.09%	0.011%
72	10.857	3050	3053	3055	rBV4	947	769	0.10%	0.012%
73	10.960	3083	3085	3088	rBV4	1366	763	0.10%	0.012%
74	11.091	3121	3126	3128	rBV6	1701	1313	0.16%	0.021%
75	11.130	3135	3138	3141	rBV5	1342	821	0.10%	0.013%
76	11.194	3146	3158	3180	rVV	402324	637890	80.00%	10.038%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042523\
 Data File : VV030865.D
 Acq On : 26 Apr 2023 03:07
 Operator : SY/MD
 Sample : 02474-19
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 44 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0AW1

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM041723WMA.M
 Title : VOC Analysis

77	11.361	3208	3210	3212	rBV3	1534	730	0.09%	0.011%
78	11.429	3228	3231	3236	rVB5	1395	1108	0.14%	0.017%
79	11.451	3236	3238	3241	rBV4	1458	990	0.12%	0.016%
80	11.567	3263	3274	3295	rBV	365997	590935	74.11%	9.299%
81	11.731	3323	3325	3328	rBV4	1381	712	0.09%	0.011%
82	11.943	3387	3391	3395	rBV5	1737	1404	0.18%	0.022%
83	12.004	3408	3410	3414	rVB4	1681	979	0.12%	0.015%
84	12.030	3416	3418	3421	rBV4	929	578	0.07%	0.009%
85	12.162	3456	3459	3462	rBV6	1619	1119	0.14%	0.018%
86	12.284	3494	3497	3498	rBV4	1466	836	0.10%	0.013%
87	12.461	3549	3552	3555	rBV5	1012	803	0.10%	0.013%
88	12.583	3587	3590	3592	rBV3	847	550	0.07%	0.009%
89	12.738	3636	3638	3641	rBV4	1652	873	0.11%	0.014%
90	12.947	3699	3703	3705	rBV5	1277	866	0.11%	0.014%
91	13.069	3738	3741	3743	rBV4	1534	916	0.11%	0.014%
92	13.098	3747	3750	3755	rBV6	1338	1221	0.15%	0.019%
93	13.445	3856	3858	3860	rBV3	1613	701	0.09%	0.011%
94	13.519	3878	3881	3885	rBV6	960	728	0.09%	0.011%
95	13.696	3935	3936	3938	rBV2	1028	537	0.07%	0.008%
96	13.763	3955	3957	3960	rBV3	1347	855	0.11%	0.013%
97	13.898	3997	3999	4001	rBV3	1464	814	0.10%	0.013%
98	13.979	4020	4024	4027	rBV6	1567	1396	0.18%	0.022%
99	14.008	4031	4033	4036	rVB4	1050	606	0.08%	0.010%
100	14.529	4194	4195	4203	rVB6	1557	1169	0.15%	0.018%




Sum of corrected areas: 6354923

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042523\
Data File : VV030865.D
Acq On : 26 Apr 2023 03:07
Operator : SY/MD
Sample : 02474-19
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 44 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0AW1

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM041723WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

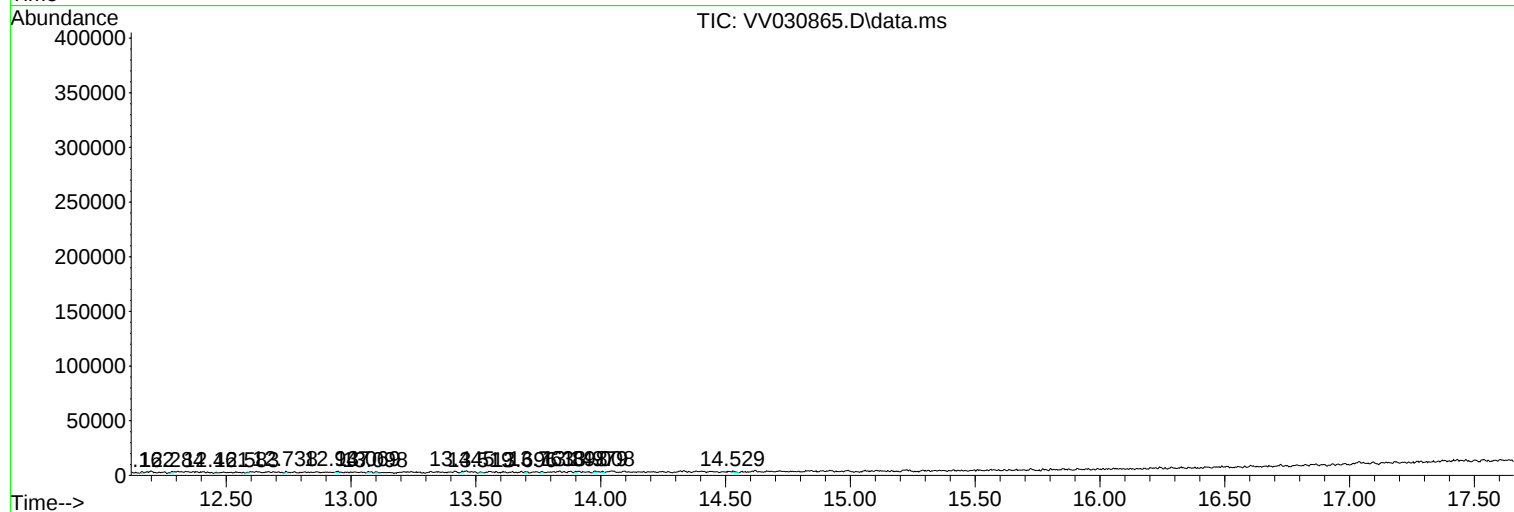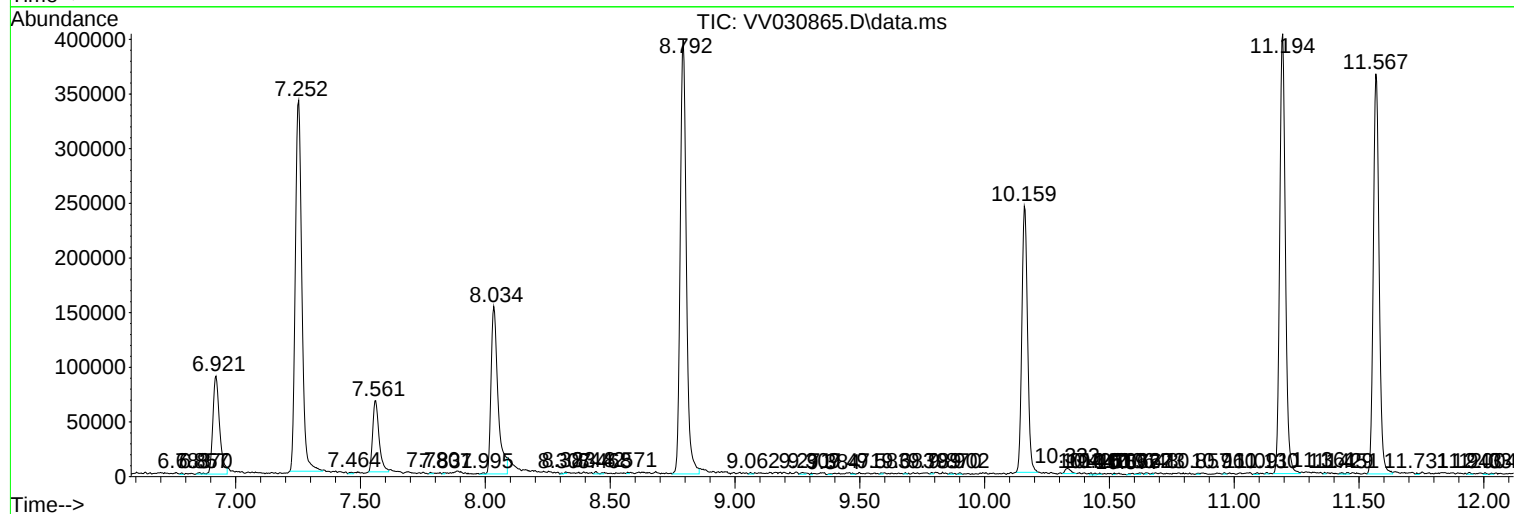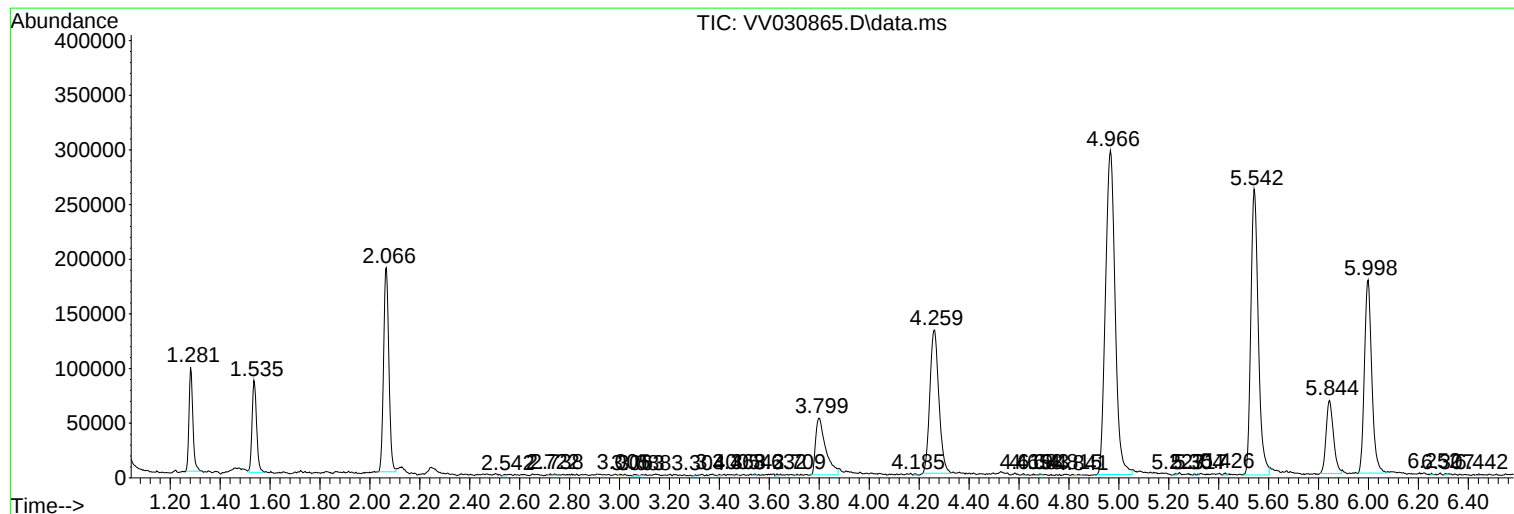

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042523\
Data File : VV030865.D
Acq On : 26 Apr 2023 03:07
Operator : SY/MD
Sample : 02474-19
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 44 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0AW1

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM041723WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042523\
Data File : VV030865.D
Acq On : 26 Apr 2023 03:07
Operator : SY/MD
Sample : 02474-19
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 44 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0AW1

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM041723WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------