

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042523\
 Data File : VV030866.D
 Acq On : 26 Apr 2023 03:31
 Operator : SY/MD
 Sample : 02474-20
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 45 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0AW2

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM041723WMA.M
 Title : VOC Analysis

Signal : TIC: VV030866.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.281	69	75	90	rBV	92322	99719	12.64%	1.482%
2	1.539	148	155	166	rVB	84506	102472	12.99%	1.523%
3	2.066	309	319	332	rBV	191007	282619	35.82%	4.200%
4	2.648	498	500	503	rBV4	1138	740	0.09%	0.011%
5	2.696	514	515	518	rBV2	1378	857	0.11%	0.013%
6	2.735	523	527	530	rBV5	1546	1194	0.15%	0.018%
7	2.770	535	538	540	rBV3	1974	1200	0.15%	0.018%
8	2.879	568	572	574	rBV6	1793	1069	0.14%	0.016%
9	2.973	592	601	606	rBV9	1949	3076	0.39%	0.046%
10	3.050	622	625	626	rBV3	1048	551	0.07%	0.008%
11	3.207	669	674	675	rBV5	1262	883	0.11%	0.013%
12	3.272	691	694	697	rBV4	1106	643	0.08%	0.010%
13	3.404	733	735	740	rBV8	1195	1107	0.14%	0.016%
14	3.432	740	744	745	rVV4	966	587	0.07%	0.009%
15	3.754	841	844	845	rBV2	1379	850	0.11%	0.013%
16	3.796	848	857	885	rVV	48701	145462	18.44%	2.162%
17	4.169	970	973	974	rBV3	990	711	0.09%	0.011%
18	4.259	984	1001	1025	rBV	130757	336958	42.71%	5.007%
19	4.522	1070	1083	1108	rVB2	115697	301058	38.16%	4.474%
20	4.966	1204	1221	1244	rVV3	296956	788958	100.00%	11.725%
21	5.291	1317	1322	1324	rBV5	1503	1380	0.17%	0.021%
22	5.365	1343	1345	1348	rBV3	1006	564	0.07%	0.008%
23	5.542	1389	1400	1425	rBV	256854	529276	67.09%	7.865%
24	5.841	1480	1493	1515	rBV2	119319	251840	31.92%	3.743%
25	5.998	1531	1542	1560	rVB	172976	346750	43.95%	5.153%
26	6.442	1678	1680	1683	rBV3	841	509	0.06%	0.008%
27	6.680	1751	1754	1757	rBV5	1556	1103	0.14%	0.016%
28	6.741	1771	1773	1776	rBV4	1302	766	0.10%	0.011%
29	6.763	1778	1780	1783	rVB3	1134	642	0.08%	0.010%
30	6.799	1788	1791	1794	rBV5	1146	733	0.09%	0.011%
31	6.921	1817	1829	1844	rBV	86967	166031	21.04%	2.467%
32	7.252	1921	1932	1951	rBV	328655	589237	74.69%	8.757%
33	7.561	2020	2028	2049	rVB	62830	110739	14.04%	1.646%
34	7.677	2062	2064	2069	rBV4	1182	993	0.13%	0.015%
35	7.831	2107	2112	2113	rBV4	1324	1154	0.15%	0.017%
36	7.873	2119	2125	2126	rBV7	2346	1686	0.21%	0.025%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW042523\
 Data File : VW030866.D
 Acq On : 26 Apr 2023 03:31
 Operator : SY/MD
 Sample : 02474-20
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 45 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0AW2

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM041723WMA.M
 Title : VOC Analysis

37	7.927	2140	2142	2144	rBV2	966	529	0.07%	0.008%
38	7.969	2151	2155	2159	rBV5	842	770	0.10%	0.011%
39	7.989	2159	2161	2162	rBV	1308	523	0.07%	0.008%
40	8.034	2165	2175	2208	rBV	148714	311512	39.48%	4.629%
41	8.435	2297	2300	2301	rBV3	1560	921	0.12%	0.014%
42	8.680	2371	2376	2379	rBV5	1266	1146	0.15%	0.017%
43	8.792	2399	2411	2432	rBV	403807	669937	84.91%	9.956%
44	9.008	2476	2478	2486	rVB8	1994	2259	0.29%	0.034%
45	9.040	2486	2488	2491	rBV4	938	733	0.09%	0.011%
46	9.275	2559	2561	2566	rVB6	1198	796	0.10%	0.012%
47	9.307	2567	2571	2574	rBV6	1308	1232	0.16%	0.018%
48	9.355	2582	2586	2587	rBV3	1005	741	0.09%	0.011%
49	9.564	2647	2651	2654	rBV6	861	742	0.09%	0.011%
50	9.606	2661	2664	2670	rBV6	1318	1287	0.16%	0.019%
51	9.670	2681	2684	2688	rVB6	2023	1440	0.18%	0.021%
52	9.857	2739	2742	2744	rBV3	1129	545	0.07%	0.008%
53	9.966	2773	2776	2779	rBV4	1516	1207	0.15%	0.018%
54	10.001	2784	2787	2790	rBV4	1062	1024	0.13%	0.015%
55	10.043	2798	2800	2803	rBV4	1114	857	0.11%	0.013%
56	10.104	2817	2819	2822	rBV4	1613	1049	0.13%	0.016%
57	10.159	2826	2836	2854	rVV	242417	392760	49.78%	5.837%
58	10.326	2884	2888	2889	rBV5	3759	2428	0.31%	0.036%
59	10.586	2965	2969	2972	rBV5	1083	892	0.11%	0.013%
60	10.657	2989	2991	2997	rVB5	1827	1290	0.16%	0.019%
61	10.789	3029	3032	3033	rBV2	1209	706	0.09%	0.010%
62	10.821	3038	3042	3048	rBV8	2151	1921	0.24%	0.029%
63	10.850	3048	3051	3052	rBV3	1525	824	0.10%	0.012%
64	10.882	3059	3061	3064	rVB5	1387	673	0.09%	0.010%
65	10.943	3075	3080	3082	rBV4	1291	1194	0.15%	0.018%
66	10.976	3088	3090	3093	rVB3	1268	782	0.10%	0.012%
67	11.033	3106	3108	3110	rBV3	988	586	0.07%	0.009%
68	11.107	3123	3131	3138	rBV8	3301	5856	0.74%	0.087%
69	11.194	3147	3158	3180	rBV	405292	641171	81.27%	9.528%
70	11.406	3223	3224	3226	rBV2	1317	594	0.08%	0.009%
71	11.439	3230	3234	3238	rBV4	1948	1588	0.20%	0.024%
72	11.567	3263	3274	3295	rBV	363360	577807	73.24%	8.587%
73	11.786	3340	3342	3345	rVB4	1512	767	0.10%	0.011%
74	11.802	3345	3347	3351	rBV5	781	649	0.08%	0.010%
75	11.834	3355	3357	3360	rVV4	2253	1115	0.14%	0.017%
76	11.921	3382	3384	3388	rVB5	1071	827	0.10%	0.012%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042523\
 Data File : VV030866.D
 Acq On : 26 Apr 2023 03:31
 Operator : SY/MD
 Sample : 02474-20
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 45 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0AW2

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM041723WMA.M
 Title : VOC Analysis

77	12.008	3409	3411	3415	rVB4	1480	742	0.09%	0.011%
78	12.030	3415	3418	3420	rBV3	882	556	0.07%	0.008%
79	12.429	3539	3542	3543	rBV2	1349	728	0.09%	0.011%
80	12.619	3598	3601	3602	rBV2	1111	597	0.08%	0.009%
81	12.799	3655	3657	3660	rBV3	1093	763	0.10%	0.011%
82	12.869	3675	3679	3683	rBV7	1299	1313	0.17%	0.020%
83	12.921	3690	3695	3696	rBV6	787	675	0.09%	0.010%
84	13.004	3718	3721	3723	rBV4	1252	966	0.12%	0.014%
85	13.049	3733	3735	3739	rBV4	1072	705	0.09%	0.010%
86	13.165	3768	3771	3772	rBV2	997	551	0.07%	0.008%
87	13.204	3782	3783	3788	rVV5	1222	735	0.09%	0.011%
88	13.500	3873	3875	3879	rBV6	950	578	0.07%	0.009%
89	13.609	3905	3909	3911	rBV5	926	871	0.11%	0.013%
90	13.747	3946	3952	3956	rBV6	2498	2457	0.31%	0.037%
91	13.766	3956	3958	3962	rVV4	1484	914	0.12%	0.014%
92	13.795	3962	3967	3972	rVV8	1951	1786	0.23%	0.027%
93	13.969	4018	4021	4022	rBV3	1377	715	0.09%	0.011%
94	14.008	4030	4033	4035	rBV4	1660	860	0.11%	0.013%
95	14.043	4043	4044	4048	rBV4	1148	742	0.09%	0.011%
96	14.127	4068	4070	4073	rVB4	1180	624	0.08%	0.009%
97	14.319	4126	4130	4133	rBV5	1093	768	0.10%	0.011%
98	14.400	4153	4155	4158	rVB4	986	511	0.06%	0.008%
99	14.419	4158	4161	4163	rBV4	1135	891	0.11%	0.013%
100	14.866	4296	4300	4304	rBV7	1301	1293	0.16%	0.019%




Sum of corrected areas: 6729138

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042523\
Data File : VV030866.D
Acq On : 26 Apr 2023 03:31
Operator : SY/MD
Sample : 02474-20
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 45 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0AW2

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM041723WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

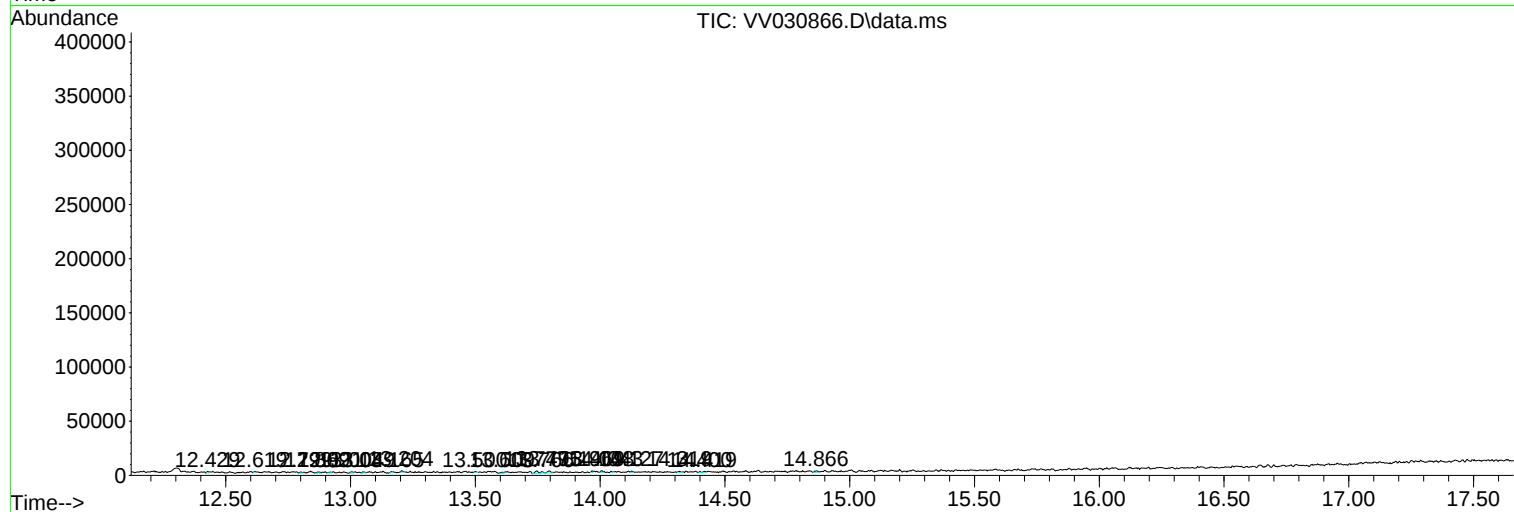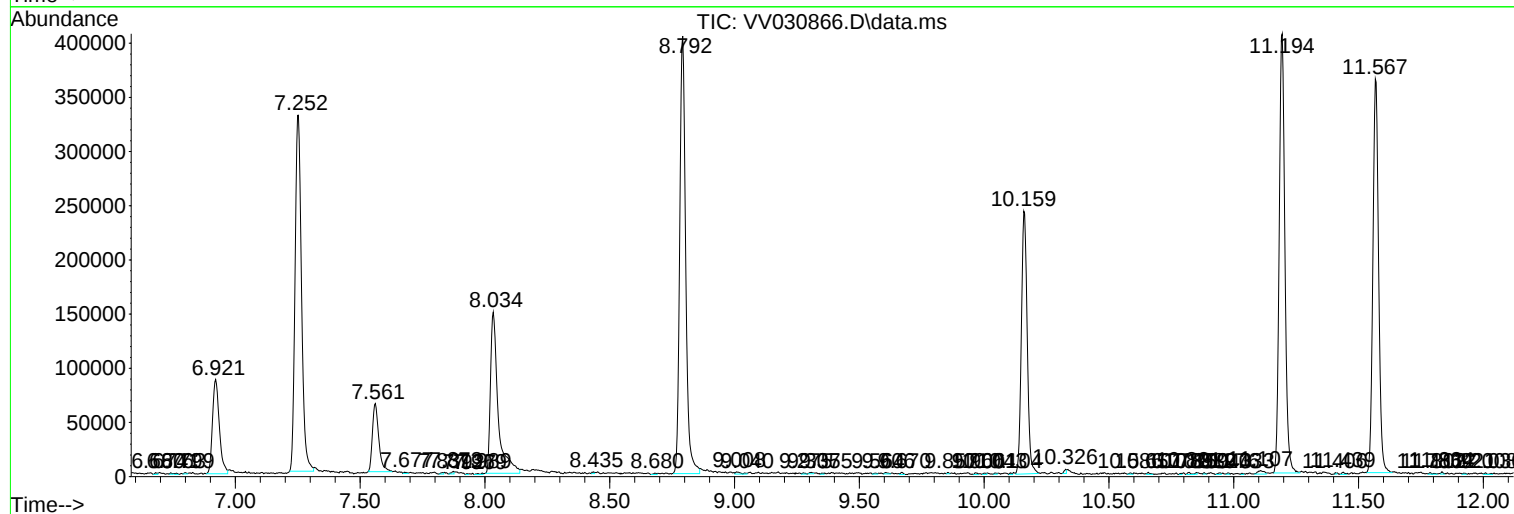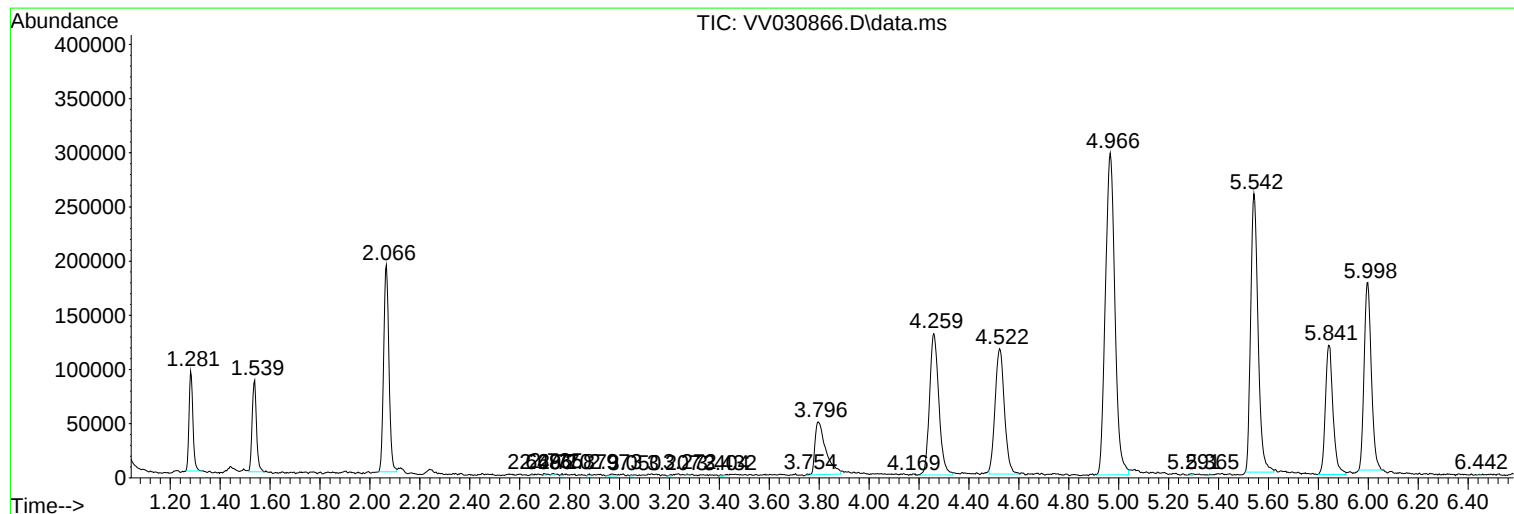

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042523\
Data File : VV030866.D
Acq On : 26 Apr 2023 03:31
Operator : SY/MD
Sample : 02474-20
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 45 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0AW2

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM041723WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042523\
Data File : VV030866.D
Acq On : 26 Apr 2023 03:31
Operator : SY/MD
Sample : 02474-20
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 45 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0AW2

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM041723WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------