

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042523\
 Data File : VV030867.D
 Acq On : 26 Apr 2023 03:55
 Operator : SY/MD
 Sample : 02474-06 10X
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 46 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0AS8

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM041723WMA.M
 Title : VOC Analysis

Signal : TIC: VV030867.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.281	69	75	85	rBV	93336	100392	12.93%	1.480%
2	1.535	148	154	171	rVB	84139	105951	13.64%	1.562%
3	2.066	310	319	332	rVB	188883	275463	35.47%	4.061%
4	2.310	393	395	397	rBV3	1537	929	0.12%	0.014%
5	2.359	408	410	413	rVB3	1468	707	0.09%	0.010%
6	2.371	413	414	417	rBV2	1189	661	0.09%	0.010%
7	2.548	466	469	473	rVB6	1578	927	0.12%	0.014%
8	2.773	535	539	541	rVB4	1240	781	0.10%	0.012%
9	2.796	541	546	550	rBV8	1841	1859	0.24%	0.027%
10	2.838	553	559	560	rBV4	1209	1078	0.14%	0.016%
11	2.924	582	586	588	rBV4	850	609	0.08%	0.009%
12	2.989	603	606	609	rBV4	908	713	0.09%	0.011%
13	3.021	613	616	618	rBV4	818	711	0.09%	0.010%
14	3.127	647	649	652	rVB3	1365	768	0.10%	0.011%
15	3.150	652	656	659	rBV6	683	623	0.08%	0.009%
16	3.265	690	692	698	rVV7	1204	783	0.10%	0.012%
17	3.336	711	714	716	rBV3	1183	843	0.11%	0.012%
18	3.490	759	762	765	rBV4	1383	1102	0.14%	0.016%
19	3.535	772	776	778	rBV4	724	582	0.07%	0.009%
20	3.603	792	797	798	rVB4	1089	705	0.09%	0.010%
21	3.619	798	802	804	rBV3	962	923	0.12%	0.014%
22	3.728	834	836	840	rVB5	1157	651	0.08%	0.010%
23	3.799	848	858	879	rBV	51461	144401	18.59%	2.129%
24	4.050	933	936	938	rBV3	1554	966	0.12%	0.014%
25	4.111	953	955	958	rBV3	1656	806	0.10%	0.012%
26	4.259	984	1001	1026	rBV	131199	338732	43.62%	4.994%
27	4.664	1124	1127	1130	rBV4	1635	920	0.12%	0.014%
28	4.966	1205	1221	1242	rBV2	291607	776586	100.00%	11.449%
29	5.330	1333	1334	1336	rBV	1246	574	0.07%	0.008%
30	5.381	1344	1350	1354	rBV6	1430	1443	0.19%	0.021%
31	5.542	1388	1400	1420	rBV	257162	535899	69.01%	7.900%
32	5.841	1479	1493	1513	rBV	303716	608581	78.37%	8.972%
33	5.998	1531	1542	1561	rVB	174834	354641	45.67%	5.228%
34	6.352	1650	1652	1655	rVB3	1680	756	0.10%	0.011%
35	6.371	1655	1658	1660	rBV3	1172	746	0.10%	0.011%
36	6.487	1689	1694	1696	rVV6	1594	1259	0.16%	0.019%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW042523\
 Data File : VW030867.D
 Acq On : 26 Apr 2023 03:55
 Operator : SY/MD
 Sample : 02474-06 10X
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 46 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0AS8

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM041723WMA.M
 Title : VOC Analysis

37	6.883	1814	1817	1819	rBV2	1117	841	0.11%	0.012%
38	6.921	1819	1829	1848	rVV	86782	166425	21.43%	2.453%
39	7.120	1889	1891	1894	rBV4	1034	702	0.09%	0.010%
40	7.252	1920	1932	1953	rBV	335165	604866	77.89%	8.917%
41	7.500	2007	2009	2012	rVB3	1427	714	0.09%	0.011%
42	7.561	2019	2028	2045	rVV	66341	118493	15.26%	1.747%
43	7.776	2092	2095	2098	rBV5	1331	937	0.12%	0.014%
44	7.995	2159	2163	2165	rVB5	1147	804	0.10%	0.012%
45	8.034	2165	2175	2203	rBV	153375	320022	41.21%	4.718%
46	8.554	2333	2337	2338	rBV4	1498	895	0.12%	0.013%
47	8.622	2354	2358	2362	rVB7	1352	1160	0.15%	0.017%
48	8.792	2400	2411	2431	rBV	397587	652860	84.07%	9.625%
49	9.059	2492	2494	2498	rBV5	1264	1065	0.14%	0.016%
50	9.429	2606	2609	2610	rBV3	1322	784	0.10%	0.012%
51	9.554	2645	2648	2650	rBV3	1330	864	0.11%	0.013%
52	9.580	2653	2656	2657	rBV3	1385	699	0.09%	0.010%
53	9.638	2672	2674	2679	rVB5	1493	926	0.12%	0.014%
54	9.664	2679	2682	2687	rBV7	1151	1144	0.15%	0.017%
55	9.876	2745	2748	2751	rBV4	1402	1132	0.15%	0.017%
56	10.014	2788	2791	2793	rBV4	1183	606	0.08%	0.009%
57	10.033	2793	2797	2800	rBV4	1158	752	0.10%	0.011%
58	10.104	2816	2819	2821	rBV3	1788	797	0.10%	0.012%
59	10.159	2826	2836	2851	rBV	239684	382926	49.31%	5.645%
60	10.297	2875	2879	2880	rBV4	1449	631	0.08%	0.009%
61	10.525	2948	2950	2953	rVV4	1023	591	0.08%	0.009%
62	10.558	2956	2960	2961	rBV3	1275	853	0.11%	0.013%
63	10.593	2967	2971	2974	rBV6	1804	1201	0.15%	0.018%
64	10.667	2990	2994	2999	rBV5	1645	1476	0.19%	0.022%
65	10.789	3030	3032	3036	rBV4	971	895	0.12%	0.013%
66	10.857	3048	3053	3056	rBV6	1539	1433	0.18%	0.021%
67	11.194	3145	3158	3178	rBV	393617	635296	81.81%	9.366%
68	11.567	3260	3274	3293	rBV	362256	585857	75.44%	8.637%
69	11.770	3333	3337	3338	rBV3	1028	748	0.10%	0.011%
70	11.905	3374	3379	3380	rBV4	950	787	0.10%	0.012%
71	12.004	3408	3410	3413	rBV4	1311	866	0.11%	0.013%
72	12.278	3492	3495	3497	rBV4	1330	1039	0.13%	0.015%
73	12.445	3545	3547	3550	rVB4	1848	851	0.11%	0.013%
74	12.474	3554	3556	3559	rBV3	1173	619	0.08%	0.009%
75	12.506	3564	3566	3571	rVV5	813	696	0.09%	0.010%
76	12.580	3583	3589	3590	rBV6	1184	971	0.13%	0.014%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042523\
 Data File : VV030867.D
 Acq On : 26 Apr 2023 03:55
 Operator : SY/MD
 Sample : 02474-06 10X
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 46 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0AS8

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM041723WMA.M
 Title : VOC Analysis

77	12.622	3599	3602	3606	rVV5	1425	968	0.12%	0.014%
78	12.712	3627	3630	3637	rBV8	776	980	0.13%	0.014%
79	12.831	3664	3667	3668	rBV3	1257	556	0.07%	0.008%
80	12.869	3675	3679	3682	rBV5	1523	1477	0.19%	0.022%
81	12.943	3699	3702	3704	rBV4	1071	713	0.09%	0.011%
82	12.988	3713	3716	3719	rBV4	748	584	0.08%	0.009%
83	13.021	3724	3726	3729	rVV4	857	576	0.07%	0.008%
84	13.143	3759	3764	3765	rBV5	908	653	0.08%	0.010%
85	13.184	3773	3777	3783	rBV8	1655	1550	0.20%	0.023%
86	13.220	3786	3788	3791	rVB4	1364	813	0.10%	0.012%
87	13.307	3808	3815	3817	rVV5	1247	1472	0.19%	0.022%
88	13.583	3898	3901	3902	rBV3	1571	854	0.11%	0.013%
89	13.680	3926	3931	3934	rBV6	1680	1887	0.24%	0.028%
90	13.795	3963	3967	3968	rBV4	1513	991	0.13%	0.015%
91	13.998	4028	4030	4034	rVB5	1512	833	0.11%	0.012%
92	14.030	4038	4040	4043	rVB3	1176	613	0.08%	0.009%
93	14.085	4055	4057	4062	rVB5	1619	1225	0.16%	0.018%
94	14.107	4062	4064	4068	rBV5	1413	1119	0.14%	0.016%
95	14.229	4100	4102	4104	rBV3	1089	671	0.09%	0.010%
96	14.477	4172	4179	4182	rBV6	1183	1524	0.20%	0.022%
97	14.503	4182	4187	4190	rBV5	1197	1111	0.14%	0.016%
98	14.580	4208	4211	4213	rVB3	1531	765	0.10%	0.011%
99	14.889	4305	4307	4310	rBV4	1670	776	0.10%	0.011%
100	14.946	4320	4325	4326	rBV5	1758	1258	0.16%	0.019%

Sum of corrected areas: 6783264




Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042523\
Data File : VV030867.D
Acq On : 26 Apr 2023 03:55
Operator : SY/MD
Sample : 02474-06 10X
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 46 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0AS8

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM041723WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L

TIC Integration Parameters: LSCINT.P

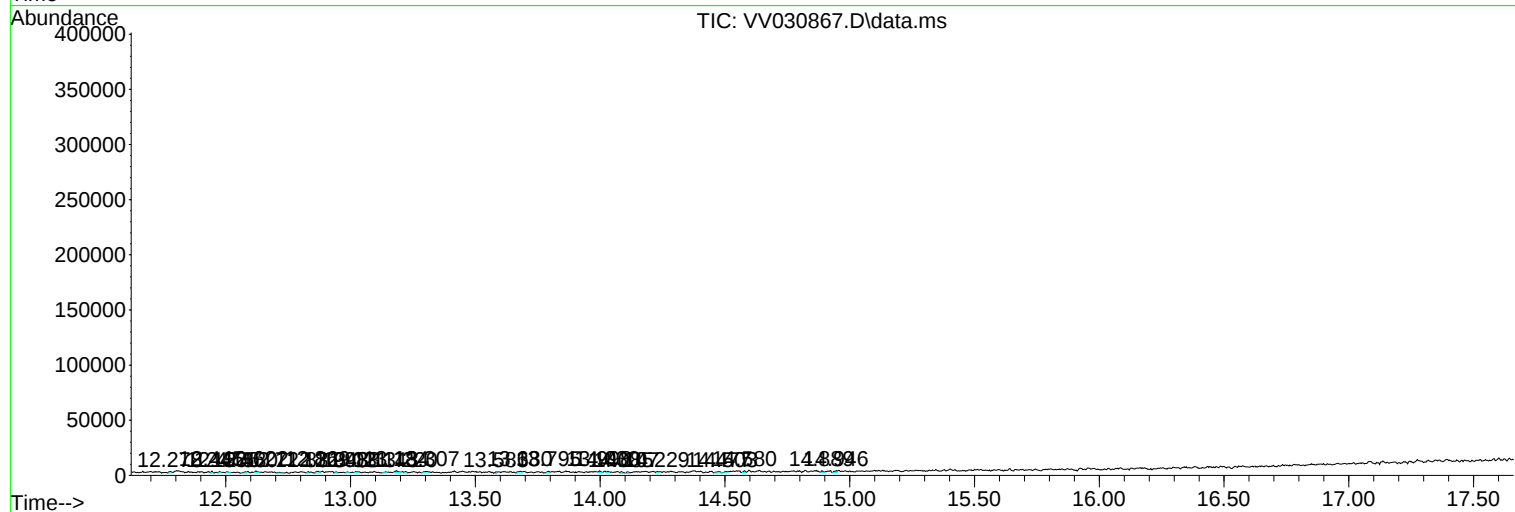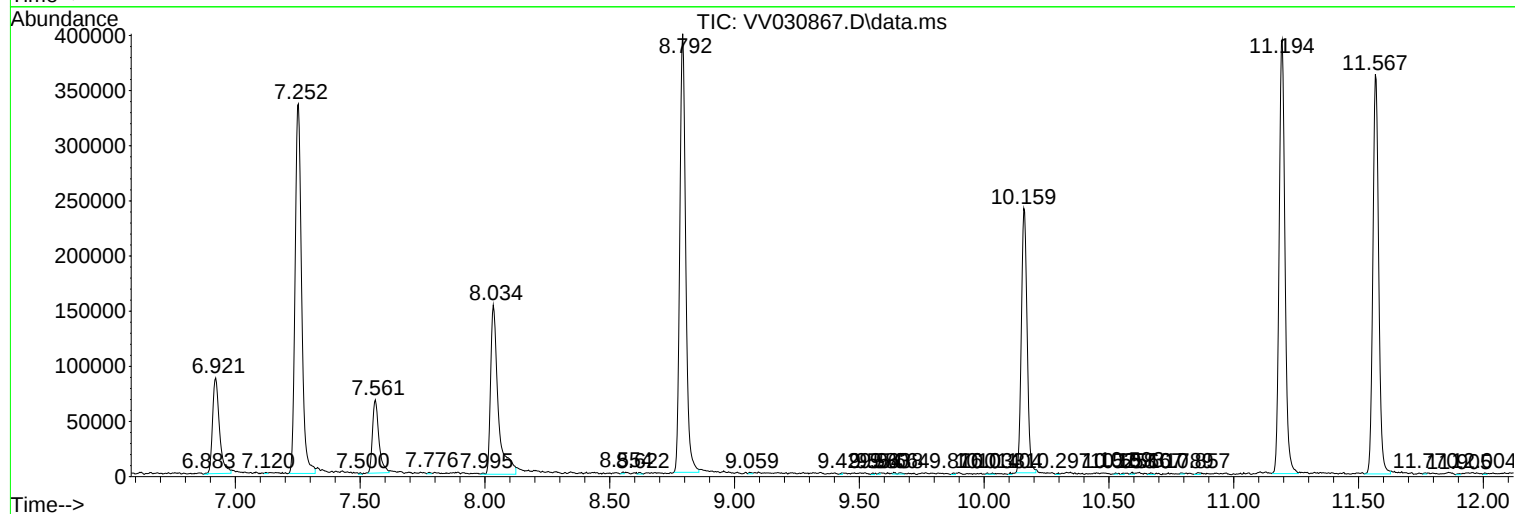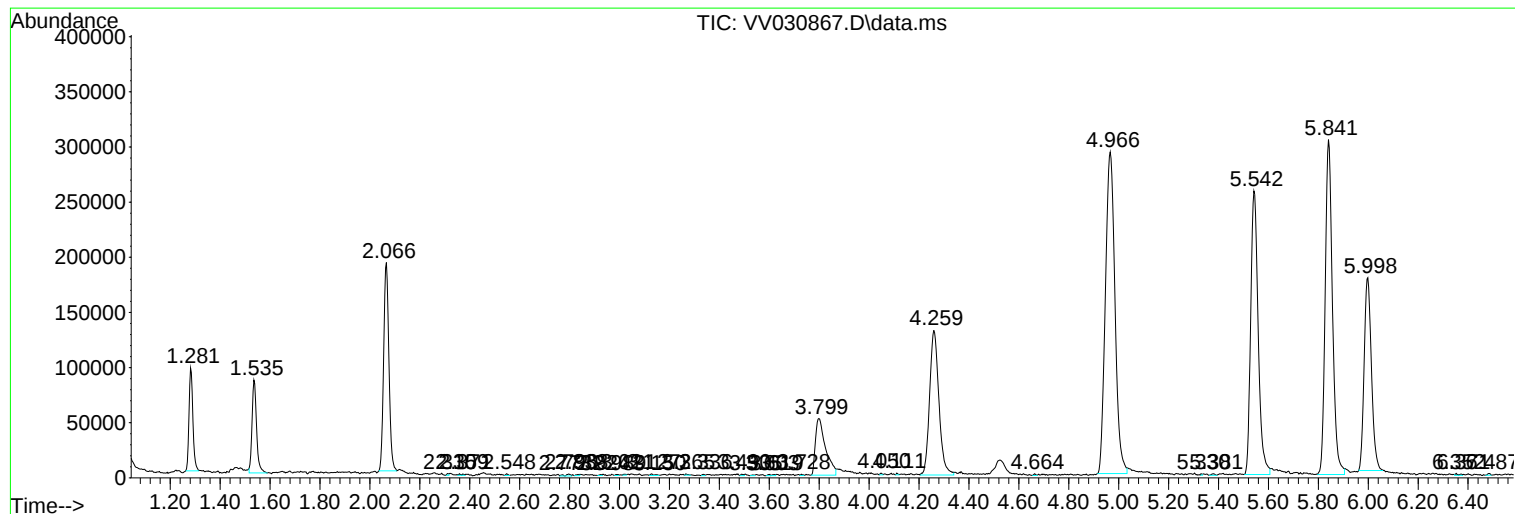

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042523\
Data File : VV030867.D
Acq On : 26 Apr 2023 03:55
Operator : SY/MD
Sample : 02474-06 10X
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 46 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0AS8

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM041723WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042523\
Data File : VV030867.D
Acq On : 26 Apr 2023 03:55
Operator : SY/MD
Sample : 02474-06 10X
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 46 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0AS8

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM041723WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------