

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042523\
 Data File : VV030868.D
 Acq On : 26 Apr 2023 04:19
 Operator : SY/MD
 Sample : 02474-08 10X
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 47 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 COATO

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM041723WMA.M
 Title : VOC Analysis

Signal : TIC: VV030868.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.281	69	75	85	rBV	91294	99332	12.57%	1.439%
2	1.539	148	155	172	rVB	86519	107428	13.60%	1.556%
3	2.066	310	319	331	rBV	189037	271102	34.32%	3.926%
4	2.365	409	412	416	rVB4	1800	1134	0.14%	0.016%
5	2.387	416	419	422	rBV4	1478	1205	0.15%	0.017%
6	2.442	433	436	437	rBV2	1771	946	0.12%	0.014%
7	2.516	457	459	462	rVB4	1450	705	0.09%	0.010%
8	2.539	463	466	469	rVV5	968	692	0.09%	0.010%
9	2.995	604	608	609	rBV4	1162	879	0.11%	0.013%
10	3.040	620	622	624	rBV3	1139	571	0.07%	0.008%
11	3.098	638	640	642	rBV2	1171	583	0.07%	0.008%
12	3.175	660	664	667	rBV6	1245	983	0.12%	0.014%
13	3.227	678	680	683	rBV4	1357	751	0.10%	0.011%
14	3.313	704	707	711	rBV6	1647	1411	0.18%	0.020%
15	3.577	786	789	790	rBV3	1459	729	0.09%	0.011%
16	3.735	834	838	839	rBV4	1570	834	0.11%	0.012%
17	3.796	847	857	880	rBV	49773	144416	18.28%	2.092%
18	4.088	946	948	951	rBV3	1309	972	0.12%	0.014%
19	4.259	987	1001	1025	rBV	129657	324741	41.11%	4.703%
20	4.657	1122	1125	1128	rBV4	1036	566	0.07%	0.008%
21	4.966	1204	1221	1247	rBV2	292977	785449	99.42%	11.376%
22	5.365	1343	1345	1349	rVV4	1473	823	0.10%	0.012%
23	5.384	1349	1351	1355	rVB5	868	517	0.07%	0.007%
24	5.490	1382	1384	1387	rBV3	1520	993	0.13%	0.014%
25	5.542	1388	1400	1424	rVV	254925	535890	67.83%	7.761%
26	5.841	1480	1493	1519	rBV2	397179	790014	100.00%	11.442%
27	5.998	1530	1542	1564	rVB	175082	361164	45.72%	5.231%
28	6.471	1686	1689	1690	rBV2	786	528	0.07%	0.008%
29	6.487	1690	1694	1698	rVV5	1989	2049	0.26%	0.030%
30	6.564	1713	1718	1722	rBV6	1765	1926	0.24%	0.028%
31	6.677	1750	1753	1757	rVB4	1283	656	0.08%	0.010%
32	6.760	1777	1779	1782	rVB4	893	513	0.06%	0.007%
33	6.921	1819	1829	1846	rBV	87537	161666	20.46%	2.341%
34	7.127	1890	1893	1895	rBV4	1731	890	0.11%	0.013%
35	7.198	1912	1915	1917	rBV4	1188	501	0.06%	0.007%
36	7.252	1920	1932	1952	rBV	335989	602285	76.24%	8.723%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW042523\
 Data File : VW030868.D
 Acq On : 26 Apr 2023 04:19
 Operator : SY/MD
 Sample : 02474-08 10X
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 47 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 COATO

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM041723WMA.M
 Title : VOC Analysis

37	7.445	1990	1992	1994	rBV3	1562	911	0.12%	0.013%
38	7.561	2018	2028	2040	rBV	64246	114822	14.53%	1.663%
39	7.847	2115	2117	2120	rBV5	1123	803	0.10%	0.012%
40	7.979	2155	2158	2160	rBV3	1953	1169	0.15%	0.017%
41	8.034	2164	2175	2190	rBV	153919	289956	36.70%	4.199%
42	8.500	2316	2320	2323	rBV6	1180	974	0.12%	0.014%
43	8.638	2358	2363	2368	rBV8	1603	2038	0.26%	0.030%
44	8.792	2398	2411	2434	rBV	394497	664599	84.12%	9.625%
45	9.014	2477	2480	2482	rBV4	1734	1361	0.17%	0.020%
46	9.078	2498	2500	2506	rBV5	1822	1323	0.17%	0.019%
47	9.197	2534	2537	2538	rBV3	1623	831	0.11%	0.012%
48	9.291	2564	2566	2570	rVB4	927	652	0.08%	0.009%
49	9.313	2570	2573	2575	rBV4	1260	675	0.09%	0.010%
50	9.458	2615	2618	2619	rBV3	985	625	0.08%	0.009%
51	9.509	2629	2634	2637	rBV5	1804	1224	0.15%	0.018%
52	9.615	2663	2667	2670	rBV5	1149	1175	0.15%	0.017%
53	9.683	2685	2688	2690	rVV3	1313	634	0.08%	0.009%
54	9.747	2706	2708	2710	rBV3	1066	705	0.09%	0.010%
55	9.783	2717	2719	2722	rBV3	1288	738	0.09%	0.011%
56	9.866	2743	2745	2748	rBV4	1092	725	0.09%	0.011%
57	9.940	2765	2768	2772	rBV4	1501	1104	0.14%	0.016%
58	9.976	2777	2779	2784	rVB5	955	753	0.10%	0.011%
59	10.159	2825	2836	2851	rBV	247306	388289	49.15%	5.624%
60	10.390	2903	2908	2910	rBV5	1306	820	0.10%	0.012%
61	10.406	2910	2913	2915	rBV4	1645	1030	0.13%	0.015%
62	10.442	2921	2924	2926	rBV3	831	532	0.07%	0.008%
63	10.455	2926	2928	2931	rVV4	759	528	0.07%	0.008%
64	10.525	2947	2950	2953	rBV4	1249	907	0.11%	0.013%
65	10.625	2978	2981	2986	rVB5	1532	1253	0.16%	0.018%
66	10.722	3008	3011	3013	rBV3	1295	757	0.10%	0.011%
67	10.767	3020	3025	3028	rBV5	1260	1361	0.17%	0.020%
68	10.818	3038	3041	3042	rBV3	872	590	0.07%	0.009%
69	11.069	3116	3119	3120	rBV2	1047	564	0.07%	0.008%
70	11.094	3125	3127	3129	rBV3	951	571	0.07%	0.008%
71	11.194	3146	3158	3174	rBV	387715	617381	78.15%	8.941%
72	11.461	3238	3241	3244	rBV4	1226	740	0.09%	0.011%
73	11.567	3263	3274	3292	rBV	354673	572439	72.46%	8.291%
74	11.760	3333	3334	3338	rVB4	1190	556	0.07%	0.008%
75	12.072	3427	3431	3432	rBV3	920	566	0.07%	0.008%
76	12.191	3465	3468	3471	rBV3	1053	773	0.10%	0.011%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042523\
 Data File : VV030868.D
 Acq On : 26 Apr 2023 04:19
 Operator : SY/MD
 Sample : 02474-08 10X
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 47 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 COATO

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM041723WMA.M
 Title : VOC Analysis

77	12.429	3538	3542	3546	rBV7	1095	984	0.12%	0.014%
78	12.516	3567	3569	3572	rBV4	1167	611	0.08%	0.009%
79	12.718	3628	3632	3634	rBV4	925	600	0.08%	0.009%
80	12.770	3645	3648	3651	rVB5	1097	749	0.09%	0.011%
81	12.783	3651	3652	3659	rVB6	844	744	0.09%	0.011%
82	12.818	3659	3663	3666	rBV5	1353	854	0.11%	0.012%
83	12.840	3666	3670	3671	rBV4	1250	786	0.10%	0.011%
84	12.934	3697	3699	3701	rVB2	1261	521	0.07%	0.008%
85	13.037	3728	3731	3734	rBV5	1438	1234	0.16%	0.018%
86	13.246	3793	3796	3799	rBV3	1401	1236	0.16%	0.018%
87	13.348	3825	3828	3830	rBV4	975	637	0.08%	0.009%
88	13.397	3840	3843	3846	rBV5	1690	1406	0.18%	0.020%
89	13.426	3848	3852	3855	rBV5	1559	1256	0.16%	0.018%
90	13.557	3892	3893	3897	rBV4	1003	499	0.06%	0.007%
91	13.779	3959	3962	3964	rBV4	1485	1003	0.13%	0.015%
92	13.889	3992	3996	3999	rBV4	1283	984	0.12%	0.014%
93	13.943	4010	4013	4015	rBV3	1176	602	0.08%	0.009%
94	13.995	4026	4029	4031	rBV4	1720	1089	0.14%	0.016%
95	14.027	4036	4039	4044	rBV6	2084	1925	0.24%	0.028%
96	14.120	4065	4068	4069	rBV3	1107	607	0.08%	0.009%
97	14.242	4103	4106	4109	rBV4	1023	609	0.08%	0.009%
98	14.409	4156	4158	4162	rBV5	1428	989	0.13%	0.014%
99	14.821	4284	4286	4288	rBV2	1470	725	0.09%	0.011%
100	15.271	4424	4426	4428	rBV3	1554	744	0.09%	0.011%




Sum of corrected areas: 6904692

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042523\
Data File : VV030868.D
Acq On : 26 Apr 2023 04:19
Operator : SY/MD
Sample : 02474-08 10X
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 47 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
COATO

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM041723WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

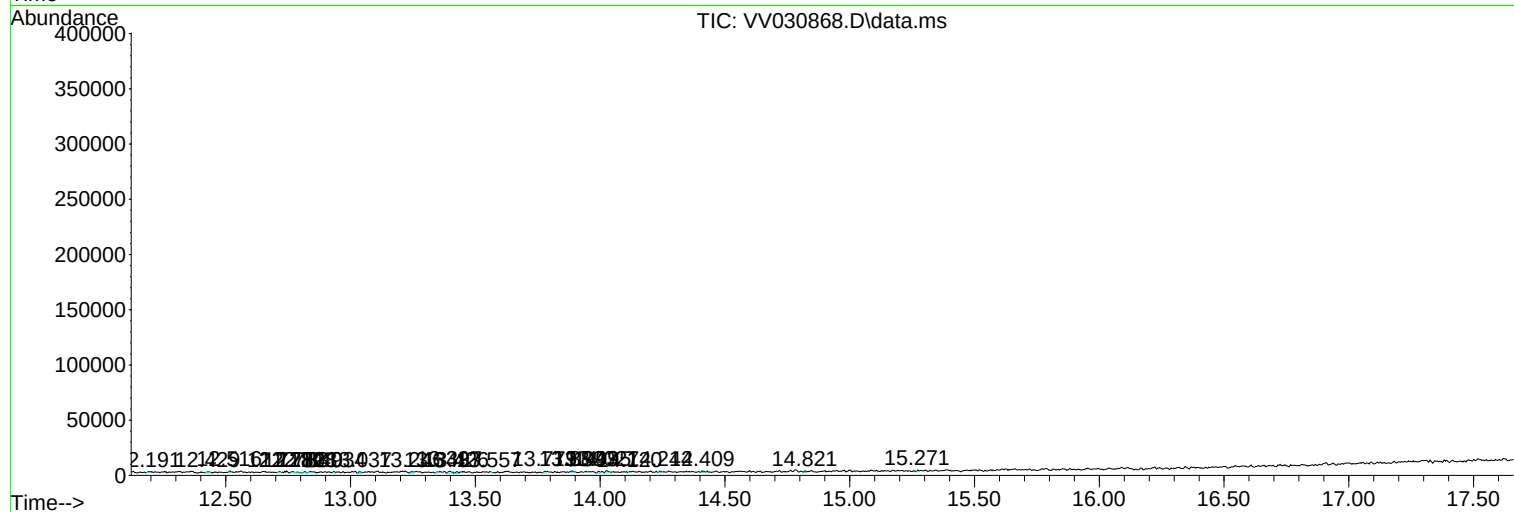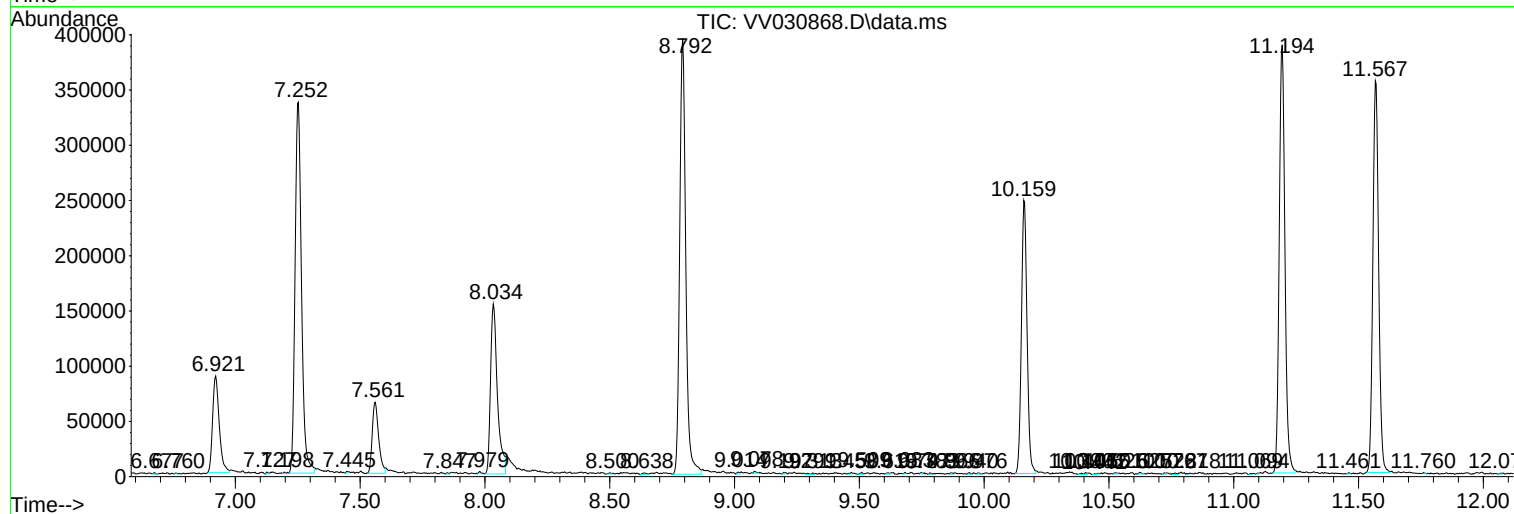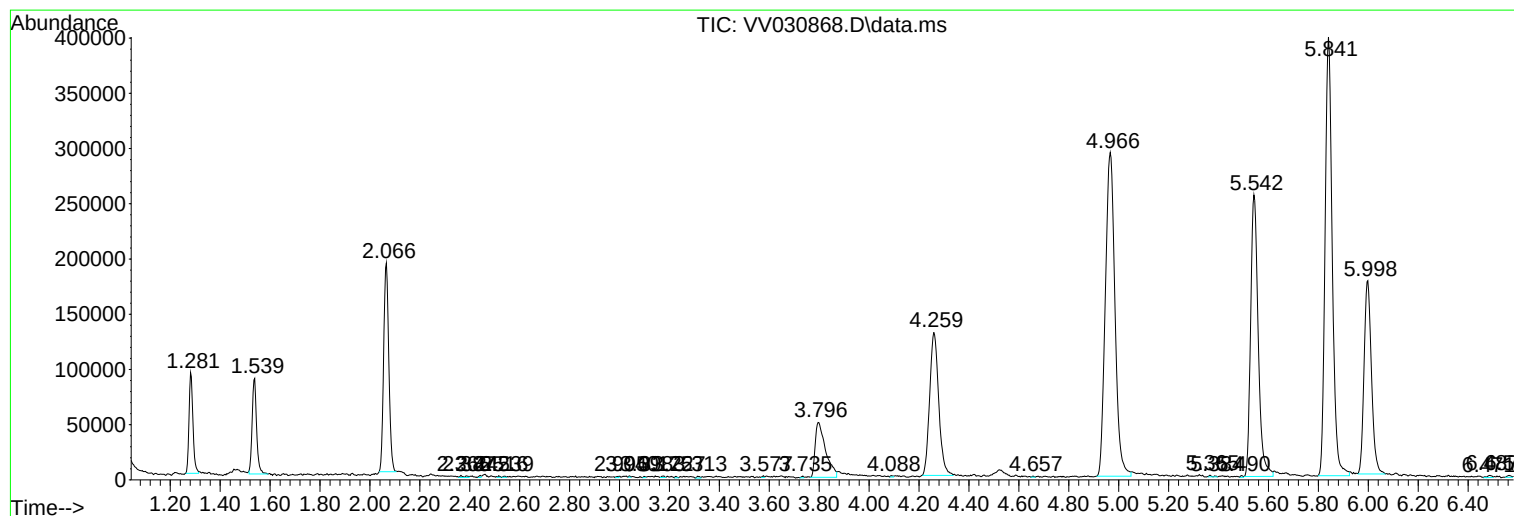

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042523\
Data File : VV030868.D
Acq On : 26 Apr 2023 04:19
Operator : SY/MD
Sample : 02474-08 10X
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 47 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0AT0

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM041723WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042523\
Data File : VV030868.D
Acq On : 26 Apr 2023 04:19
Operator : SY/MD
Sample : 02474-08 10X
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 47 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0AT0

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM041723WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc