

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042523\
 Data File : VV030869.D
 Acq On : 26 Apr 2023 04:42
 Operator : SY/MD
 Sample : 02474-14 10X
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 48 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0AT6

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM041723WMA.M
 Title : VOC Analysis

Signal : TIC: VV030869.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.281	69	75	85	rBV	91851	97441	7.01%	1.282%
2	1.535	148	154	168	rVB	84631	102407	7.37%	1.348%
3	2.066	310	319	334	rBV	189469	277661	19.99%	3.654%
4	2.416	424	428	432	rBV6	1269	1002	0.07%	0.013%
5	2.442	432	436	437	rBV4	2886	2025	0.15%	0.027%
6	2.609	484	488	491	rBV6	1782	1529	0.11%	0.020%
7	2.690	509	513	514	rBV3	1086	734	0.05%	0.010%
8	2.725	522	524	528	rBV4	1512	990	0.07%	0.013%
9	2.767	535	537	541	rBV4	1203	785	0.06%	0.010%
10	2.896	575	577	581	rBV5	835	522	0.04%	0.007%
11	3.031	615	619	623	rBV5	1106	920	0.07%	0.012%
12	3.059	625	628	629	rBV3	1155	674	0.05%	0.009%
13	3.182	662	666	667	rBV3	625	515	0.04%	0.007%
14	3.278	692	696	700	rBV5	1119	873	0.06%	0.011%
15	3.397	732	733	737	rVB5	1072	573	0.04%	0.008%
16	3.426	740	742	745	rBV5	914	608	0.04%	0.008%
17	3.458	751	752	756	rBV4	1085	749	0.05%	0.010%
18	3.477	756	758	764	rVB5	1426	944	0.07%	0.012%
19	3.564	783	785	788	rVB2	1387	717	0.05%	0.009%
20	3.580	788	790	793	rBV3	961	700	0.05%	0.009%
21	3.799	849	858	892	rBV	52862	173417	12.48%	2.282%
22	4.259	985	1001	1025	rBV	133679	337810	24.32%	4.445%
23	4.638	1115	1119	1122	rBV4	1499	1184	0.09%	0.016%
24	4.680	1130	1132	1136	rBV3	1389	920	0.07%	0.012%
25	4.764	1152	1158	1161	rBV7	1669	1956	0.14%	0.026%
26	4.789	1163	1166	1171	rBV5	1137	1008	0.07%	0.013%
27	4.873	1185	1192	1194	rBV7	1658	1409	0.10%	0.019%
28	4.892	1195	1198	1201	rBV5	903	708	0.05%	0.009%
29	4.966	1204	1221	1244	rBV3	295379	791223	56.95%	10.412%
30	5.223	1299	1301	1304	rVB4	1618	813	0.06%	0.011%
31	5.243	1304	1307	1310	rBV5	1581	1210	0.09%	0.016%
32	5.448	1369	1371	1374	rBV4	1447	815	0.06%	0.011%
33	5.542	1388	1400	1423	rBV	256844	534282	38.46%	7.031%
34	5.841	1480	1493	1515	rBV	713705	1389294	100.00%	18.283%
35	5.998	1532	1542	1563	rVB	176581	360695	25.96%	4.747%
36	6.320	1639	1642	1644	rBV3	1236	868	0.06%	0.011%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042523\
 Data File : VV030869.D
 Acq On : 26 Apr 2023 04:42
 Operator : SY/MD
 Sample : 02474-14 10X
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 48 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0AT6

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM041723WMA.M
 Title : VOC Analysis

37	6.519	1703	1704	1711	rVB5	1395	1406	0.10%	0.019%
38	6.583	1721	1724	1728	rVB6	1101	629	0.05%	0.008%
39	6.770	1779	1782	1785	rBV5	965	730	0.05%	0.010%
40	6.921	1820	1829	1846	rBV	88071	161799	11.65%	2.129%
41	7.069	1873	1875	1880	rVB5	1292	915	0.07%	0.012%
42	7.172	1903	1907	1909	rBV4	1392	1245	0.09%	0.016%
43	7.252	1921	1932	1949	rBV	335431	597358	43.00%	7.861%
44	7.561	2019	2028	2048	rVB	63559	113553	8.17%	1.494%
45	7.918	2137	2139	2141	rBV2	1357	826	0.06%	0.011%
46	8.034	2166	2175	2206	rBV	155445	319574	23.00%	4.205%
47	8.439	2296	2301	2305	rBV6	1683	2087	0.15%	0.027%
48	8.509	2320	2323	2325	rBV3	1235	889	0.06%	0.012%
49	8.577	2342	2344	2345	rBV2	1277	511	0.04%	0.007%
50	8.792	2400	2411	2432	rBV	392751	662951	47.72%	8.724%
51	9.140	2516	2519	2520	rBV3	1450	805	0.06%	0.011%
52	9.172	2527	2529	2531	rBV3	1068	583	0.04%	0.008%
53	9.336	2577	2580	2582	rBV4	1931	1310	0.09%	0.017%
54	9.349	2582	2584	2588	rVB4	1123	794	0.06%	0.010%
55	9.683	2684	2688	2691	rBV5	1079	838	0.06%	0.011%
56	9.718	2697	2699	2704	rVB5	1100	541	0.04%	0.007%
57	9.866	2742	2745	2746	rBV2	860	574	0.04%	0.008%
58	9.886	2747	2751	2752	rVV3	1102	759	0.05%	0.010%
59	9.911	2757	2759	2763	rVB4	964	585	0.04%	0.008%
60	10.159	2825	2836	2852	rBV	245602	392174	28.23%	5.161%
61	10.249	2861	2864	2868	rBV6	1578	1435	0.10%	0.019%
62	10.374	2898	2903	2904	rVB4	1143	800	0.06%	0.011%
63	10.451	2923	2927	2929	rBV5	1216	1176	0.08%	0.015%
64	10.593	2969	2971	2974	rBV2	772	519	0.04%	0.007%
65	10.622	2976	2980	2985	rVB7	1310	1072	0.08%	0.014%
66	10.796	3029	3034	3036	rBV6	1555	1529	0.11%	0.020%
67	10.824	3041	3043	3046	rBV4	866	548	0.04%	0.007%
68	10.953	3081	3083	3085	rVV3	1434	632	0.05%	0.008%
69	11.194	3146	3158	3176	rBV	398233	624320	44.94%	8.216%
70	11.368	3209	3212	3214	rBV4	1619	812	0.06%	0.011%
71	11.458	3237	3240	3242	rBV3	1239	700	0.05%	0.009%
72	11.519	3253	3259	3262	rBV7	1535	1894	0.14%	0.025%
73	11.567	3263	3274	3293	rVV	364716	583984	42.03%	7.685%
74	11.738	3323	3327	3330	rBV6	1382	1320	0.10%	0.017%
75	11.988	3402	3405	3406	rBV3	1345	891	0.06%	0.012%
76	12.027	3413	3417	3419	rBV5	1283	830	0.06%	0.011%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042523\
 Data File : VV030869.D
 Acq On : 26 Apr 2023 04:42
 Operator : SY/MD
 Sample : 02474-14 10X
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 48 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0AT6

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM041723WMA.M
 Title : VOC Analysis

77	12.213	3473	3475	3479	rBV5	1027	677	0.05%	0.009%
78	12.323	3506	3509	3514	rBV6	1633	1207	0.09%	0.016%
79	12.445	3545	3547	3552	rVB5	989	826	0.06%	0.011%
80	12.503	3562	3565	3568	rBV6	1751	1362	0.10%	0.018%
81	12.590	3589	3592	3593	rBV	1697	926	0.07%	0.012%
82	12.612	3597	3599	3601	rBV3	1153	684	0.05%	0.009%
83	12.876	3675	3681	3684	rBV8	1361	1541	0.11%	0.020%
84	13.056	3733	3737	3739	rBV5	965	783	0.06%	0.010%
85	13.162	3768	3770	3775	rVB4	1147	944	0.07%	0.012%
86	13.184	3775	3777	3779	rBV3	1182	734	0.05%	0.010%
87	13.239	3790	3794	3797	rVB5	1690	1491	0.11%	0.020%
88	13.258	3799	3800	3805	rVB5	1485	744	0.05%	0.010%
89	13.326	3818	3821	3824	rVB4	1579	1006	0.07%	0.013%
90	13.345	3824	3827	3828	rBV2	874	560	0.04%	0.007%
91	13.451	3858	3860	3863	rBV3	984	505	0.04%	0.007%
92	13.525	3880	3883	3885	rBV3	1446	955	0.07%	0.013%
93	13.564	3892	3895	3897	rBV4	946	519	0.04%	0.007%
94	13.596	3903	3905	3908	rBV3	1379	738	0.05%	0.010%
95	13.660	3922	3925	3928	rBV5	1525	964	0.07%	0.013%
96	13.821	3973	3975	3980	rBV6	847	858	0.06%	0.011%
97	14.464	4173	4175	4178	rVB3	1170	681	0.05%	0.009%
98	14.532	4194	4196	4199	rBV3	1560	1083	0.08%	0.014%
99	14.590	4211	4214	4216	rBV4	1298	864	0.06%	0.011%
100	14.991	4336	4339	4347	rBV7	1661	2483	0.18%	0.033%




Sum of corrected areas: 7599014

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042523\
Data File : VV030869.D
Acq On : 26 Apr 2023 04:42
Operator : SY/MD
Sample : 02474-14 10X
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 48 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0AT6

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM041723WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

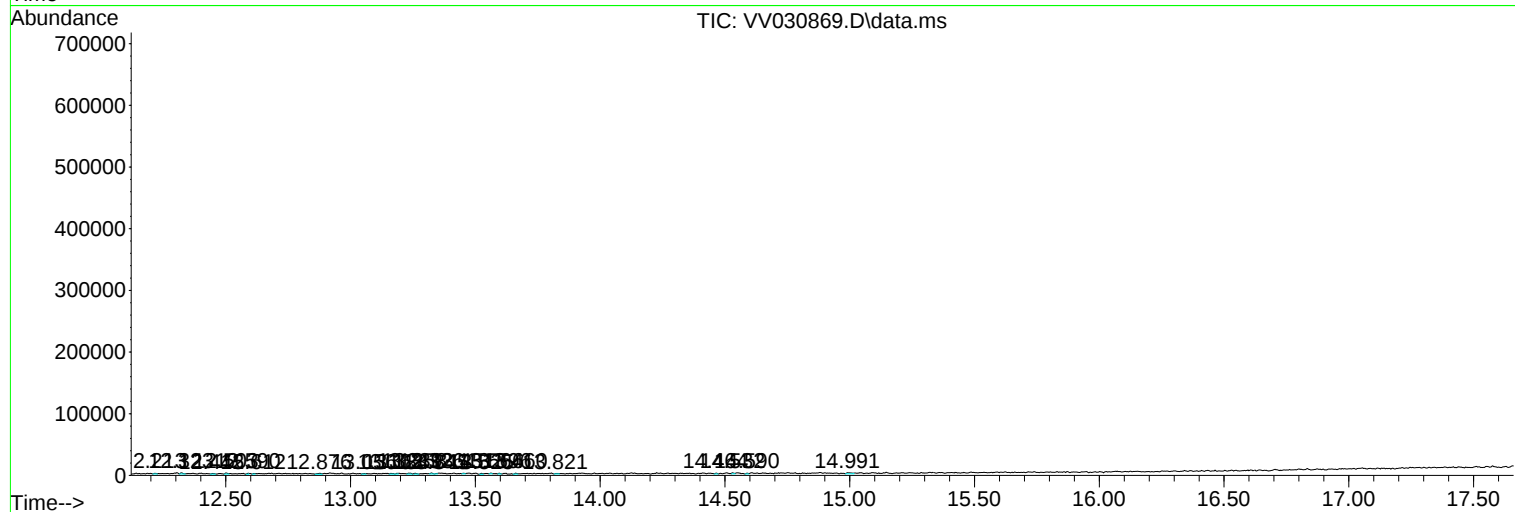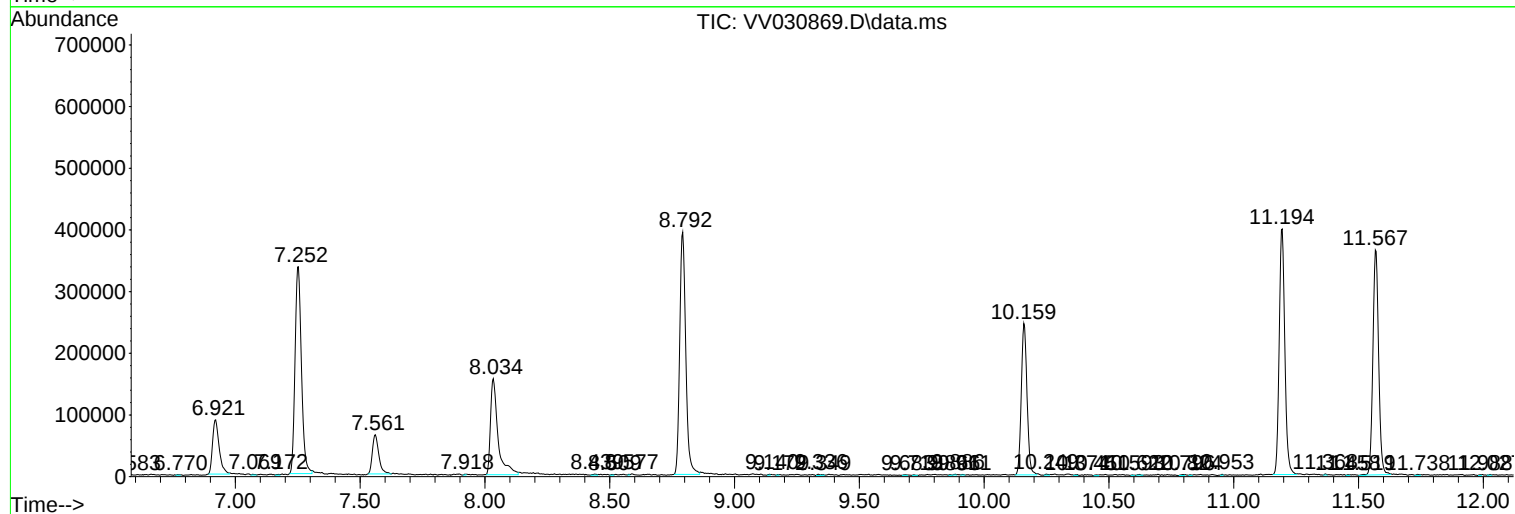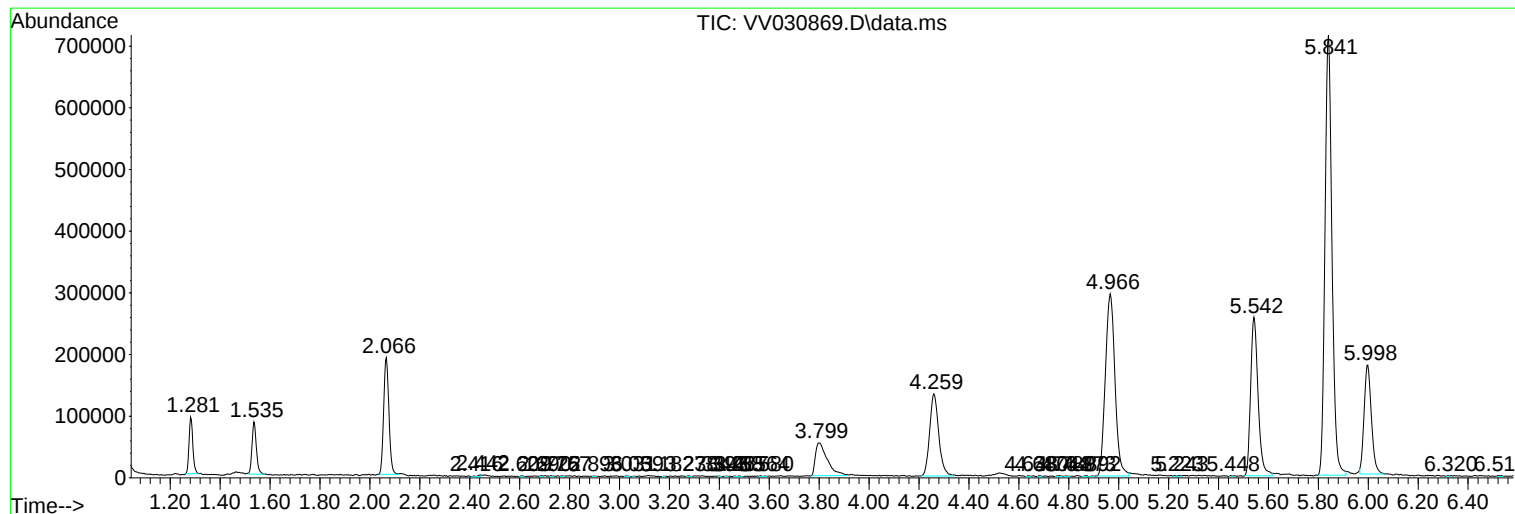

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042523\
Data File : VV030869.D
Acq On : 26 Apr 2023 04:42
Operator : SY/MD
Sample : 02474-14 10X
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 48 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0AT6

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM041723WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042523\
Data File : VV030869.D
Acq On : 26 Apr 2023 04:42
Operator : SY/MD
Sample : 02474-14 10X
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 48 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0AT6

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM041723WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc