

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042523\
 Data File : VV030870.D
 Acq On : 26 Apr 2023 05:06
 Operator : SY/MD
 Sample : 02474-15 10X
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 49 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0AT7

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM041723WMA.M
 Title : VOC Analysis

Signal : TIC: VV030870.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.281	69	75	86	rBV	90694	97386	6.72%	1.286%
2	1.535	148	154	168	rVB	84606	101825	7.02%	1.345%
3	2.066	310	319	333	rVB	185190	265967	18.35%	3.513%
4	2.301	389	392	395	rBV3	1053	648	0.04%	0.009%
5	2.452	432	439	442	rBV8	2860	3378	0.23%	0.045%
6	2.519	457	460	462	rBV4	1134	707	0.05%	0.009%
7	2.844	558	561	562	rBV3	928	512	0.04%	0.007%
8	2.879	569	572	573	rBV3	1118	615	0.04%	0.008%
9	3.047	620	624	629	rBV8	1371	1181	0.08%	0.016%
10	3.069	629	631	633	rBV	947	469	0.03%	0.006%
11	3.121	643	647	649	rVB3	1229	711	0.05%	0.009%
12	3.275	693	695	697	rBV3	991	497	0.03%	0.007%
13	3.410	734	737	740	rVB5	1273	941	0.06%	0.012%
14	3.455	749	751	754	rBV4	1081	744	0.05%	0.010%
15	3.683	819	822	825	rBV4	1187	822	0.06%	0.011%
16	3.799	845	858	887	rBV	52106	176573	12.18%	2.332%
17	4.095	947	950	954	rBV5	1366	936	0.06%	0.012%
18	4.259	986	1001	1025	rBV2	127400	326704	22.54%	4.315%
19	4.645	1115	1121	1124	rBV7	1639	1717	0.12%	0.023%
20	4.850	1183	1185	1187	rBV3	1508	634	0.04%	0.008%
21	4.966	1202	1221	1242	rBV2	290631	777984	53.67%	10.276%
22	5.223	1298	1301	1306	rBV6	1808	2205	0.15%	0.029%
23	5.294	1321	1323	1326	rVB3	1411	715	0.05%	0.009%
24	5.317	1326	1330	1331	rBV3	1575	1198	0.08%	0.016%
25	5.542	1389	1400	1420	rBV	256771	521806	36.00%	6.892%
26	5.841	1479	1493	1520	rBV	736112	1449607	100.00%	19.148%
27	5.998	1531	1542	1559	rVB	170893	346659	23.91%	4.579%
28	6.381	1658	1661	1663	rBV4	1202	955	0.07%	0.013%
29	6.638	1737	1741	1742	rBV3	1090	788	0.05%	0.010%
30	6.773	1781	1783	1785	rBV3	1114	494	0.03%	0.007%
31	6.921	1819	1829	1852	rBV	85543	161570	11.15%	2.134%
32	7.153	1899	1901	1903	rBV3	1167	740	0.05%	0.010%
33	7.249	1919	1931	1952	rBV	325911	594147	40.99%	7.848%
34	7.561	2019	2028	2043	rBV2	63021	114490	7.90%	1.512%
35	7.722	2074	2078	2082	rBV7	1610	1681	0.12%	0.022%
36	7.792	2096	2100	2101	rBV4	1338	699	0.05%	0.009%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042523\
 Data File : VV030870.D
 Acq On : 26 Apr 2023 05:06
 Operator : SY/MD
 Sample : 02474-15 10X
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 49 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0AT7

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM041723WMA.M
 Title : VOC Analysis

37	7.989	2159	2161	2164	rVB4	1536	838	0.06%	0.011%
38	8.034	2164	2175	2205	rBV	151097	321479	22.18%	4.246%
39	8.323	2260	2265	2267	rBV5	1877	1826	0.13%	0.024%
40	8.792	2400	2411	2434	rBV	397324	666804	46.00%	8.808%
41	9.079	2497	2500	2502	rVB4	1538	714	0.05%	0.009%
42	9.275	2558	2561	2562	rBV3	1578	794	0.05%	0.010%
43	9.300	2566	2569	2570	rBV3	1518	764	0.05%	0.010%
44	9.400	2595	2600	2605	rBV8	1314	1747	0.12%	0.023%
45	9.439	2608	2612	2615	rBV5	1527	1463	0.10%	0.019%
46	9.487	2623	2627	2629	rBV4	1243	924	0.06%	0.012%
47	9.513	2632	2635	2636	rBV2	889	520	0.04%	0.007%
48	9.805	2724	2726	2730	rBV4	980	542	0.04%	0.007%
49	9.860	2740	2743	2746	rBV4	1519	1049	0.07%	0.014%
50	10.066	2803	2807	2808	rBV4	1046	581	0.04%	0.008%
51	10.085	2811	2813	2819	rVV7	1295	1154	0.08%	0.015%
52	10.159	2825	2836	2855	rBV	235945	377937	26.07%	4.992%
53	10.307	2876	2882	2884	rBV7	2347	2265	0.16%	0.030%
54	10.403	2910	2912	2915	rBV4	894	596	0.04%	0.008%
55	10.452	2924	2927	2931	rVB4	2183	1674	0.12%	0.022%
56	10.484	2931	2937	2939	rBV6	1644	1893	0.13%	0.025%
57	10.561	2959	2961	2964	rVV4	1063	509	0.04%	0.007%
58	10.895	3060	3065	3068	rBV6	903	1094	0.08%	0.014%
59	10.934	3074	3077	3079	rBV4	940	512	0.04%	0.007%
60	10.950	3079	3082	3083	rBV3	922	582	0.04%	0.008%
61	11.017	3098	3103	3105	rBV5	1021	1029	0.07%	0.014%
62	11.056	3111	3115	3118	rBV4	925	757	0.05%	0.010%
63	11.194	3145	3158	3176	rBV	391069	626938	43.25%	8.281%
64	11.423	3225	3229	3230	rBV3	764	483	0.03%	0.006%
65	11.567	3263	3274	3296	rVB	350444	563896	38.90%	7.448%
66	11.673	3305	3307	3310	rBV4	1499	903	0.06%	0.012%
67	11.744	3327	3329	3333	rBV5	1256	619	0.04%	0.008%
68	11.940	3386	3390	3394	rBV6	1276	1020	0.07%	0.013%
69	12.030	3416	3418	3419	rBV2	1133	470	0.03%	0.006%
70	12.140	3451	3452	3454	rBV2	891	479	0.03%	0.006%
71	12.439	3542	3545	3550	rBV6	1396	1348	0.09%	0.018%
72	12.461	3550	3552	3554	rBV3	915	599	0.04%	0.008%
73	12.516	3564	3569	3573	rVB6	2302	1799	0.12%	0.024%
74	12.535	3573	3575	3577	rBV4	832	496	0.03%	0.007%
75	12.615	3596	3600	3601	rBV4	1262	672	0.05%	0.009%
76	12.683	3619	3621	3625	rBV5	922	760	0.05%	0.010%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042523\
 Data File : VV030870.D
 Acq On : 26 Apr 2023 05:06
 Operator : SY/MD
 Sample : 02474-15 10X
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 49 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0AT7

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM041723WMA.M
 Title : VOC Analysis

77	12.722	3629	3633	3636	rVB4	910	643	0.04%	0.008%
78	12.885	3680	3684	3691	rVB7	1263	1059	0.07%	0.014%
79	12.914	3691	3693	3695	rBV3	1110	612	0.04%	0.008%
80	12.992	3715	3717	3719	rVV2	1155	594	0.04%	0.008%
81	13.008	3719	3722	3723	rVB3	1261	597	0.04%	0.008%
82	13.033	3728	3730	3732	rVV3	1205	483	0.03%	0.006%
83	13.066	3735	3740	3743	rBV7	1261	947	0.07%	0.013%
84	13.107	3750	3753	3758	rVB4	1171	1109	0.08%	0.015%
85	13.133	3758	3761	3765	rBV3	1507	1117	0.08%	0.015%
86	13.159	3765	3769	3771	rBV5	1301	1001	0.07%	0.013%
87	13.197	3775	3781	3784	rVB7	1303	1360	0.09%	0.018%
88	13.217	3784	3787	3789	rBV4	1200	705	0.05%	0.009%
89	13.426	3847	3852	3853	rBV4	1084	868	0.06%	0.011%
90	13.606	3901	3908	3911	rBV9	1280	1755	0.12%	0.023%
91	13.741	3944	3950	3952	rBV6	1312	931	0.06%	0.012%
92	13.776	3958	3961	3962	rBV2	1482	672	0.05%	0.009%
93	13.795	3966	3967	3972	rVB4	1581	802	0.06%	0.011%
94	13.821	3972	3975	3977	rBV3	874	566	0.04%	0.007%
95	13.934	4007	4010	4012	rVB4	1420	844	0.06%	0.011%
96	13.953	4012	4016	4017	rBV4	1273	857	0.06%	0.011%
97	14.027	4036	4039	4040	rBV2	977	486	0.03%	0.006%
98	14.146	4073	4076	4079	rVB4	1806	947	0.07%	0.013%
99	14.265	4108	4113	4118	rBV7	1511	1690	0.12%	0.022%
100	15.020	4346	4348	4353	rBV5	1309	833	0.06%	0.011%




Sum of corrected areas: 7570712

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042523\
Data File : VV030870.D
Acq On : 26 Apr 2023 05:06
Operator : SY/MD
Sample : 02474-15 10X
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 49 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0AT7

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM041723WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

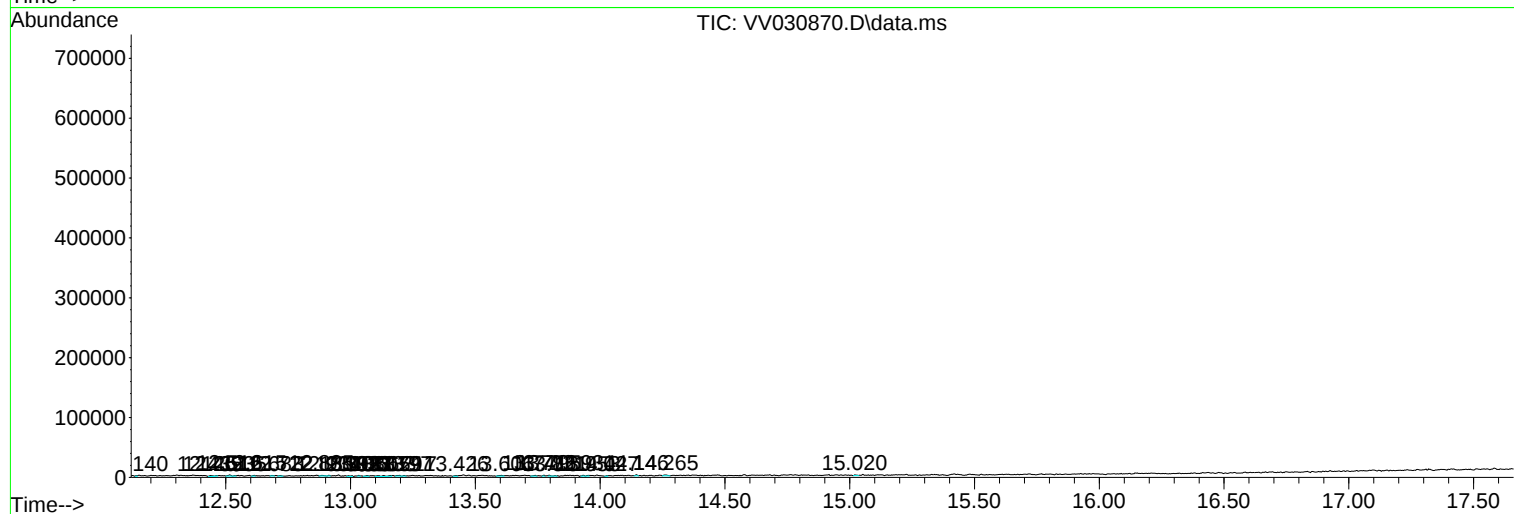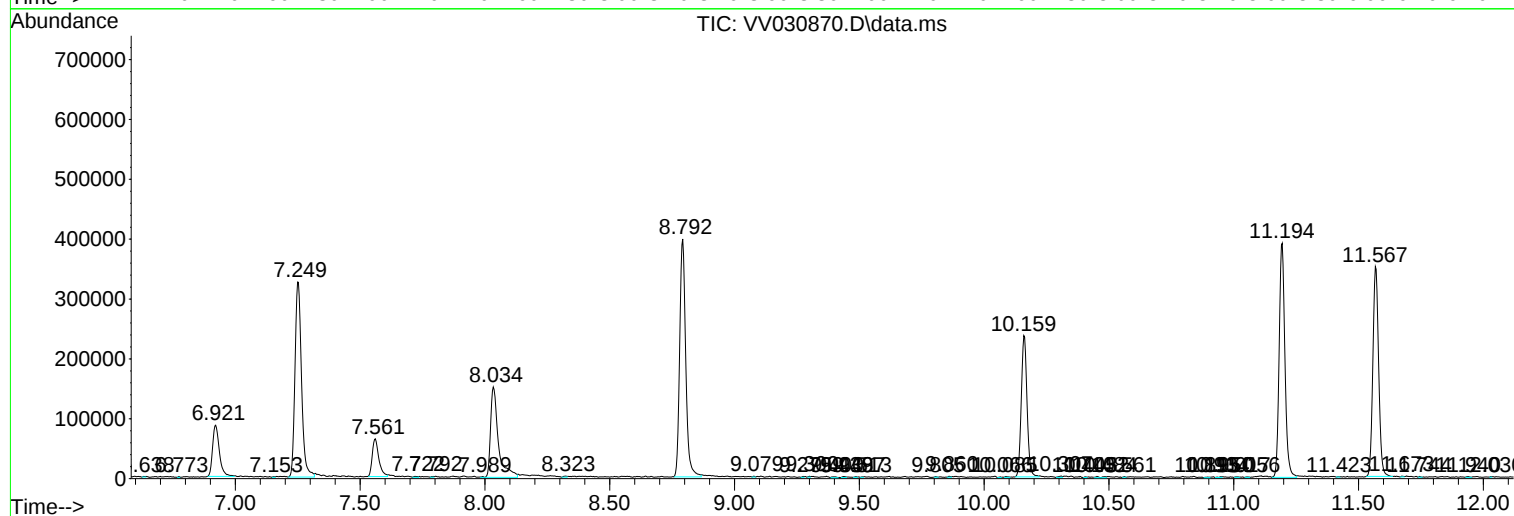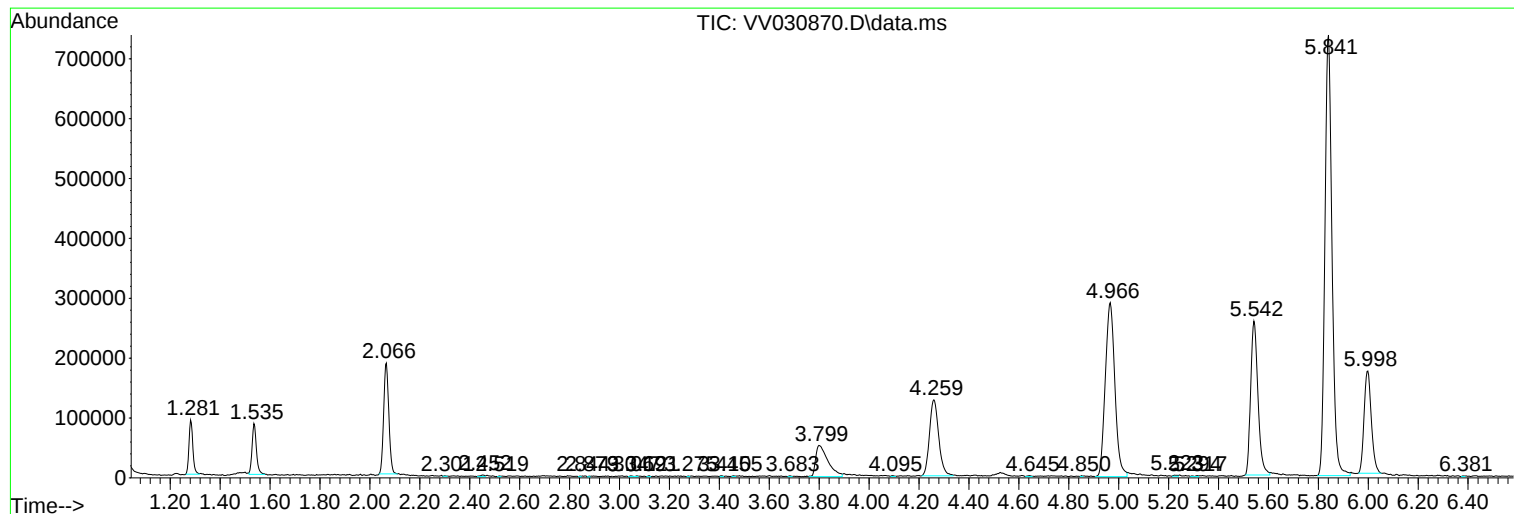

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042523\
Data File : VV030870.D
Acq On : 26 Apr 2023 05:06
Operator : SY/MD
Sample : 02474-15 10X
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 49 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0AT7

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM041723WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042523\
Data File : VV030870.D
Acq On : 26 Apr 2023 05:06
Operator : SY/MD
Sample : 02474-15 10X
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 49 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0AT7

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM041723WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc