
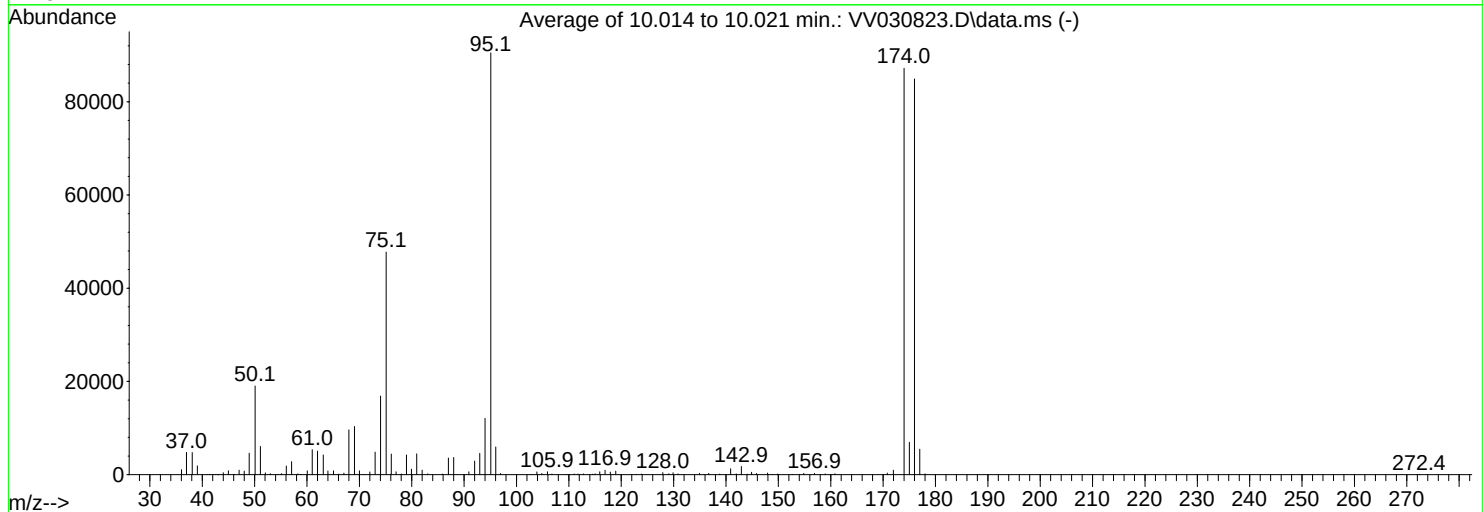


Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042523\
Data File : VV030823.D
Acq On : 25 Apr 2023 09:20
Operator : SY/MD
Sample : BFB372
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BFB372

Integration File: LSCINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM041723WMA.M
Title : VOC Analysis
Last Update : Thu Apr 27 04:45:18 2023

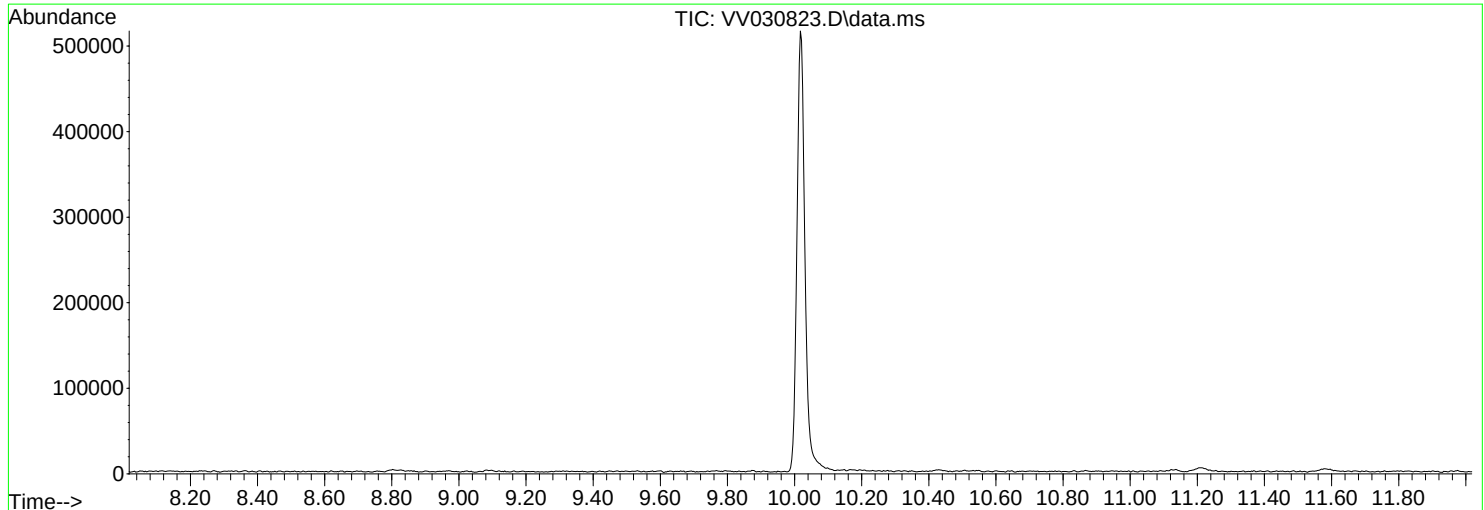

AutoFind: Scans 2791, 2792, 2793; Background Corrected with Scan 2779

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	21.0	19008	PASS
75	95	30	80	52.8	47768	PASS
95	95	100	100	100.0	90507	PASS
96	95	5	9	6.5	5927	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	120	96.3	87197	PASS
175	174	5	9	7.9	6928	PASS
176	174	95	105	97.4	84915	PASS
177	176	5	10	6.4	5466	PASS

m/z	Abundance
35.10	120.0
35.60	134.0
37.00	129.0
38.30	110.0
39.10	116.0
40.10	232.0
40.90	104.0
42.10	146.0
43.10	138.0
44.00	321.0
45.00	122.0
48.20	102.0
48.80	110.0
49.40	108.0
52.70	112.0
60.40	116.0
82.20	106.0
137.50	103.0

Instrument :
MSVOA_V
ClientSampleId :
BFB372

m/z	Abundance
36.00	1074.0
37.00	4695.0
38.10	4753.0
39.10	1999.0
40.10	265.0
41.00	162.0
43.00	185.0
44.10	723.0
45.00	961.0
46.10	179.0
47.10	883.0
48.00	793.0
49.00	4618.0
50.10	18104.0
51.10	5970.0
52.10	374.0
53.00	231.0
55.00	262.0
56.00	1833.0
57.00	2665.0
58.30	183.0
60.10	747.0
61.00	5283.0
62.00	4656.0
63.10	4040.0
64.00	756.0
65.00	710.0
66.10	153.0
67.10	350.0
68.00	9178.0
69.10	9871.0
70.00	829.0
72.00	540.0
73.00	4530.0
74.00	16222.0
75.10	46472.0
76.10	4497.0
77.00	611.0
78.00	406.0
79.00	4219.0
79.90	1056.0
80.90	4143.0
82.00	968.0
83.00	143.0
85.90	170.0
87.00	3406.0
88.00	3600.0
90.90	620.0
92.00	2919.0
93.00	4491.0
94.00	11751.0
95.10	86960.0
96.00	6076.0
96.90	260.0
103.90	557.0
104.80	221.0
105.90	654.0
106.70	132.0
111.00	150.0
111.80	140.0
112.70	164.0
114.60	140.0
115.00	165.0
115.90	493.0
116.90	955.0
117.90	517.0
118.90	714.0
123.00	110.0
123.90	177.0
128.00	435.0
129.10	200.0
129.90	379.0
130.90	189.0
135.00	330.0
135.80	118.0
136.70	232.0
138.80	127.0
140.90	1205.0
141.90	149.0
143.00	1672.0
144.90	542.0
145.90	224.0
147.90	340.0
148.80	148.0
149.80	153.0
152.70	102.0
154.80	283.0
156.90	321.0
158.90	133.0
160.80	170.0
170.80	327.0
171.90	815.0

Instrument :
MSVOA_V
ClientSampleId :
BFB372

174.00	82000.0
175.00	6587.0
176.00	79984.0
177.00	5278.0
178.00	172.0

Instrument :
MSVOA_V
ClientSampleId :
BFB372

m/z	Abundance
36.00	1078.0
37.00	4957.0
38.10	5021.0
39.10	2086.0
40.00	306.0
41.00	149.0
41.50	109.0
42.00	132.0
42.60	131.0
43.00	152.0
44.10	762.0
45.10	996.0
47.10	971.0
48.00	901.0
49.00	4846.0
50.10	19792.0
51.10	6260.0
52.10	402.0
53.00	208.0
54.30	142.0
55.20	295.0
56.00	1925.0
57.10	2899.0
58.30	187.0
60.00	810.0
61.00	5616.0
62.00	5148.0
63.10	4332.0
64.00	790.0
65.10	842.0
66.10	120.0
67.00	343.0
68.00	9880.0
69.10	10721.0
70.00	828.0
72.00	590.0
73.00	5067.0
74.00	17440.0
75.10	49304.0
76.10	4574.0
77.00	605.0
79.00	4425.0
79.90	1185.0
81.00	4652.0
82.00	1104.0
83.00	178.0
85.90	152.0
87.00	3647.0
88.00	3743.0
90.90	617.0
92.00	3011.0
93.00	4716.0
94.00	12572.0
95.10	93720.0
96.00	6104.0
96.90	276.0
103.90	600.0
104.90	261.0
105.90	646.0
106.80	155.0
111.00	127.0
111.70	151.0
112.80	175.0
114.50	163.0
115.00	177.0
115.90	633.0
116.90	976.0
117.90	565.0
119.00	755.0
122.80	101.0
123.90	150.0
128.00	424.0
129.10	220.0
129.90	420.0
130.80	170.0
134.90	289.0
136.70	270.0
138.80	144.0
140.90	1318.0
142.00	164.0
143.00	1845.0
144.10	115.0
144.90	557.0
145.80	247.0
147.90	340.0
149.80	136.0
154.10	115.0
154.80	282.0
156.90	313.0
159.00	177.0
160.80	214.0
170.10	124.0

Instrument :
MSVOA_V
ClientSampleId :
BFB372

170.80	360.0
172.00	977.0
174.00	89960.0
175.00	7155.0
176.00	87992.0
177.00	5620.0
178.00	163.0

Instrument :
MSVOA_V
ClientSampleId :
BFB372

m/z	Abundance
36.10	1022.0
37.10	5017.0
38.10	4758.0
39.00	1980.0
40.00	380.0
40.90	155.0
41.40	115.0
42.00	163.0
42.60	111.0
42.90	122.0
44.00	771.0
45.10	925.0
47.00	1007.0
48.00	937.0
49.00	4662.0
50.10	19128.0
51.10	5945.0
52.00	380.0
53.00	174.0
54.00	184.0
55.10	363.0
56.10	1842.0
57.10	2802.0
58.10	183.0
58.80	114.0
60.00	955.0
61.00	5209.0
62.00	5334.0
63.10	4338.0
64.00	783.0
65.10	915.0
67.00	338.0
68.00	9788.0
69.00	10457.0
70.00	774.0
70.80	112.0
72.00	645.0
73.00	4960.0
74.10	16952.0
75.10	47528.0
76.10	4271.0
77.00	615.0
79.00	4076.0
80.00	1260.0
81.00	4636.0
82.00	1090.0
83.10	194.0
85.80	120.0
87.00	3703.0
88.00	3638.0
90.90	576.0
92.00	2823.0
93.00	4474.0
94.00	11952.0
95.10	90840.0
96.10	5600.0
97.00	232.0
102.80	100.0
103.90	626.0
104.90	222.0
105.90	562.0
106.80	148.0
109.60	114.0
111.00	132.0
111.70	133.0
112.90	198.0
115.00	178.0
115.90	692.0
116.90	960.0
117.90	578.0
119.00	800.0
123.90	110.0
127.80	451.0
129.10	208.0
129.90	432.0
130.80	160.0
134.90	238.0
136.70	277.0
138.80	122.0
140.90	1262.0
142.00	209.0
142.90	1750.0
144.10	152.0
144.90	481.0
145.80	281.0
148.00	344.0
149.90	122.0
152.60	100.0
154.10	124.0
154.90	301.0
156.90	246.0
158.00	102.0

Instrument :
MSVOA_V
ClientSampleId :
BFB372

159.00	234.0
160.80	195.0
170.10	129.0
170.80	332.0
172.00	1086.0
174.00	89632.0
175.00	7041.0
176.00	86768.0
177.00	5499.0
178.00	175.0
272.40	102.0

Instrument :
MSVOA_V
ClientSampleId :
BFB372