

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042524\
 Data File : VV035404.D
 Acq On : 25 Apr 2024 15:12
 Operator : SY/MD
 Sample : P2158-14
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VHBLK001

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM032624WMA.M
 Title : VOC Analysis

Signal : TIC: VV035404.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.278	67	74	93	rVB	257393	285779	16.43%	2.358%
2	1.523	145	150	174	rVB	148879	195467	11.24%	1.613%
3	2.053	306	315	333	rBV	422124	609268	35.03%	5.027%
4	2.449	429	438	449	rBV3	5054	7943	0.46%	0.066%
5	2.725	522	524	527	rBV	253	143	0.01%	0.001%
6	2.745	527	530	534	rVV2	280	208	0.01%	0.002%
7	2.761	534	535	540	rVV2	248	140	0.01%	0.001%
8	2.931	584	588	591	rBV2	327	282	0.02%	0.002%
9	3.005	608	611	614	rVB3	324	192	0.01%	0.002%
10	3.140	650	653	655	rBV2	254	195	0.01%	0.002%
11	3.166	659	661	662	rVB	174	48	0.00%	0.000%
12	3.195	669	670	671	rBV	148	44	0.00%	0.000%
13	3.269	691	693	696	rBV	217	144	0.01%	0.001%
14	3.323	708	710	713	rBV2	147	91	0.01%	0.001%
15	3.413	735	738	739	rBV2	145	67	0.00%	0.001%
16	3.458	749	752	756	rBV2	237	148	0.01%	0.001%
17	3.500	761	765	766	rBV	220	116	0.01%	0.001%
18	3.523	770	772	776	rVB	171	98	0.01%	0.001%
19	3.581	788	790	791	rBV	144	47	0.00%	0.000%
20	3.642	806	809	813	rBV2	247	198	0.01%	0.002%
21	3.696	823	826	828	rBV2	185	108	0.01%	0.001%
22	3.719	828	833	836	rVB2	211	209	0.01%	0.002%
23	3.741	836	840	841	rBV	165	112	0.01%	0.001%
24	3.761	843	846	849	rBV2	150	117	0.01%	0.001%
25	3.796	849	857	901	rBV	103113	325143	18.69%	2.683%
26	4.246	983	997	1038	rVB	268763	692509	39.82%	5.714%
27	4.693	1132	1136	1140	rBV3	335	349	0.02%	0.003%
28	4.738	1148	1150	1153	rVB2	319	100	0.01%	0.001%
29	4.757	1154	1156	1159	rVB3	404	201	0.01%	0.002%
30	4.780	1159	1163	1168	rBV2	330	347	0.02%	0.003%
31	4.867	1187	1190	1193	rBV3	332	237	0.01%	0.002%
32	4.883	1193	1195	1198	rBV	249	82	0.00%	0.001%
33	4.953	1202	1217	1254	rBV2	660579	1739309	100.00%	14.350%
34	5.445	1368	1370	1373	rBV3	254	144	0.01%	0.001%
35	5.532	1386	1397	1435	rBV	401291	853691	49.08%	7.043%
36	5.834	1482	1491	1507	rBV4	7004	16520	0.95%	0.136%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042524\
 Data File : VV035404.D
 Acq On : 25 Apr 2024 15:12
 Operator : SY/MD
 Sample : P2158-14
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VHBLK001

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM032624WMA.M
 Title : VOC Analysis

37	5.986	1526	1538	1567	rBV	374209	780775	44.89%	6.442%
38	6.304	1635	1637	1639	rVB2	437	170	0.01%	0.001%
39	6.407	1666	1669	1671	rBV	71	43	0.00%	0.000%
40	6.420	1671	1673	1674	rBV	143	39	0.00%	0.000%
41	6.432	1674	1677	1682	rBV3	297	251	0.01%	0.002%
42	6.539	1707	1710	1712	rBV	227	137	0.01%	0.001%
43	6.645	1740	1743	1749	rVB2	247	198	0.01%	0.002%
44	6.683	1753	1755	1760	rBV2	270	181	0.01%	0.001%
45	6.732	1768	1770	1772	rBV2	108	59	0.00%	0.000%
46	6.793	1788	1789	1791	rBV	133	41	0.00%	0.000%
47	6.834	1799	1802	1805	rBV	278	146	0.01%	0.001%
48	6.850	1805	1807	1810	rVB	209	128	0.01%	0.001%
49	6.876	1812	1815	1816	rBV	225	129	0.01%	0.001%
50	6.912	1816	1826	1855	rBV	184594	357873	20.58%	2.953%
51	7.243	1918	1929	1963	rBV	738761	1326157	76.25%	10.942%
52	7.555	2016	2026	2062	rBV	127869	246886	14.19%	2.037%
53	7.847	2115	2117	2119	rBV2	264	113	0.01%	0.001%
54	8.031	2164	2174	2222	rBV2	291882	709734	40.81%	5.856%
55	8.561	2336	2339	2342	rBV3	669	493	0.03%	0.004%
56	8.783	2397	2408	2447	rBV	637359	1070737	61.56%	8.834%
57	9.153	2521	2523	2527	rBV2	230	156	0.01%	0.001%
58	9.175	2527	2530	2533	rBV3	501	391	0.02%	0.003%
59	9.220	2542	2544	2546	rBV	349	194	0.01%	0.002%
60	9.410	2601	2603	2606	rVB	234	108	0.01%	0.001%
61	9.429	2606	2609	2610	rBV	197	86	0.00%	0.001%
62	9.439	2610	2612	2615	rBV2	146	66	0.00%	0.001%
63	9.574	2652	2654	2657	rVB2	368	204	0.01%	0.002%
64	9.593	2657	2660	2663	rBV	221	163	0.01%	0.001%
65	9.966	2774	2776	2778	rBV	125	82	0.00%	0.001%
66	10.153	2822	2834	2865	rBV	546100	872210	50.15%	7.196%
67	10.374	2898	2903	2906	rVB3	486	444	0.03%	0.004%
68	10.429	2918	2920	2923	rBV	217	161	0.01%	0.001%
69	10.567	2960	2963	2967	rBV2	274	192	0.01%	0.002%
70	10.747	3016	3019	3020	rBV2	171	86	0.00%	0.001%
71	10.792	3031	3033	3039	rBV2	191	135	0.01%	0.001%
72	10.834	3042	3046	3050	rBV2	235	277	0.02%	0.002%
73	11.185	3144	3155	3183	rBV	555477	901295	51.82%	7.436%
74	11.558	3259	3271	3307	rBV	707588	1117372	64.24%	9.219%
75	11.969	3397	3399	3400	rBV	264	132	0.01%	0.001%
76	12.310	3502	3505	3508	rBV3	447	351	0.02%	0.003%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042524\
Data File : VV035404.D
Acq On : 25 Apr 2024 15:12
Operator : SY/MD
Sample : P2158-14
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 6 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VHBLK001

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM032624WMA.M
Title : VOC Analysis

77	12.715	3629	3631	3632	rBV3	441	162	0.01%	0.001%
78	13.059	3734	3738	3740	rBV	541	422	0.02%	0.003%
79	13.159	3767	3769	3773	rBV	291	142	0.01%	0.001%
80	13.191	3778	3779	3781	rVB2	330	80	0.00%	0.001%
81	13.214	3781	3786	3790	rBV4	1277	1369	0.08%	0.011%




Sum of corrected areas: 12120366

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042524\
Data File : VV035404.D
Acq On : 25 Apr 2024 15:12
Operator : SY/MD
Sample : P2158-14
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 6 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM032624WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

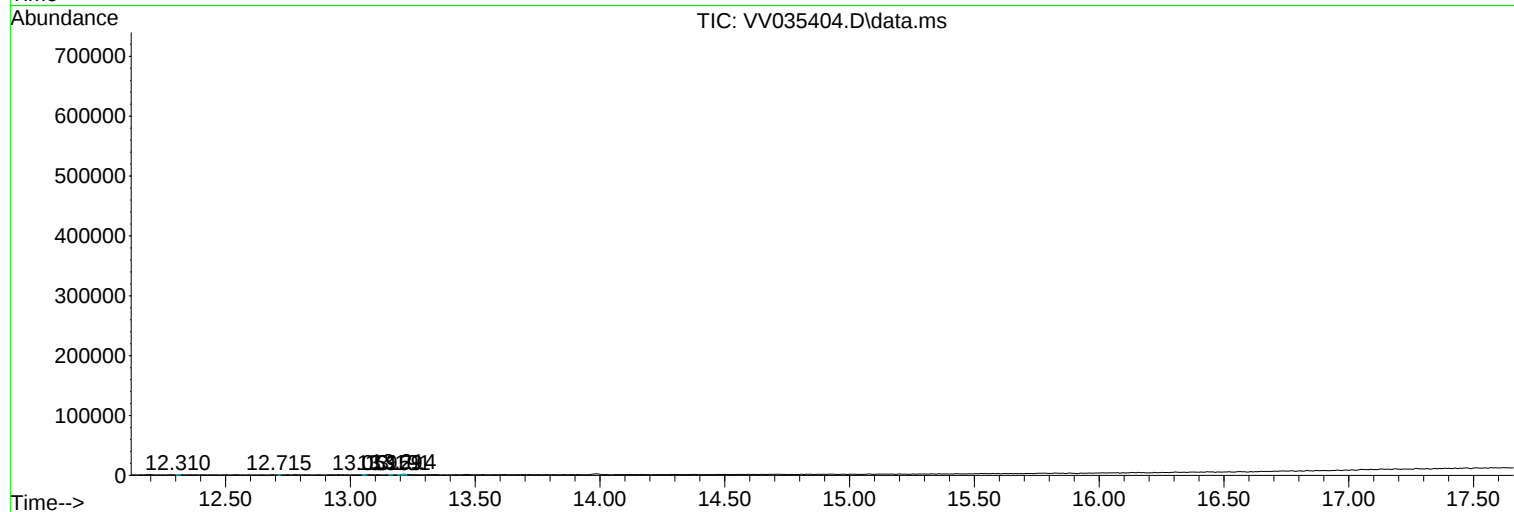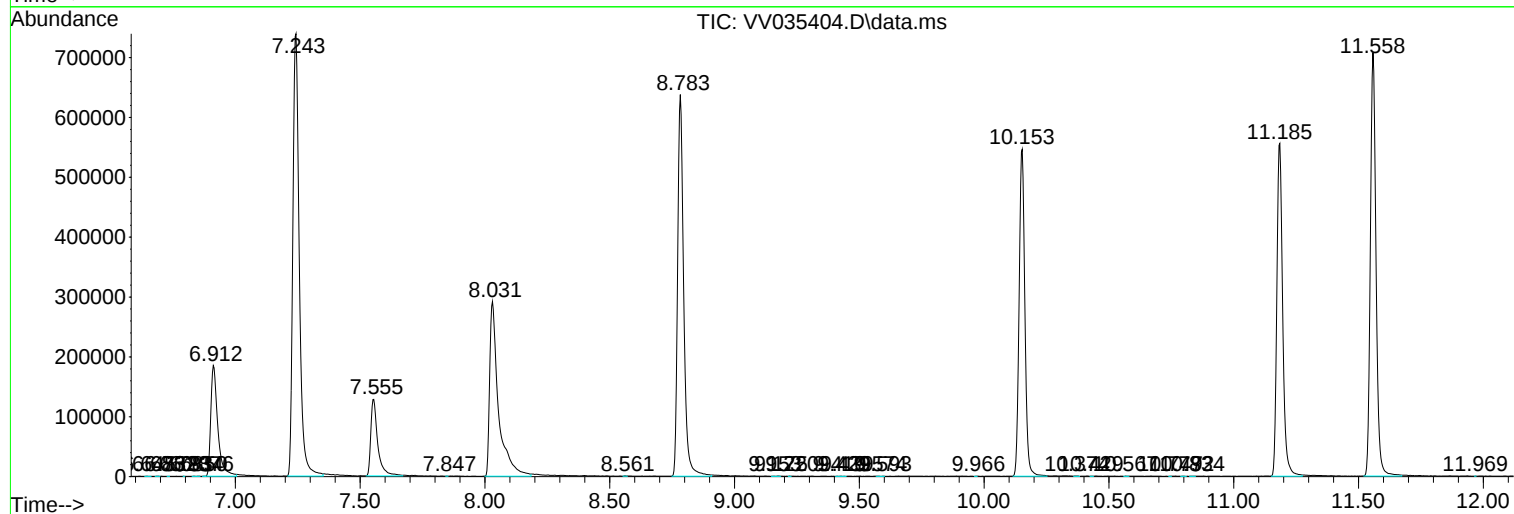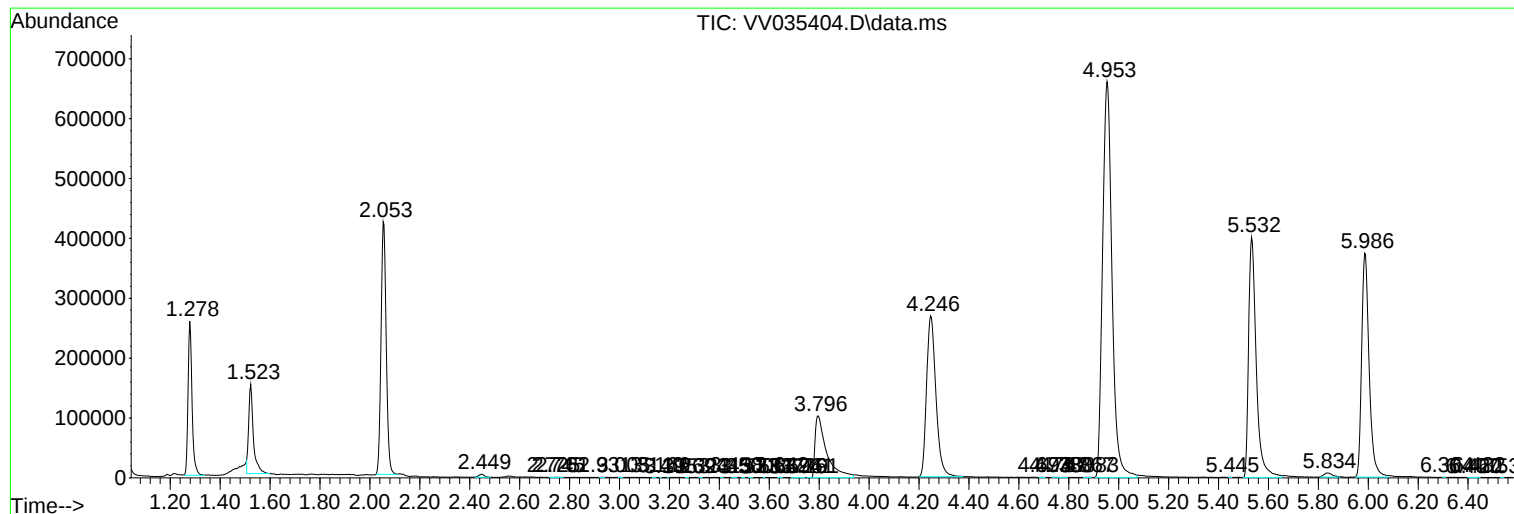

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042524\
Data File : VV035404.D
Acq On : 25 Apr 2024 15:12
Operator : SY/MD
Sample : P2158-14
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 6 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM032624WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042524\
Data File : VV035404.D
Acq On : 25 Apr 2024 15:12
Operator : SY/MD
Sample : P2158-14
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 6 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM032624WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc