

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042524\
 Data File : VV035405.D
 Acq On : 25 Apr 2024 15:36
 Operator : SY/MD
 Sample : P2182-08 100X
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 MCORD1

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM032624WMA.M
 Title : VOC Analysis

Signal : TIC: VV035405.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.278	68	74	90	rVB	216521	238561	13.44%	1.858%
2	1.526	145	151	185	rVB	148257	233476	13.15%	1.819%
3	2.053	306	315	334	rVB	381452	546570	30.79%	4.258%
4	2.558	463	472	476	rBV2	1624	2620	0.15%	0.020%
5	2.863	563	567	570	rBV2	393	311	0.02%	0.002%
6	2.892	575	576	577	rBV2	164	47	0.00%	0.000%
7	2.937	588	590	594	rBV2	374	270	0.02%	0.002%
8	2.970	597	600	603	rVB2	417	259	0.01%	0.002%
9	3.060	626	628	631	rVB2	222	81	0.00%	0.001%
10	3.076	631	633	635	rBV2	160	89	0.01%	0.001%
11	3.114	644	645	648	rBV	138	70	0.00%	0.001%
12	3.191	667	669	671	rBV	189	90	0.01%	0.001%
13	3.236	680	683	685	rBV2	245	140	0.01%	0.001%
14	3.262	689	691	694	rBV	80	41	0.00%	0.000%
15	3.298	697	702	704	rBV2	229	188	0.01%	0.001%
16	3.307	704	705	708	rBV	185	70	0.00%	0.001%
17	3.336	711	714	715	rBV	216	102	0.01%	0.001%
18	3.404	731	735	738	rBV	149	124	0.01%	0.001%
19	3.420	738	740	744	rVB2	249	137	0.01%	0.001%
20	3.458	748	752	754	rBV3	267	211	0.01%	0.002%
21	3.513	764	769	770	rBV2	286	197	0.01%	0.002%
22	3.577	786	789	792	rBV2	213	127	0.01%	0.001%
23	3.661	813	815	819	rBV2	153	82	0.00%	0.001%
24	3.796	848	857	912	rBV	133378	452523	25.49%	3.525%
25	4.246	982	997	1029	rBV	280200	730505	41.15%	5.691%
26	4.744	1148	1152	1155	rBV2	449	361	0.02%	0.003%
27	4.805	1169	1171	1172	rBV	232	66	0.00%	0.001%
28	4.847	1181	1184	1189	rBV3	343	302	0.02%	0.002%
29	4.953	1201	1217	1254	rBV2	671780	1775378	100.00%	13.830%
30	5.362	1342	1344	1345	rBV	449	130	0.01%	0.001%
31	5.532	1386	1397	1433	rBV	434967	918795	51.75%	7.157%
32	5.834	1480	1491	1508	rBV4	9354	22808	1.28%	0.178%
33	5.985	1525	1538	1565	rBV	394853	821026	46.25%	6.396%
34	6.310	1637	1639	1642	rVB2	416	229	0.01%	0.002%
35	6.503	1695	1699	1702	rVB2	311	219	0.01%	0.002%
36	6.548	1711	1713	1715	rBV	222	73	0.00%	0.001%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042524\
 Data File : VV035405.D
 Acq On : 25 Apr 2024 15:36
 Operator : SY/MD
 Sample : P2182-08 100X
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 MC0RD1

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM032624WMA.M
 Title : VOC Analysis

37	6.584	1723	1724	1725	rBV	139	48	0.00%	0.000%
38	6.612	1730	1733	1736	rBV2	402	336	0.02%	0.003%
39	6.696	1756	1759	1761	rBV3	242	145	0.01%	0.001%
40	6.818	1793	1797	1798	rBV	137	108	0.01%	0.001%
41	6.825	1798	1799	1803	rVV	274	176	0.01%	0.001%
42	6.844	1803	1805	1808	rVB	237	121	0.01%	0.001%
43	6.912	1816	1826	1858	rBV	182481	364770	20.55%	2.842%
44	7.153	1899	1901	1909	rBV4	567	588	0.03%	0.005%
45	7.239	1917	1928	1963	rBV	704711	1276510	71.90%	9.944%
46	7.551	2016	2025	2053	rBV	129514	247924	13.96%	1.931%
47	7.866	2120	2123	2125	rVB2	441	207	0.01%	0.002%
48	7.928	2135	2142	2147	rBV4	475	591	0.03%	0.005%
49	7.953	2148	2150	2152	rVB2	326	113	0.01%	0.001%
50	8.030	2165	2174	2223	rBV2	383272	937565	52.81%	7.304%
51	8.783	2396	2408	2441	rBV	678789	1134810	63.92%	8.840%
52	9.198	2535	2537	2541	rVB	381	191	0.01%	0.001%
53	9.223	2541	2545	2547	rBV2	372	279	0.02%	0.002%
54	9.272	2557	2560	2563	rBV2	266	186	0.01%	0.001%
55	9.288	2563	2565	2568	rVV2	318	141	0.01%	0.001%
56	9.381	2591	2594	2599	rBV2	320	232	0.01%	0.002%
57	9.407	2599	2602	2603	rVV	261	154	0.01%	0.001%
58	9.432	2607	2610	2616	rVB2	295	276	0.02%	0.002%
59	9.493	2624	2629	2632	rBV2	346	343	0.02%	0.003%
60	9.535	2639	2642	2643	rBV2	146	65	0.00%	0.001%
61	9.870	2745	2746	2748	rBV	132	34	0.00%	0.000%
62	10.069	2805	2808	2809	rBV	304	147	0.01%	0.001%
63	10.153	2821	2834	2864	rBV	620767	1014019	57.12%	7.899%
64	10.429	2918	2920	2921	rBV	143	70	0.00%	0.001%
65	10.577	2964	2966	2967	rBV	292	112	0.01%	0.001%
66	10.718	3006	3010	3011	rBV2	260	172	0.01%	0.001%
67	10.751	3018	3020	3021	rBV	326	159	0.01%	0.001%
68	10.789	3029	3032	3037	rVB2	576	511	0.03%	0.004%
69	10.825	3037	3043	3046	rBV2	361	322	0.02%	0.003%
70	10.969	3083	3088	3090	rBV	291	242	0.01%	0.002%
71	10.982	3090	3092	3096	rBV	197	166	0.01%	0.001%
72	11.027	3103	3106	3108	rBV	227	124	0.01%	0.001%
73	11.088	3123	3125	3127	rBV	247	95	0.01%	0.001%
74	11.185	3144	3155	3177	rBV	601540	944071	53.18%	7.354%
75	11.452	3235	3238	3241	rBV2	323	250	0.01%	0.002%
76	11.558	3259	3271	3304	rBV	722865	1163006	65.51%	9.060%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042524\
Data File : VV035405.D
Acq On : 25 Apr 2024 15:36
Operator : SY/MD
Sample : P2182-08 100X
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 7 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
MC0RD1

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM032624WMA.M

Title : VOC Analysis

77	11.905	3376	3379	3380	rBV2	459	289	0.02%	0.002%
78	12.033	3417	3419	3423	rVB2	457	223	0.01%	0.002%
79	12.053	3423	3425	3427	rBV2	350	182	0.01%	0.001%
80	12.455	3547	3550	3553	rBV	320	188	0.01%	0.001%
81	12.664	3612	3615	3619	rVB3	469	313	0.02%	0.002%
82	13.271	3800	3804	3807	rBV2	383	340	0.02%	0.003%




Sum of corrected areas: 12837192

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042524\
Data File : VV035405.D
Acq On : 25 Apr 2024 15:36
Operator : SY/MD
Sample : P2182-08 100X
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 7 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
MC0RD1

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM032624WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

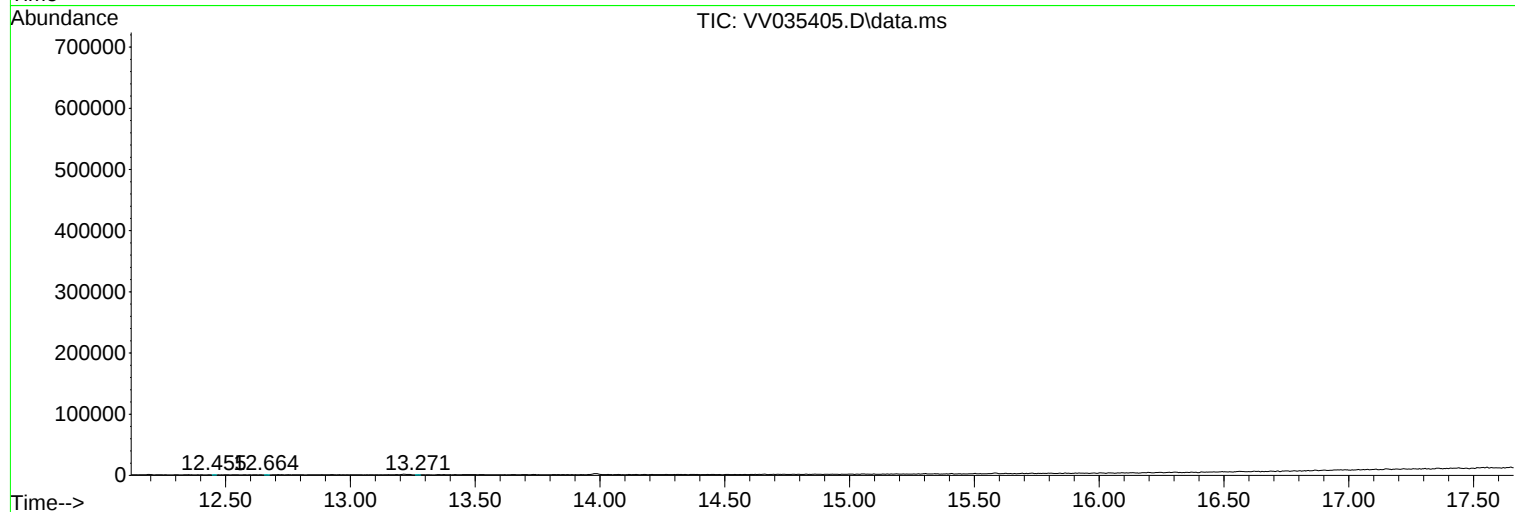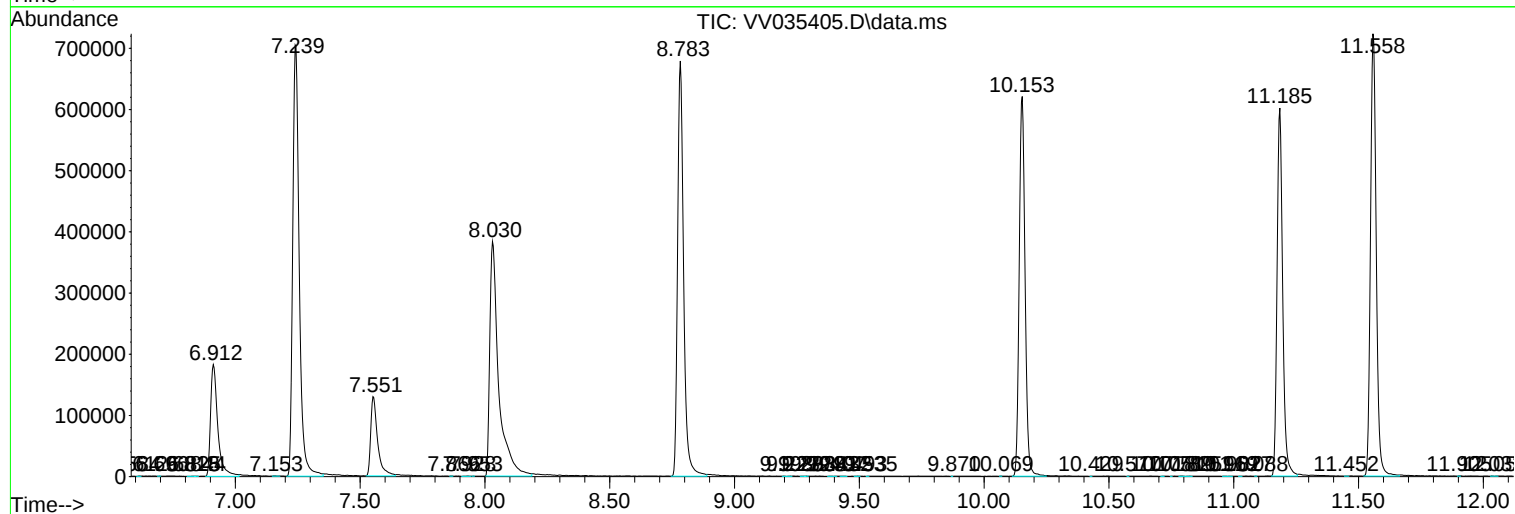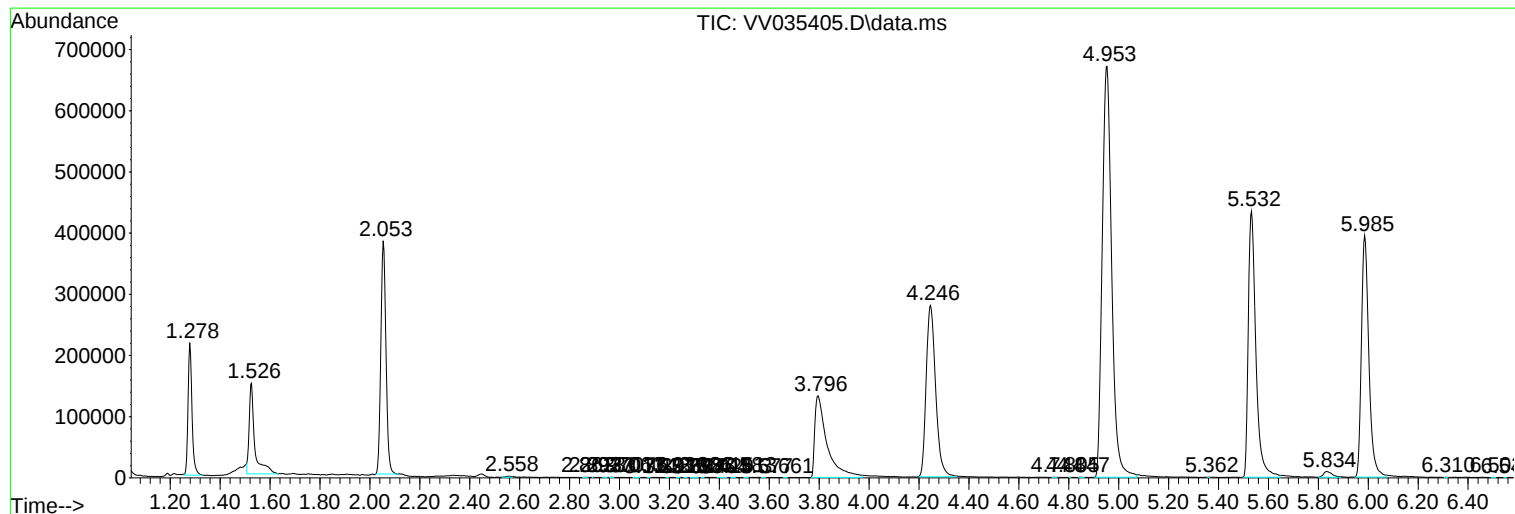

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042524\
Data File : VV035405.D
Acq On : 25 Apr 2024 15:36
Operator : SY/MD
Sample : P2182-08 100X
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 7 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
MC0RD1

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM032624WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042524\
Data File : VV035405.D
Acq On : 25 Apr 2024 15:36
Operator : SY/MD
Sample : P2182-08 100X
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 7 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
MC0RD1

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM032624WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc