

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042524\
 Data File : VV035406.D
 Acq On : 25 Apr 2024 16:05
 Operator : SY/MD
 Sample : P2164-07
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VHBLK002

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM032624WMA.M
 Title : VOC Analysis

Signal : TIC: VV035406.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.278	68	74	91	rVB	256478	289070	15.31%	2.177%
2	1.532	146	153	167	rBV	223432	264130	13.99%	1.989%
3	2.053	306	315	334	rVB	443161	639695	33.89%	4.817%
4	2.491	449	451	455	rVB3	423	229	0.01%	0.002%
5	2.680	508	510	513	rBV2	160	81	0.00%	0.001%
6	2.799	545	547	548	rBV	214	97	0.01%	0.001%
7	2.995	606	608	610	rBV	230	107	0.01%	0.001%
8	3.047	621	624	625	rBV	215	128	0.01%	0.001%
9	3.156	656	658	662	rVB2	199	85	0.00%	0.001%
10	3.195	669	670	676	rVB3	321	237	0.01%	0.002%
11	3.220	676	678	680	rBV	270	149	0.01%	0.001%
12	3.240	680	684	685	rBV	166	121	0.01%	0.001%
13	3.327	704	711	713	rBV2	272	277	0.01%	0.002%
14	3.359	718	721	722	rVV2	143	66	0.00%	0.000%
15	3.407	734	736	739	rVB2	247	130	0.01%	0.001%
16	3.439	743	746	750	rBV2	187	152	0.01%	0.001%
17	3.497	758	764	767	rBV2	243	307	0.02%	0.002%
18	3.510	767	768	772	rVV	190	88	0.00%	0.001%
19	3.542	776	778	780	rBV	223	77	0.00%	0.001%
20	3.558	780	783	787	rBV2	139	107	0.01%	0.001%
21	3.581	787	790	796	rVB	223	174	0.01%	0.001%
22	3.610	796	799	801	rBV	124	77	0.00%	0.001%
23	3.658	812	814	816	rBV	204	90	0.00%	0.001%
24	3.802	849	859	893	rBV	115470	386235	20.46%	2.908%
25	4.243	981	996	1031	rBV	292644	758743	40.19%	5.713%
26	4.741	1147	1151	1154	rBV2	354	219	0.01%	0.002%
27	4.950	1201	1216	1257	rBV2	720418	1887672	100.00%	14.213%
28	5.532	1386	1397	1438	rBV	439563	933930	49.48%	7.032%
29	5.835	1480	1491	1514	rVB5	9170	23297	1.23%	0.175%
30	5.986	1524	1538	1563	rBV	403246	844451	44.74%	6.358%
31	6.288	1630	1632	1635	rBV2	385	228	0.01%	0.002%
32	6.346	1647	1650	1653	rBV2	456	286	0.02%	0.002%
33	6.391	1662	1664	1668	rVB2	328	170	0.01%	0.001%
34	6.410	1668	1670	1671	rBV2	234	91	0.00%	0.001%
35	6.449	1679	1682	1684	rBV	213	131	0.01%	0.001%
36	6.458	1684	1685	1689	rVV	367	188	0.01%	0.001%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042524\
 Data File : VV035406.D
 Acq On : 25 Apr 2024 16:05
 Operator : SY/MD
 Sample : P2164-07
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VHBLK002

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM032624WMA.M
 Title : VOC Analysis

37	6.481	1689	1692	1694	rVV2	423	326	0.02%	0.002%
38	6.507	1696	1700	1705	rVB2	396	372	0.02%	0.003%
39	6.555	1712	1715	1720	rVB	176	115	0.01%	0.001%
40	6.580	1720	1723	1724	rBV2	407	243	0.01%	0.002%
41	6.619	1731	1735	1736	rBV	270	130	0.01%	0.001%
42	6.744	1770	1774	1779	rVB2	702	602	0.03%	0.005%
43	6.767	1779	1781	1782	rBV2	131	54	0.00%	0.000%
44	6.812	1792	1795	1798	rVB2	225	140	0.01%	0.001%
45	6.831	1798	1801	1802	rBV	211	109	0.01%	0.001%
46	6.912	1816	1826	1866	rBV	194997	388015	20.56%	2.922%
47	7.240	1917	1928	1960	rBV	811334	1447043	76.66%	10.895%
48	7.551	2016	2025	2046	rBV	138043	256930	13.61%	1.935%
49	7.870	2122	2124	2128	rVB2	671	283	0.01%	0.002%
50	7.902	2132	2134	2139	rVB2	438	337	0.02%	0.003%
51	7.934	2143	2144	2146	rBV	228	94	0.00%	0.001%
52	7.973	2150	2156	2159	rBV2	314	287	0.02%	0.002%
53	7.992	2159	2162	2163	rBV	330	119	0.01%	0.001%
54	8.034	2165	2175	2211	rBV2	338098	850747	45.07%	6.406%
55	8.407	2287	2291	2295	rBV4	660	560	0.03%	0.004%
56	8.568	2338	2341	2343	rBV2	574	384	0.02%	0.003%
57	8.715	2385	2387	2389	rBV2	344	144	0.01%	0.001%
58	8.783	2397	2408	2437	rBV	689473	1151560	61.00%	8.671%
59	9.040	2485	2488	2493	rBV3	767	712	0.04%	0.005%
60	9.130	2514	2516	2520	rVB2	452	253	0.01%	0.002%
61	9.182	2528	2532	2533	rBV2	441	289	0.02%	0.002%
62	9.339	2580	2581	2583	rBV	136	58	0.00%	0.000%
63	9.358	2584	2587	2590	rVB	350	215	0.01%	0.002%
64	9.429	2606	2609	2614	rBV2	185	236	0.01%	0.002%
65	9.449	2614	2615	2617	rVV2	250	83	0.00%	0.001%
66	9.474	2620	2623	2628	rBV2	163	161	0.01%	0.001%
67	9.539	2641	2643	2645	rBV	171	79	0.00%	0.001%
68	9.616	2665	2667	2672	rVB2	311	148	0.01%	0.001%
69	9.638	2672	2674	2676	rBV	128	62	0.00%	0.000%
70	9.690	2688	2690	2694	rBV2	200	127	0.01%	0.001%
71	9.715	2696	2698	2701	rBV2	192	103	0.01%	0.001%
72	9.873	2745	2747	2748	rBV	256	88	0.00%	0.001%
73	9.953	2770	2772	2774	rBV	120	74	0.00%	0.001%
74	10.027	2792	2795	2796	rBV	200	118	0.01%	0.001%
75	10.059	2802	2805	2809	rBV	308	224	0.01%	0.002%
76	10.101	2816	2818	2819	rBV	138	38	0.00%	0.000%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042524\
 Data File : VV035406.D
 Acq On : 25 Apr 2024 16:05
 Operator : SY/MD
 Sample : P2164-07
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VHBLK002

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM032624WMA.M

Title : VOC Analysis

77	10.153	2822	2834	2869	rBV	590517	958031	50.75%	7.213%
78	10.500	2940	2942	2945	rVB2	254	93	0.00%	0.001%
79	10.657	2989	2991	2997	rVB	470	310	0.02%	0.002%
80	10.712	3003	3008	3011	rBV2	283	279	0.01%	0.002%
81	10.989	3091	3094	3096	rBV2	213	160	0.01%	0.001%
82	11.002	3096	3098	3103	rVB2	308	238	0.01%	0.002%
83	11.185	3144	3155	3178	rBV	608607	972925	51.54%	7.326%
84	11.558	3259	3271	3299	rBV	755337	1214717	64.35%	9.146%
85	12.085	3433	3435	3436	rBV	239	100	0.01%	0.001%
86	12.439	3542	3545	3547	rBV2	318	169	0.01%	0.001%
87	12.555	3574	3581	3586	rBV3	426	649	0.03%	0.005%
88	12.606	3593	3597	3600	rBV2	308	245	0.01%	0.002%
89	13.307	3812	3815	3817	rBV2	467	288	0.02%	0.002%




Sum of corrected areas: 13281181

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042524\
Data File : VV035406.D
Acq On : 25 Apr 2024 16:05
Operator : SY/MD
Sample : P2164-07
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 8 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VHBLK002

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM032624WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

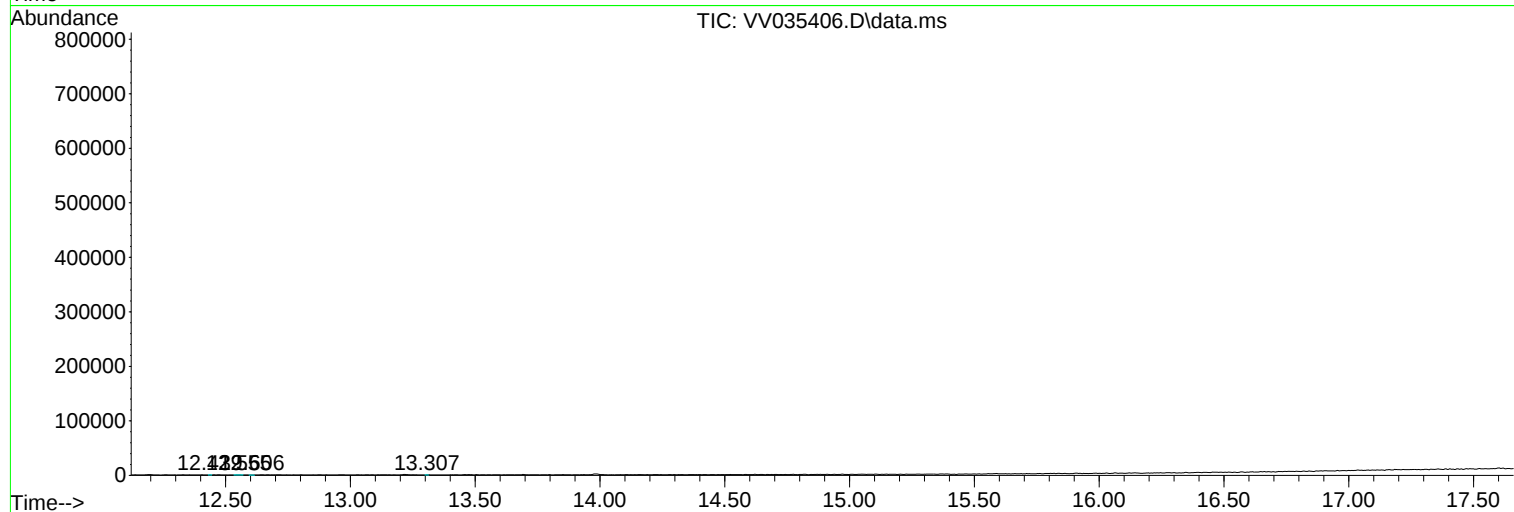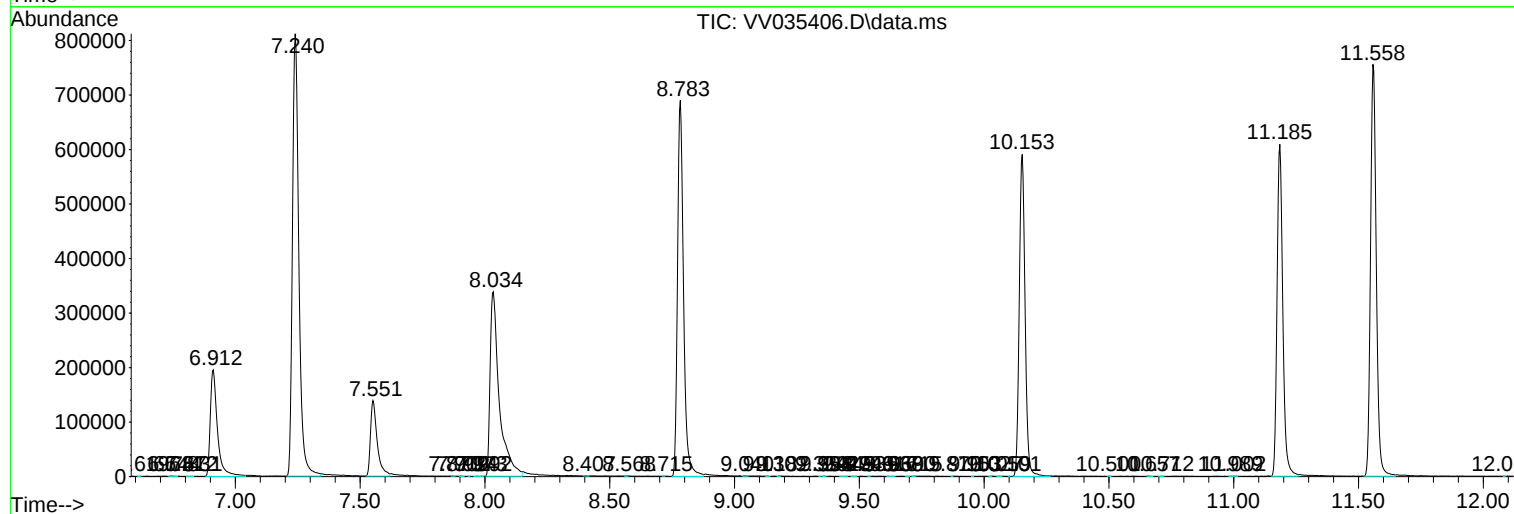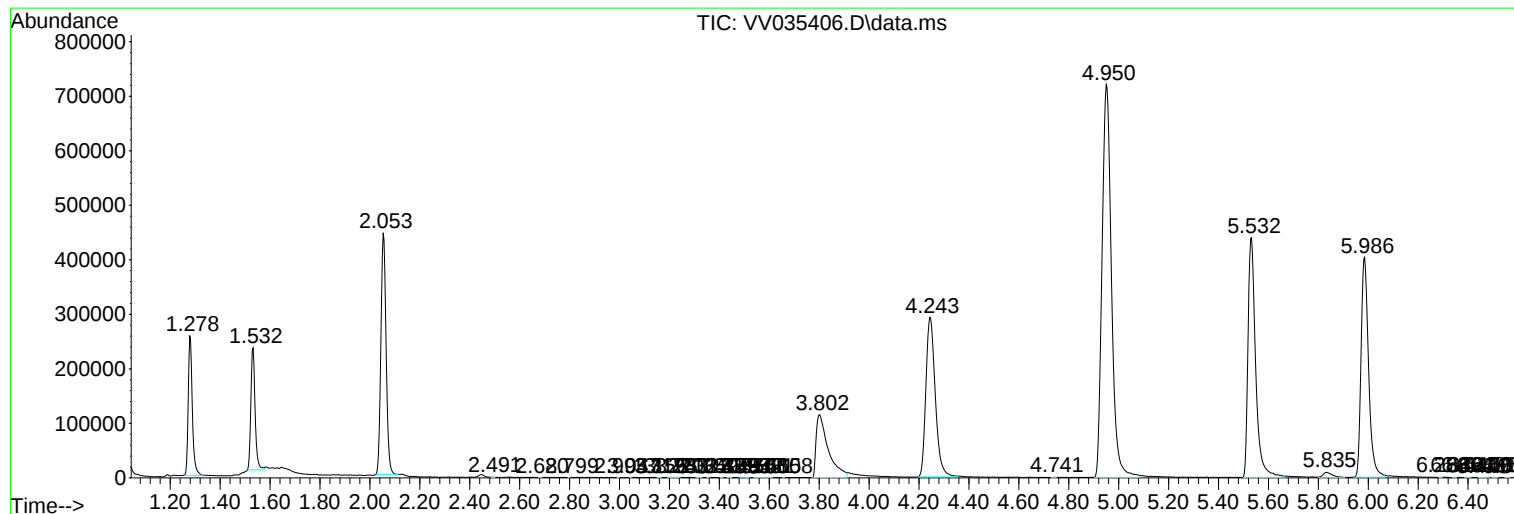

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042524\
Data File : VV035406.D
Acq On : 25 Apr 2024 16:05
Operator : SY/MD
Sample : P2164-07
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 8 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VHBLK002

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM032624WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042524\
Data File : VV035406.D
Acq On : 25 Apr 2024 16:05
Operator : SY/MD
Sample : P2164-07
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 8 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VHBLK002

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM032624WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc