

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042524\
 Data File : VV035407.D
 Acq On : 25 Apr 2024 16:29
 Operator : SY/MD
 Sample : P2238-06
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VHBLK001

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM032624WMA.M
 Title : VOC Analysis

Signal : TIC: VV035407.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.188	42	46	50	rBV	2983	2469	0.14%	0.020%
2	1.278	67	74	91	rVB	242928	272216	15.08%	2.168%
3	1.529	145	152	168	rBV	218942	262398	14.53%	2.089%
4	2.053	305	315	332	rBV	423126	612531	33.93%	4.877%
5	2.233	366	371	379	rVB6	1123	1464	0.08%	0.012%
6	2.410	423	426	429	rVV3	452	276	0.02%	0.002%
7	2.445	429	437	451	rVB3	4418	7688	0.43%	0.061%
8	2.561	462	473	477	rBV6	1133	1944	0.11%	0.015%
9	2.613	485	489	492	rBV2	362	311	0.02%	0.002%
10	2.654	499	502	508	rBV2	321	236	0.01%	0.002%
11	3.127	642	649	651	rBV2	192	215	0.01%	0.002%
12	3.288	696	699	706	rVB2	332	319	0.02%	0.003%
13	3.658	809	814	820	rVB2	180	220	0.01%	0.002%
14	3.709	827	830	835	rBV2	252	203	0.01%	0.002%
15	3.802	850	859	912	rBV	98847	349529	19.36%	2.783%
16	4.246	981	997	1029	rBV	278566	718219	39.78%	5.719%
17	4.632	1113	1117	1119	rBV2	294	245	0.01%	0.002%
18	4.670	1126	1129	1132	rBV2	250	246	0.01%	0.002%
19	4.764	1154	1158	1161	rVB2	373	252	0.01%	0.002%
20	4.953	1198	1217	1250	rBV2	681836	1805452	100.00%	14.376%
21	5.256	1309	1311	1314	rVB2	452	198	0.01%	0.002%
22	5.336	1329	1336	1343	rBV5	616	926	0.05%	0.007%
23	5.416	1355	1361	1364	rBV5	403	396	0.02%	0.003%
24	5.439	1364	1368	1372	rVB3	295	275	0.02%	0.002%
25	5.532	1386	1397	1433	rBV	414671	884670	49.00%	7.044%
26	5.834	1480	1491	1506	rBV4	9791	23453	1.30%	0.187%
27	5.937	1518	1523	1525	rBV2	569	541	0.03%	0.004%
28	5.985	1525	1538	1568	rBV	385415	815041	45.14%	6.490%
29	6.246	1617	1619	1627	rVB5	640	611	0.03%	0.005%
30	6.278	1627	1629	1633	rBV2	340	229	0.01%	0.002%
31	6.358	1650	1654	1656	rBV2	240	207	0.01%	0.002%
32	6.420	1671	1673	1679	rVB3	525	361	0.02%	0.003%
33	6.632	1734	1739	1743	rVV3	333	343	0.02%	0.003%
34	6.719	1764	1766	1770	rVB2	333	234	0.01%	0.002%
35	6.757	1775	1778	1783	rBV3	457	392	0.02%	0.003%
36	6.912	1815	1826	1861	rBV	184272	362407	20.07%	2.886%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042524\
 Data File : VV035407.D
 Acq On : 25 Apr 2024 16:29
 Operator : SY/MD
 Sample : P2238-06
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VHBLK001

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM032624WMA.M
 Title : VOC Analysis

37	7.156	1897	1902	1904	rBV4	345	321	0.02%	0.003%
38	7.178	1906	1909	1912	rVB3	586	442	0.02%	0.004%
39	7.239	1917	1928	1970	rBV	761903	1382306	76.56%	11.007%
40	7.551	2016	2025	2055	rBV	130187	245449	13.59%	1.954%
41	7.850	2115	2118	2120	rBV3	480	350	0.02%	0.003%
42	7.902	2131	2134	2142	rVB3	325	399	0.02%	0.003%
43	7.934	2142	2144	2146	rBV2	340	189	0.01%	0.002%
44	8.034	2165	2175	2214	rBV2	282336	740068	40.99%	5.893%
45	8.317	2260	2263	2264	rBV3	548	303	0.02%	0.002%
46	8.352	2272	2274	2279	rVB5	602	354	0.02%	0.003%
47	8.555	2333	2337	2342	rBV3	756	790	0.04%	0.006%
48	8.580	2342	2345	2350	rVB3	612	522	0.03%	0.004%
49	8.628	2355	2360	2363	rBV4	453	355	0.02%	0.003%
50	8.667	2369	2372	2373	rBV2	411	222	0.01%	0.002%
51	8.696	2379	2381	2384	rBV2	414	277	0.02%	0.002%
52	8.783	2397	2408	2444	rBV	645944	1095241	60.66%	8.721%
53	9.111	2507	2510	2512	rVB	465	205	0.01%	0.002%
54	9.419	2602	2606	2609	rBV2	295	263	0.01%	0.002%
55	9.471	2617	2622	2626	rBV	358	356	0.02%	0.003%
56	9.490	2626	2628	2630	rVV	383	192	0.01%	0.002%
57	9.558	2645	2649	2655	rBV	405	410	0.02%	0.003%
58	9.876	2744	2748	2753	rVB3	345	276	0.02%	0.002%
59	10.153	2819	2834	2860	rBV	553537	893508	49.49%	7.115%
60	10.358	2893	2898	2903	rVB5	582	663	0.04%	0.005%
61	10.390	2903	2908	2910	rBV3	457	390	0.02%	0.003%
62	10.564	2958	2962	2968	rVB2	258	270	0.01%	0.002%
63	10.754	3018	3021	3029	rVB3	435	431	0.02%	0.003%
64	10.796	3029	3034	3035	rBV2	518	354	0.02%	0.003%
65	10.879	3057	3060	3063	rVV	379	258	0.01%	0.002%
66	11.027	3100	3106	3108	rBV2	213	234	0.01%	0.002%
67	11.085	3116	3124	3127	rBV	252	323	0.02%	0.003%
68	11.185	3144	3155	3182	rBV	568630	909327	50.37%	7.241%
69	11.416	3225	3227	3231	rVB	435	225	0.01%	0.002%
70	11.558	3258	3271	3297	rBV	706762	1144784	63.41%	9.116%
71	11.802	3344	3347	3349	rBV3	569	404	0.02%	0.003%
72	11.837	3355	3358	3365	rVB4	544	703	0.04%	0.006%
73	11.870	3365	3368	3370	rBV2	539	393	0.02%	0.003%
74	11.963	3394	3397	3399	rBV2	530	254	0.01%	0.002%
75	12.053	3420	3425	3427	rBV2	352	349	0.02%	0.003%
76	12.085	3433	3435	3437	rBV	427	223	0.01%	0.002%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042524\
 Data File : VV035407.D
 Acq On : 25 Apr 2024 16:29
 Operator : SY/MD
 Sample : P2238-06
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VHBLK001

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM032624WMA.M
 Title : VOC Analysis

77	12.191	3462	3468	3469	rBV3	577	546	0.03%	0.004%
78	12.262	3487	3490	3498	rBV3	419	523	0.03%	0.004%
79	12.320	3502	3508	3509	rBV3	476	440	0.02%	0.004%
80	12.406	3531	3535	3538	rBV2	313	307	0.02%	0.002%
81	12.551	3573	3580	3583	rBV2	526	609	0.03%	0.005%
82	12.606	3591	3597	3601	rBV3	462	449	0.02%	0.004%
83	12.680	3618	3620	3627	rBV3	366	321	0.02%	0.003%
84	13.043	3730	3733	3736	rBV2	532	374	0.02%	0.003%
85	13.088	3743	3747	3750	rBV3	446	376	0.02%	0.003%
86	13.214	3782	3786	3788	rBV2	503	438	0.02%	0.003%
87	13.265	3797	3802	3806	rBV2	348	456	0.03%	0.004%
88	13.468	3861	3865	3867	rBV4	403	331	0.02%	0.003%
89	13.548	3884	3890	3891	rBV	319	315	0.02%	0.003%
90	13.622	3911	3913	3917	rBV2	295	269	0.01%	0.002%
91	13.776	3957	3961	3962	rBV	361	224	0.01%	0.002%
92	13.853	3981	3985	3989	rBV4	588	531	0.03%	0.004%
93	13.953	4013	4016	4018	rBV	468	351	0.02%	0.003%
94	13.979	4021	4024	4025	rBV	894	481	0.03%	0.004%
95	14.082	4052	4056	4057	rBV	321	262	0.01%	0.002%
96	14.197	4089	4092	4093	rBV	424	190	0.01%	0.002%
97	14.326	4128	4132	4136	rBV4	611	552	0.03%	0.004%
98	14.345	4136	4138	4142	rBV3	456	338	0.02%	0.003%
99	14.496	4182	4185	4188	rBV3	630	399	0.02%	0.003%
100	14.776	4270	4272	4275	rVB3	564	275	0.02%	0.002%




Sum of corrected areas: 12558457

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042524\
Data File : VV035407.D
Acq On : 25 Apr 2024 16:29
Operator : SY/MD
Sample : P2238-06
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 9 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM032624WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

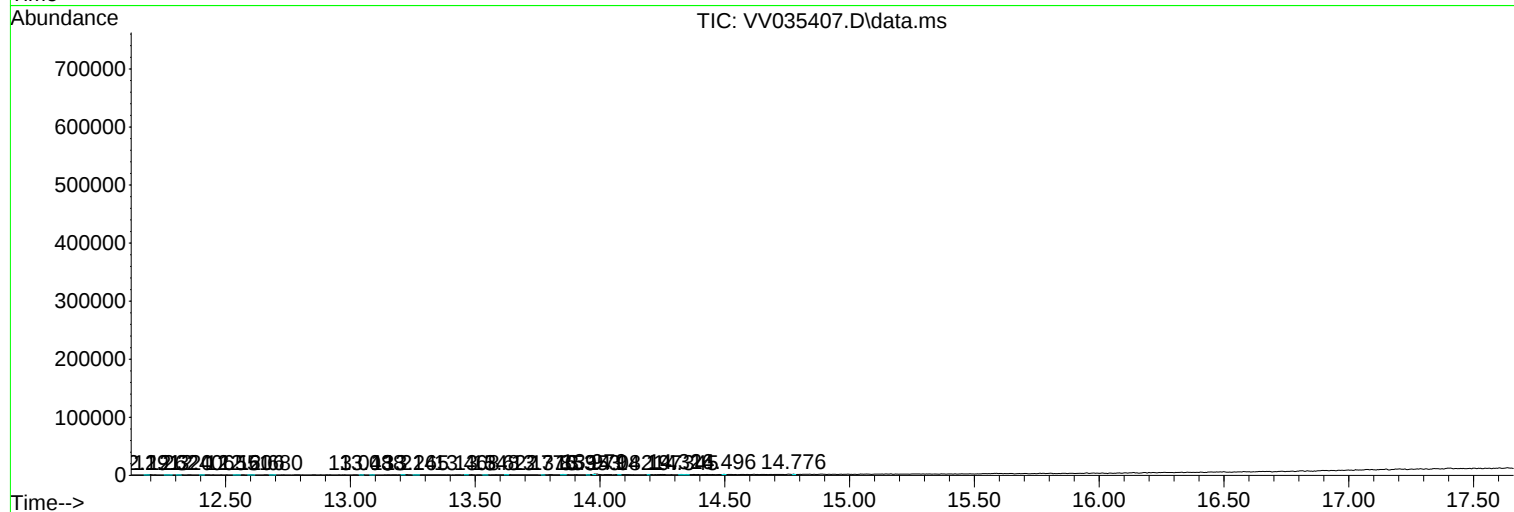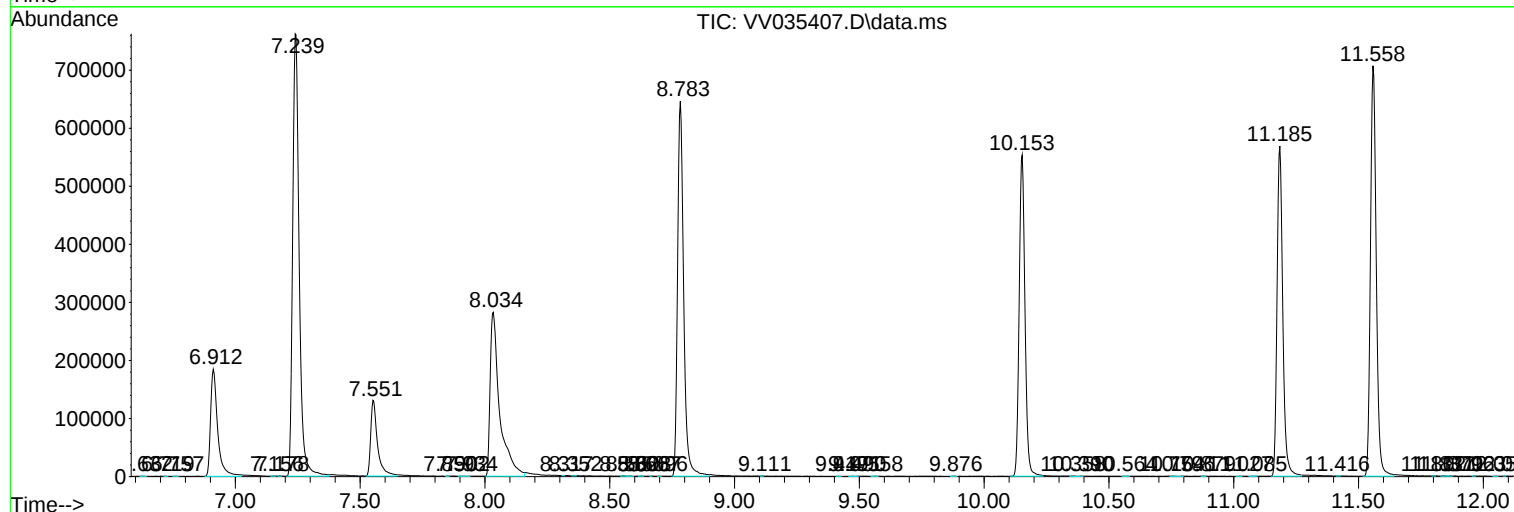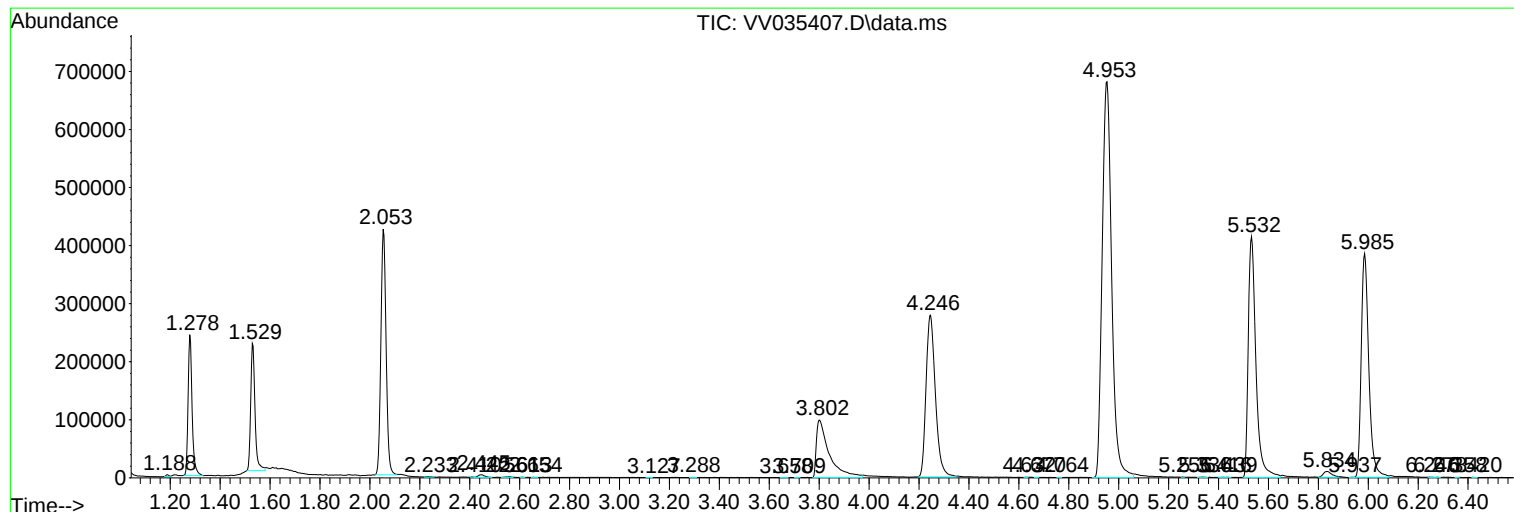

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042524\
Data File : VV035407.D
Acq On : 25 Apr 2024 16:29
Operator : SY/MD
Sample : P2238-06
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 9 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM032624WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042524\
Data File : VV035407.D
Acq On : 25 Apr 2024 16:29
Operator : SY/MD
Sample : P2238-06
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 9 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM032624WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------