

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042524\
 Data File : VV035408.D
 Acq On : 25 Apr 2024 16:53
 Operator : SY/MD
 Sample : P2182-07
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 MC0RC9

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM032624WMA.M

Title : VOC Analysis

Signal : TIC: VV035408.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.278	67	74	91	rBV	255720	278661	14.38%	2.074%
2	1.532	146	153	164	rBV	236595	273904	14.13%	2.039%
3	2.056	306	316	333	rBV	431646	627031	32.35%	4.667%
4	2.551	463	470	471	rBV2	1120	1137	0.06%	0.008%
5	2.815	549	552	554	rBV	383	230	0.01%	0.002%
6	2.847	559	562	565	rBV2	237	161	0.01%	0.001%
7	2.870	566	569	570	rVB	256	98	0.01%	0.001%
8	2.895	575	577	579	rBV	222	124	0.01%	0.001%
9	2.960	594	597	603	rVB	335	310	0.02%	0.002%
10	2.992	604	607	610	rBV2	198	116	0.01%	0.001%
11	3.066	628	630	637	rVB	355	323	0.02%	0.002%
12	3.104	639	642	645	rBV2	146	88	0.00%	0.001%
13	3.172	660	663	665	rVB2	216	127	0.01%	0.001%
14	3.188	665	668	673	rBV3	218	152	0.01%	0.001%
15	3.214	673	676	678	rBV2	196	145	0.01%	0.001%
16	3.268	684	693	698	rBV2	283	381	0.02%	0.003%
17	3.330	706	712	715	rBV2	186	188	0.01%	0.001%
18	3.397	730	733	735	rBV	164	113	0.01%	0.001%
19	3.477	755	758	761	rVB2	280	165	0.01%	0.001%
20	3.506	761	767	770	rVB	98	83	0.00%	0.001%
21	3.532	770	775	778	rBV2	282	273	0.01%	0.002%
22	3.580	785	790	794	rBV2	197	179	0.01%	0.001%
23	3.619	799	802	804	rBV2	140	85	0.00%	0.001%
24	3.677	817	820	823	rVB2	350	200	0.01%	0.001%
25	3.702	823	828	832	rBV2	318	247	0.01%	0.002%
26	3.735	834	838	841	rVB2	278	172	0.01%	0.001%
27	3.799	849	858	906	rBV	100592	343127	17.70%	2.554%
28	4.246	982	997	1031	rBV	284557	752020	38.80%	5.598%
29	4.735	1136	1149	1167	rBV5	6491	15720	0.81%	0.117%
30	4.953	1198	1217	1263	rBV2	699356	1938337	100.00%	14.428%
31	5.355	1340	1342	1347	rVB3	508	253	0.01%	0.002%
32	5.413	1357	1360	1361	rBV2	234	125	0.01%	0.001%
33	5.532	1386	1397	1434	rBV	419305	889175	45.87%	6.619%
34	5.834	1482	1491	1505	rBV3	8794	18250	0.94%	0.136%
35	5.985	1526	1538	1574	rBV	392226	814706	42.03%	6.064%
36	6.236	1613	1616	1619	rBV4	530	337	0.02%	0.003%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042524\
 Data File : VV035408.D
 Acq On : 25 Apr 2024 16:53
 Operator : SY/MD
 Sample : P2182-07
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 MC0RC9

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM032624WMA.M
 Title : VOC Analysis

37	6.329	1643	1645	1646	rBV2	206	100	0.01%	0.001%
38	6.400	1663	1667	1670	rBV	398	239	0.01%	0.002%
39	6.439	1677	1679	1681	rBV	282	132	0.01%	0.001%
40	6.461	1684	1686	1689	rBV2	283	168	0.01%	0.001%
41	6.497	1694	1697	1702	rBV2	167	158	0.01%	0.001%
42	6.526	1702	1706	1709	rVB2	250	167	0.01%	0.001%
43	6.551	1709	1714	1716	rBV	240	208	0.01%	0.002%
44	6.587	1723	1725	1729	rVB2	275	163	0.01%	0.001%
45	6.622	1730	1736	1737	rBV2	173	140	0.01%	0.001%
46	6.715	1762	1765	1769	rBV4	483	299	0.02%	0.002%
47	6.735	1769	1771	1772	rBV	183	96	0.00%	0.001%
48	6.844	1801	1805	1807	rBV2	409	240	0.01%	0.002%
49	6.911	1816	1826	1856	rBV	191317	369635	19.07%	2.751%
50	7.239	1917	1928	1961	rBV	792928	1405526	72.51%	10.462%
51	7.551	2016	2025	2057	rBV	129556	247680	12.78%	1.844%
52	7.908	2133	2136	2145	rVB4	1823	2542	0.13%	0.019%
53	7.947	2146	2148	2151	rVB2	376	186	0.01%	0.001%
54	8.030	2164	2174	2223	rBV2	295680	748963	38.64%	5.575%
55	8.371	2279	2280	2282	rBV2	497	253	0.01%	0.002%
56	8.619	2354	2357	2359	rBV	264	136	0.01%	0.001%
57	8.667	2370	2372	2374	rBV2	217	122	0.01%	0.001%
58	8.738	2392	2394	2396	rBV2	246	164	0.01%	0.001%
59	8.783	2397	2408	2445	rVV2	674250	1280926	66.08%	9.535%
60	9.143	2518	2520	2526	rBV2	420	350	0.02%	0.003%
61	9.246	2550	2552	2553	rBV	270	105	0.01%	0.001%
62	9.275	2557	2561	2562	rBV2	212	175	0.01%	0.001%
63	9.316	2571	2574	2576	rBV2	177	129	0.01%	0.001%
64	9.361	2586	2588	2594	rBV2	283	256	0.01%	0.002%
65	9.397	2597	2599	2602	rVV2	193	122	0.01%	0.001%
66	9.468	2618	2621	2623	rBV2	321	199	0.01%	0.001%
67	9.545	2643	2645	2650	rVB	376	246	0.01%	0.002%
68	9.587	2656	2658	2662	rBV2	221	141	0.01%	0.001%
69	9.615	2662	2667	2671	rVB3	312	284	0.01%	0.002%
70	9.670	2680	2684	2686	rBV2	194	137	0.01%	0.001%
71	9.889	2751	2752	2756	rVB	248	112	0.01%	0.001%
72	9.934	2763	2766	2770	rBV2	239	222	0.01%	0.002%
73	9.956	2771	2773	2775	rVV2	232	109	0.01%	0.001%
74	9.976	2776	2779	2783	rVB	332	223	0.01%	0.002%
75	10.004	2786	2788	2795	rVB3	288	210	0.01%	0.002%
76	10.059	2801	2805	2808	rBV	231	186	0.01%	0.001%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042524\
 Data File : VV035408.D
 Acq On : 25 Apr 2024 16:53
 Operator : SY/MD
 Sample : P2182-07
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 MC0RC9

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM032624WMA.M
 Title : VOC Analysis

77	10.095	2814	2816	2821	rBV	615	234	0.01%	0.002%
78	10.149	2821	2833	2851	rBV	570430	896104	46.23%	6.670%
79	10.467	2929	2932	2934	rBV	236	139	0.01%	0.001%
80	10.484	2934	2937	2940	rVV2	208	183	0.01%	0.001%
81	10.612	2974	2977	2980	rBV	171	139	0.01%	0.001%
82	10.750	3017	3020	3024	rBV2	250	200	0.01%	0.001%
83	10.918	3066	3072	3075	rBV2	262	273	0.01%	0.002%
84	10.937	3075	3078	3081	rBV2	211	134	0.01%	0.001%
85	11.123	3127	3136	3145	rBV	23914	37903	1.96%	0.282%
86	11.185	3145	3155	3184	rVB	593283	1047440	54.04%	7.797%
87	11.506	3249	3255	3260	rBV6	4049	6538	0.34%	0.049%
88	11.557	3261	3271	3301	rVB2	784381	1373846	70.88%	10.226%
89	11.863	3364	3366	3370	rVB2	696	441	0.02%	0.003%
90	11.924	3381	3385	3388	rBV2	372	376	0.02%	0.003%
91	12.091	3434	3437	3438	rBV	234	137	0.01%	0.001%
92	12.426	3538	3541	3545	rBV	217	165	0.01%	0.001%
93	12.448	3545	3548	3551	rBV2	244	173	0.01%	0.001%
94	12.959	3705	3707	3711	rVB	456	275	0.01%	0.002%
95	13.030	3724	3729	3734	rBV	333	359	0.02%	0.003%
96	13.056	3734	3737	3742	rBV2	404	369	0.02%	0.003%
97	13.094	3747	3749	3751	rBV	403	154	0.01%	0.001%
98	13.204	3774	3783	3793	rBV3	21155	33577	1.73%	0.250%
99	13.319	3816	3819	3824	rBV	515	500	0.03%	0.004%
100	13.683	3923	3932	3941	rBV4	10273	16737	0.86%	0.125%




Sum of corrected areas: 13434588

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042524\
Data File : VV035408.D
Acq On : 25 Apr 2024 16:53
Operator : SY/MD
Sample : P2182-07
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 9 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
MC0RC9

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM032624WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

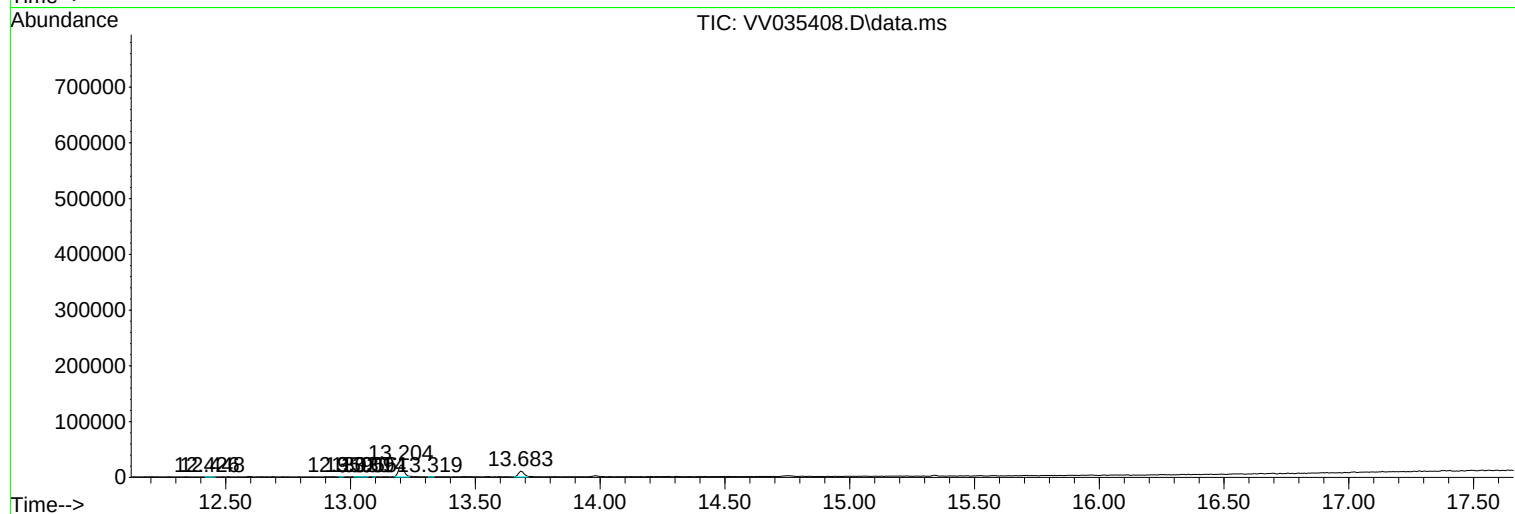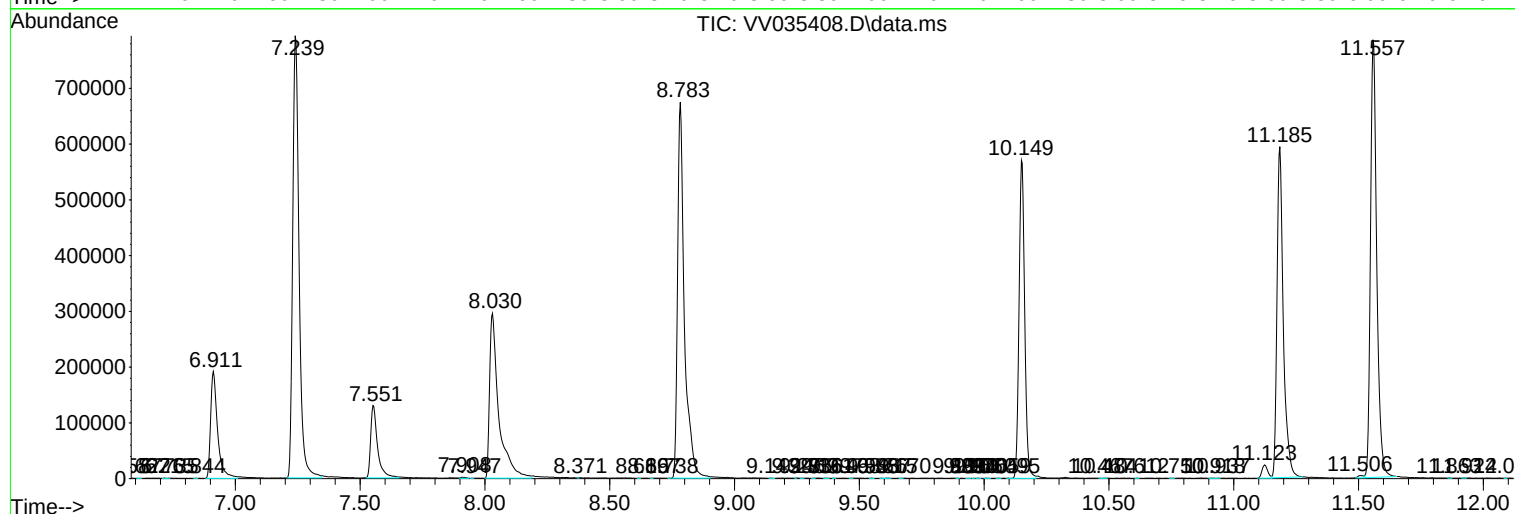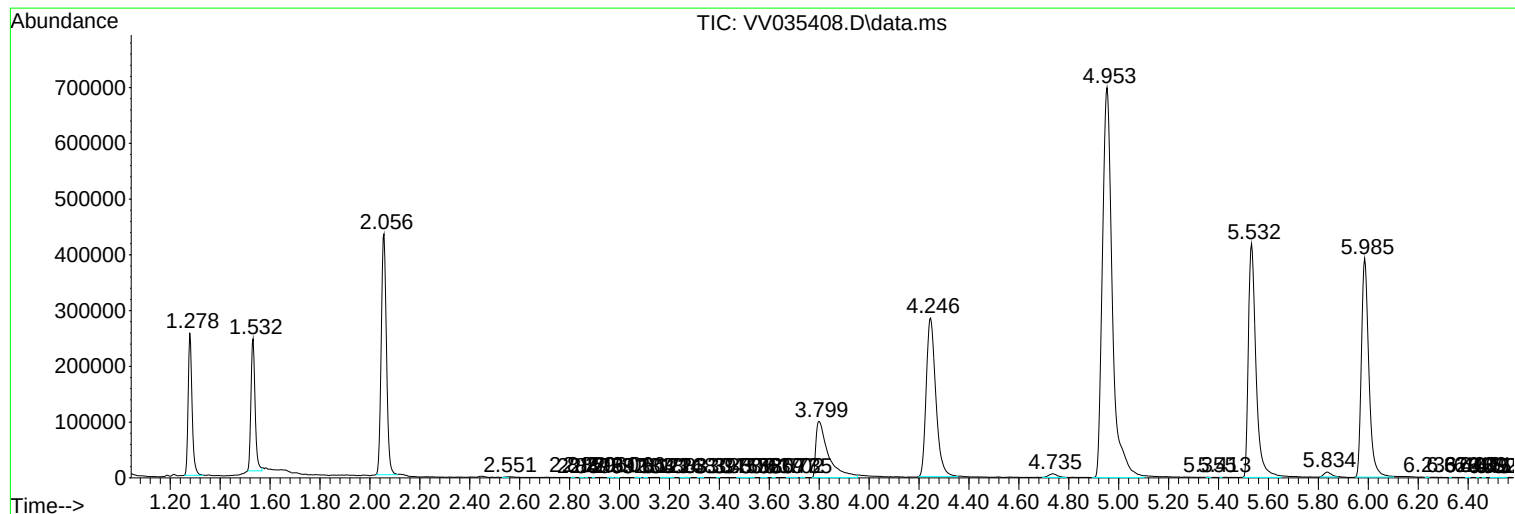

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042524\
Data File : VV035408.D
Acq On : 25 Apr 2024 16:53
Operator : SY/MD
Sample : P2182-07
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 9 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
MC0RC9

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM032624WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042524\
Data File : VV035408.D
Acq On : 25 Apr 2024 16:53
Operator : SY/MD
Sample : P2182-07
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 9 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
MC0RC9

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM032624WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------