

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042524\
 Data File : VV035411.D
 Acq On : 25 Apr 2024 18:05
 Operator : SY/MD
 Sample : P2182-13
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VHBLK001

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM032624WMA.M

Title : VOC Analysis

Signal : TIC: VV035411.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.188	41	46	50	rBV	2974	2945	0.16%	0.023%
2	1.217	50	55	60	rVV3	3158	3660	0.20%	0.029%
3	1.278	67	74	89	rBV	278547	303456	16.88%	2.414%
4	1.532	145	153	168	rBV	244180	292584	16.28%	2.328%
5	2.056	305	316	334	rBV	449068	656210	36.51%	5.221%
6	2.445	428	437	448	rVB3	4653	7698	0.43%	0.061%
7	2.542	460	467	468	rBV3	529	571	0.03%	0.005%
8	2.555	468	471	479	rVV2	803	901	0.05%	0.007%
9	2.709	514	519	520	rBV2	408	330	0.02%	0.003%
10	2.728	522	525	531	rVB2	504	502	0.03%	0.004%
11	2.764	531	536	538	rBV	260	215	0.01%	0.002%
12	2.921	580	585	588	rBV2	198	194	0.01%	0.002%
13	3.069	628	631	637	rVB3	314	273	0.02%	0.002%
14	3.105	637	642	646	rBV2	322	347	0.02%	0.003%
15	3.269	688	693	697	rVB2	278	279	0.02%	0.002%
16	3.362	718	722	726	rVV2	311	285	0.02%	0.002%
17	3.426	739	742	747	rBV2	232	215	0.01%	0.002%
18	3.600	794	796	800	rVB2	364	195	0.01%	0.002%
19	3.629	800	805	807	rBV3	313	306	0.02%	0.002%
20	3.757	840	845	850	rBV3	311	360	0.02%	0.003%
21	3.799	850	858	907	rBV	94800	324894	18.08%	2.585%
22	4.246	981	997	1030	rBV	277509	714532	39.75%	5.685%
23	4.436	1052	1056	1062	rBV4	535	464	0.03%	0.004%
24	4.529	1082	1085	1087	rBV	321	214	0.01%	0.002%
25	4.777	1158	1162	1165	rBV3	298	246	0.01%	0.002%
26	4.834	1175	1180	1182	rBV3	359	257	0.01%	0.002%
27	4.953	1200	1217	1264	rBV2	677586	1797442	100.00%	14.301%
28	5.252	1308	1310	1315	rVB2	708	478	0.03%	0.004%
29	5.400	1348	1356	1359	rBV4	539	648	0.04%	0.005%
30	5.532	1386	1397	1434	rBV	425321	899875	50.06%	7.160%
31	5.831	1478	1490	1516	rBV3	10954	27013	1.50%	0.215%
32	5.985	1522	1538	1574	rBV	383297	799347	44.47%	6.360%
33	6.243	1615	1618	1621	rVB2	571	410	0.02%	0.003%
34	6.262	1621	1624	1626	rVB2	403	227	0.01%	0.002%
35	6.278	1627	1629	1633	rBV2	386	259	0.01%	0.002%
36	6.346	1647	1650	1653	rBV2	282	191	0.01%	0.002%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042524\
 Data File : VV035411.D
 Acq On : 25 Apr 2024 18:05
 Operator : SY/MD
 Sample : P2182-13
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VHBLK001

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM032624WMA.M
 Title : VOC Analysis

37	6.436	1674	1678	1680	rBV3	325	227	0.01%	0.002%
38	6.516	1700	1703	1710	rVV	229	226	0.01%	0.002%
39	6.809	1791	1794	1797	rBV2	295	192	0.01%	0.002%
40	6.912	1816	1826	1860	rBV	183490	360171	20.04%	2.866%
41	7.239	1917	1928	1963	rBV	757430	1374719	76.48%	10.938%
42	7.551	2016	2025	2052	rBV	126117	240438	13.38%	1.913%
43	7.793	2098	2100	2105	rVB3	435	358	0.02%	0.003%
44	7.821	2105	2109	2112	rBV4	434	320	0.02%	0.003%
45	7.902	2130	2134	2136	rVB4	390	249	0.01%	0.002%
46	8.027	2164	2173	2224	rBV3	265644	702618	39.09%	5.590%
47	8.378	2278	2282	2283	rBV3	427	316	0.02%	0.003%
48	8.407	2289	2291	2294	rVB4	465	248	0.01%	0.002%
49	8.442	2298	2302	2304	rVB3	406	249	0.01%	0.002%
50	8.455	2304	2306	2309	rVB	472	329	0.02%	0.003%
51	8.487	2313	2316	2321	rVB4	487	409	0.02%	0.003%
52	8.516	2321	2325	2329	rBV2	265	268	0.01%	0.002%
53	8.558	2335	2338	2343	rBV4	570	418	0.02%	0.003%
54	8.783	2396	2408	2442	rBV	661903	1121087	62.37%	8.920%
55	9.066	2493	2496	2497	rBV3	525	292	0.02%	0.002%
56	9.075	2497	2499	2504	rVB4	423	259	0.01%	0.002%
57	9.101	2504	2507	2509	rBV2	504	296	0.02%	0.002%
58	9.149	2516	2522	2525	rVB2	676	747	0.04%	0.006%
59	9.172	2525	2529	2530	rBV2	337	196	0.01%	0.002%
60	9.349	2582	2584	2587	rVB	434	229	0.01%	0.002%
61	9.503	2630	2632	2637	rBV2	338	235	0.01%	0.002%
62	9.619	2665	2668	2675	rVB	194	193	0.01%	0.002%
63	9.657	2675	2680	2684	rBV2	423	379	0.02%	0.003%
64	9.712	2690	2697	2700	rBV2	219	244	0.01%	0.002%
65	9.870	2739	2746	2751	rBV4	309	403	0.02%	0.003%
66	9.937	2763	2767	2769	rBV2	377	323	0.02%	0.003%
67	10.149	2821	2833	2857	rVV	539957	847643	47.16%	6.744%
68	10.320	2883	2886	2888	rBV3	390	234	0.01%	0.002%
69	10.362	2897	2899	2901	rBV2	350	196	0.01%	0.002%
70	10.519	2946	2948	2953	rVB2	282	195	0.01%	0.002%
71	10.722	3007	3011	3014	rVB	280	188	0.01%	0.001%
72	10.789	3029	3032	3037	rBV2	427	273	0.02%	0.002%
73	10.992	3090	3095	3098	rBV2	188	199	0.01%	0.002%
74	11.136	3134	3140	3143	rBV4	688	702	0.04%	0.006%
75	11.181	3143	3154	3180	rBV	586725	934917	52.01%	7.438%
76	11.471	3241	3244	3249	rVB4	264	269	0.01%	0.002%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042524\
 Data File : VV035411.D
 Acq On : 25 Apr 2024 18:05
 Operator : SY/MD
 Sample : P2182-13
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VHBLK001

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM032624WMA.M
 Title : VOC Analysis

77	11.558	3259	3271	3292	rBV	706844	1124994	62.59%	8.951%
78	11.815	3348	3351	3353	rBV2	253	190	0.01%	0.002%
79	11.921	3381	3384	3387	rVB3	396	232	0.01%	0.002%
80	11.943	3387	3391	3394	rBV2	465	353	0.02%	0.003%
81	12.011	3407	3412	3417	rVB5	555	660	0.04%	0.005%
82	12.046	3417	3423	3425	rBV3	426	460	0.03%	0.004%
83	12.085	3432	3435	3438	rBV2	294	206	0.01%	0.002%
84	12.178	3457	3464	3466	rBV4	644	732	0.04%	0.006%
85	12.236	3477	3482	3486	rBV3	328	408	0.02%	0.003%
86	12.535	3572	3575	3581	rVB2	259	212	0.01%	0.002%
87	12.583	3586	3590	3597	rVB3	393	490	0.03%	0.004%
88	12.873	3675	3680	3682	rBV2	485	425	0.02%	0.003%
89	13.053	3734	3736	3742	rVB	498	367	0.02%	0.003%
90	13.210	3776	3785	3795	rBV4	2743	4789	0.27%	0.038%
91	13.400	3841	3844	3845	rBV	332	201	0.01%	0.002%
92	13.599	3904	3906	3909	rBV2	346	189	0.01%	0.002%
93	13.648	3917	3921	3923	rBV	362	220	0.01%	0.002%
94	13.664	3923	3926	3929	rBV2	372	208	0.01%	0.002%
95	13.683	3929	3932	3933	rBV2	479	286	0.02%	0.002%
96	13.824	3972	3976	3983	rBV	624	729	0.04%	0.006%
97	13.979	4020	4024	4032	rVB3	1496	1742	0.10%	0.014%
98	14.258	4109	4111	4115	rBV2	338	288	0.02%	0.002%
99	14.297	4121	4123	4130	rVB3	520	440	0.02%	0.004%
100	15.043	4352	4355	4357	rBV3	668	448	0.02%	0.004%




Sum of corrected areas: 12568746

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042524\
Data File : VV035411.D
Acq On : 25 Apr 2024 18:05
Operator : SY/MD
Sample : P2182-13
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 12 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM032624WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

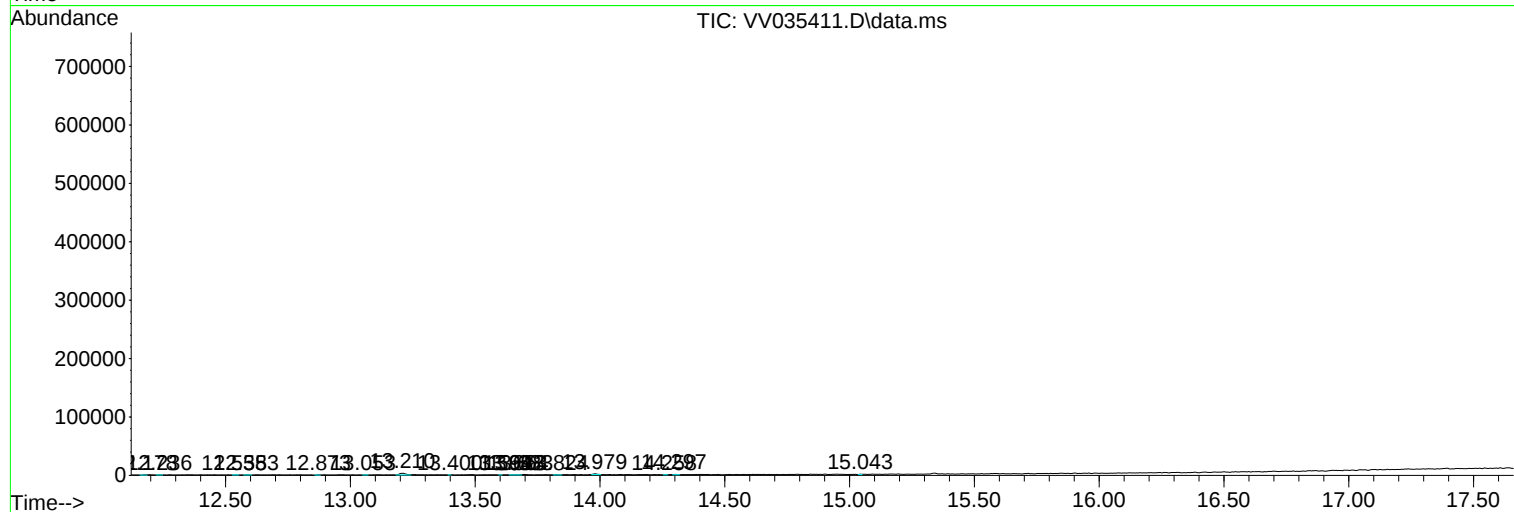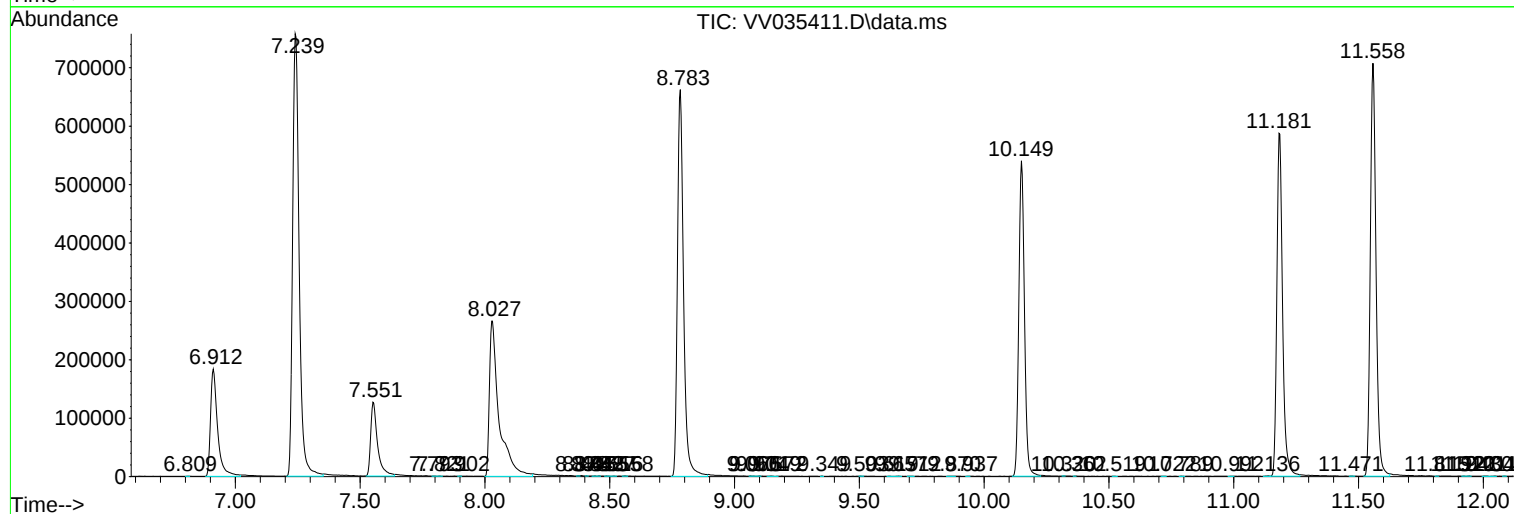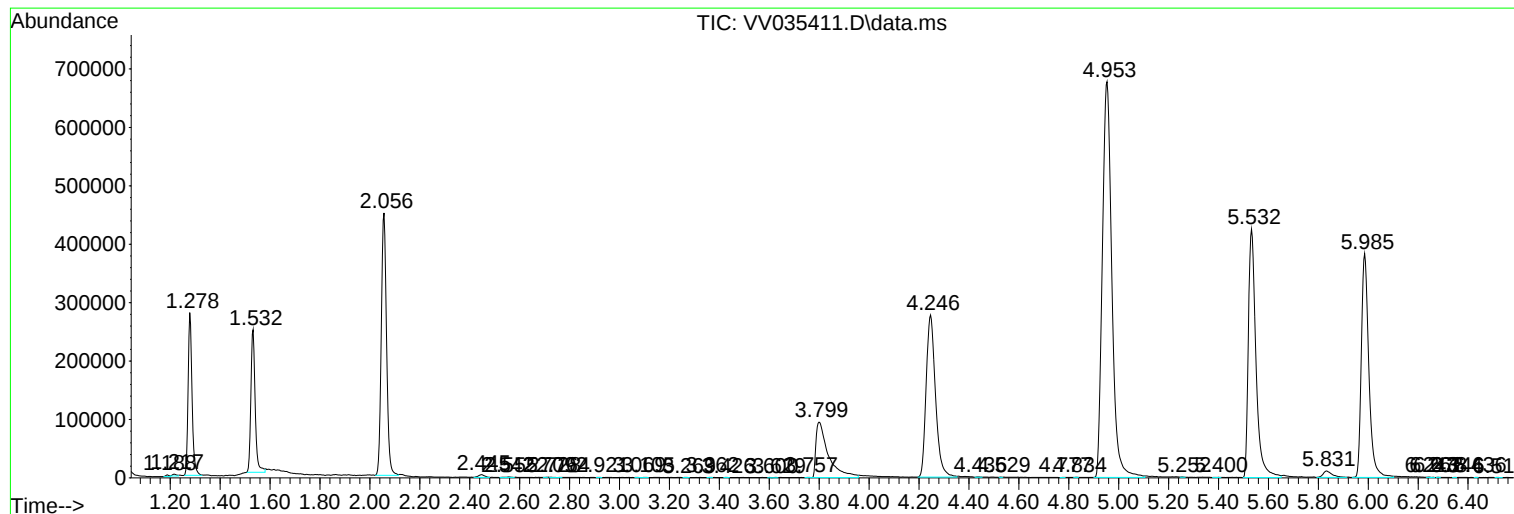

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042524\
Data File : VV035411.D
Acq On : 25 Apr 2024 18:05
Operator : SY/MD
Sample : P2182-13
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 12 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM032624WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042524\
Data File : VV035411.D
Acq On : 25 Apr 2024 18:05
Operator : SY/MD
Sample : P2182-13
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 12 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM032624WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------