

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042524\
 Data File : VV035412.D
 Acq On : 25 Apr 2024 18:29
 Operator : SY/MD
 Sample : P2158-14
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VHBLK001

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM032624WMA.M
 Title : VOC Analysis

Signal : TIC: VV035412.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.278	67	74	90	rVB	267931	291646	16.73%	2.398%
2	1.529	146	152	165	rVB	229757	254252	14.58%	2.091%
3	2.056	306	316	336	rVB	433478	633783	36.36%	5.212%
4	2.445	429	437	446	rBV2	4263	6746	0.39%	0.055%
5	2.828	554	556	557	rBV	138	63	0.00%	0.001%
6	2.879	567	572	574	rBV2	299	258	0.01%	0.002%
7	2.963	596	598	601	rBV2	285	154	0.01%	0.001%
8	2.995	603	608	612	rBV3	399	477	0.03%	0.004%
9	3.114	642	645	649	rVB2	230	163	0.01%	0.001%
10	3.175	658	664	668	rBV3	317	321	0.02%	0.003%
11	3.195	668	670	673	rVV	302	153	0.01%	0.001%
12	3.211	673	675	678	rVB2	235	96	0.01%	0.001%
13	3.246	684	686	689	rVB	219	97	0.01%	0.001%
14	3.291	696	700	703	rBV2	221	157	0.01%	0.001%
15	3.323	708	710	713	rBV	292	244	0.01%	0.002%
16	3.407	731	736	739	rBV2	252	224	0.01%	0.002%
17	3.494	759	763	769	rVB2	391	339	0.02%	0.003%
18	3.564	784	785	789	rVB	244	91	0.01%	0.001%
19	3.587	789	792	795	rVB	160	111	0.01%	0.001%
20	3.609	795	799	800	rBV	149	97	0.01%	0.001%
21	3.712	828	831	832	rBV	127	59	0.00%	0.000%
22	3.799	849	858	904	rBV	96725	321559	18.45%	2.644%
23	4.246	982	997	1029	rBV	266800	690266	39.60%	5.676%
24	4.722	1142	1145	1146	rBV	282	163	0.01%	0.001%
25	4.789	1163	1166	1168	rBV3	378	273	0.02%	0.002%
26	4.870	1187	1191	1192	rBV	469	277	0.02%	0.002%
27	4.953	1201	1217	1271	rBV2	659854	1743280	100.00%	14.335%
28	5.426	1362	1364	1365	rBV2	295	164	0.01%	0.001%
29	5.532	1386	1397	1435	rBV	415028	878464	50.39%	7.224%
30	5.834	1480	1491	1512	rBV4	10517	26078	1.50%	0.214%
31	5.985	1525	1538	1568	rBV	374286	780695	44.78%	6.420%
32	6.307	1635	1638	1641	rVB2	430	236	0.01%	0.002%
33	6.323	1641	1643	1644	rBV	292	153	0.01%	0.001%
34	6.358	1649	1654	1658	rVB2	580	383	0.02%	0.003%
35	6.394	1662	1665	1666	rBV2	270	117	0.01%	0.001%
36	6.490	1690	1695	1698	rVB2	333	309	0.02%	0.003%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042524\
 Data File : VV035412.D
 Acq On : 25 Apr 2024 18:29
 Operator : SY/MD
 Sample : P2158-14
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VHBLK001

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM032624WMA.M
 Title : VOC Analysis

37	6.510	1698	1701	1703	rBV2	238	142	0.01%	0.001%
38	6.561	1715	1717	1719	rBV	228	113	0.01%	0.001%
39	6.654	1744	1746	1748	rBV2	94	51	0.00%	0.000%
40	6.674	1749	1752	1754	rVV2	192	114	0.01%	0.001%
41	6.690	1754	1757	1758	rBV2	186	98	0.01%	0.001%
42	6.773	1776	1783	1787	rBV2	319	326	0.02%	0.003%
43	6.809	1793	1794	1796	rBV2	126	29	0.00%	0.000%
44	6.876	1812	1815	1816	rBV	433	222	0.01%	0.002%
45	6.911	1816	1826	1855	rVV	177488	347206	19.92%	2.855%
46	7.156	1898	1902	1905	rBV4	411	324	0.02%	0.003%
47	7.239	1918	1928	1957	rBV	729709	1320245	75.73%	10.856%
48	7.551	2017	2025	2060	rBV	120354	234193	13.43%	1.926%
49	7.841	2111	2115	2118	rBV2	460	382	0.02%	0.003%
50	7.963	2151	2153	2156	rVB2	227	117	0.01%	0.001%
51	7.995	2156	2163	2165	rBV3	516	501	0.03%	0.004%
52	8.030	2165	2174	2215	rBV4	263335	688568	39.50%	5.662%
53	8.503	2318	2321	2322	rBV2	370	184	0.01%	0.002%
54	8.645	2362	2365	2366	rBV	403	235	0.01%	0.002%
55	8.706	2380	2384	2386	rBV2	286	213	0.01%	0.002%
56	8.783	2397	2408	2438	rBV	649807	1080887	62.00%	8.888%
57	9.185	2532	2533	2534	rBV	224	68	0.00%	0.001%
58	9.239	2548	2550	2553	rBV	274	116	0.01%	0.001%
59	9.265	2557	2558	2560	rVB	195	52	0.00%	0.000%
60	9.407	2598	2602	2609	rBV2	303	439	0.03%	0.004%
61	9.458	2616	2618	2620	rVB2	175	50	0.00%	0.000%
62	9.480	2620	2625	2628	rBV2	213	227	0.01%	0.002%
63	9.628	2668	2671	2675	rBV2	341	256	0.01%	0.002%
64	9.693	2689	2691	2694	rVB	161	79	0.00%	0.001%
65	9.725	2699	2701	2703	rBV	118	57	0.00%	0.000%
66	9.741	2703	2706	2709	rVB2	252	159	0.01%	0.001%
67	9.841	2731	2737	2738	rBV	274	228	0.01%	0.002%
68	9.931	2761	2765	2767	rBV	298	210	0.01%	0.002%
69	10.005	2786	2788	2790	rVB	162	47	0.00%	0.000%
70	10.024	2791	2794	2796	rBV	283	148	0.01%	0.001%
71	10.091	2812	2815	2821	rBV	248	224	0.01%	0.002%
72	10.149	2821	2833	2859	rBV	534533	838379	48.09%	6.894%
73	10.413	2913	2915	2919	rBV	299	258	0.01%	0.002%
74	10.452	2925	2927	2930	rBV	209	115	0.01%	0.001%
75	10.567	2956	2963	2967	rBV2	549	693	0.04%	0.006%
76	10.632	2982	2983	2988	rVB2	297	185	0.01%	0.002%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042524\
Data File : VV035412.D
Acq On : 25 Apr 2024 18:29
Operator : SY/MD
Sample : P2158-14
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 13 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VHBLK001

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM032624WMA.M

Title : VOC Analysis

77	10.712	3005	3008	3012	rVB4	456	367	0.02%	0.003%
78	10.763	3021	3024	3026	rBV2	431	246	0.01%	0.002%
79	10.850	3048	3051	3053	rBV2	220	146	0.01%	0.001%
80	11.107	3126	3131	3135	rBV2	331	392	0.02%	0.003%
81	11.185	3143	3155	3180	rBV	572131	915499	52.52%	7.528%
82	11.558	3260	3271	3296	rBV	684762	1095240	62.83%	9.006%
83	11.931	3384	3387	3390	rBV3	471	400	0.02%	0.003%
84	11.985	3402	3404	3405	rBV3	298	108	0.01%	0.001%
85	12.040	3418	3421	3427	rBV	394	358	0.02%	0.003%
86	12.098	3436	3439	3442	rBV3	284	246	0.01%	0.002%




Sum of corrected areas: 12161090

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042524\
Data File : VV035412.D
Acq On : 25 Apr 2024 18:29
Operator : SY/MD
Sample : P2158-14
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 13 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM032624WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

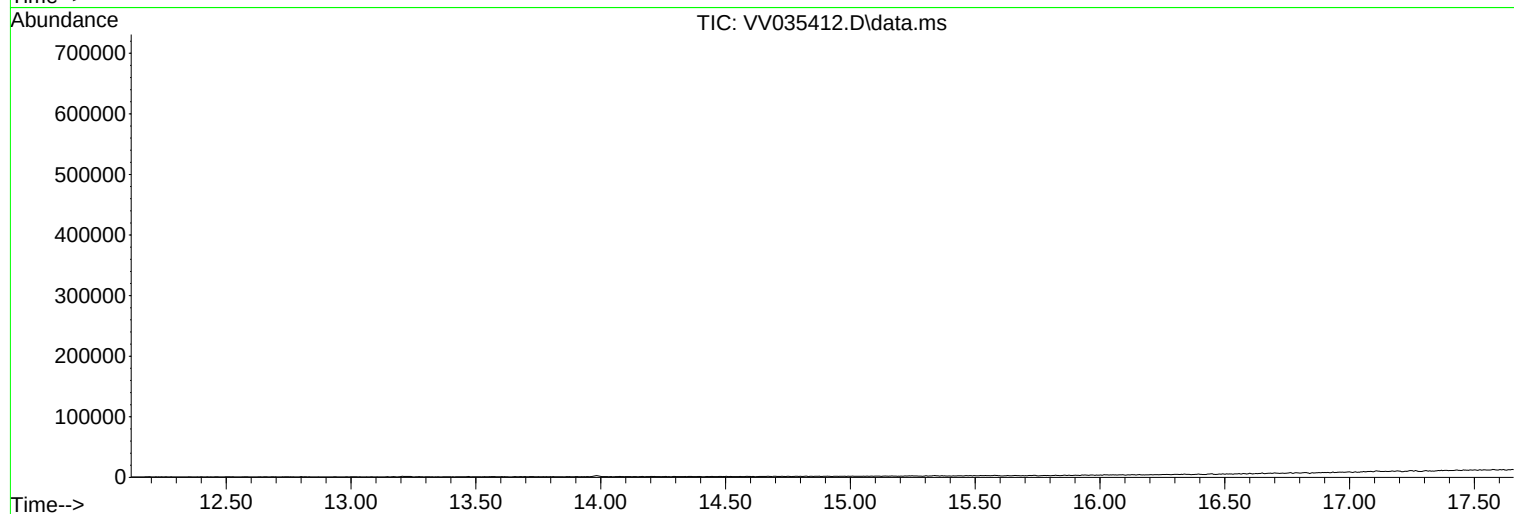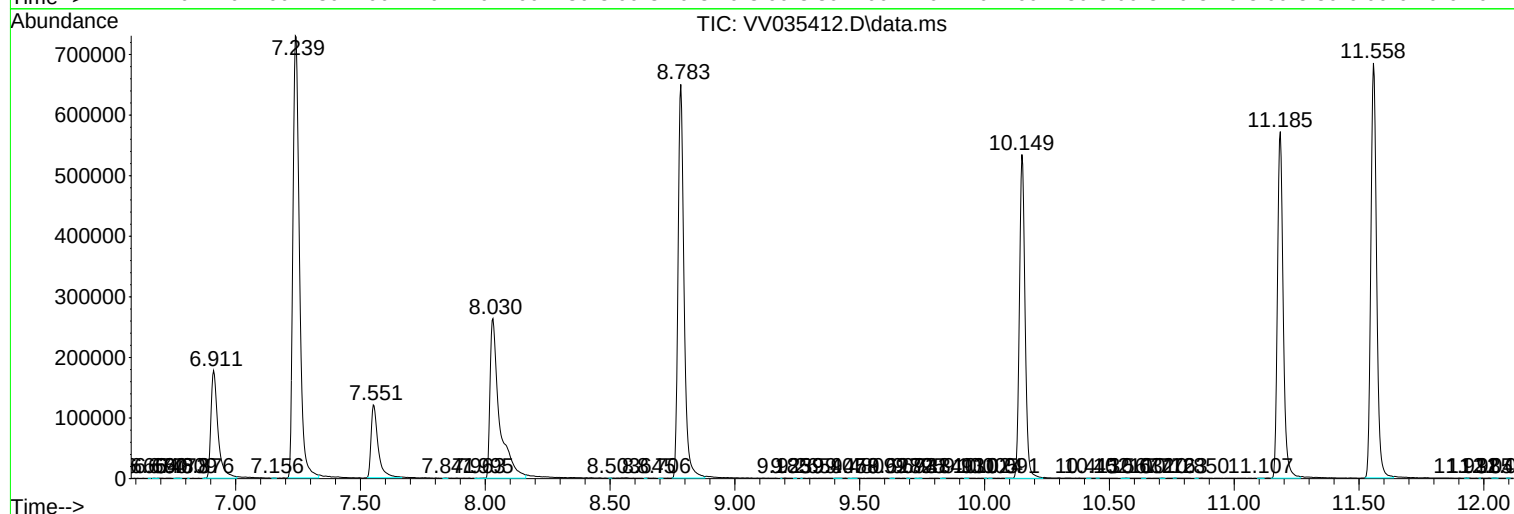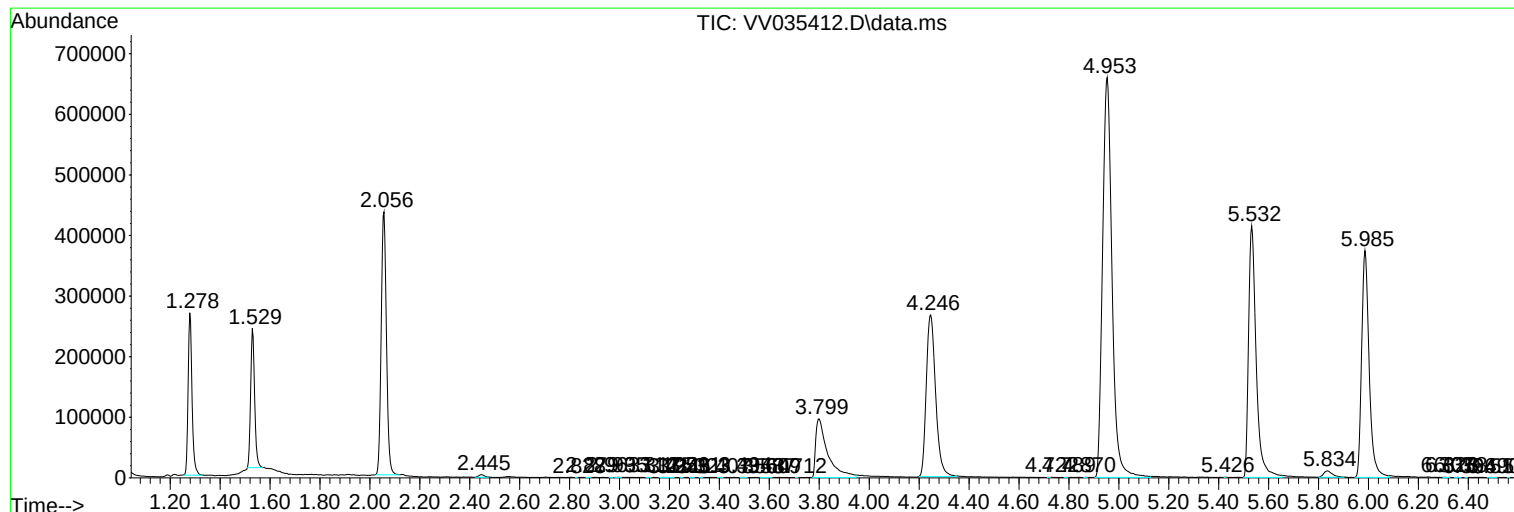

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042524\
Data File : VV035412.D
Acq On : 25 Apr 2024 18:29
Operator : SY/MD
Sample : P2158-14
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 13 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM032624WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042524\
Data File : VV035412.D
Acq On : 25 Apr 2024 18:29
Operator : SY/MD
Sample : P2158-14
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 13 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM032624WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------