


Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042524\
Data File : VV035400.D
Acq On : 25 Apr 2024 08:55
Operator : SY/MD
Sample : BFB291
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BFB291

Integration File: LSCINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM032624WMA.M
Title : VOC Analysis
Last Update : Fri Apr 26 01:37:05 2024

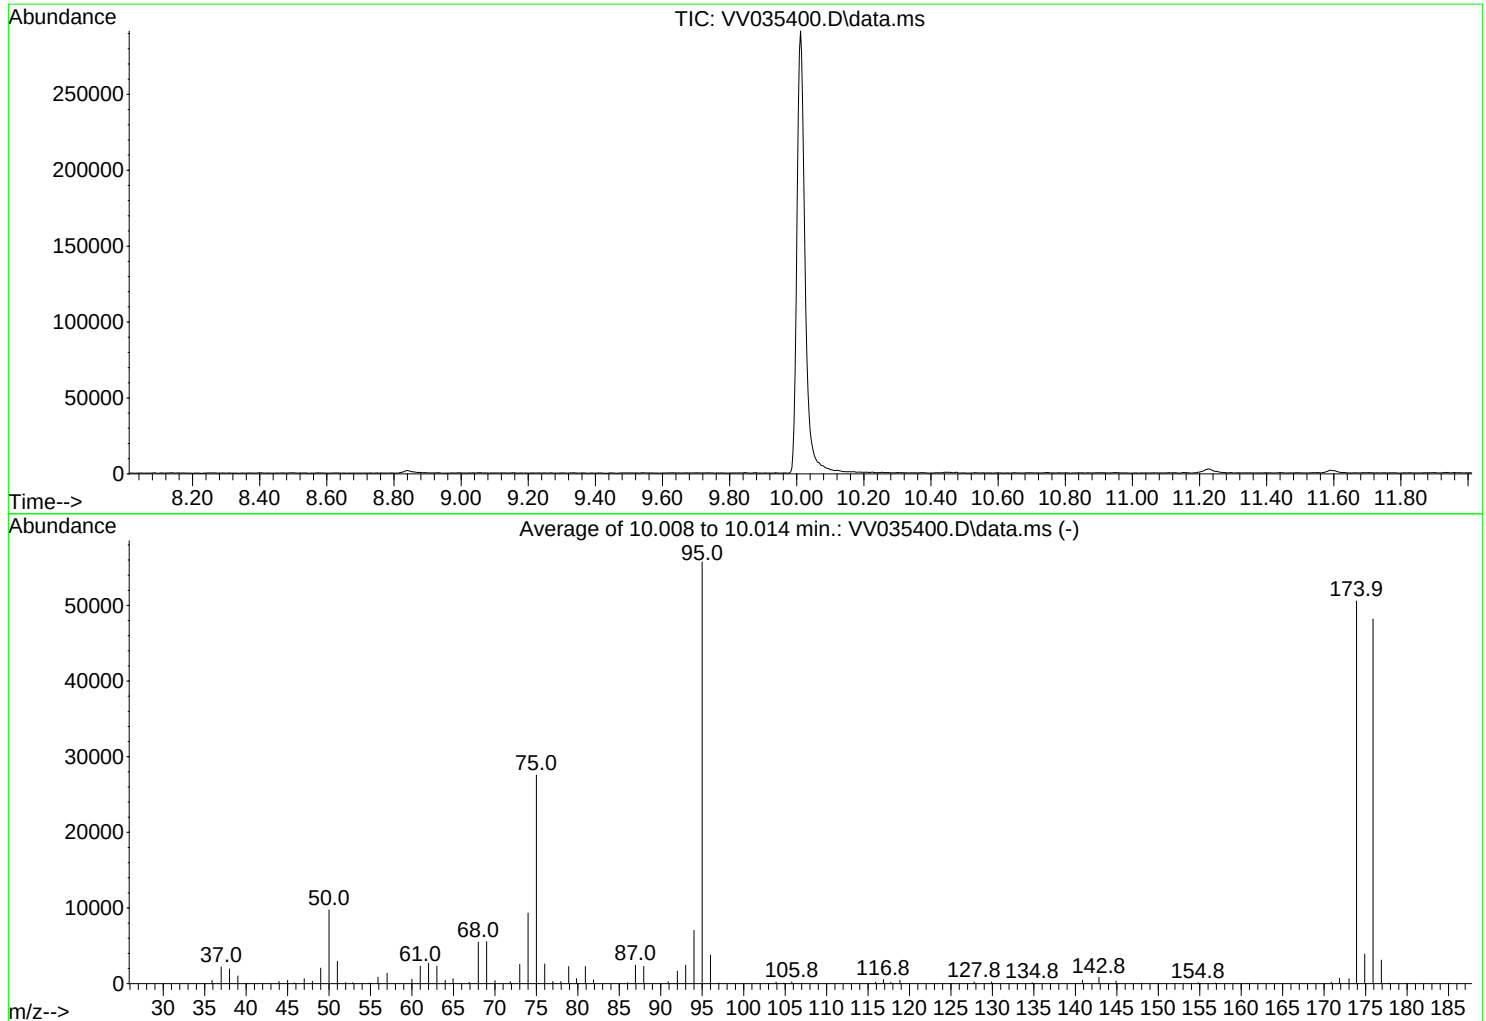

AutoFind: Scans 2789, 2790, 2791; Background Corrected with Scan 2779

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
50	95	15	40	17.5	9761	PASS
75	95	30	80	49.5	27584	PASS
95	95	100	100	100.0	55760	PASS
96	95	5	9	6.8	3775	PASS
173	174	0.00	2	1.3	654	PASS
174	95	50	120	90.7	50584	PASS
175	174	5	9	7.7	3909	PASS
176	174	95	105	95.3	48197	PASS
177	176	5	10	6.4	3104	PASS

m/z	Abundance
40.00	219.0
43.90	350.0

Instrument :
MSVOA_V
ClientSampleId :
BFB291

m/z	Abundance
35.90	452.0
37.00	2286.0
38.00	1968.0
39.00	1045.0
40.00	221.0
44.00	578.0
45.00	492.0
45.80	118.0
47.00	690.0
48.00	295.0
49.00	2113.0
50.00	9660.0
51.00	2983.0
52.00	128.0
52.80	108.0
55.10	109.0
55.90	790.0
57.00	1354.0
60.00	543.0
61.00	2231.0
62.00	2702.0
63.00	2417.0
64.00	470.0
64.90	607.0
66.90	145.0
68.00	5371.0
69.00	5329.0
70.00	491.0
71.80	273.0
73.00	2491.0
74.00	9154.0
75.00	27296.0
76.00	2596.0
77.00	273.0
77.90	253.0
78.90	2334.0
79.80	680.0
80.90	2216.0
81.90	432.0
86.00	132.0
87.00	2410.0
88.00	2255.0
90.90	252.0
92.00	1708.0
93.00	2498.0
94.00	7142.0
95.00	55880.0
96.00	3805.0
97.00	125.0
104.00	205.0
104.80	101.0
105.80	217.0
115.90	194.0
116.80	521.0
117.70	175.0
118.80	413.0
127.80	231.0
129.90	221.0
134.90	113.0
140.80	503.0
142.80	813.0
144.90	409.0
154.70	127.0
156.90	124.0
170.80	186.0
171.90	640.0
173.00	634.0
173.90	48944.0
174.90	3906.0
175.90	46592.0
176.90	3101.0
177.80	117.0

Instrument :
MSVOA_V
ClientSampleId :
BFB291

m/z	Abundance
35.90	481.0
37.00	2307.0
38.00	1979.0
39.00	1043.0
40.00	232.0
44.00	683.0
45.00	443.0
45.80	108.0
47.00	696.0
48.00	331.0
49.00	2111.0
50.00	10154.0
51.00	3046.0
52.00	166.0
52.90	124.0
54.80	112.0
55.00	110.0
55.90	908.0
57.00	1411.0
60.00	614.0
61.00	2353.0
62.00	2804.0
63.00	2389.0
64.00	453.0
65.00	673.0
66.90	180.0
68.00	5682.0
69.00	5721.0
70.00	412.0
71.80	251.0
73.00	2624.0
74.00	9688.0
75.00	28432.0
76.00	2678.0
77.00	311.0
78.00	291.0
78.90	2313.0
79.90	688.0
80.90	2343.0
81.90	493.0
86.00	137.0
86.90	2507.0
88.00	2348.0
90.90	273.0
92.00	1738.0
93.00	2486.0
94.00	7306.0
95.00	57576.0
96.00	3900.0
97.00	106.0
103.90	203.0
104.90	101.0
105.80	237.0
115.90	193.0
116.90	532.0
117.80	193.0
118.80	488.0
127.80	257.0
129.90	250.0
134.80	128.0
140.80	460.0
142.80	875.0
144.90	361.0
147.90	102.0
154.80	138.0
156.90	118.0
160.70	103.0
170.80	187.0
171.80	726.0
173.00	681.0
173.90	52104.0
174.90	4024.0
175.90	49768.0
176.90	3163.0
177.80	113.0

Instrument :
MSVOA_V
ClientSampleId :
BFB291

m/z	Abundance
35.90	419.0
37.00	2107.0
38.00	1923.0
39.00	932.0
40.00	252.0
44.00	711.0
45.00	419.0
45.80	115.0
47.00	605.0
48.00	323.0
49.00	1934.0
50.00	9470.0
51.00	2846.0
52.00	180.0
52.90	132.0
54.00	102.0
54.90	158.0
55.90	845.0
57.00	1405.0
60.00	603.0
61.00	2330.0
62.00	2649.0
63.00	2203.0
64.00	428.0
65.00	690.0
65.90	107.0
66.90	191.0
68.00	5383.0
69.00	5546.0
70.00	321.0
71.90	207.0
73.00	2524.0
74.00	9158.0
75.00	27024.0
76.00	2517.0
77.00	319.0
77.90	309.0
78.90	2150.0
79.90	683.0
80.90	2225.0
81.90	536.0
86.00	109.0
86.90	2381.0
87.90	2225.0
90.90	264.0
92.00	1535.0
93.00	2287.0
94.00	6717.0
95.00	53824.0
96.00	3621.0
103.80	208.0
105.80	263.0
115.90	198.0
116.80	541.0
117.80	212.0
118.90	484.0
127.80	239.0
129.90	221.0
134.70	112.0
140.90	439.0
142.90	771.0
144.90	329.0
148.00	103.0
154.90	143.0
170.90	189.0
171.90	765.0
173.00	646.0
173.90	50704.0
174.90	3798.0
175.90	48232.0
176.90	3048.0

Instrument :
MSVOA_V
ClientSampleId :
BFB291