

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV042619\
 Data File : VV010508.D
 Acq On : 26 Apr 2019 14:03
 Operator : SY/MD
 Sample : MDL02
 Misc : 25mL/MSVOA V/WATER
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 MDL02

Manual Integrations
 APPROVED

MMDadoda
 5/28/2019 3:13:30 PM

Quant Time: Apr 29 11:41:29 2019
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR042619SIM.M
 Quant Title : TRACE VOA SOM01.0
 QLast Update : Sat Apr 27 04:44:38 2019
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	5.67	114	6139	0.50	ug/L	0.00
5) Chlorobenzene-d5	8.89	117	5732	0.50	ug/L	0.00
10) 1,4-Dichlorobenzene-d4	11.29	152	2716	0.50	ug/L	0.00

System Monitoring Compounds

2) Vinyl Chloride-d3	1.32	65	2430	0.53	ug/L	0.00
Spiked Amount	0.500	Range	40 - 130	Recovery	=	106.00%
4) 1,2-Dichloroethane-d4	5.07	65	2427	0.59	ug/L	0.00
Spiked Amount	0.500	Range	70 - 130	Recovery	=	118.00%
7) Toluene-d8	7.35	98	6870	0.57	ug/L	0.00
Spiked Amount	0.500	Range	70 - 130	Recovery	=	114.00%
9) 1,1,2,2-Tetrachloroethane-	10.25	84	1989	0.60	ug/L	0.00
Spiked Amount	0.500	Range	65 - 120	Recovery	=	120.00%
11) 1-2-dichlorobenzene-d4	11.67	152	2978	0.55	ug/L	0.00
Spiked Amount	0.500	Range	80 - 120	Recovery	=	110.00%

Target Compounds

					Qvalue
3) Vinyl chloride	1.32	62	152	0.033 ug/L #	1
6) Trichloroethene	5.96	95	137	0.028 ug/L	89
8) 1,2-Dibromoethane	8.40	107	79	0.028 ug/L #	81
12) 1,2,3-Trichloropropane	10.32	75	72	0.031 ug/L #	87
13) 1,2-Dibromo-3-chloropropan	12.48	75	24m	0.038 ug/L	

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\V0ASRV\HPCHEM1\MSVOA V\DATA\VV042619\
Data File : VV010508.D
Acq On : 26 Apr 2019 14:03
Operator : SY/MD
Sample : MDL02
Misc : 25mL/MSVOA V/WATER
ALS Vial : 14 Sample Multiplier: 1


Instrument :
MSVOA_V
ClientSampleId :
MDL02

Manual Integrations
APPROVED

MMDadoda
5/28/2019 3:13:30 PM

Quant Time: Apr 29 11:41:29 2019
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR042619SIM.M
Quant Title : TRACE VOA SOM01.0
QLast Update : Sat Apr 27 04:44:38 2019
Response via : Initial Calibration

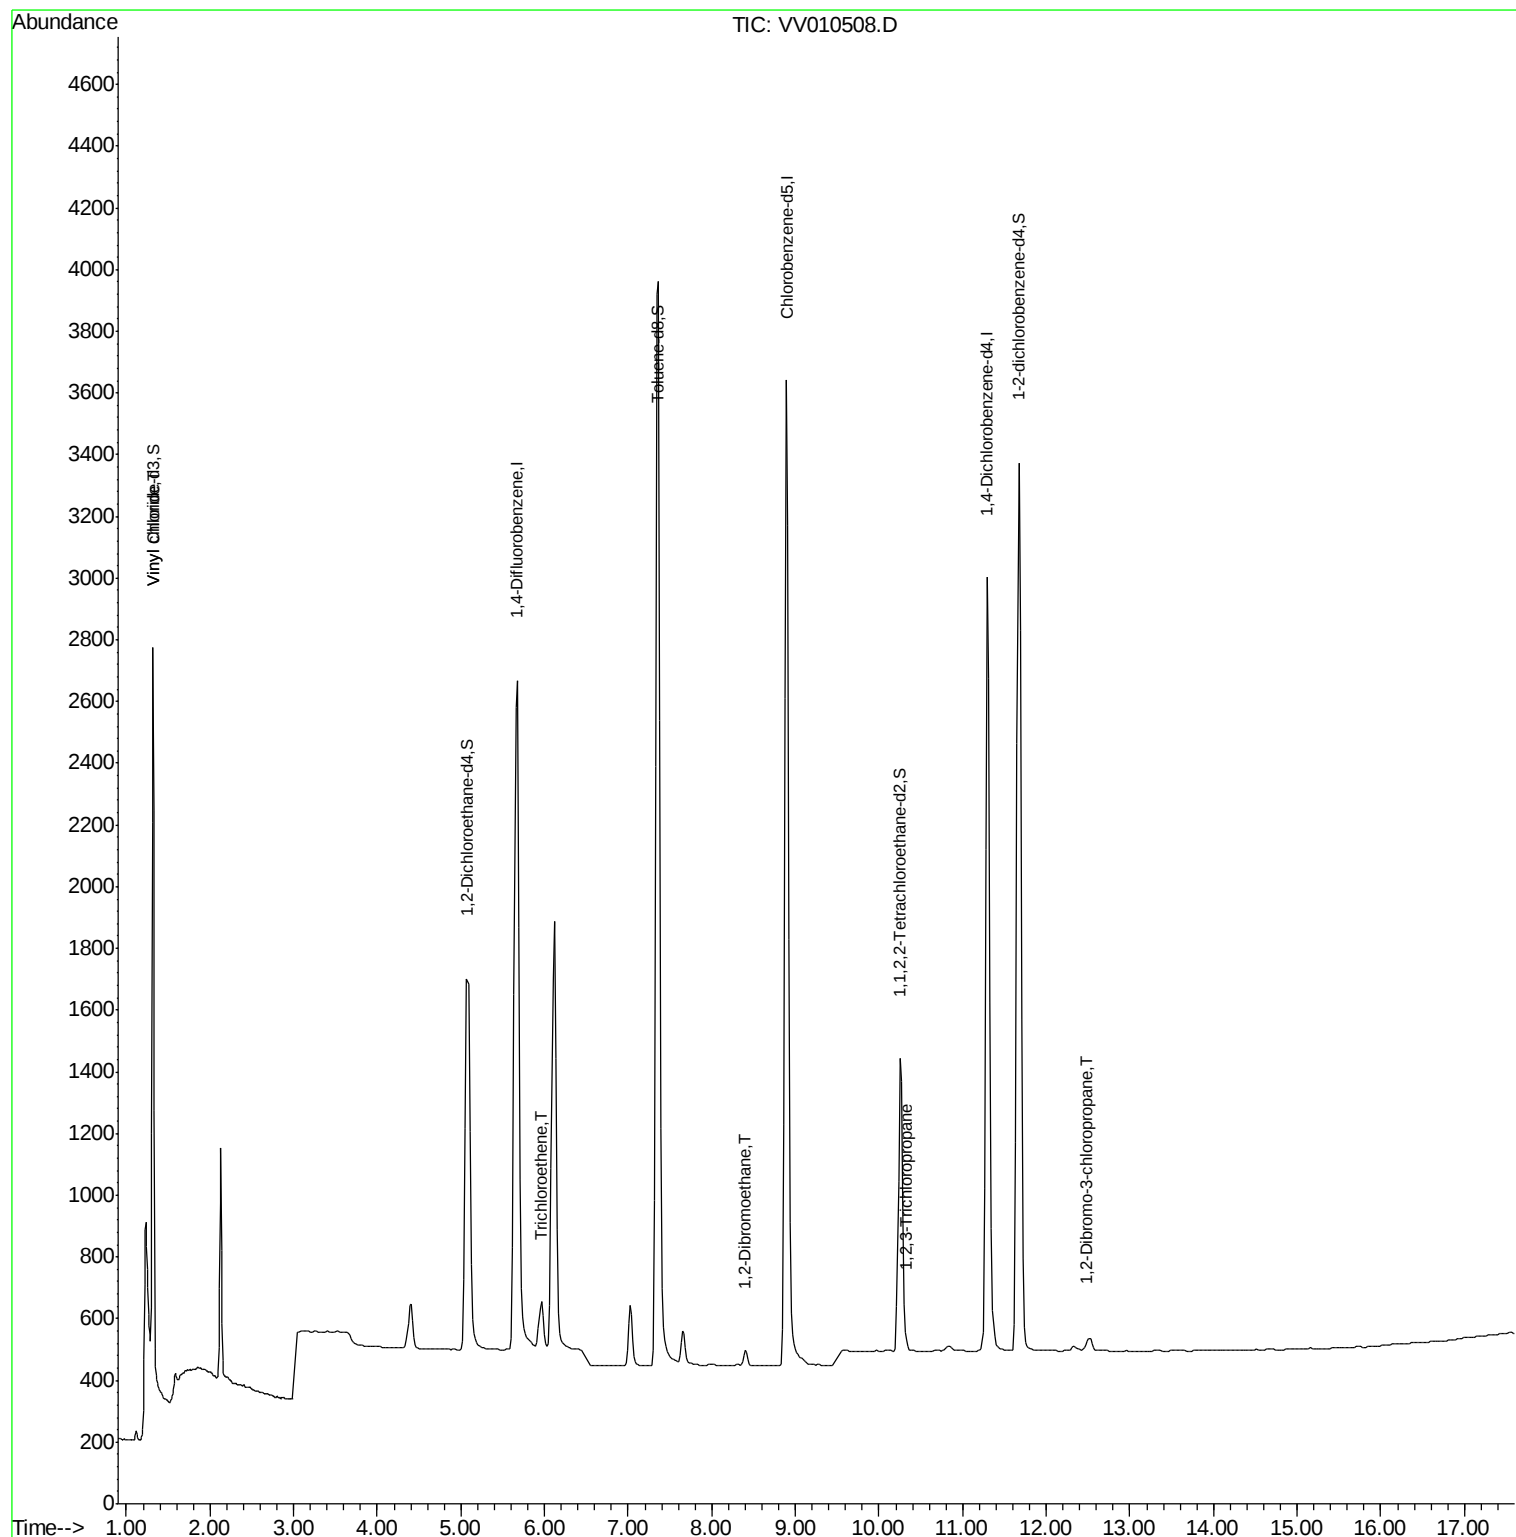

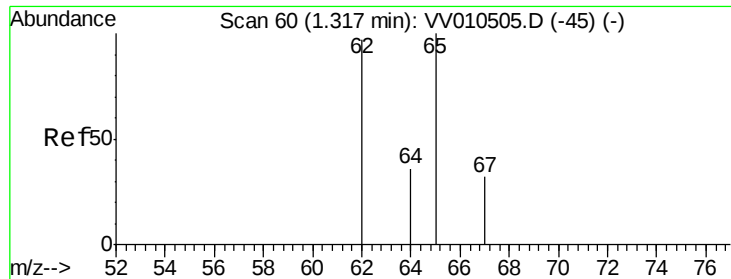

#3

Vinyl chloride

Concen: 0.033 ug/L

RT: 1.32 min Scan# 60

Delta R.T. 0.00 min

Lab File: VV010508.D

Acq: 26 Apr 2019 14:03

Instrument :

MSVOA_V

ClientSampled :

MDL02

Tot Ion: 62 Resp: 152

Ion Ratio Lower Upper





62 100

64 241.4 28.9 53.7#

Manual Integrations
APPROVED

MMDadoda

5/28/2019 3:13:30 PM

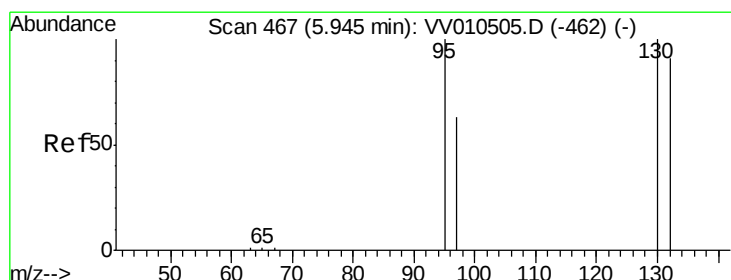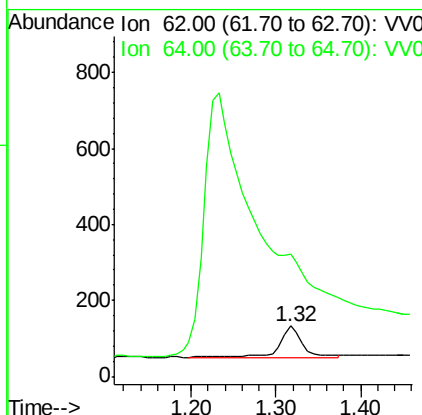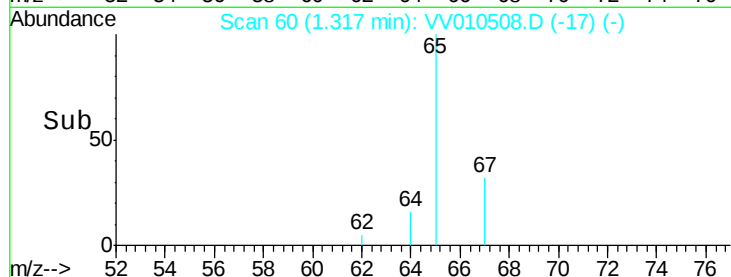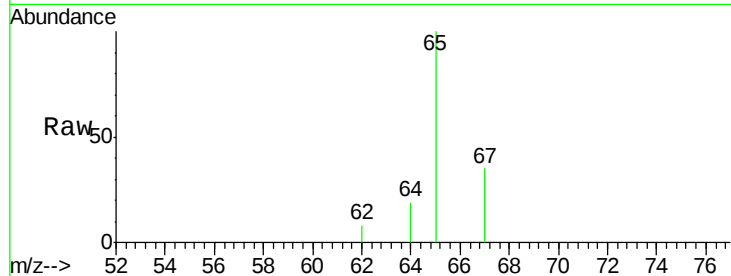

#6

Trichloroethene

Concen: 0.028 ug/L

RT: 5.96 min Scan# 468

Delta R.T. 0.02 min

Lab File: VV010508.D

Acq: 26 Apr 2019 14:03

Tgt Ion: 95 Resp: 137




Ion Ratio Lower Upper


95 100

97 84.1 48.0 89.2

132 103.4 78.1 145.1

130 104.5 80.5 149.5

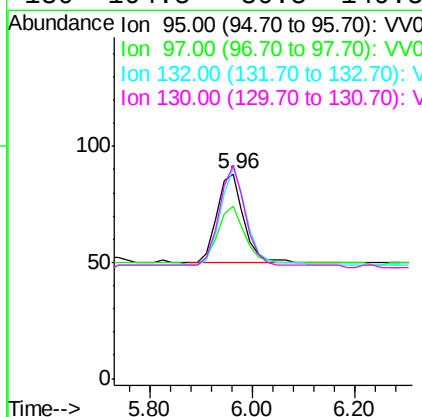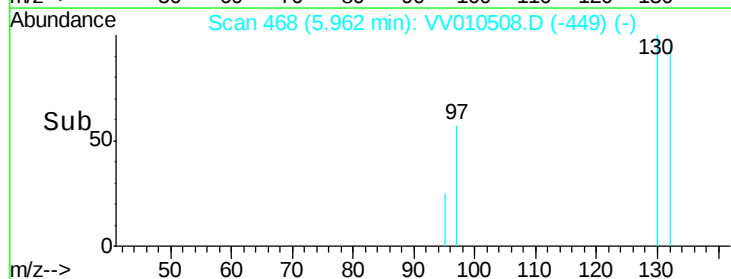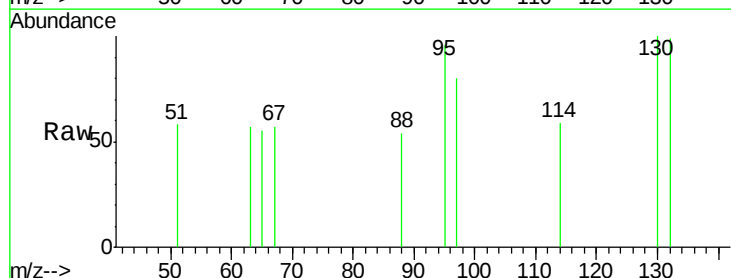

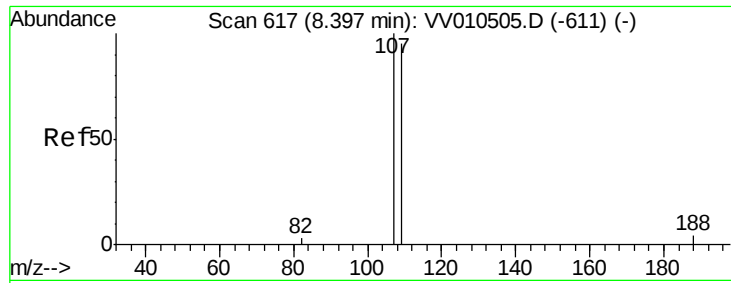

#8

1,2-Dibromoethane

Concen: 0.028 ug/L

RT: 8.40 min Scan# 617

Delta R.T. 0.00 min

Lab File: VV010508.D

Acq: 26 Apr 2019 14:03

Instrument :

MSVOA_V





ClientSampled :

MDL02

Tot Ion:	107	Resp:	79
Ion Ratio	Lower	Upper	
107	100		
109	98.6	67.2	124.8
188	67.1	10.6	16.0#

Manual Integrations
APPROVED

MMDadoda
5/28/2019 3:13:30 PM

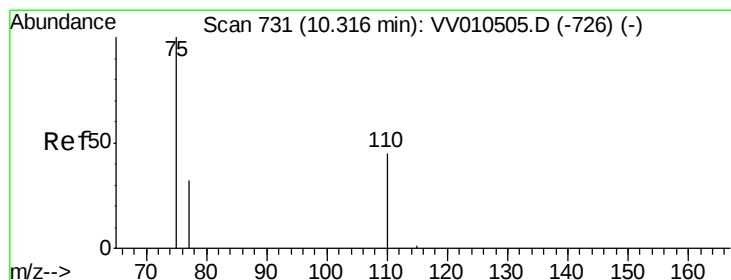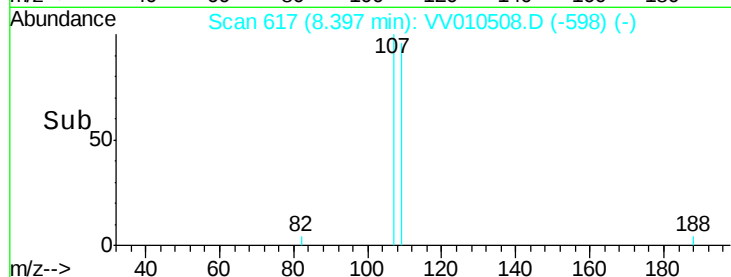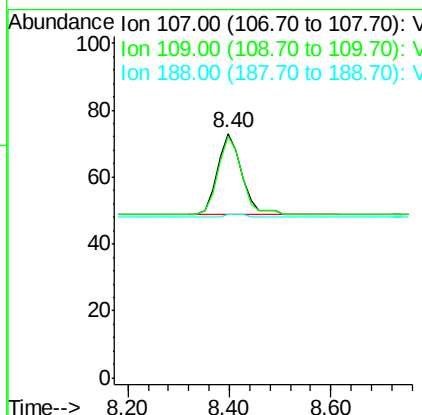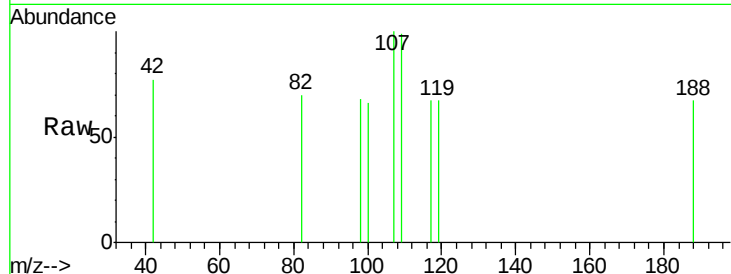

#12

1,2,3-Trichloropropane

Concen: 0.031 ug/L




RT: 10.32 min Scan# 731


Delta R.T. 0.00 min

Lab File: VV010508.D

Acq: 26 Apr 2019 14:03

Tgt Ion:	75	Resp:	72
Ion Ratio	Lower	Upper	
75	100		
110	51.4	33.9	50.9#
77	26.4	26.0	39.0

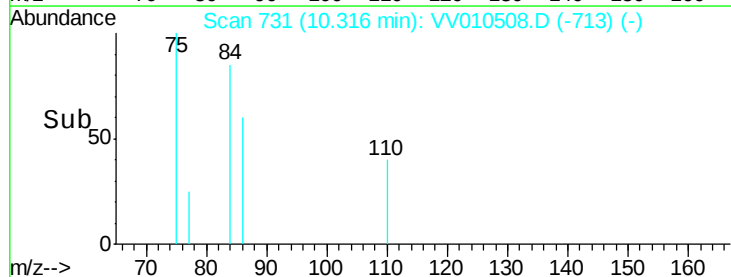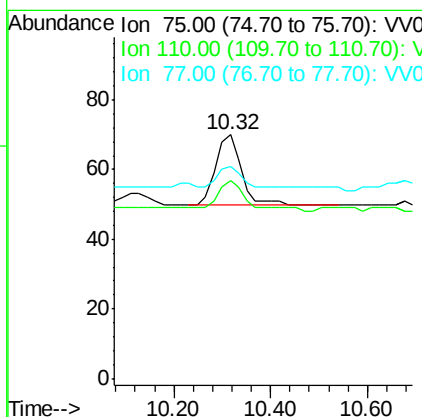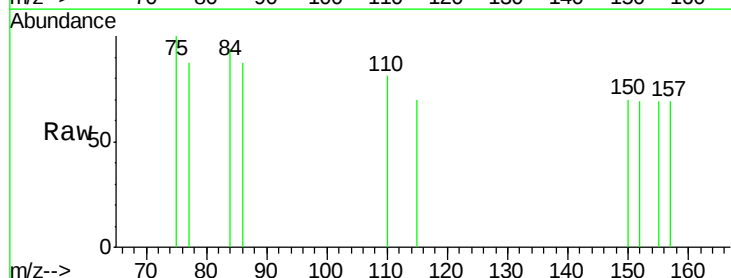

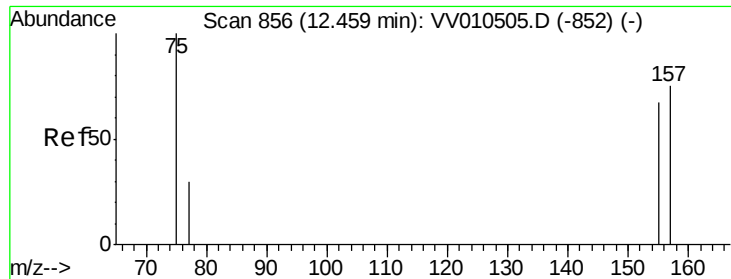

#13

1,2-Dibromo-3-chloropropane

Concen: 0.038 ug/L m

RT: 12.48 min Scan# 857

Delta R.T. 0.02 min

Lab File: VV010508.D

Acq: 26 Apr 2019 14:03

Instrument :

MSVOA_V

ClientSampleId :

MDL02

Tot Ion	Ratio	Lower	Upper
75	100		
157	94.6	67.2	100.8
155	92.9	61.4	92.2

Manual Integrations
APPROVED

MMDadoda
5/28/2019 3:13:30 PM

