


Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042619\
Data File : VV010497.D
Acq On : 25 Apr 2019 16:24
Operator : SY/MD
Sample : BFB02
Misc : 25mL/MSVOA_V/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BFB02

Integration File: rteint.p

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR042619SIM.M
Title : TRACE VOA SOM01.0
Last Update : Tue Apr 30 01:23:26 2019

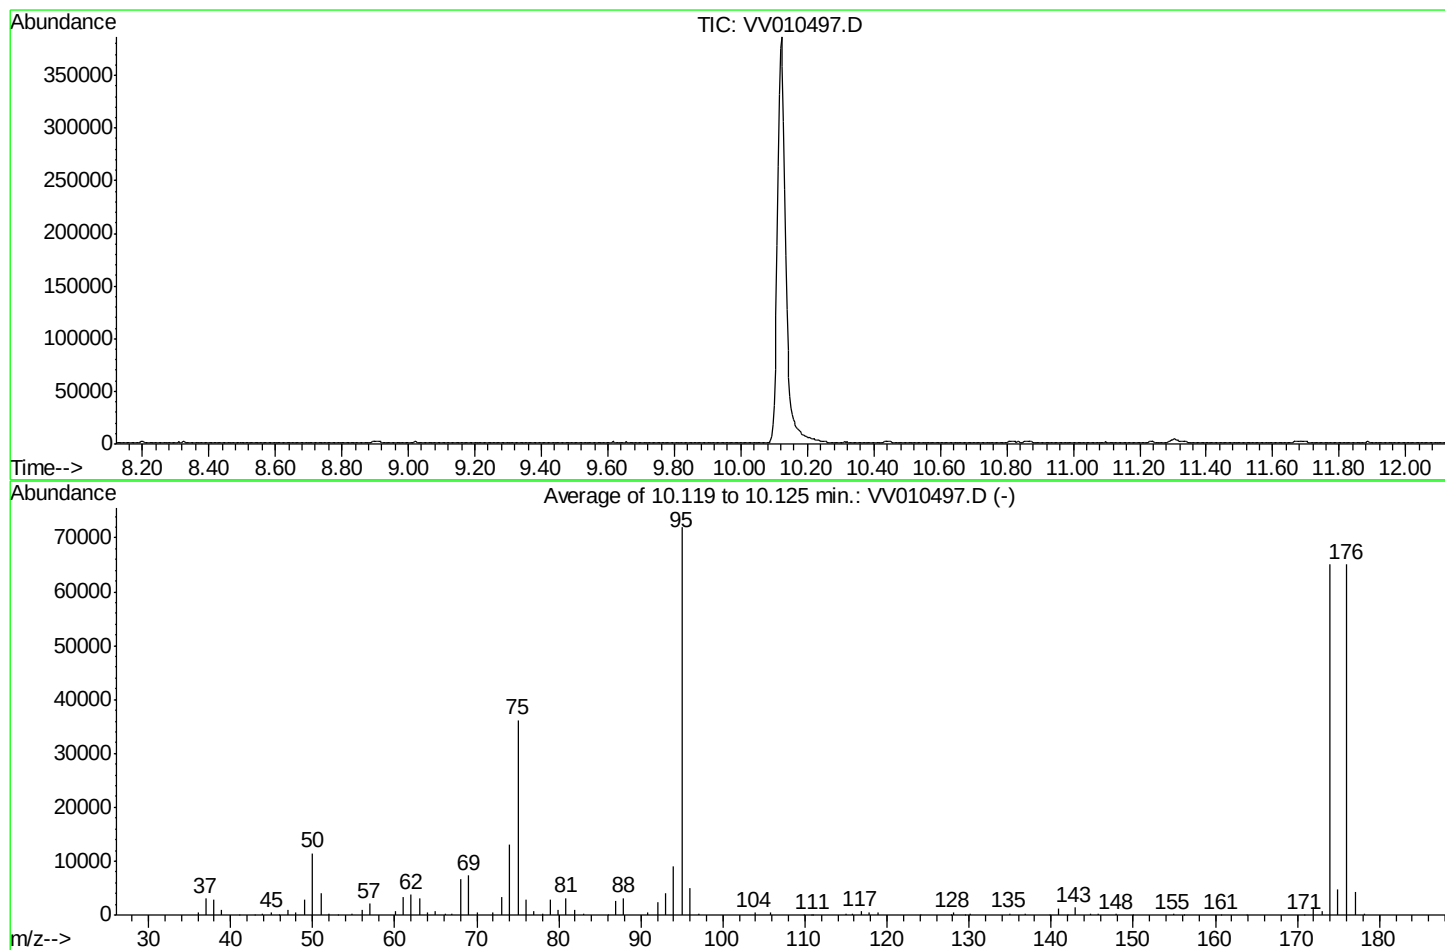

AutoFind: Scans 2808, 2809, 2810; Background Corrected with Scan 2795

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	15.9	11464	PASS
75	95	30	80	50.2	36157	PASS
95	95	100	100	100.0	71965	PASS
96	95	5	9	7.0	5046	PASS
173	174	0.00	2	1.0	681	PASS
174	95	50	120	90.4	65064	PASS
175	174	5	9	7.5	4851	PASS
176	174	95	101	100.0	65085	PASS
177	176	5	9	6.5	4260	PASS

m/z	Abundance
36.10	549.0
37.00	3100.0
38.00	3205.0
39.00	1130.0
39.90	847.0
44.00	746.0
45.00	529.0
45.80	124.0
46.90	721.0
48.00	397.0
49.00	2899.0
50.00	12283.0
51.00	4041.0
51.90	182.0
54.80	259.0
56.00	1070.0
57.00	2198.0
60.10	867.0
61.00	3618.0
62.00	3888.0
63.00	3187.0
64.00	416.0
65.00	869.0
66.20	131.0
66.90	225.0
68.00	6949.0
69.00	7578.0
70.10	521.0
71.90	474.0
73.00	3184.0
74.00	12855.0
75.00	36048.0
76.00	3150.0
77.00	543.0
78.90	3024.0
80.00	886.0
80.90	3295.0
82.00	883.0
83.10	162.0
86.90	2868.0
87.90	3153.0
90.90	342.0
92.00	2460.0
93.00	4211.0
94.00	8905.0
95.00	73304.0
96.00	5048.0
97.10	196.0
103.90	468.0
105.90	336.0
110.80	127.0
115.00	182.0
115.80	317.0
116.90	623.0
117.80	402.0
118.90	470.0
128.10	462.0
130.10	311.0
134.80	207.0
136.80	221.0
139.80	137.0
140.80	1266.0
142.00	217.0
142.90	1462.0
144.80	428.0
145.70	245.0
148.00	300.0
154.90	205.0
172.00	1324.0
173.00	1041.0
174.00	64120.0
175.00	5126.0
176.00	64056.0
177.00	4413.0
178.10	125.0

Instrument :
MSVOA_V
ClientSampleId :
BFB02

m/z	Abundance
36.10	538.0
37.00	3138.0
38.00	2965.0
38.90	1032.0
39.90	860.0
41.10	127.0
42.90	108.0
44.00	819.0
45.00	457.0
45.90	103.0
47.00	878.0
48.00	574.0
49.00	2868.0
50.00	11707.0
51.00	4236.0
51.90	243.0
53.10	162.0
54.80	180.0
56.00	979.0
56.90	2230.0
60.10	780.0
61.00	3565.0
62.00	3937.0
63.00	3215.0
64.00	502.0
65.00	806.0
66.20	193.0
66.90	310.0
68.00	6661.0
69.00	7623.0
70.20	534.0
71.90	519.0
73.00	3330.0
74.00	13565.0
75.00	37472.0
76.00	2981.0
77.00	689.0
78.00	231.0
78.90	3021.0
80.00	904.0
80.90	3222.0
82.00	889.0
83.00	206.0
86.90	2814.0
87.90	3262.0
90.90	425.0
92.00	2498.0
93.00	4155.0
94.00	9429.0
95.00	74080.0
96.00	5269.0
97.10	175.0
103.90	401.0
105.90	382.0
109.90	130.0
111.00	174.0
114.90	201.0
115.80	339.0
116.90	679.0
117.80	422.0
118.90	634.0
128.10	465.0
130.00	275.0
134.90	258.0
136.80	180.0
140.80	1359.0
142.90	1422.0
144.80	377.0
145.70	232.0
147.90	242.0
149.90	124.0
154.80	165.0
160.70	106.0
163.80	103.0
170.90	146.0
172.00	1364.0
173.00	1002.0
174.00	66912.0
175.00	4948.0
176.00	67504.0
177.00	4431.0
178.20	168.0

Instrument :
MSVOA_V
ClientSampleId :
BFB02

m/z	Abundance
36.10	431.0
37.00	2882.0
38.00	2590.0
38.90	858.0
39.90	877.0
41.10	115.0
42.90	108.0
44.00	815.0
45.00	409.0
46.00	148.0
47.00	956.0
47.90	670.0
49.00	2545.0
50.00	10402.0
51.00	3966.0
52.00	252.0
53.10	214.0
54.90	118.0
56.00	892.0
56.90	1959.0
60.10	565.0
61.00	3099.0
62.00	3508.0
63.00	2876.0
64.10	561.0
65.00	703.0
66.10	181.0
66.90	307.0
68.00	6023.0
69.00	6870.0
70.20	519.0
71.90	542.0
73.00	3216.0
74.00	12592.0
75.00	34952.0
76.00	2541.0
77.00	636.0
78.00	311.0
78.90	2696.0
79.90	926.0
80.90	2794.0
81.90	868.0
82.90	194.0
86.00	145.0
86.90	2426.0
87.90	2977.0
90.80	419.0
92.00	2145.0
93.00	3663.0
94.00	9061.0
95.00	68512.0
96.00	4821.0
97.00	119.0
103.80	303.0
105.80	391.0
109.90	157.0
111.00	180.0
114.90	246.0
115.80	309.0
116.80	749.0
117.90	434.0
118.90	610.0
124.00	136.0
127.80	343.0
128.10	314.0
129.50	105.0
130.00	223.0
135.00	277.0
136.80	117.0
140.90	1200.0
142.90	1223.0
144.80	244.0
145.70	210.0
147.90	162.0
149.90	133.0
154.80	144.0
156.10	109.0
170.80	216.0
171.90	1364.0
174.00	64160.0
174.90	4481.0
176.00	63696.0
177.00	3937.0
178.20	130.0

Instrument :
MSVOA_V
ClientSampleId :
BFB02

Scan 2795 (10.077 min): VV010497.D
BFB02

m/z	Abundance
39.90	968.0
43.80	578.0

Instrument :
MSVOA_V
ClientSampleId :
BFB02