


Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042619\
 Data File : VV010504.D
 Acq On : 26 Apr 2019 09:55
 Operator : SY/MD
 Sample : BFB03
 Misc : 25mL/MSVOA_V/WATER
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BFB03

Integration File: rteint.p

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR042619SIM.M
 Title : TRACE VOA SOM01.0
 Last Update : Tue Apr 30 01:23:26 2019

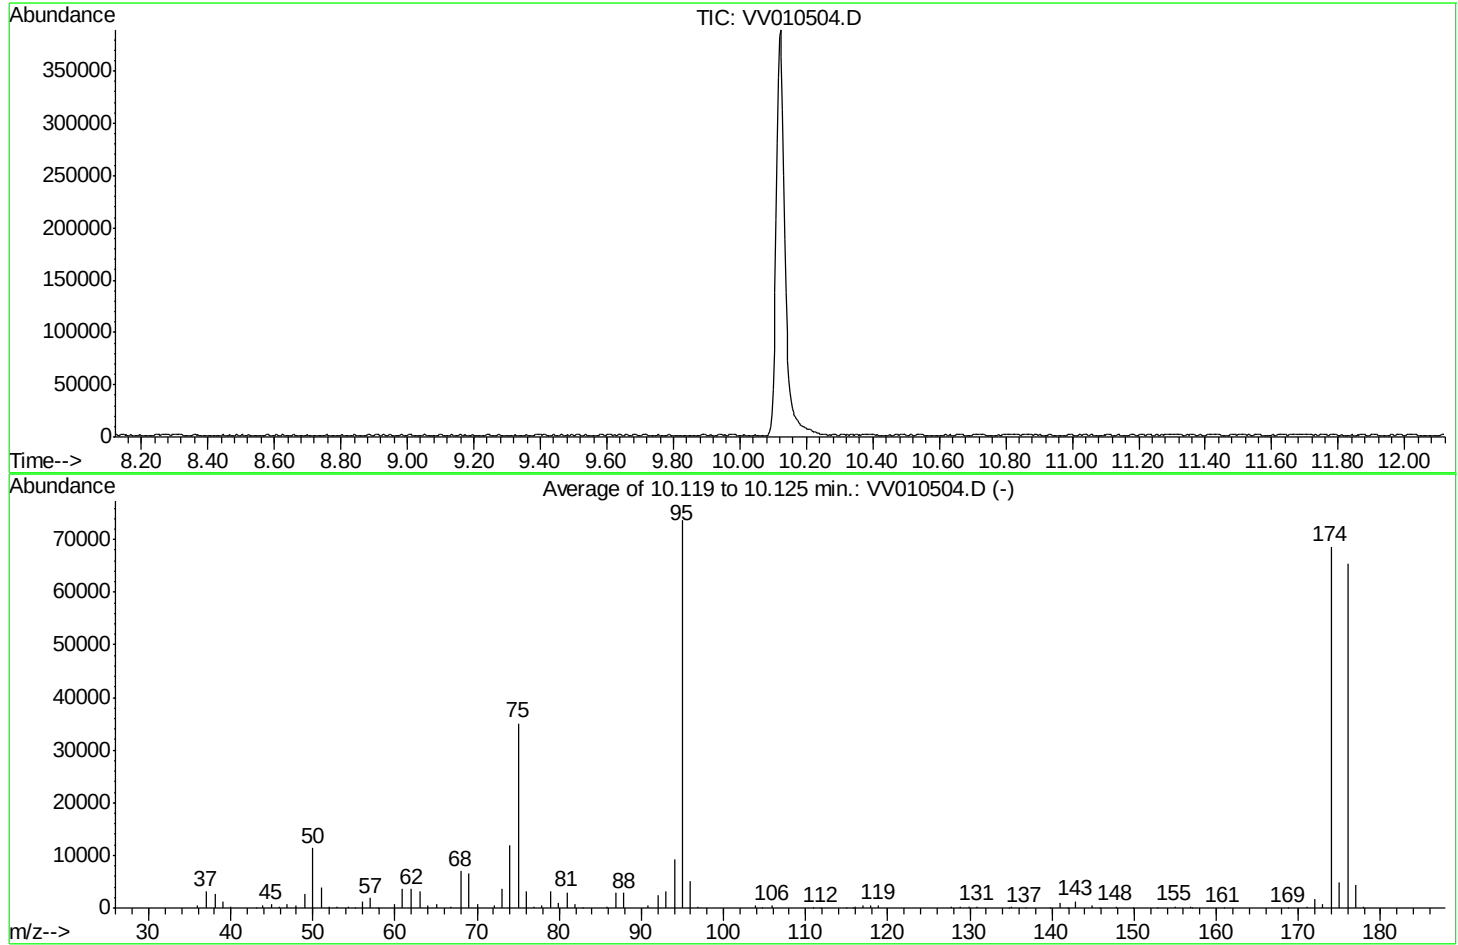

AutoFind: Scans 2808, 2809, 2810; Background Corrected with Scan 2794

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	15.5	11424	PASS
75	95	30	80	47.6	35045	PASS
95	95	100	100	100.0	73674	PASS
96	95	5	9	6.8	5005	PASS
173	174	0.00	2	1.2	850	PASS
174	95	50	120	93.2	68688	PASS
175	174	5	9	7.3	4995	PASS
176	174	95	101	95.4	65504	PASS
177	176	5	9	6.5	4268	PASS

m/z	Abundance
35.90	445.0
37.00	3119.0
38.00	2919.0
39.10	1315.0
39.90	1269.0
43.10	110.0
43.90	741.0
45.00	710.0
45.90	257.0
46.90	613.0
47.90	612.0
49.00	2960.0
50.00	11700.0
51.00	4158.0
52.00	217.0
52.90	181.0
54.30	181.0
55.10	182.0
56.00	1261.0
57.00	2046.0
57.90	103.0
59.90	830.0
60.90	3615.0
62.00	3885.0
63.00	3078.0
64.10	547.0
65.10	874.0
66.90	154.0
68.00	6828.0
69.00	6542.0
70.10	803.0
72.10	412.0
72.90	3482.0
74.00	12165.0
75.00	36392.0
76.10	3185.0
77.00	458.0
77.90	450.0
78.90	3370.0
79.90	1032.0
80.90	3166.0
81.90	787.0
85.80	269.0
87.00	2907.0
87.90	2993.0
90.90	405.0
92.00	2157.0
93.00	3149.0
94.00	9038.0
95.00	74736.0
96.00	5211.0
96.90	230.0
103.80	476.0
104.70	139.0
106.00	441.0
110.90	107.0
115.80	367.0
116.90	402.0
117.90	362.0
118.90	475.0
127.70	308.0
128.90	163.0
129.90	339.0
130.90	323.0
135.10	275.0
136.80	170.0
139.70	126.0
140.90	851.0
141.90	125.0
142.90	1306.0
144.80	435.0
145.90	170.0
147.80	376.0
149.90	136.0
155.00	354.0
156.80	248.0
160.90	168.0
168.80	109.0
171.00	261.0
171.90	1507.0
173.00	790.0
174.00	68960.0
175.00	4987.0
176.00	65352.0
177.00	4372.0
177.90	196.0

Instrument :
MSVOA_V
ClientSampleId :
BFB03

m/z	Abundance
35.90	454.0
37.00	3219.0
38.10	2791.0
39.10	1226.0
39.90	1404.0
43.00	102.0
43.90	786.0
44.90	797.0
45.90	296.0
46.90	817.0
48.00	601.0
49.00	2697.0
50.00	11696.0
51.00	3989.0
52.00	214.0
52.90	192.0
54.30	166.0
56.00	1258.0
57.00	1889.0
59.90	840.0
60.90	3689.0
62.00	3687.0
63.00	3121.0
64.00	609.0
65.10	872.0
66.80	155.0
68.00	7258.0
69.00	6821.0
70.10	652.0
72.10	404.0
73.00	3616.0
74.00	12268.0
75.00	35952.0
76.00	3233.0
77.90	425.0
78.90	3301.0
79.90	1035.0
80.90	3121.0
81.90	708.0
85.80	253.0
86.90	2801.0
87.90	3041.0
90.90	487.0
92.00	2583.0
93.00	3213.0
94.00	9439.0
95.00	75912.0
96.00	5188.0
96.90	264.0
103.80	390.0
104.70	126.0
106.00	452.0
111.80	113.0
116.00	381.0
117.00	482.0
118.00	432.0
118.80	495.0
127.70	321.0
128.80	171.0
129.90	333.0
130.90	400.0
134.70	177.0
135.00	180.0
136.70	118.0
139.70	131.0
140.90	1027.0
142.90	1352.0
144.80	409.0
145.80	155.0
147.80	372.0
149.80	111.0
155.00	353.0
156.80	226.0
160.90	122.0
168.80	124.0
171.00	300.0
172.00	1728.0
173.00	828.0
174.00	70888.0
175.00	5141.0
176.00	67288.0
177.00	4392.0
177.90	270.0

Instrument :
MSVOA_V
ClientSampleId :
BFB03

m/z	Abundance
36.00	501.0
37.00	2961.0
38.00	2312.0
39.10	1007.0
39.90	1583.0
43.80	880.0
44.90	673.0
45.90	222.0
46.90	744.0
48.00	501.0
49.00	2282.0
50.00	10876.0
51.00	3593.0
52.00	187.0
52.90	193.0
54.30	111.0
54.90	108.0
56.00	1223.0
57.00	1687.0
59.90	756.0
60.90	3403.0
62.00	3206.0
63.00	2957.0
64.00	544.0
65.00	785.0
66.90	170.0
68.00	7009.0
69.00	6366.0
70.00	512.0
71.90	418.0
73.00	3563.0
74.00	11488.0
75.00	32792.0
76.00	2967.0
76.80	399.0
77.80	318.0
78.90	2908.0
79.90	1070.0
80.90	2784.0
81.90	708.0
82.80	113.0
85.90	186.0
86.90	2870.0
87.90	2584.0
90.80	473.0
92.00	2615.0
93.00	3227.0
94.00	9091.0
95.00	70376.0
96.00	4616.0
96.90	246.0
103.90	350.0
105.90	368.0
111.00	123.0
111.90	156.0
115.00	106.0
116.00	375.0
117.00	534.0
118.00	390.0
118.80	510.0
127.80	348.0
128.80	181.0
129.90	284.0
130.90	360.0
134.70	144.0
141.00	1101.0
142.90	1332.0
144.80	407.0
147.80	269.0
149.80	110.0
152.90	126.0
154.90	330.0
157.00	164.0
171.00	292.0
172.00	1816.0
172.90	934.0
174.00	66216.0
175.00	4858.0
176.00	63872.0
177.00	4042.0
177.90	245.0

Instrument :
MSVOA_V
ClientSampleId :
BFB03

Scan 2794 (10.074 min): VV010504.D
BFB03

m/z	Abundance
39.90	1247.0
43.80	375.0
44.20	235.0

Instrument :
MSVOA_V
ClientSampleId :
BFB03