

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042621\
 Data File : VV021136.D
 Acq On : 26 Apr 2021 12:22
 Operator : SY/MD
 Sample : VV0426MBL01
 Misc : 5.0g/5.0mL/100uL/5.0mL/MSVOA_V/MEOH
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :

Quant Time: Apr 27 04:16:33 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM042121WMA.M
 Quant Title : VOC Analysis
 QLast Update : Tue Apr 27 04:16:04 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	5.619	114	701391	50.00	ug/L	0.00
28) Chlorobenzene-d5	8.857	117	679448	50.00	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.255	152	318487	50.00	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.307	65	189339	32.85	ug/L	0.00
Spiked Amount	50.000	Range	60 - 135	Recovery	=	65.70%
7) Chloroethane-d5	1.571	69	165588	39.06	ug/L	0.00
Spiked Amount	50.000	Range	70 - 130	Recovery	=	78.12%
11) 1,1-Dichloroethene-d2	2.108	63	291385	27.41	ug/L	0.00
Spiked Amount	50.000	Range	60 - 125	Recovery	=	54.82%#
21) 2-Butanone-d5	3.902	46	282344	100.32	ug/L	0.00
Spiked Amount	100.000	Range	40 - 130	Recovery	=	100.32%
24) Chloroform-d	4.349	84	442203	43.04	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	86.08%
26) 1,2-Dichloroethane-d4	5.034	65	297108	45.49	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	90.98%
32) Benzene-d6	5.053	84	768954	42.49	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	84.98%
36) 1,2-Dichloropropane-d6	6.072	67	246870	45.71	ug/L	0.00
Spiked Amount	50.000	Range	70 - 120	Recovery	=	91.42%
41) Toluene-d8	7.320	98	709371	40.51	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	81.02%
43) trans-1,3-Dichloroprop...	7.625	79	123883	41.97	ug/L	0.00
Spiked Amount	50.000	Range	60 - 125	Recovery	=	83.94%
47) 2-Hexanone-d5	8.091	63	210590	98.30	ug/L	0.00
Spiked Amount	100.000	Range	45 - 130	Recovery	=	98.30%
56) 1,1,2,2-Tetrachloroeth...	10.220	84	367113	45.06	ug/L	0.00
Spiked Amount	50.000	Range	65 - 120	Recovery	=	90.12%
66) 1,2-Dichlorobenzene-d4	11.631	152	306504	48.72	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	97.44%
Target Compounds						
44) trans-1,3-Dichloropropene	7.628	75	5978	0.76	ug/L	Qvalue 92


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042621\
Data File : VV021136.D
Acq On : 26 Apr 2021 12:22
Operator : SY/MD
Sample : VV0426MBL01
Misc : 5.0g/5.0mL/100uL/5.0mL/MSVOA_V/MEOH
ALS Vial : 3 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :


Quant Time: Apr 27 04:16:33 2021
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM042121WMA.M
Quant Title : VOC Analysis
QLast Update : Tue Apr 27 04:16:04 2021
Response via : Initial Calibration

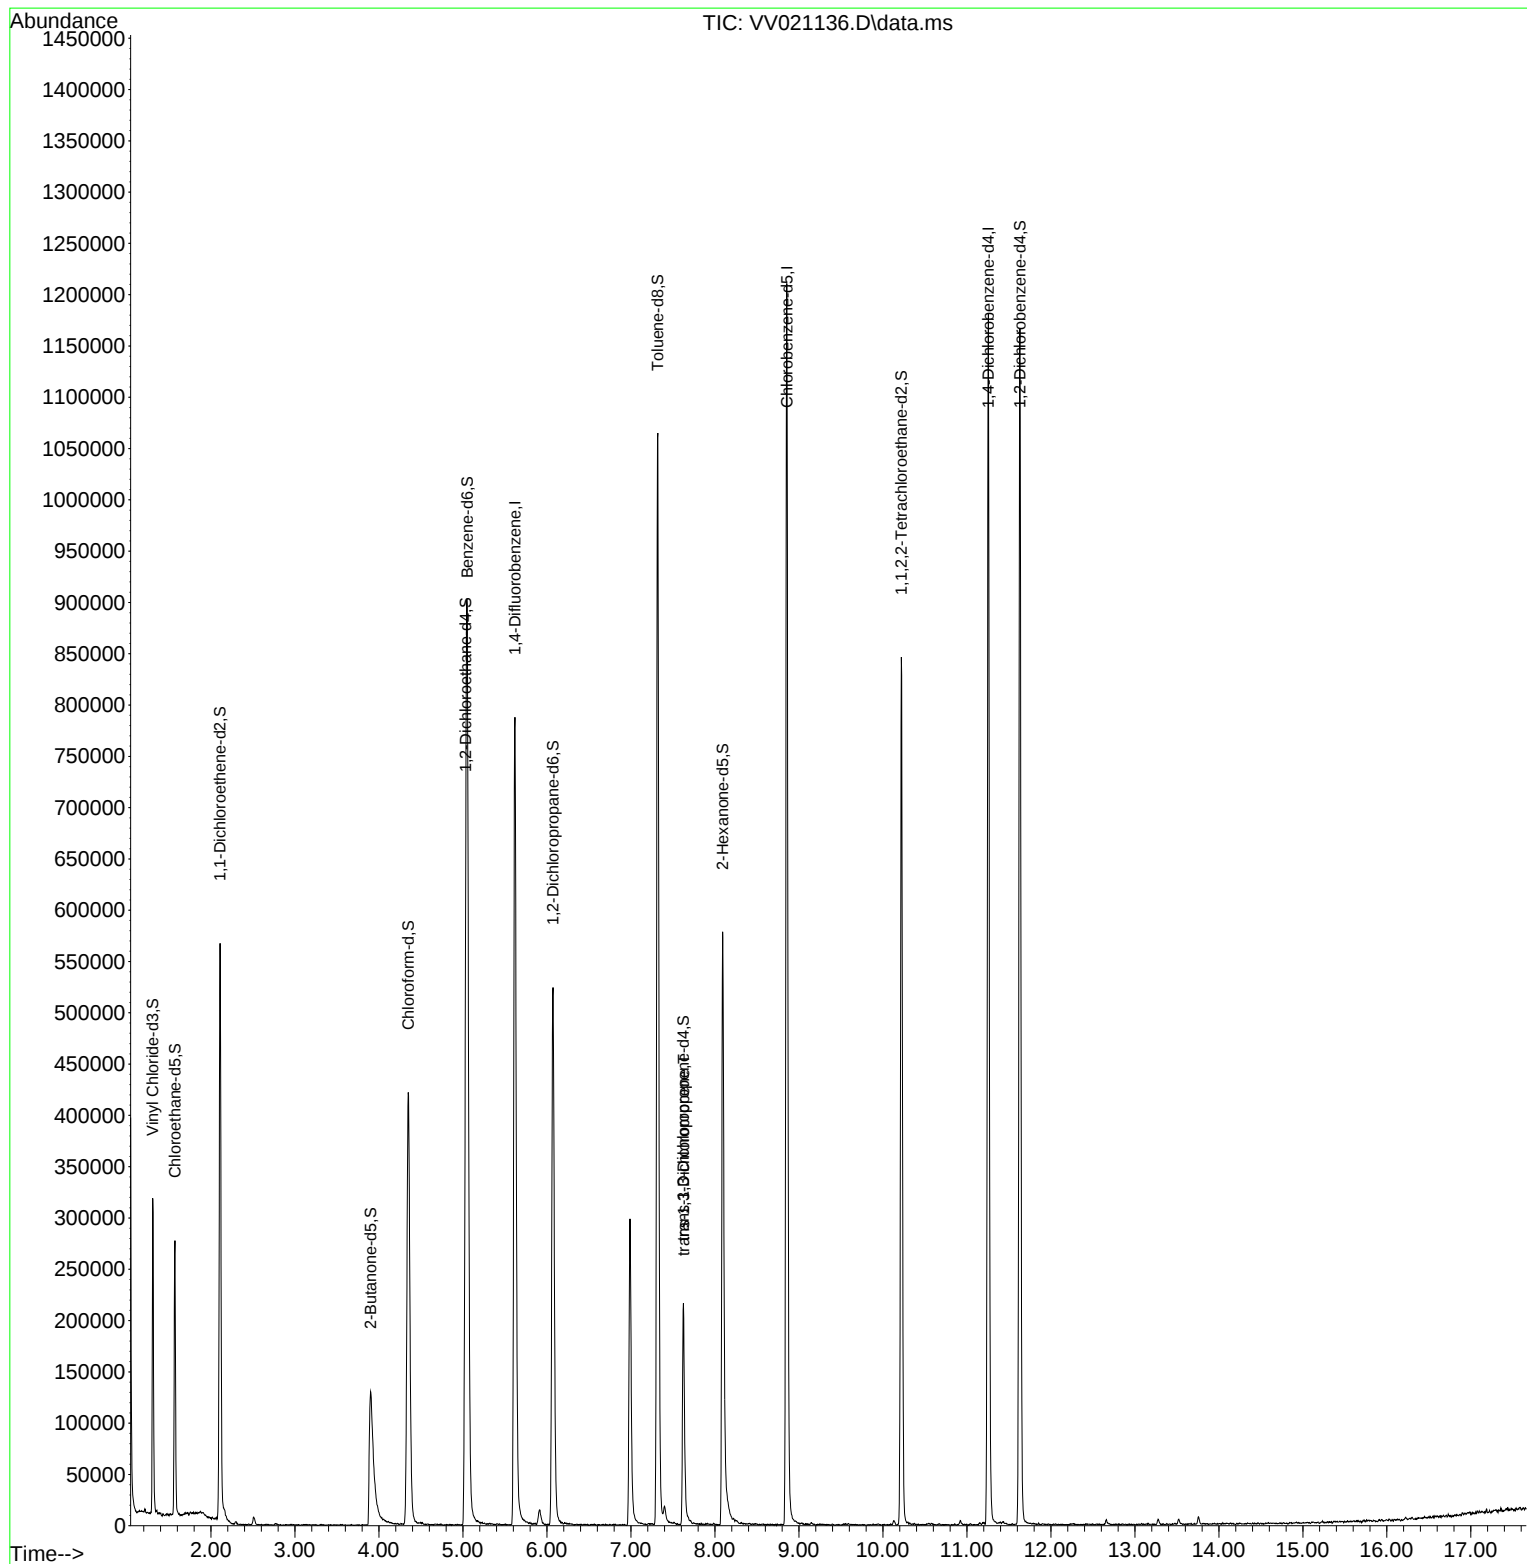

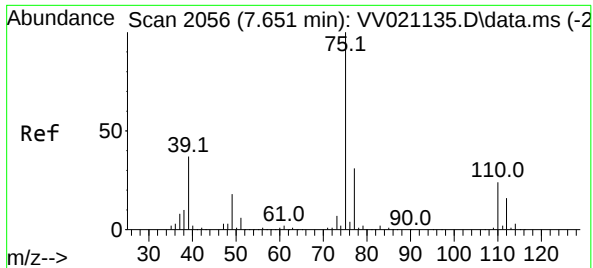

#44
 trans-1,3-Dichloropropene
 Concen: 0.76 ug/L
 RT: 7.628 min Scan# 2049
 Delta R.T. -0.023 min
 Lab File: VV021136.D
 Acq: 26 Apr 2021 12:22

Instrument :
 MSVOA_V
 ClientSampleId :

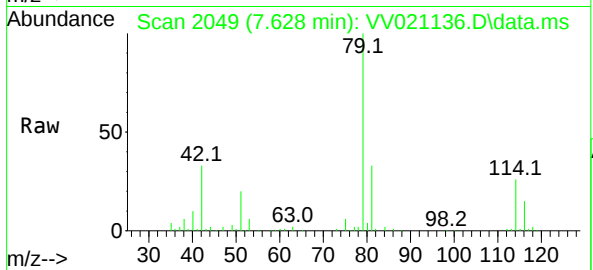

Tgt Ion: 75 Resp: 5978
 Ion Ratio Lower Upper
 75 100
 77 35.5 21.8 40.6

