

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042621\
 Data File : VV021146.D
 Acq On : 26 Apr 2021 16:25
 Operator : SY/MD
 Sample : M2121-03ME
 Misc : 2.80g/5.0mL/100uL/5.0mL/MSVOA_V/MEOH
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :

Quant Time: Apr 27 04:18:10 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM042121WMA.M
 Quant Title : VOC Analysis
 QLast Update : Tue Apr 27 04:16:04 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	5.616	114	753293	50.00	ug/L	0.00
28) Chlorobenzene-d5	8.860	117	730771	50.00	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.262	152	351274	50.00	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.307	65	186131	30.07	ug/L	0.00
Spiked Amount	50.000	Range	60 - 135	Recovery	=	60.14%
7) Chloroethane-d5	1.571	69	140392	30.83	ug/L	0.00
Spiked Amount	50.000	Range	70 - 130	Recovery	=	61.66%#
11) 1,1-Dichloroethene-d2	2.092	63	291765	25.56	ug/L	-0.02
Spiked Amount	50.000	Range	60 - 125	Recovery	=	51.12%#
21) 2-Butanone-d5	3.912	46	235799	78.01	ug/L	0.02
Spiked Amount	100.000	Range	40 - 130	Recovery	=	78.01%
24) Chloroform-d	4.349	84	411569	37.30	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	74.60%
26) 1,2-Dichloroethane-d4	5.034	65	284061	40.50	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	81.00%
32) Benzene-d6	5.050	84	718765	36.93	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	73.86%
36) 1,2-Dichloropropane-d6	6.072	67	233809	40.25	ug/L	0.00
Spiked Amount	50.000	Range	70 - 120	Recovery	=	80.50%
41) Toluene-d8	7.320	98	660320	35.06	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	70.12%#
43) trans-1,3-Dichloroprop...	7.625	79	114679	36.12	ug/L	0.00
Spiked Amount	50.000	Range	60 - 125	Recovery	=	72.24%
47) 2-Hexanone-d5	8.323	63	246	0.11	ug/L	0.23
Spiked Amount	100.000	Range	45 - 130	Recovery	=	0.11%#
56) 1,1,2,2-Tetrachloroeth...	10.230	84	349118	39.84	ug/L	0.00
Spiked Amount	50.000	Range	65 - 120	Recovery	=	79.68%
66) 1,2-Dichlorobenzene-d4	11.635	152	294974	42.51	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	85.02%
Target Compounds						
44) trans-1,3-Dichloropropene	7.632	75	5664	0.67	ug/L	Qvalue 84


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042621\
Data File : VV021146.D
Acq On : 26 Apr 2021 16:25
Operator : SY/MD
Sample : M2121-03ME
Misc : 2.80g/5.0mL/100uL/5.0mL/MSVOA_V/MEOH
ALS Vial : 13 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :

Quant Time: Apr 27 04:18:10 2021
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM042121WMA.M
Quant Title : VOC Analysis
QLast Update : Tue Apr 27 04:16:04 2021
Response via : Initial Calibration

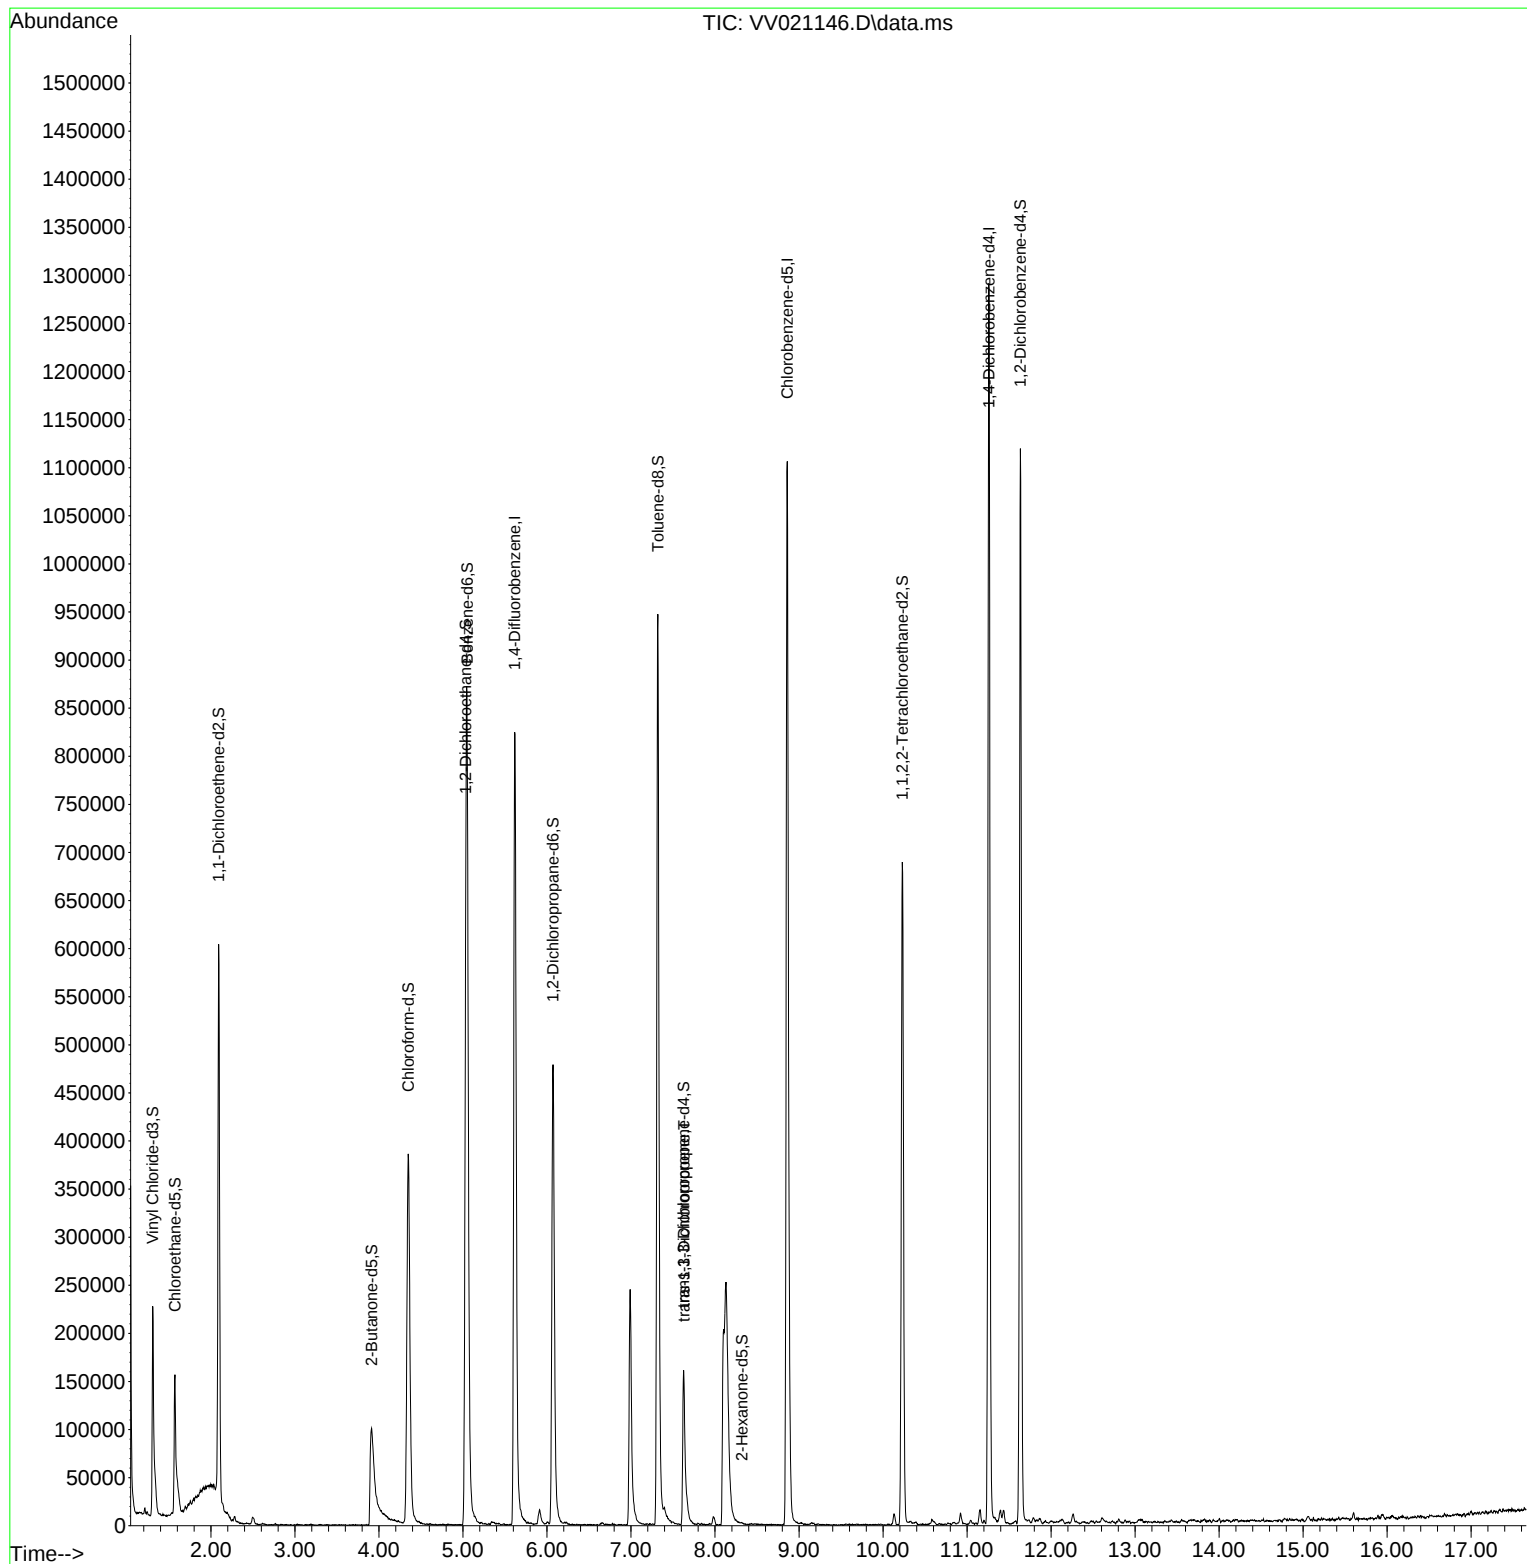


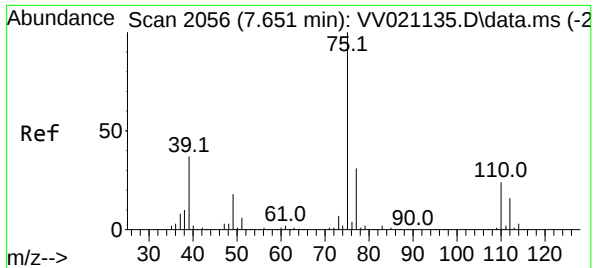

#44

trans-1,3-Dichloropropene
 Concen: 0.67 ug/L
 RT: 7.632 min Scan# 2050
 Delta R.T. -0.019 min
 Lab File: VV021146.D
 Acq: 26 Apr 2021 16:25

Instrument :
 MSVOA_V
 ClientSampleId :

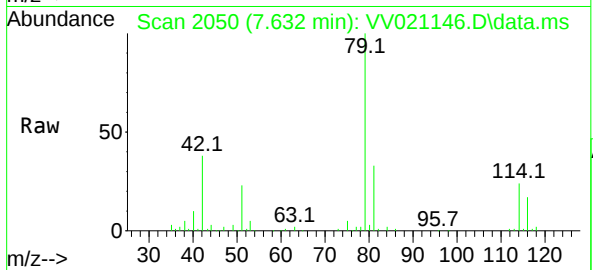

Tgt Ion: 75 Resp: 5664
 Ion Ratio Lower Upper
 75 100
 77 39.9 21.8 40.6

