


Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042621\
Data File : VV021140.D
Acq On : 26 Apr 2021 14:05
Operator : SY/MD
Sample : M2123-07
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 7 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BG7A7

Manual Integrations
APPROVED

MMDadoda
4/27/2021 10:43:04 AM

Quant Time: Apr 27 04:17:13 2021
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM042121WMA.M
Quant Title : VOC Analysis
QLast Update : Tue Apr 27 04:16:04 2021
Response via : Initial Calibration

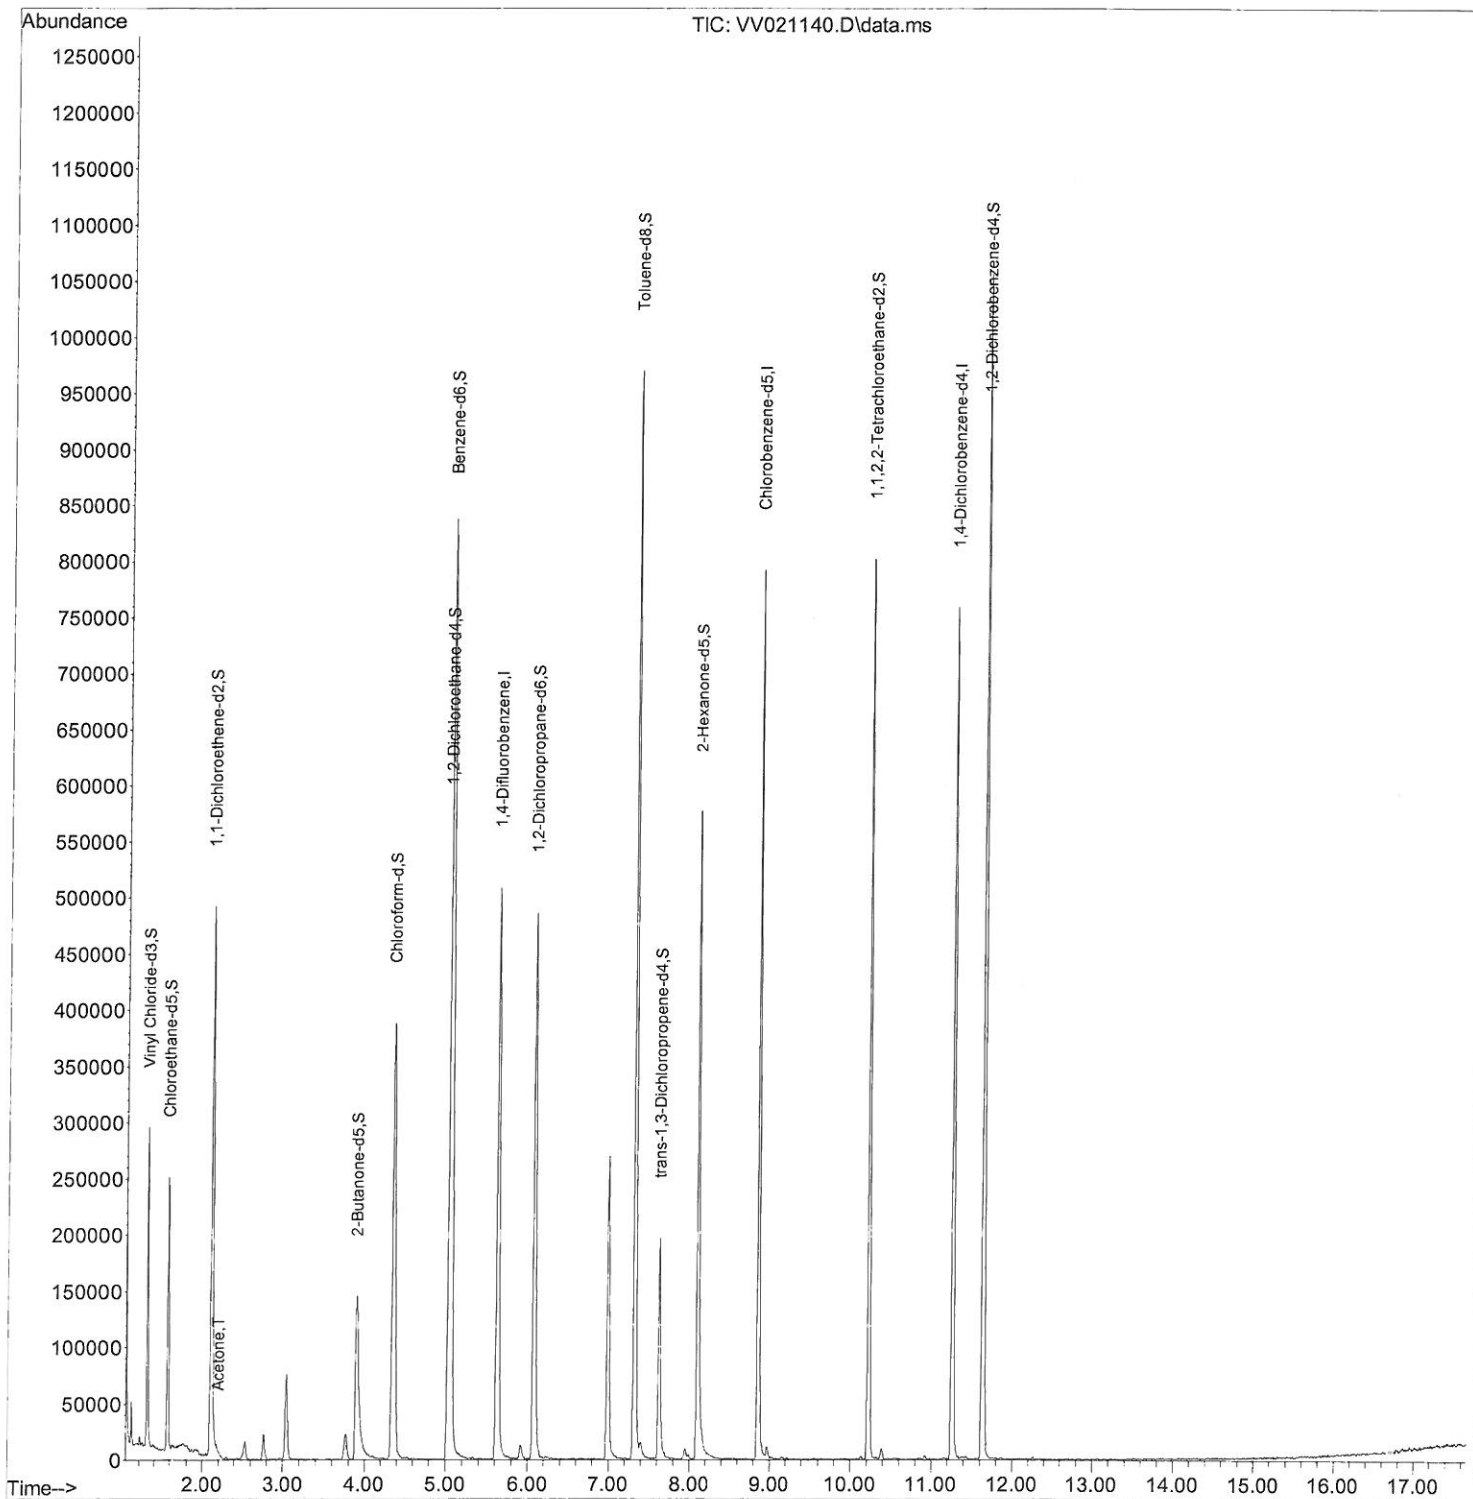

Quantitation Report (Qedit)




Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042621\
Data File : VV021140.D
Acq On : 26 Apr 2021 14:05
Operator : SY/MD
Sample : M2123-07
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 7 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BG7A7

Manual Integrations
APPROVED

MMDadoda
4/27/2021 10:43:04 AM

Quant Time: Apr 27 04:17:13 2021
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM042121WMA.M
Quant Title : VOC Analysis
QLast Update : Tue Apr 27 04:16:04 2021
Response via : Initial Calibration

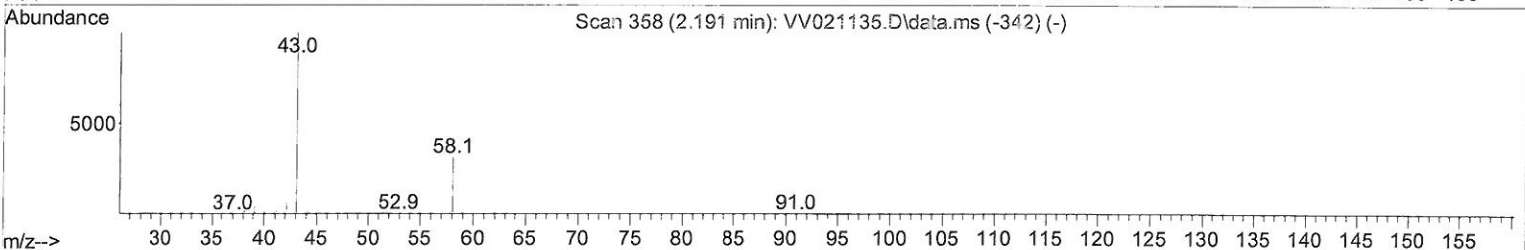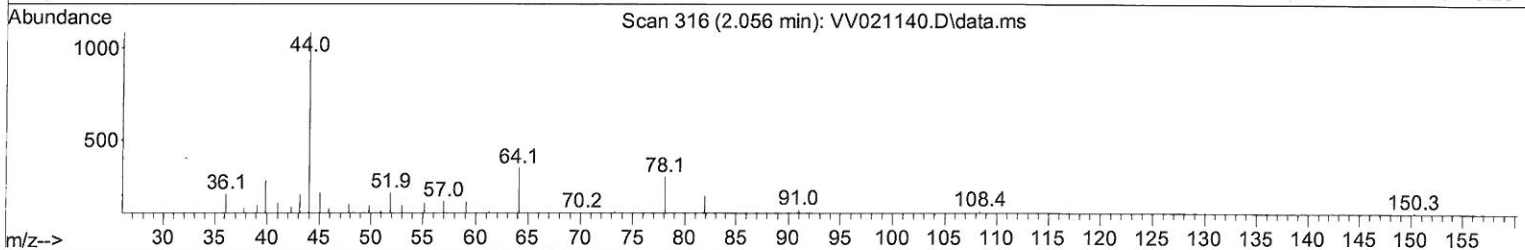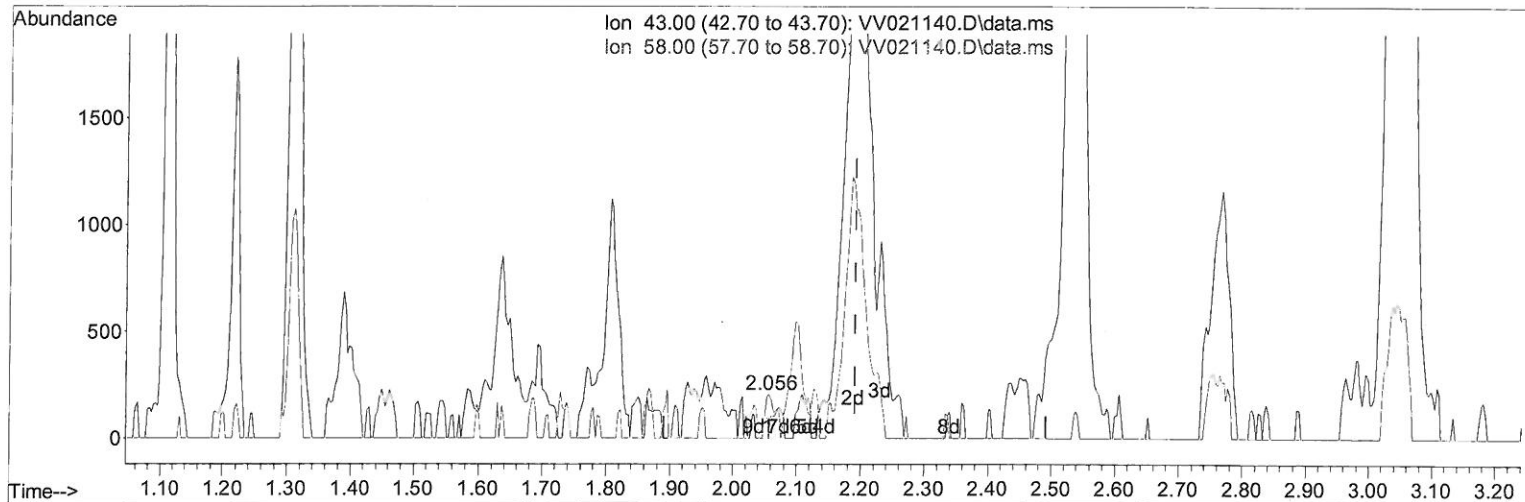

TIC: VV021140.D\data.ms

(13) Acetone (T)

2.056min (-0.135) 0.11 ug/L

response 182

Ion	Exp%	Act%
43.00	100.00	100.00
58.00	15.40	22.53
0.00	0.00	0.00
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042621\
Data File : VV021140.D
Acq On : 26 Apr 2021 14:05
Operator : SY/MD
Sample : M2123-07
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 7 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BG7A7

Manual Integrations
APPROVED

MMDadoda
4/27/2021 10:43:04 AM

Quant Time: Apr 27 04:17:13 2021
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM042121WMA.M
Quant Title : VOC Analysis
QLast Update : Tue Apr 27 04:16:04 2021
Response via : Initial Calibration

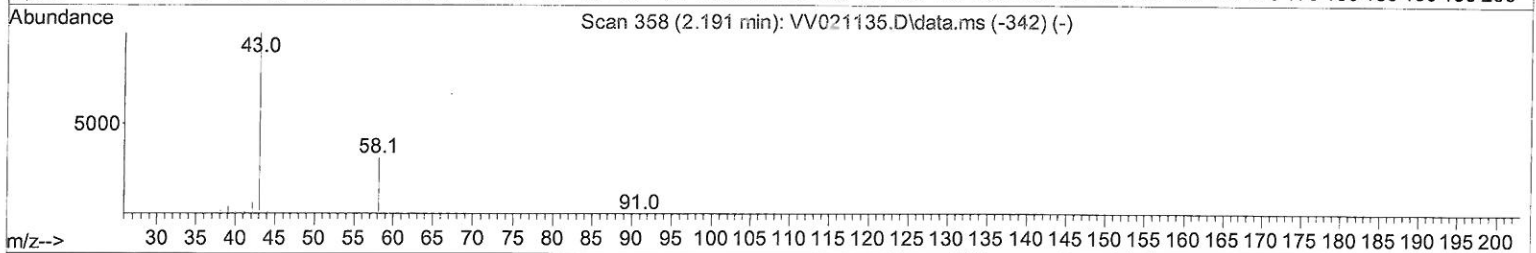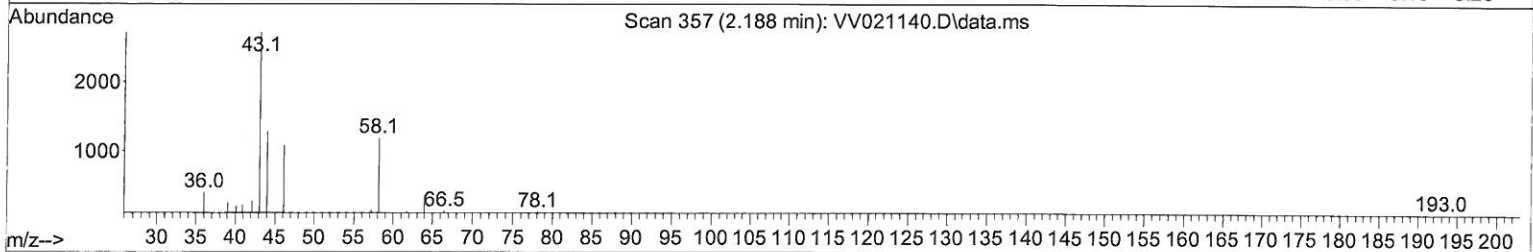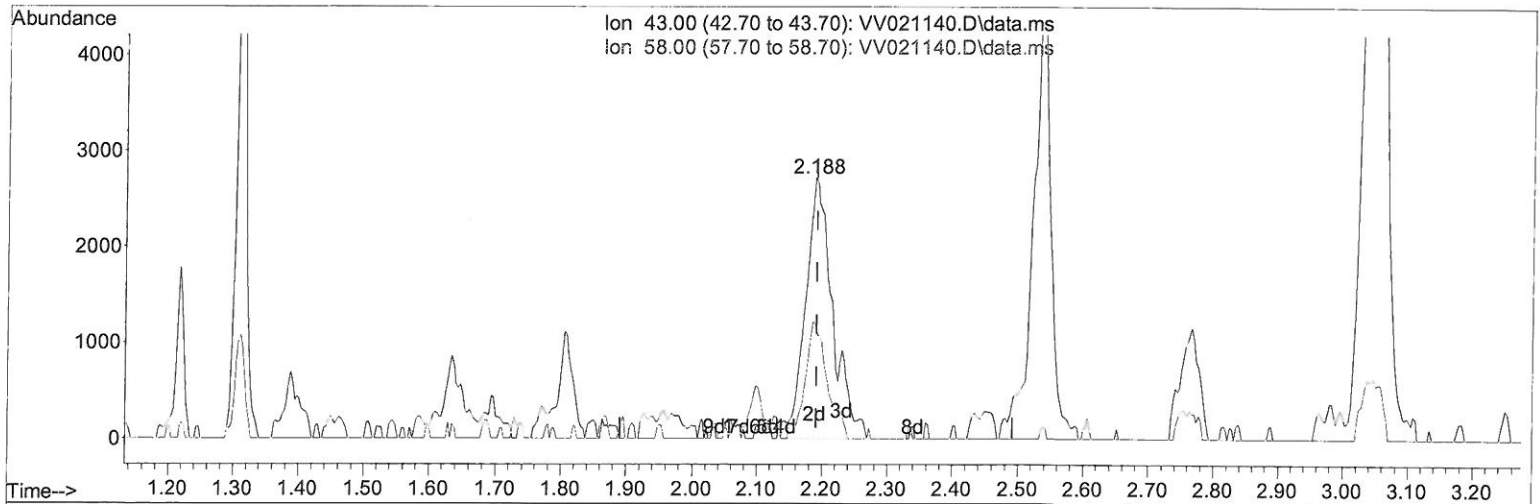

TIC: VV021140.D\data.ms

(13) Acetone (T)

2.188min (-0.003) 4.77 ug/L m

response 7848

Ion	Exp%	Act%
43.00	100.00	100.00
58.00	15.40	0.52
0.00	0.00	0.00
0.00	0.00	0.00

7 MD
4/29/21

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW042621\
 Data File : VW021140.D
 Acq On : 26 Apr 2021 14:05
 Operator : SY/MD
 Sample : M2123-07
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BG7A7

Manual Integrations
 APPROVED

MMDadoda
 4/27/2021 10:43:04 AM

Quant Time: Apr 27 04:17:13 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM042121WMA.M
 Quant Title : VOC Analysis
 QLast Update : Tue Apr 27 04:16:04 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)
Internal Standards						
1) 1,4-Difluorobenzene	5.622	114	439328	50.00	ug/L	0.00
28) Chlorobenzene-d5	8.857	117	437149	50.00	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.255	152	199622	50.00	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.307	65	168501	46.68	ug/L	0.00
Spiked Amount	50.000	Range	60 - 135	Recovery	=	93.36%
7) Chloroethane-d5	1.571	69	145755	54.88	ug/L	0.00
Spiked Amount	50.000	Range	70 - 130	Recovery	=	109.76%
11) 1,1-Dichloroethene-d2	2.111	63	256887	38.58	ug/L	0.00
Spiked Amount	50.000	Range	60 - 125	Recovery	=	77.16%
21) 2-Butanone-d5	3.899	46	271022	153.74	ug/L	0.00
Spiked Amount	100.000	Range	40 - 130	Recovery	=	153.74%#
24) Chloroform-d	4.352	84	400725	62.27	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	124.54%
26) 1,2-Dichloroethane-d4	5.034	65	276539	67.60	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	135.20%#
32) Benzene-d6	5.053	84	710055	60.99	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	121.98%
36) 1,2-Dichloropropane-d6	6.076	67	229979	66.18	ug/L	0.00
Spiked Amount	50.000	Range	70 - 120	Recovery	=	132.36%#
41) Toluene-d8	7.320	98	640889	56.88	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	113.76%
43) trans-1,3-Dichloroprop...	7.625	79	118783	62.55	ug/L	0.00
Spiked Amount	50.000	Range	60 - 125	Recovery	=	125.10%#
47) 2-Hexanone-d5	8.092	63	202373	146.83	ug/L	0.00
Spiked Amount	100.000	Range	45 - 130	Recovery	=	146.83%#
56) 1,1,2,2-Tetrachloroeth...	10.220	84	355601	67.84	ug/L	0.00
Spiked Amount	50.000	Range	65 - 120	Recovery	=	135.68%#
66) 1,2-Dichlorobenzene-d4	11.632	152	286889	72.75	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	145.50%#
Target Compounds						
13) Acetone	2.188	43	7848m	4.77	ug/L	Qvalue

7 MD
 4/29/21

(#) = qualifier out of range (m) = manual integration (+) = signals summed