

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW042621\
 Data File : VW021144.D
 Acq On : 26 Apr 2021 15:38
 Operator : SY/MD
 Sample : M2326-04
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BG7C6

Manual Integrations
 APPROVED

MMDadoda
 5/6/2021 2:51:03 PM

Quant Time: Apr 27 04:17:52 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM042121WMA.M
 Quant Title : VOC Analysis
 QLast Update : Tue Apr 27 04:16:04 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Difluorobenzene	5.622	114	676273	50.00	ug/L	0.00
28) Chlorobenzene-d5	8.857	117	677255	50.00	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.255	152	310787	50.00	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.310	65	183644	33.05	ug/L	0.00
Spiked Amount 50.000	Range 60 - 135		Recovery =	66.10%		
7) Chloroethane-d5	1.571	69	157181	38.45	ug/L	0.00
Spiked Amount 50.000	Range 70 - 130		Recovery =	76.90%		
11) 1,1-Dichloroethene-d2	2.111	63	281500	27.46	ug/L	0.00
Spiked Amount 50.000	Range 60 - 125		Recovery =	54.92%#		
21) 2-Butanone-d5	3.902	46	260567	96.02	ug/L	0.00
Spiked Amount 100.000	Range 40 - 130		Recovery =	96.02%		
24) Chloroform-d	4.355	84	402640	40.64	ug/L	0.00
Spiked Amount 50.000	Range 70 - 125		Recovery =	81.28%		
26) 1,2-Dichloroethane-d4	5.037	65	275248	43.71	ug/L	0.00
Spiked Amount 50.000	Range 70 - 125		Recovery =	87.42%		
32) Benzene-d6	5.053	84	699623	38.79	ug/L	0.00
Spiked Amount 50.000	Range 70 - 125		Recovery =	77.58%		
36) 1,2-Dichloropropane-d6	6.075	67	228152	42.38	ug/L	0.00
Spiked Amount 50.000	Range 70 - 120		Recovery =	84.76%		
41) Toluene-d8	7.320	98	630665	36.13	ug/L	0.00
Spiked Amount 50.000	Range 80 - 120		Recovery =	72.26%#		
43) trans-1,3-Dichloroprop...	7.625	79	110033	37.40	ug/L	0.00
Spiked Amount 50.000	Range 60 - 125		Recovery =	74.80%		
47) 2-Hexanone-d5	8.095	63	190450	89.19	ug/L	0.00
Spiked Amount 100.000	Range 45 - 130		Recovery =	89.19%		
56) 1,1,2,2-Tetrachloroeth...	10.220	84	329251	40.54	ug/L	0.00
Spiked Amount 50.000	Range 65 - 120		Recovery =	81.08%		
66) 1,2-Dichlorobenzene-d4	11.632	152	267660	43.60	ug/L	0.00
Spiked Amount 50.000	Range 80 - 120		Recovery =	87.20%		
Target Compounds						Qvalue
13) Acetone	2.207	43	10370m	4.09	ug/L	

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042621\
Data File : VV021144.D
Acq On : 26 Apr 2021 15:38
Operator : SY/MD
Sample : M2326-04
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 11 Sample Multiplier: 1


Instrument :
MSVOA_V
ClientSampled :
BG7C6

Manual Integrations
APPROVED

MMDadoda
5/6/2021 2:51:03 PM

Quant Time: Apr 27 04:17:52 2021
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM042121WMA.M
Quant Title : VOC Analysis
QLast Update : Tue Apr 27 04:16:04 2021
Response via : Initial Calibration

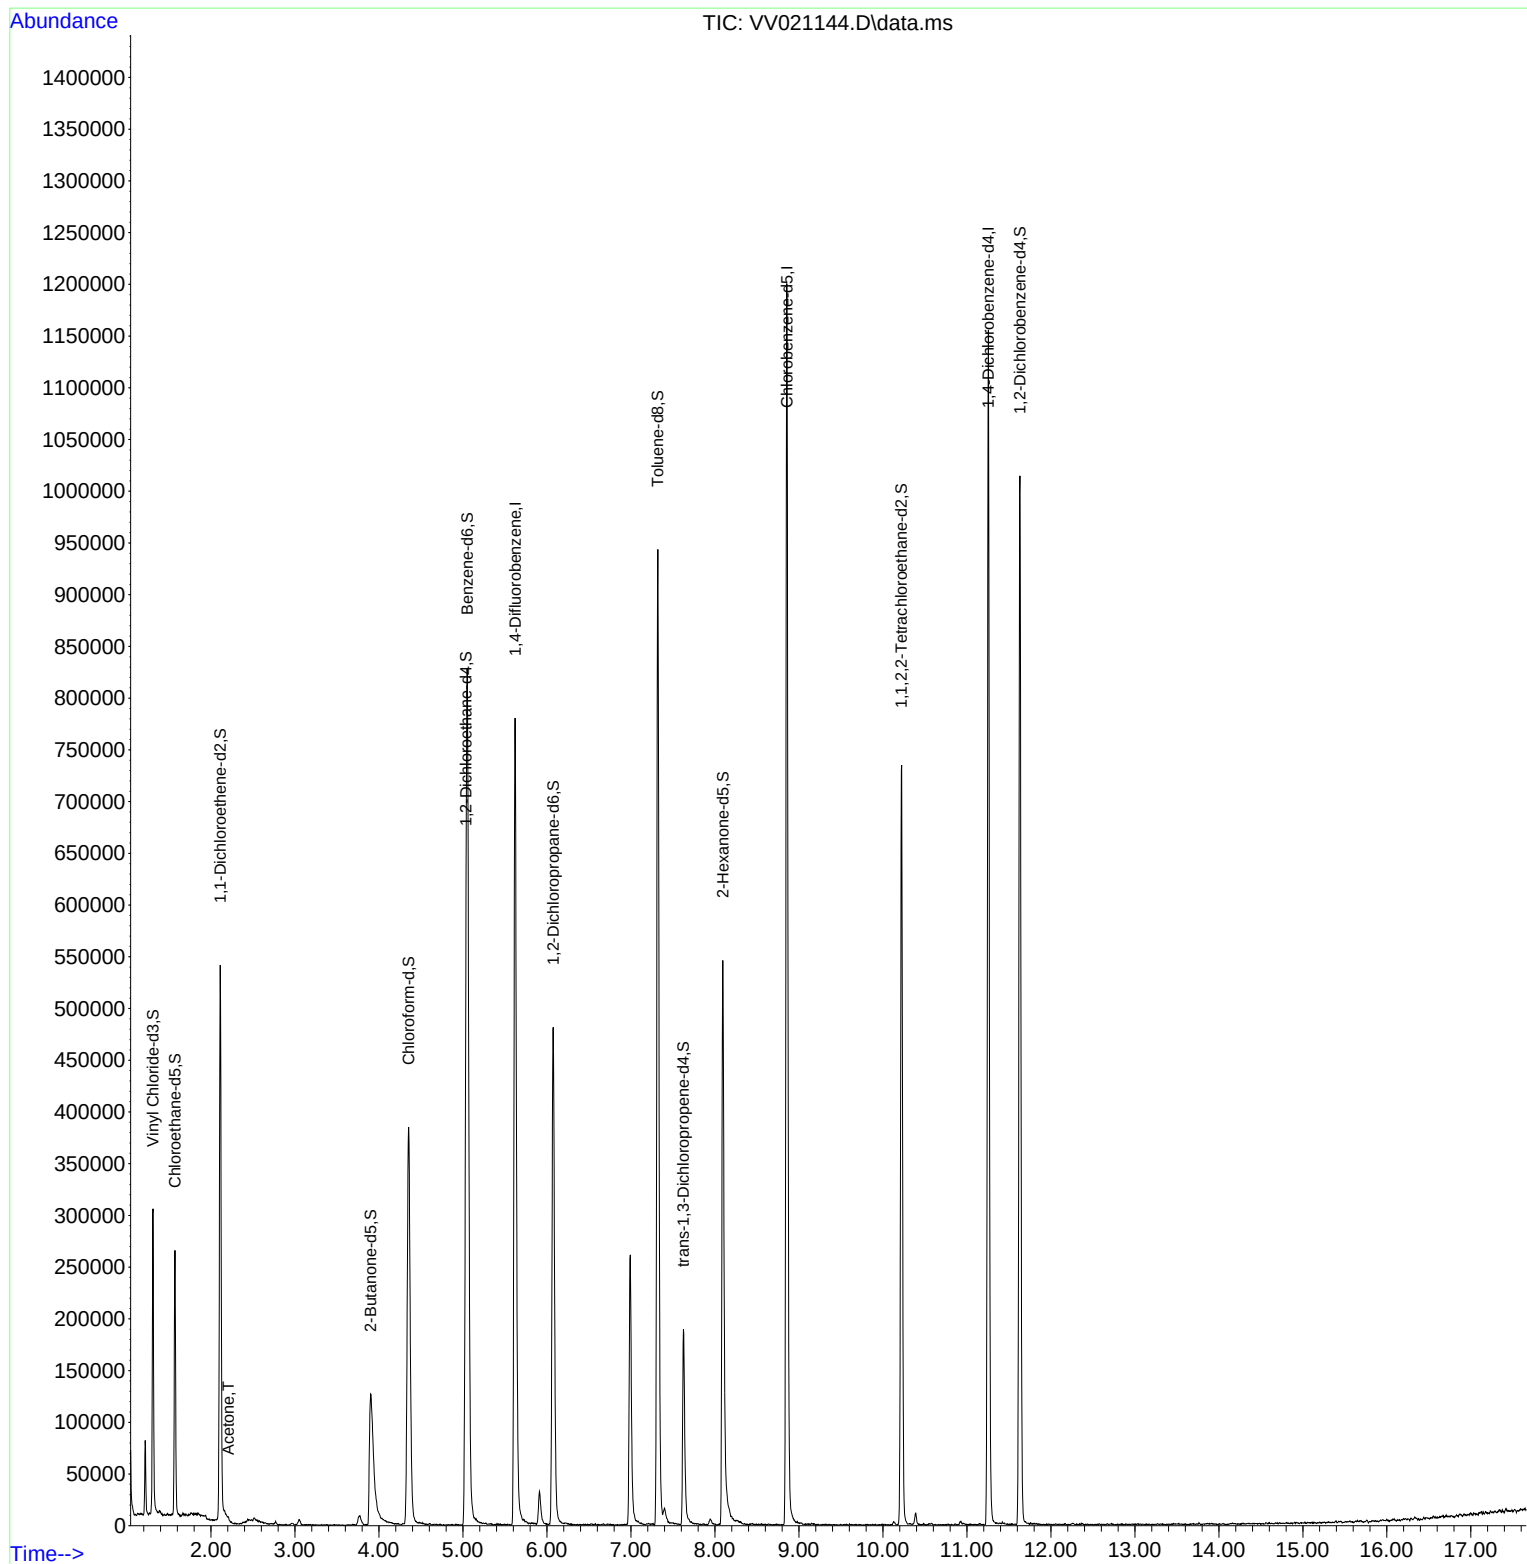

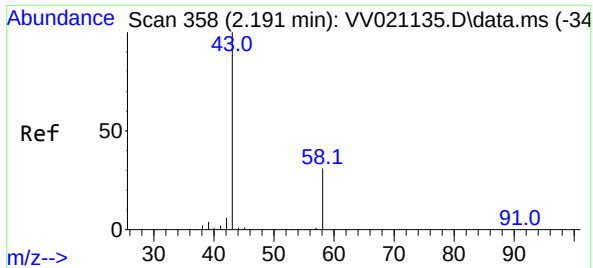

#13
Acetone
Concen: 4.09 ug/L m
RT: 2.207 min Scan# 363
Delta R.T. 0.016 min
Lab File: VV021144.D
Acq: 26 Apr 2021 15:38

Tgt Ion: 43 Resp: 10370
Ion Ratio Lower Upper
43 100
58 1.5 0.0 30.8

Instrument :
MSVOA_V
ClientSampleId :
BG7C6

Manual Integrations
APPROVED

MMDadoda
5/6/2021 2:51:03 PM

