

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW042621\
 Data File : VW021149.D
 Acq On : 26 Apr 2021 17:59
 Operator : SY/MD
 Sample : M2165-15ME
 Misc : 7.10g/5.0mL/100uL/5.0mL/MSVOA_V/MEOH
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 GB3F6ME

Quant Time: Apr 27 04:18:43 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM042121WMA.M
 Quant Title : VOC Analysis
 QLast Update : Tue Apr 27 04:16:04 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	5.616	114	656916	50.00	ug/L	0.00
28) Chlorobenzene-d5	8.860	117	636435	50.00	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.262	152	306121	50.00	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.307	65	238290	44.15	ug/L	0.00
Spiked Amount 50.000	Range 60 - 135		Recovery = 88.30%			
7) Chloroethane-d5	1.571	69	199184	50.16	ug/L	0.00
Spiked Amount 50.000	Range 70 - 130		Recovery = 100.32%			
11) 1,1-Dichloroethene-d2	2.092	63	380049	38.17	ug/L	-0.02
Spiked Amount 50.000	Range 60 - 125		Recovery = 76.34%			
21) 2-Butanone-d5	3.908	46	383215	145.38	ug/L	0.01
Spiked Amount 100.000	Range 40 - 130		Recovery = 145.38%#			
24) Chloroform-d	4.346	84	642737	66.79	ug/L	0.00
Spiked Amount 50.000	Range 70 - 125		Recovery = 133.58%#			
26) 1,2-Dichloroethane-d4	5.031	65	446744	73.03	ug/L	0.00
Spiked Amount 50.000	Range 70 - 125		Recovery = 146.06%#			
32) Benzene-d6	5.047	84	1113221	65.68	ug/L	0.00
Spiked Amount 50.000	Range 70 - 125		Recovery = 131.36%#			
36) 1,2-Dichloropropane-d6	6.072	67	368073	72.75	ug/L	0.00
Spiked Amount 50.000	Range 70 - 120		Recovery = 145.50%#			
41) Toluene-d8	7.317	98	1044198	63.65	ug/L	0.00
Spiked Amount 50.000	Range 80 - 120		Recovery = 127.30%#			
43) trans-1,3-Dichloroprop...	7.625	79	185997	67.27	ug/L	0.00
Spiked Amount 50.000	Range 60 - 125		Recovery = 134.54%#			
47) 2-Hexanone-d5	8.133	63	357434	178.12	ug/L	0.04
Spiked Amount 100.000	Range 45 - 130		Recovery = 178.12%#			
56) 1,1,2,2-Tetrachloroeth...	10.233	84	563999	73.91	ug/L	0.01
Spiked Amount 50.000	Range 65 - 120		Recovery = 147.82%#			
66) 1,2-Dichlorobenzene-d4	11.635	152	478401	79.11	ug/L	0.00
Spiked Amount 50.000	Range 80 - 120		Recovery = 158.22%#			
Target Compounds						Qvalue
46) Tetrachloroethene	7.979	164	100648	22.92	ug/L	93


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042621\
Data File : VV021149.D
Acq On : 26 Apr 2021 17:59
Operator : SY/MD
Sample : M2165-15ME
Misc : 7.10g/5.0mL/100uL/5.0mL/MSVOA_V/MEOH
ALS Vial : 17 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
GB3F6ME


Quant Time: Apr 27 04:18:43 2021
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM042121WMA.M
Quant Title : VOC Analysis
QLast Update : Tue Apr 27 04:16:04 2021
Response via : Initial Calibration

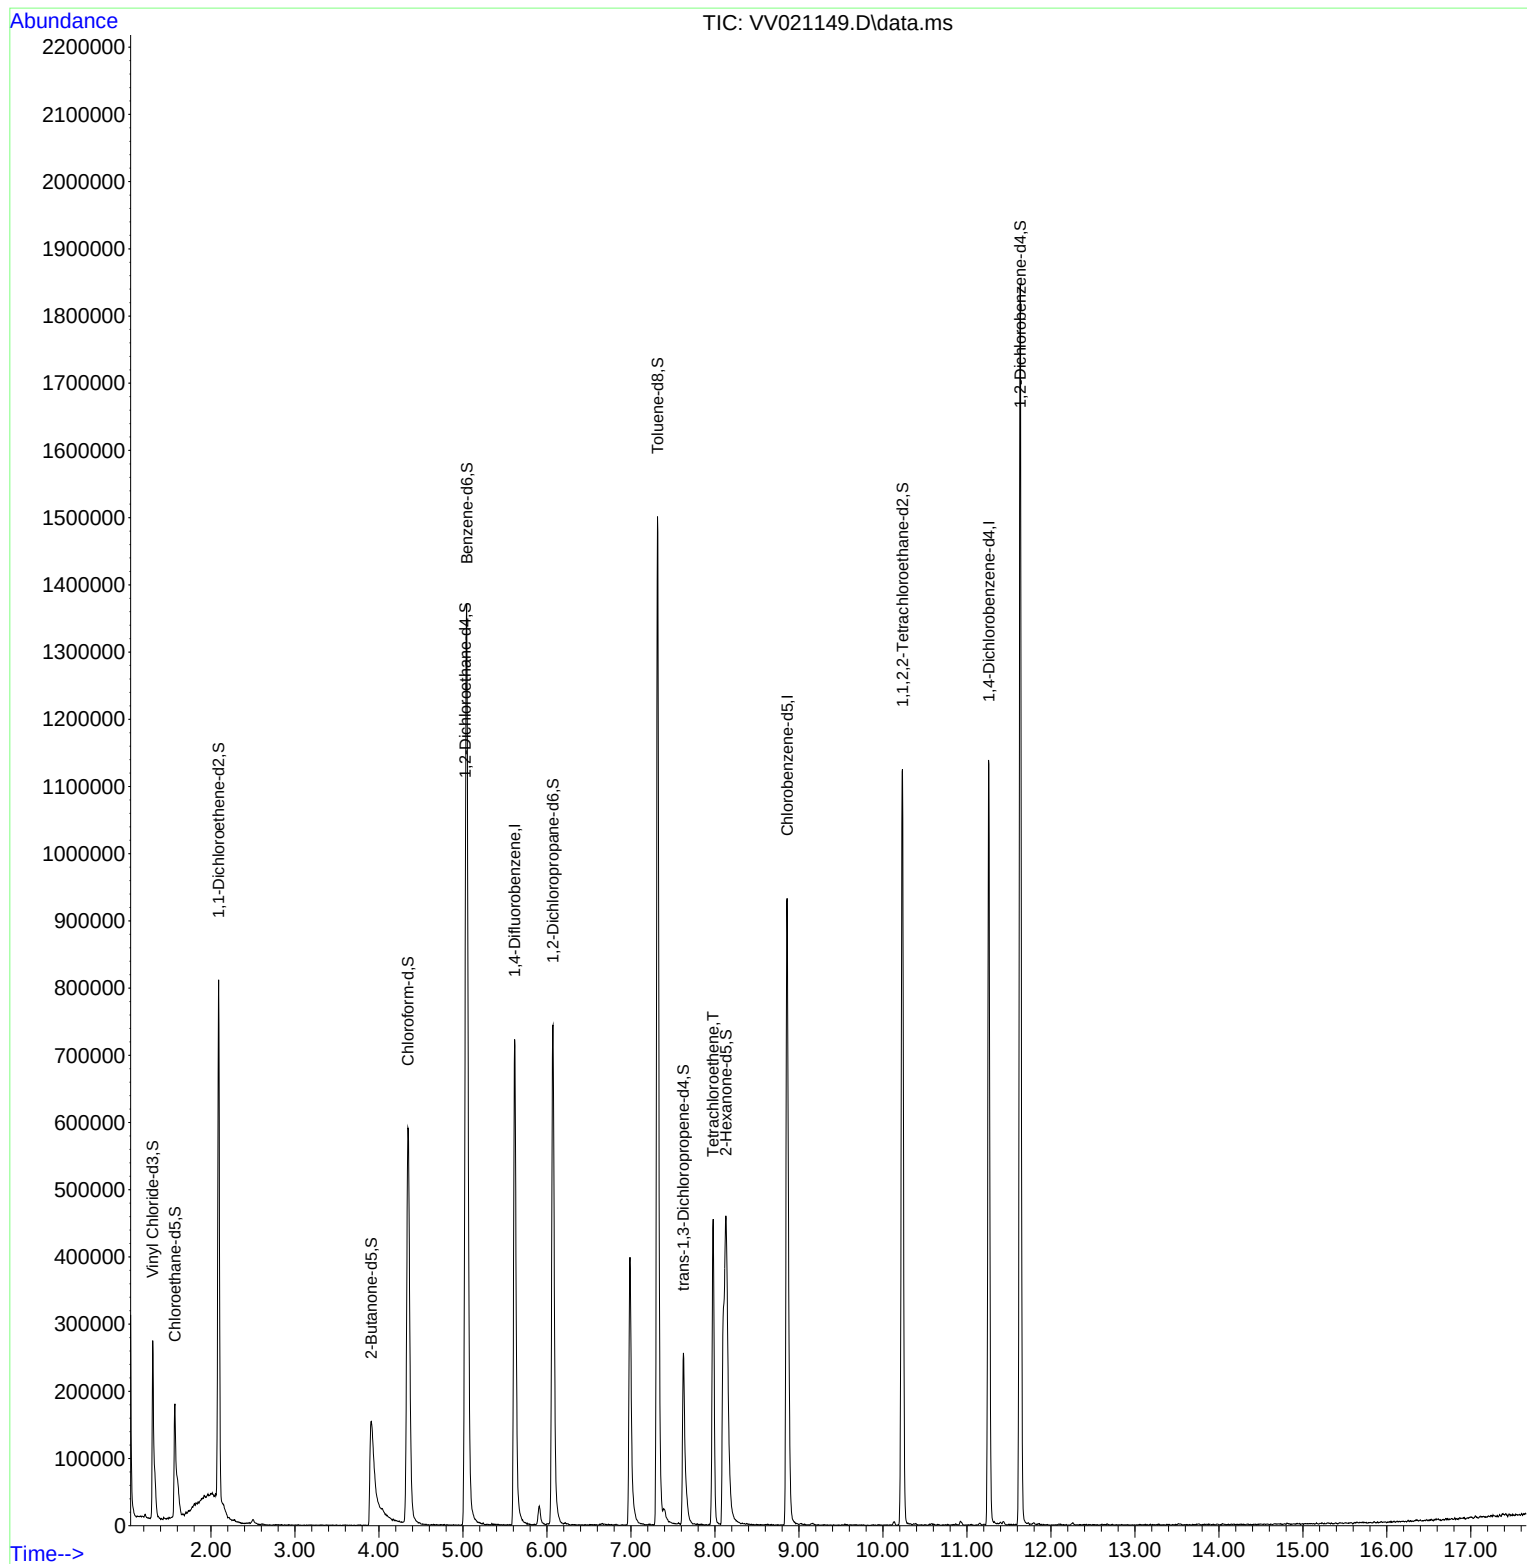

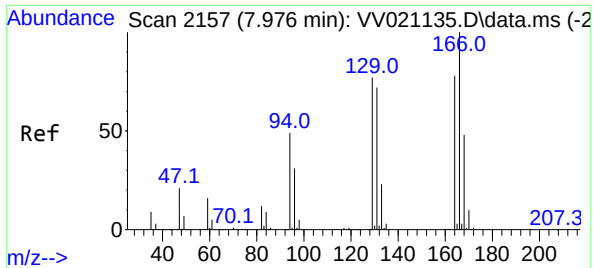

#46
Tetrachloroethene
Concen: 22.92 ug/L
RT: 7.979 min Scan# 2158
Delta R.T. 0.003 min
Lab File: VV021149.D
Acq: 26 Apr 2021 17:59

Instrument :
MSVOA_V
ClientSampleId :
GB3F6ME

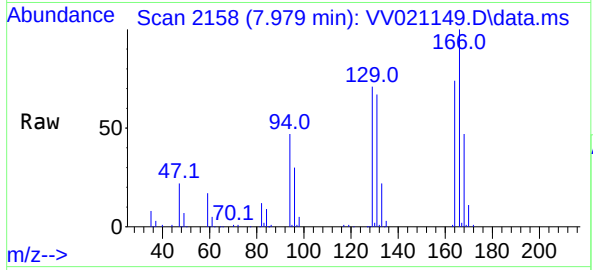

Tgt Ion:164 Resp: 100648

Ion	Ratio	Lower	Upper
164	100		
129	95.6	63.8	118.4
131	90.3	59.3	110.1
166	135.3	87.7	162.9

