

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW042621\
 Data File : VW021158.D
 Acq On : 26 Apr 2021 21:31
 Operator : SY/MD
 Sample : M2165-05 10X
 Misc : 5.44g/5.0mL/100uL/5.0mL/MSVOA_V/MEOH
 ALS Vial : 26 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 GB3E6

Quant Time: Apr 27 04:20:32 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM042121WMA.M
 Quant Title : VOC Analysis
 QLast Update : Tue Apr 27 04:16:04 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	5.619	114	653382	50.00	ug/L	0.00
28) Chlorobenzene-d5	8.857	117	638147	50.00	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.255	152	303847	50.00	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.307	65	242261	45.12	ug/L	0.00
Spiked Amount 50.000	Range 60 - 135		Recovery = 90.24%			
7) Chloroethane-d5	1.568	69	184548	46.73	ug/L	0.00
Spiked Amount 50.000	Range 70 - 130		Recovery = 93.46%			
11) 1,1-Dichloroethene-d2	2.104	63	341581	34.49	ug/L	0.00
Spiked Amount 50.000	Range 60 - 125		Recovery = 68.98%			
21) 2-Butanone-d5	3.899	46	253939	96.86	ug/L	0.00
Spiked Amount 100.000	Range 40 - 130		Recovery = 96.86%			
24) Chloroform-d	4.349	84	438226	45.78	ug/L	0.00
Spiked Amount 50.000	Range 70 - 125		Recovery = 91.56%			
26) 1,2-Dichloroethane-d4	5.034	65	301218	49.51	ug/L	0.00
Spiked Amount 50.000	Range 70 - 125		Recovery = 99.02%			
32) Benzene-d6	5.053	84	809788	47.65	ug/L	0.00
Spiked Amount 50.000	Range 70 - 125		Recovery = 95.30%			
36) 1,2-Dichloropropane-d6	6.072	67	246420	48.58	ug/L	0.00
Spiked Amount 50.000	Range 70 - 120		Recovery = 97.16%			
41) Toluene-d8	7.320	98	771791	46.92	ug/L	0.00
Spiked Amount 50.000	Range 80 - 120		Recovery = 93.84%			
43) trans-1,3-Dichloroprop...	7.625	79	130495	47.07	ug/L	0.00
Spiked Amount 50.000	Range 60 - 125		Recovery = 94.14%			
47) 2-Hexanone-d5	8.095	63	207667	103.21	ug/L	0.00
Spiked Amount 100.000	Range 45 - 130		Recovery = 103.21%			
56) 1,1,2,2-Tetrachloroeth...	10.223	84	344471	45.02	ug/L	0.00
Spiked Amount 50.000	Range 65 - 120		Recovery = 90.04%			
66) 1,2-Dichlorobenzene-d4	11.631	152	320755	53.44	ug/L	0.00
Spiked Amount 50.000	Range 80 - 120		Recovery = 106.88%			
Target Compounds						Qvalue
46) Tetrachloroethene	7.982	164	9301947	2112.35	ug/L	97

(#) = qualifier out of range (m) = manual integration (+) = signals summed




Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042621\
Data File : VV021158.D
Acq On : 26 Apr 2021 21:31
Operator : SY/MD
Sample : M2165-05 10X
Misc : 5.44g/5.0mL/100uL/5.0mL/MSVOA_V/MEOH
ALS Vial : 26 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
GB3E6

Quant Time: Apr 27 04:20:32 2021
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM042121WMA.M
Quant Title : VOC Analysis
QLast Update : Tue Apr 27 04:16:04 2021
Response via : Initial Calibration

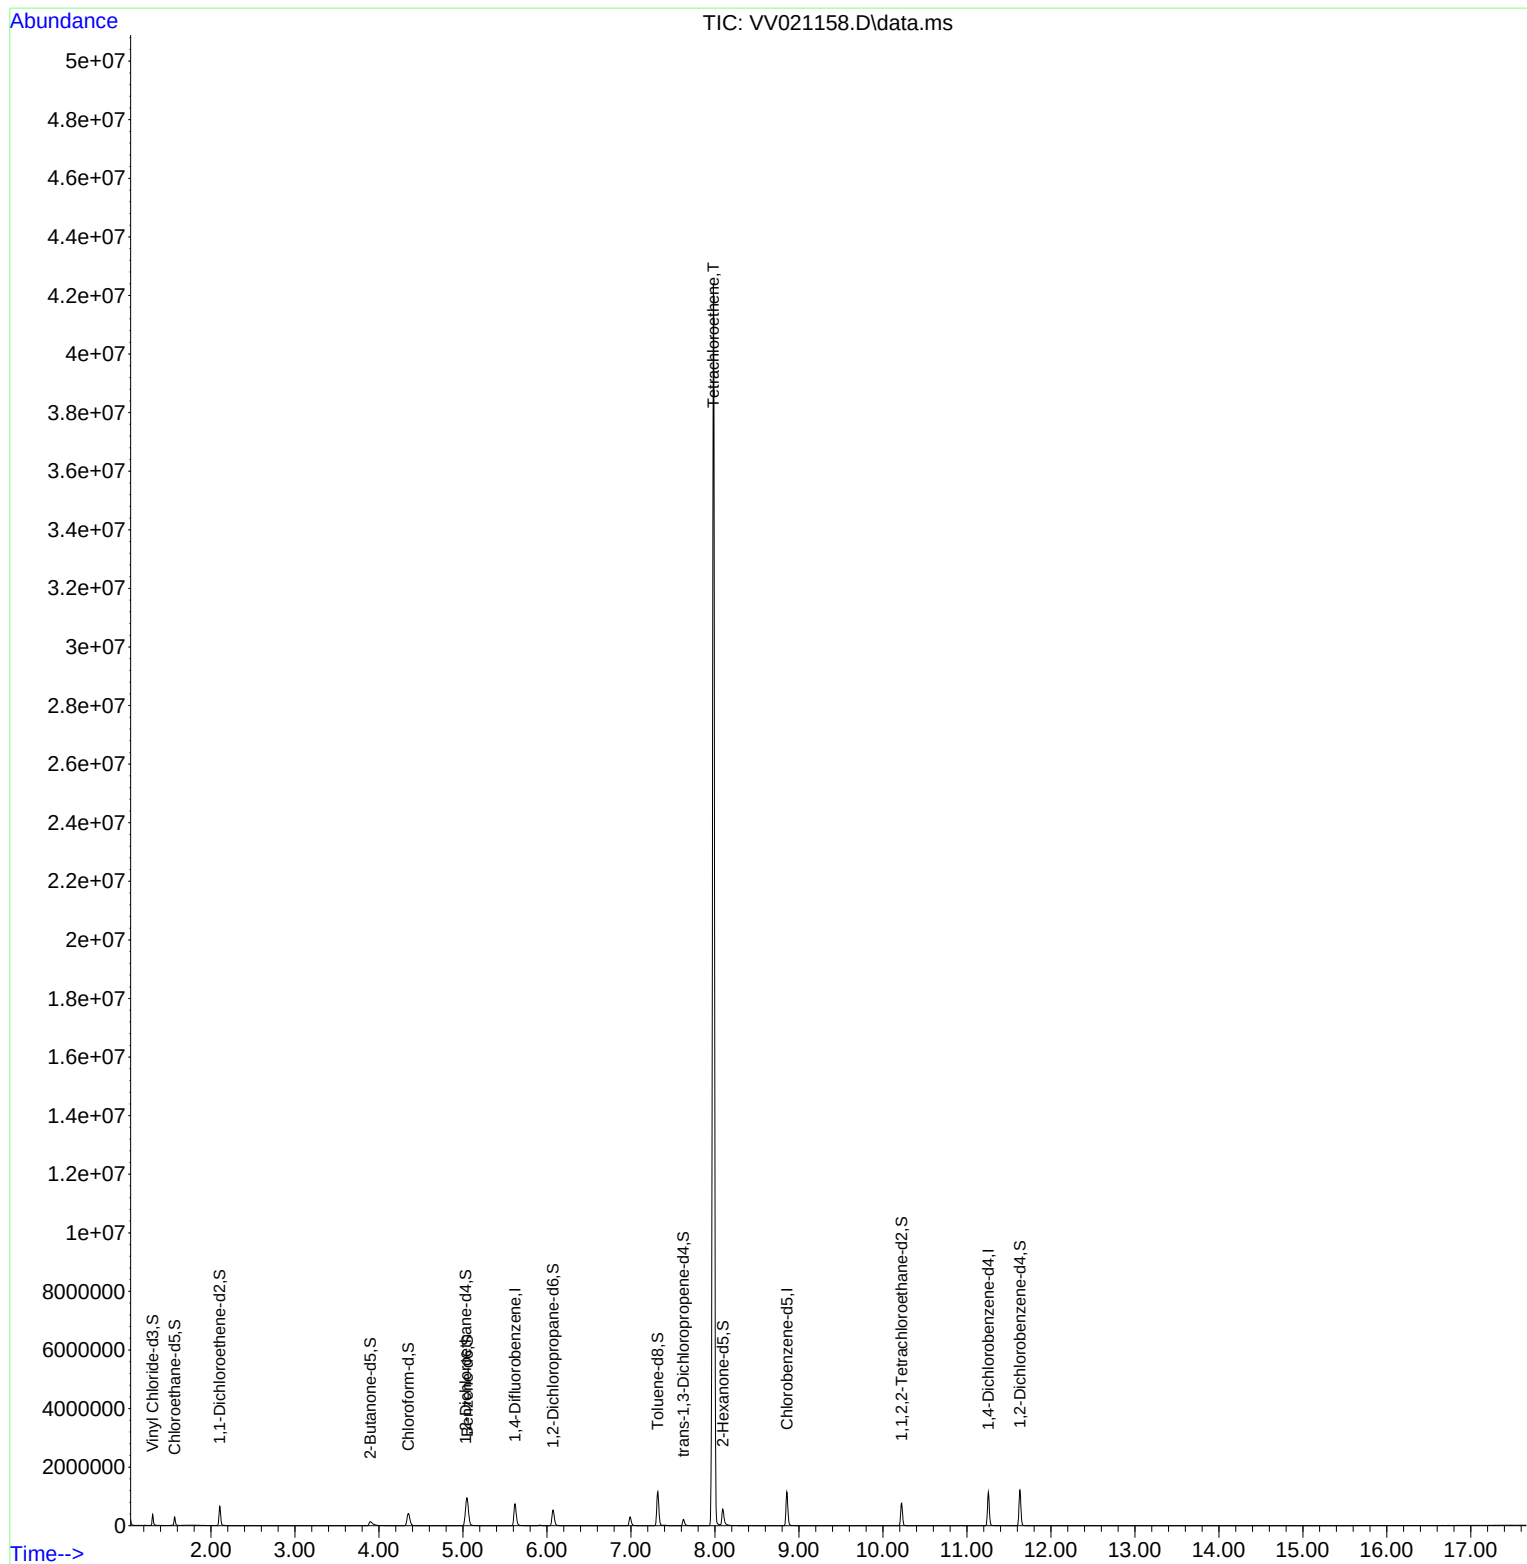


Abundance Scan 2157 (7.976 min): VV021135.D\data.ms (-2

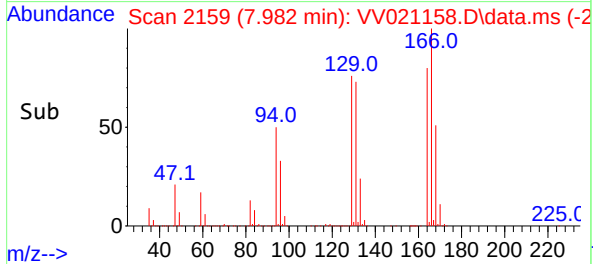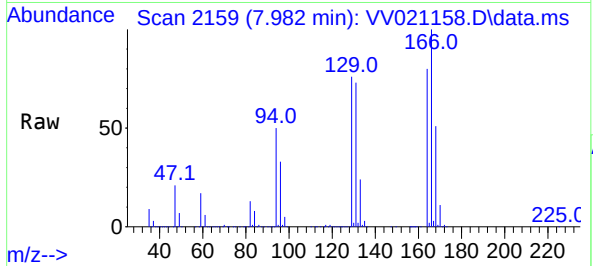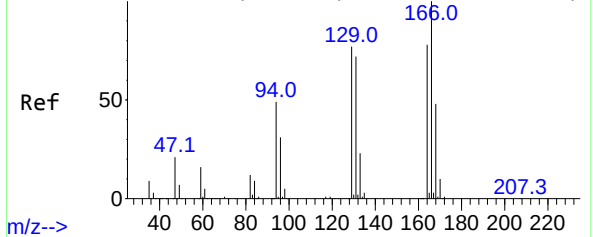

#46
Tetrachloroethene
Concen: 2112.35 ug/L
RT: 7.982 min Scan# 2159
Delta R.T. 0.006 min
Lab File: VV021158.D
Acq: 26 Apr 2021 21:31

Tgt Ion:164 Resp: 9301947

Ion	Ratio	Lower	Upper
164	100		
129	94.4	63.8	118.4
131	91.4	59.3	110.1
166	124.7	87.7	162.9

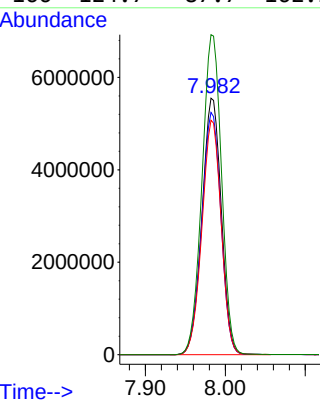

Instrument :
MSVOA_V
ClientSampleId :
GB3E6