

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042621\
 Data File : VV021137.D
 Acq On : 26 Apr 2021 12:53
 Operator : SY/MD
 Sample : VV0426WBL01
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VBLK172

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM042121WMA.M
 Title : VOC Analysis

Signal : TIC: VV021137.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.307	77	83	95	rVB	423193	424323	17.22%	2.174%
2	1.571	158	165	177	rVB	318129	356175	14.45%	1.825%
3	2.111	323	333	361	rVB	676045	1017493	41.29%	5.214%
4	2.442	433	436	440	rBV2	806	731	0.03%	0.004%
5	2.674	506	508	512	rVB3	481	302	0.01%	0.002%
6	2.696	512	515	517	rVB2	789	468	0.02%	0.002%
7	2.712	517	520	521	rBV	430	237	0.01%	0.001%
8	2.818	549	553	557	rVV	471	453	0.02%	0.002%
9	2.860	565	566	569	rVB	775	353	0.01%	0.002%
10	2.883	569	573	576	rBV2	316	253	0.01%	0.001%
11	2.905	576	580	585	rVB4	704	594	0.02%	0.003%
12	2.944	590	592	594	rBV	644	267	0.01%	0.001%
13	2.966	594	599	600	rBV3	345	249	0.01%	0.001%
14	3.005	606	611	615	rBV4	706	617	0.03%	0.003%
15	3.076	630	633	637	rBV	520	416	0.02%	0.002%
16	3.098	637	640	644	rVB2	1071	823	0.03%	0.004%
17	3.130	647	650	652	rBV	585	336	0.01%	0.002%
18	3.211	673	675	680	rVB3	538	389	0.02%	0.002%
19	3.233	680	682	683	rBV3	565	279	0.01%	0.001%
20	3.269	690	693	695	rBV2	655	451	0.02%	0.002%
21	3.281	695	697	700	rVV3	523	342	0.01%	0.002%
22	3.320	706	709	711	rVB2	626	335	0.01%	0.002%
23	3.359	716	721	725	rBV3	785	611	0.02%	0.003%
24	3.381	725	728	729	rBV	521	257	0.01%	0.001%
25	3.465	751	754	755	rBV2	662	308	0.01%	0.002%
26	3.503	763	766	768	rVB2	388	217	0.01%	0.001%
27	3.519	768	771	774	rBV2	702	447	0.02%	0.002%
28	3.597	792	795	796	rBV2	602	293	0.01%	0.002%
29	3.625	801	804	808	rVB3	758	473	0.02%	0.002%
30	3.648	808	811	812	rBV2	646	370	0.02%	0.002%
31	3.674	816	819	822	rVV2	632	315	0.01%	0.002%
32	3.732	835	837	839	rBV2	661	335	0.01%	0.002%
33	3.780	850	852	853	rBV2	467	233	0.01%	0.001%
34	3.896	876	888	920	rBV	122945	414983	16.84%	2.126%
35	4.349	1013	1029	1056	rBV	427883	1056957	42.89%	5.416%
36	4.613	1108	1111	1112	rBV2	741	368	0.01%	0.002%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042621\
 Data File : VV021137.D
 Acq On : 26 Apr 2021 12:53
 Operator : SY/MD
 Sample : VV0426WBL01
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VBLK172

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM042121WMA.M
 Title : VOC Analysis

37	4.709	1139	1141	1144	rVB3	627	342	0.01%	0.002%
38	4.728	1144	1147	1151	rVB3	465	342	0.01%	0.002%
39	4.770	1158	1160	1163	rBV3	640	403	0.02%	0.002%
40	4.834	1178	1180	1183	rBV	429	287	0.01%	0.001%
41	4.857	1183	1187	1190	rVV3	455	379	0.02%	0.002%
42	4.902	1197	1201	1205	rBV3	755	733	0.03%	0.004%
43	4.944	1210	1214	1216	rBV3	607	420	0.02%	0.002%
44	5.047	1229	1246	1276	rBV2	946216	2464428	100.00%	12.628%
45	5.468	1373	1377	1378	rBV2	585	449	0.02%	0.002%
46	5.529	1393	1396	1397	rVB2	671	306	0.01%	0.002%
47	5.542	1397	1400	1402	rBV2	732	399	0.02%	0.002%
48	5.561	1403	1406	1407	rBV	606	269	0.01%	0.001%
49	5.619	1412	1424	1455	rBV	794352	1612570	65.43%	8.263%
50	5.915	1504	1516	1530	rBV5	14475	30792	1.25%	0.158%
51	5.995	1539	1541	1544	rBV3	692	417	0.02%	0.002%
52	6.072	1551	1565	1586	rBV	539497	1095593	44.46%	5.614%
53	6.426	1673	1675	1679	rVB4	516	275	0.01%	0.001%
54	6.625	1734	1737	1739	rBV2	1010	734	0.03%	0.004%
55	6.738	1769	1772	1773	rBV2	452	225	0.01%	0.001%
56	6.748	1773	1775	1778	rVV3	596	353	0.01%	0.002%
57	6.796	1789	1790	1793	rVV	539	337	0.01%	0.002%
58	6.812	1793	1795	1798	rVB2	892	510	0.02%	0.003%
59	6.866	1810	1812	1816	rBV2	789	406	0.02%	0.002%
60	6.908	1821	1825	1827	rBV2	572	315	0.01%	0.002%
61	6.989	1839	1850	1876	rVV2	306658	567168	23.01%	2.906%
62	7.227	1921	1924	1925	rBV	624	304	0.01%	0.002%
63	7.320	1940	1953	1972	rBV	1169357	2035958	82.61%	10.433%
64	7.625	2038	2048	2064	rBV2	218383	384829	15.62%	1.972%
65	7.985	2156	2160	2165	rVB5	1226	1081	0.04%	0.006%
66	8.091	2183	2193	2229	rBV	513479	974481	39.54%	4.993%
67	8.857	2419	2431	2458	rBV	1213071	1985572	80.57%	10.174%
68	9.146	2518	2521	2527	rBV6	2185	2585	0.10%	0.013%
69	9.323	2573	2576	2578	rBV2	653	500	0.02%	0.003%
70	9.355	2582	2586	2588	rBV2	580	489	0.02%	0.003%
71	9.378	2591	2593	2595	rBV2	518	296	0.01%	0.002%
72	9.509	2631	2634	2636	rVB3	476	235	0.01%	0.001%
73	9.532	2638	2641	2642	rBV2	747	353	0.01%	0.002%
74	9.673	2682	2685	2688	rBV2	734	523	0.02%	0.003%
75	9.770	2712	2715	2720	rVB2	536	466	0.02%	0.002%
76	9.805	2722	2726	2730	rBV4	1136	1042	0.04%	0.005%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042621\
 Data File : VV021137.D
 Acq On : 26 Apr 2021 12:53
 Operator : SY/MD
 Sample : VV0426WBL01
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VBLK172

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM042121WMA.M
 Title : VOC Analysis

77	9.921	2759	2762	2765	rBV	1170	834	0.03%	0.004%
78	9.937	2765	2767	2770	rVB	979	541	0.02%	0.003%
79	10.130	2819	2827	2836	rBV4	6803	10119	0.41%	0.052%
80	10.178	2840	2842	2843	rBV	478	227	0.01%	0.001%
81	10.220	2843	2855	2879	rBV	780013	1227358	49.80%	6.289%
82	10.667	2988	2994	2999	rVB7	1486	1595	0.06%	0.008%
83	10.693	2999	3002	3005	rBV2	423	343	0.01%	0.002%
84	10.773	3024	3027	3030	rBV2	796	690	0.03%	0.004%
85	10.837	3043	3047	3050	rBV4	1238	957	0.04%	0.005%
86	10.898	3064	3066	3067	rBV2	943	412	0.02%	0.002%
87	10.924	3068	3074	3083	rVB6	5743	7543	0.31%	0.039%
88	11.024	3102	3105	3106	rBV2	1307	667	0.03%	0.003%
89	11.146	3139	3143	3153	rVB9	3174	4496	0.18%	0.023%
90	11.255	3165	3177	3197	rBV	1232777	1907557	77.40%	9.775%
91	11.570	3273	3275	3277	rBV	811	378	0.02%	0.002%
92	11.632	3282	3294	3317	rVV	1213062	1895284	76.91%	9.712%
93	12.336	3511	3513	3517	rBV3	755	749	0.03%	0.004%
94	12.406	3532	3535	3540	rVV5	847	740	0.03%	0.004%
95	12.529	3571	3573	3576	rBV2	740	417	0.02%	0.002%
96	12.603	3594	3596	3600	rBV5	966	832	0.03%	0.004%
97	12.741	3636	3639	3642	rBV	671	623	0.03%	0.003%
98	13.381	3835	3838	3840	rBV	1059	749	0.03%	0.004%
99	13.667	3922	3927	3931	rBV4	1216	1201	0.05%	0.006%
100	14.223	4097	4100	4105	rBV3	1637	1660	0.07%	0.009%




Sum of corrected areas: 19515191

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042621\
Data File : VV021137.D
Acq On : 26 Apr 2021 12:53
Operator : SY/MD
Sample : VV0426WBL01
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK172

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM042121WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

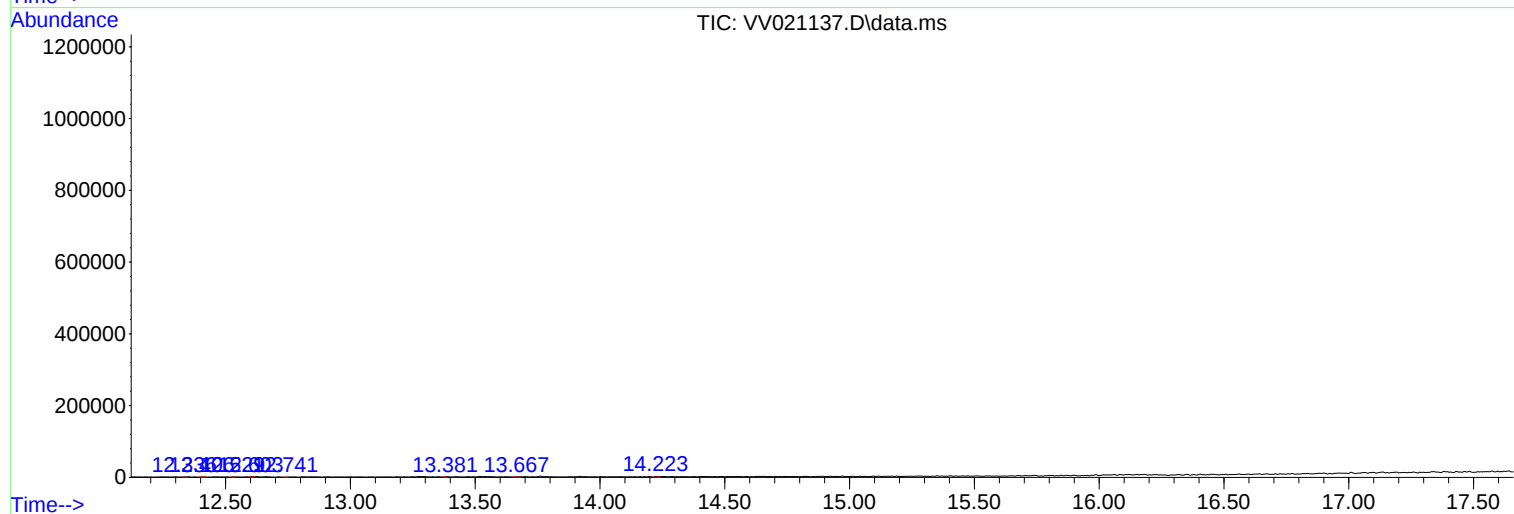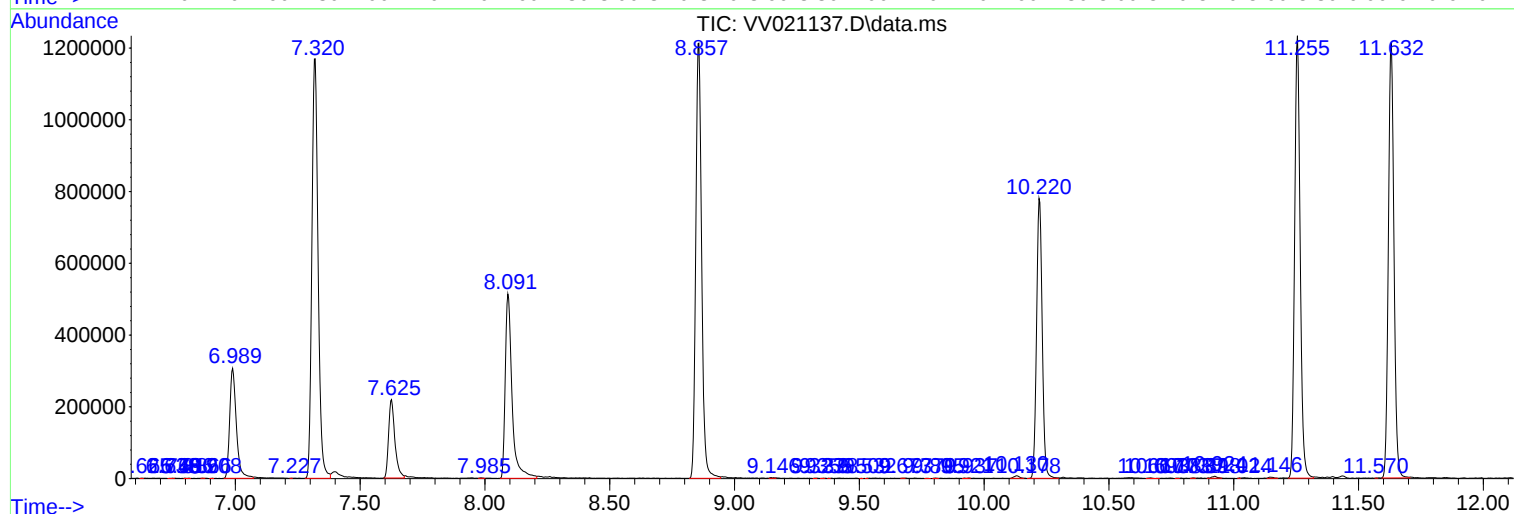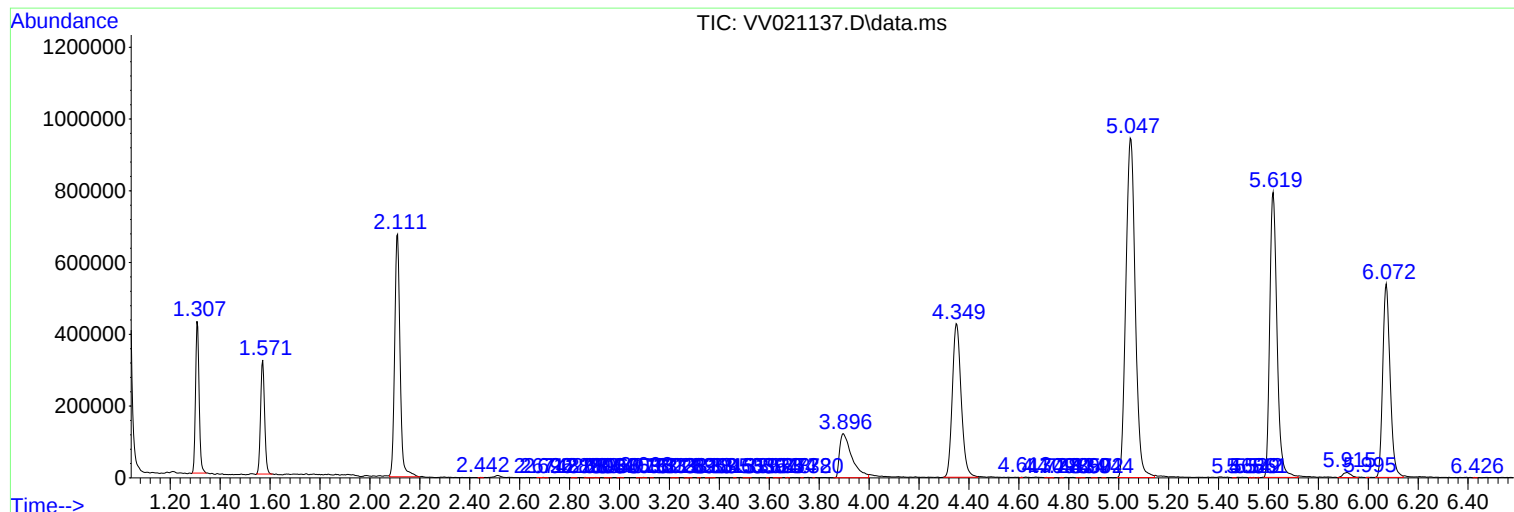

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042621\
Data File : VV021137.D
Acq On : 26 Apr 2021 12:53
Operator : SY/MD
Sample : VV0426WBL01
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK172

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM042121WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042621\
Data File : VV021137.D
Acq On : 26 Apr 2021 12:53
Operator : SY/MD
Sample : VV0426WBL01
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK172

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM042121WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
