

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042621\
 Data File : VV021138.D
 Acq On : 26 Apr 2021 13:18
 Operator : SY/MD
 Sample : M2121-21
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VHBLK002

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM042121WMA.M

Title : VOC Analysis

Signal : TIC: VV021138.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.307	77	83	100	rVB	431269	442238	17.18%	2.258%
2	1.571	158	165	180	rVB	326244	368675	14.32%	1.883%
3	2.108	323	332	356	rVB	688220	1011055	39.28%	5.163%
4	2.285	384	387	388	rBV2	1069	653	0.03%	0.003%
5	2.378	413	416	419	rBV3	506	345	0.01%	0.002%
6	2.426	428	431	433	rBV3	765	514	0.02%	0.003%
7	2.478	445	447	450	rBV2	605	480	0.02%	0.002%
8	2.510	450	457	467	rVB3	7010	11322	0.44%	0.058%
9	2.645	496	499	501	rBV2	371	218	0.01%	0.001%
10	2.725	521	524	526	rBV3	431	270	0.01%	0.001%
11	2.761	533	535	539	rBV	869	522	0.02%	0.003%
12	2.925	584	586	592	rBV2	669	629	0.02%	0.003%
13	2.953	592	595	599	rVB4	601	483	0.02%	0.002%
14	2.976	599	602	605	rBV4	470	335	0.01%	0.002%
15	3.008	609	612	614	rBV3	748	470	0.02%	0.002%
16	3.047	620	624	627	rVB3	828	617	0.02%	0.003%
17	3.108	637	643	645	rVB2	739	655	0.03%	0.003%
18	3.121	645	647	649	rBV	447	242	0.01%	0.001%
19	3.130	649	650	654	rVB	472	307	0.01%	0.002%
20	3.191	664	669	673	rVB3	510	446	0.02%	0.002%
21	3.269	689	693	696	rBV2	1212	806	0.03%	0.004%
22	3.394	729	732	736	rVB	911	520	0.02%	0.003%
23	3.449	746	749	752	rBV2	431	358	0.01%	0.002%
24	3.503	763	766	768	rBV2	812	609	0.02%	0.003%
25	3.587	789	792	794	rVB2	617	257	0.01%	0.001%
26	3.603	794	797	801	rBV	540	428	0.02%	0.002%
27	3.635	801	807	812	rBV5	547	587	0.02%	0.003%
28	3.658	812	814	816	rBV2	662	398	0.02%	0.002%
29	3.690	822	824	825	rBV2	631	232	0.01%	0.001%
30	3.799	857	858	862	rVB2	392	241	0.01%	0.001%
31	3.857	873	876	878	rBV2	601	415	0.02%	0.002%
32	3.896	878	888	928	rBV2	129400	461529	17.93%	2.357%
33	4.352	1014	1030	1059	rBV2	442690	1095949	42.58%	5.597%
34	4.712	1140	1142	1144	rBV2	452	224	0.01%	0.001%
35	4.812	1169	1173	1177	rVB2	927	818	0.03%	0.004%
36	4.834	1177	1180	1181	rBV2	740	383	0.01%	0.002%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW042621\
 Data File : VW021138.D
 Acq On : 26 Apr 2021 13:18
 Operator : SY/MD
 Sample : M2121-21
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VHBLK002

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM042121WMA.M
 Title : VOC Analysis

37	4.905	1200	1202	1204	rBV	421	229	0.01%	0.001%
38	4.953	1214	1217	1220	rBV2	734	415	0.02%	0.002%
39	5.050	1230	1247	1277	rBV3	998475	2573818	100.00%	13.143%
40	5.442	1365	1369	1372	rBV5	978	668	0.03%	0.003%
41	5.484	1380	1382	1384	rBV3	911	608	0.02%	0.003%
42	5.619	1412	1424	1455	rBV	721350	1459132	56.69%	7.451%
43	6.024	1547	1550	1551	rBV2	796	479	0.02%	0.002%
44	6.072	1552	1565	1590	rVV	555939	1138341	44.23%	5.813%
45	6.323	1640	1643	1646	rVB3	1114	653	0.03%	0.003%
46	6.403	1666	1668	1672	rBV3	354	218	0.01%	0.001%
47	6.497	1693	1697	1698	rBV3	943	534	0.02%	0.003%
48	6.548	1711	1713	1716	rBV2	523	385	0.01%	0.002%
49	6.593	1725	1727	1732	rVB4	877	729	0.03%	0.004%
50	6.619	1732	1735	1736	rBV2	449	236	0.01%	0.001%
51	6.629	1736	1738	1742	rVV2	621	503	0.02%	0.003%
52	6.722	1764	1767	1769	rBV2	919	637	0.02%	0.003%
53	6.786	1785	1787	1790	rVB2	523	226	0.01%	0.001%
54	6.805	1791	1793	1799	rVB3	600	497	0.02%	0.003%
55	6.831	1799	1801	1803	rBV2	636	403	0.02%	0.002%
56	6.883	1814	1817	1819	rBV4	726	469	0.02%	0.002%
57	6.934	1831	1833	1836	rVB2	589	236	0.01%	0.001%
58	6.989	1839	1850	1879	rBV	316926	592878	23.03%	3.028%
59	7.320	1941	1953	1970	rBV	1221627	2095899	81.43%	10.703%
60	7.625	2038	2048	2071	rBV	234566	410741	15.96%	2.097%
61	7.825	2109	2110	2114	rVB3	1062	616	0.02%	0.003%
62	7.866	2114	2123	2128	rBV6	1593	2284	0.09%	0.012%
63	7.934	2139	2144	2147	rBV3	1405	1346	0.05%	0.007%
64	7.989	2157	2161	2162	rBV3	1074	869	0.03%	0.004%
65	8.014	2167	2169	2173	rVB2	786	471	0.02%	0.002%
66	8.034	2173	2175	2178	rVB	898	501	0.02%	0.003%
67	8.095	2183	2194	2220	rBV	593999	1089821	42.34%	5.565%
68	8.577	2341	2344	2347	rBV2	643	588	0.02%	0.003%
69	8.648	2364	2366	2368	rBV2	715	386	0.01%	0.002%
70	8.718	2386	2388	2390	rVB2	524	258	0.01%	0.001%
71	8.802	2411	2414	2417	rVB3	1000	537	0.02%	0.003%
72	8.857	2419	2431	2458	rBV	1108182	1800331	69.95%	9.193%
73	9.114	2509	2511	2514	rBV3	766	404	0.02%	0.002%
74	9.188	2532	2534	2537	rVB4	953	436	0.02%	0.002%
75	9.294	2564	2567	2569	rBV	956	596	0.02%	0.003%
76	9.612	2663	2666	2670	rBV2	398	328	0.01%	0.002%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW042621\
 Data File : VW021138.D
 Acq On : 26 Apr 2021 13:18
 Operator : SY/MD
 Sample : M2121-21
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VHBLK002

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM042121WMA.M
 Title : VOC Analysis

77	9.860	2741	2743	2747	rVB2	805	385	0.01%	0.002%
78	9.882	2747	2750	2751	rBV	554	332	0.01%	0.002%
79	9.911	2757	2759	2760	rBV	559	235	0.01%	0.001%
80	9.989	2777	2783	2786	rBV2	920	1082	0.04%	0.006%
81	10.037	2792	2798	2801	rBV4	639	770	0.03%	0.004%
82	10.130	2822	2827	2837	rVB3	7570	9164	0.36%	0.047%
83	10.220	2843	2855	2877	rBV	842129	1336837	51.94%	6.827%
84	10.815	3038	3040	3043	rBV	808	501	0.02%	0.003%
85	10.886	3058	3062	3064	rBV3	1058	883	0.03%	0.005%
86	11.120	3131	3135	3138	rBV2	891	789	0.03%	0.004%
87	11.149	3139	3144	3147	rBV2	3091	3261	0.13%	0.017%
88	11.255	3166	3177	3196	rBV	1100014	1693840	65.81%	8.650%
89	11.632	3282	3294	3314	rBV	1231272	1942611	75.48%	9.920%
90	11.831	3353	3356	3359	rBV5	1470	1052	0.04%	0.005%
91	11.992	3404	3406	3410	rVB3	1183	735	0.03%	0.004%
92	12.017	3410	3414	3417	rBV4	998	785	0.03%	0.004%
93	12.590	3589	3592	3600	rBV6	1201	1699	0.07%	0.009%
94	12.886	3682	3684	3687	rBV2	1217	807	0.03%	0.004%
95	12.947	3700	3703	3705	rBV	933	488	0.02%	0.002%
96	13.056	3734	3737	3740	rVB2	1124	706	0.03%	0.004%
97	13.185	3774	3777	3780	rBV2	554	318	0.01%	0.002%
98	13.416	3847	3849	3852	rBV2	1137	632	0.02%	0.003%
99	13.831	3973	3978	3981	rBV2	1122	1028	0.04%	0.005%
100	13.959	4015	4018	4020	rBV2	1236	822	0.03%	0.004%




Sum of corrected areas: 19582698

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042621\
Data File : VV021138.D
Acq On : 26 Apr 2021 13:18
Operator : SY/MD
Sample : M2121-21
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 5 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VHBLK002

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM042121WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

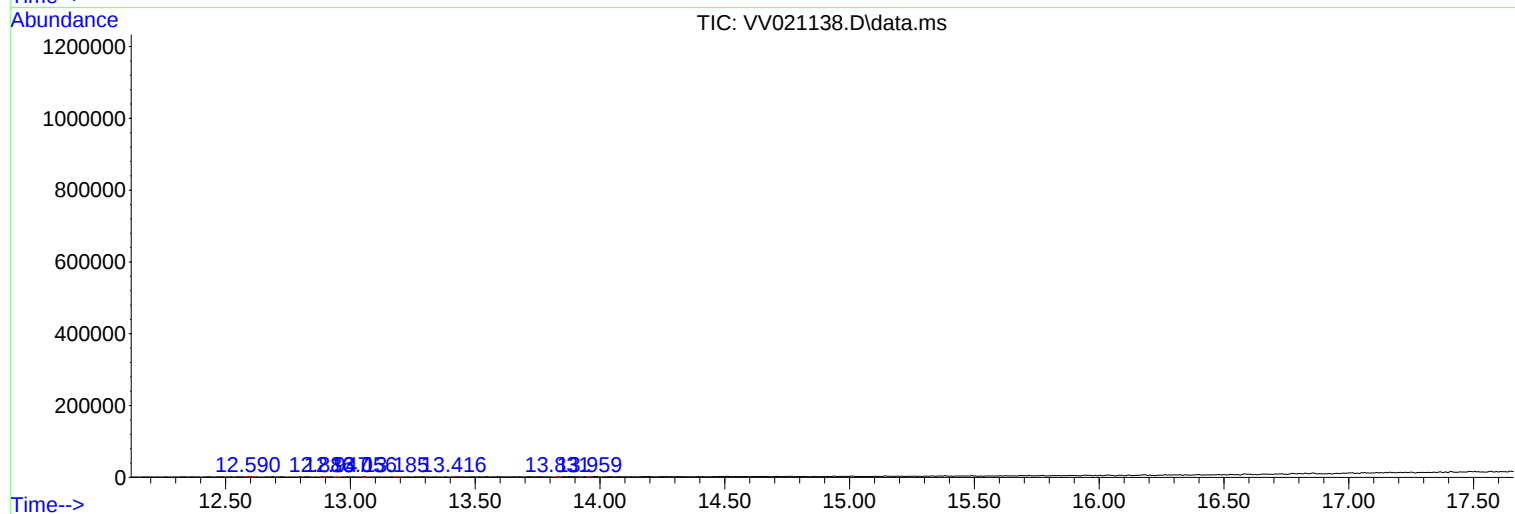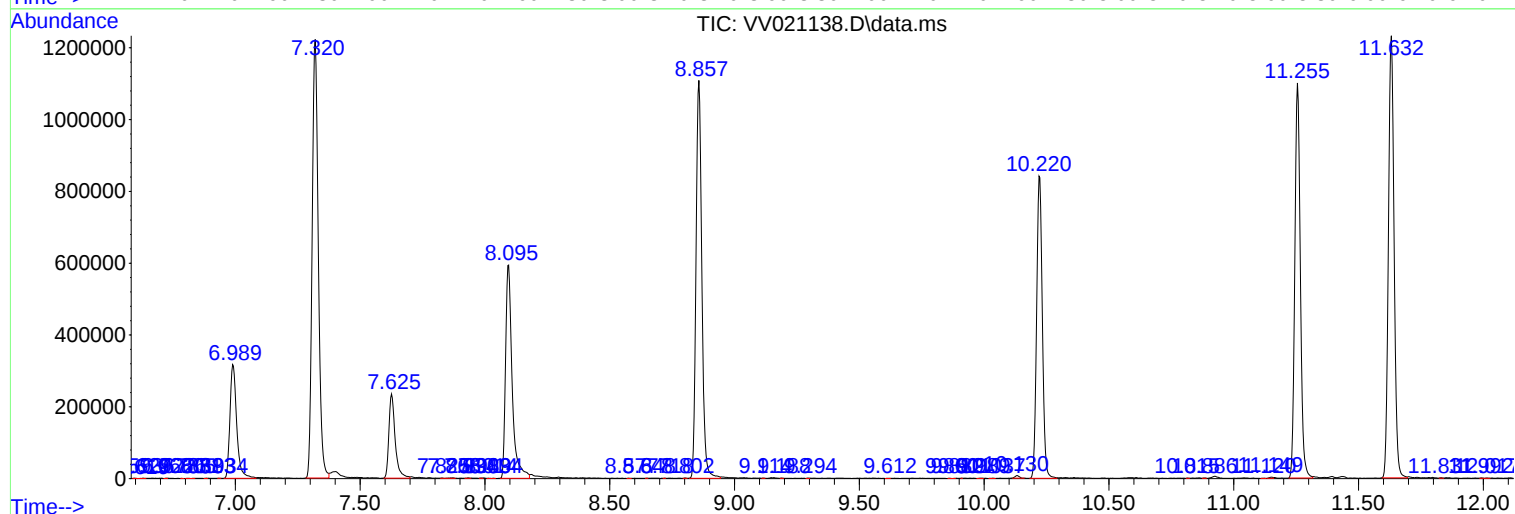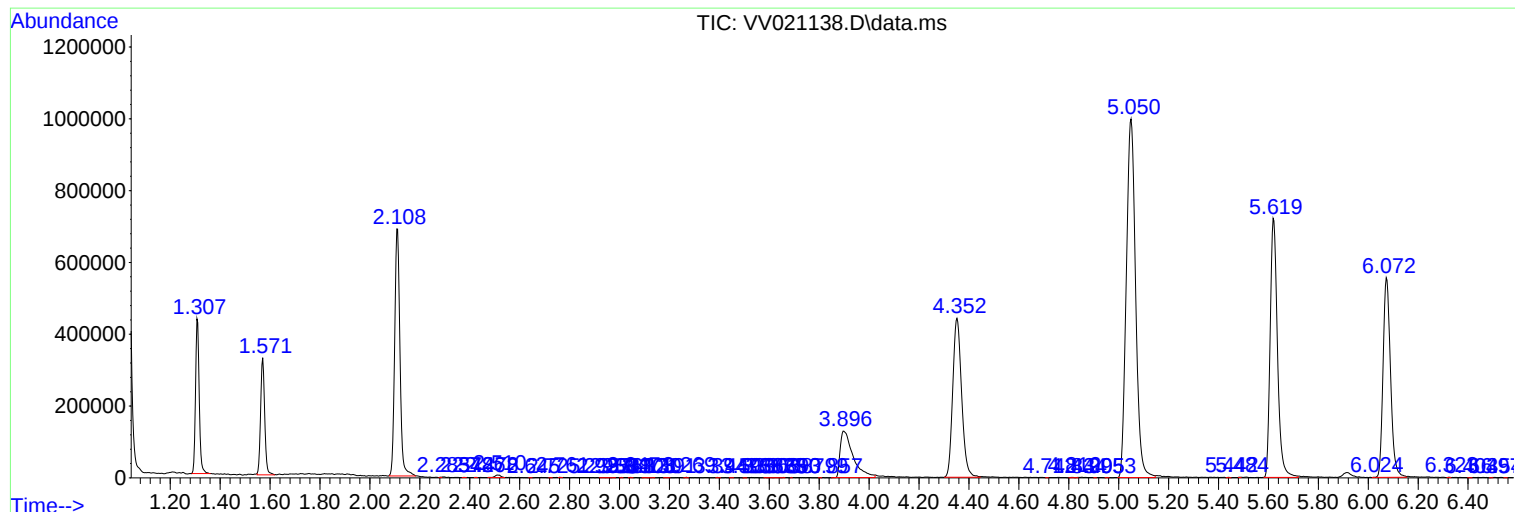

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042621\
Data File : VV021138.D
Acq On : 26 Apr 2021 13:18
Operator : SY/MD
Sample : M2121-21
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 5 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VHBLK002

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM042121WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042621\
Data File : VV021138.D
Acq On : 26 Apr 2021 13:18
Operator : SY/MD
Sample : M2121-21
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 5 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VHBLK002

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM042121WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
