

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042621\
 Data File : VV021139.D
 Acq On : 26 Apr 2021 13:41
 Operator : SY/MD
 Sample : M2123-06DL 40X
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BG7A6DL

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM042121WMA.M

Title : VOC Analysis

Signal : TIC: VV021139.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.310	77	84	97	rBV	312659	326616	13.70%	1.592%
2	1.571	158	165	181	rVB	267386	306204	12.84%	1.493%
3	2.111	323	333	366	rVB	542385	830949	34.85%	4.051%
4	2.352	406	408	412	rBV3	646	425	0.02%	0.002%
5	2.471	442	445	449	rBV4	1082	806	0.03%	0.004%
6	2.513	450	458	471	rVB5	8886	15533	0.65%	0.076%
7	2.606	485	487	488	rBV2	530	269	0.01%	0.001%
8	2.642	495	498	500	rBV2	483	333	0.01%	0.002%
9	2.738	527	528	529	rBV	392	99	0.00%	0.000%
10	2.767	529	537	547	rVV3	8429	15828	0.66%	0.077%
11	2.934	585	589	590	rBV2	436	264	0.01%	0.001%
12	2.947	590	593	594	rBV	823	392	0.02%	0.002%
13	3.098	638	640	645	rVB3	735	523	0.02%	0.003%
14	3.124	645	648	651	rBV	810	457	0.02%	0.002%
15	3.137	651	652	654	rBV	341	124	0.01%	0.001%
16	3.259	688	690	691	rBV	281	91	0.00%	0.000%
17	3.326	709	711	713	rBV	487	212	0.01%	0.001%
18	3.352	717	719	722	rVB2	451	237	0.01%	0.001%
19	3.461	748	753	754	rBV3	595	475	0.02%	0.002%
20	3.516	768	770	773	rVB	441	149	0.01%	0.001%
21	3.545	776	779	782	rVB2	450	233	0.01%	0.001%
22	3.568	782	786	790	rBV3	1076	1083	0.05%	0.005%
23	3.596	793	795	797	rBV2	318	209	0.01%	0.001%
24	3.625	802	804	805	rBV	452	204	0.01%	0.001%
25	3.658	812	814	817	rBV	437	225	0.01%	0.001%
26	3.677	817	820	825	rVB3	922	475	0.02%	0.002%
27	3.706	825	829	833	rVB3	828	685	0.03%	0.003%
28	3.735	835	838	840	rBV2	591	389	0.02%	0.002%
29	3.764	843	847	850	rVB2	495	395	0.02%	0.002%
30	3.783	850	853	855	rBV	367	187	0.01%	0.001%
31	3.799	855	858	860	rBV3	596	395	0.02%	0.002%
32	3.915	878	894	919	rBV3	612058	1714940	71.93%	8.361%
33	4.352	1015	1030	1056	rBV	431026	1043136	43.75%	5.086%
34	4.825	1176	1177	1179	rBV2	1047	446	0.02%	0.002%
35	4.850	1182	1185	1190	rVB2	1148	799	0.03%	0.004%
36	4.876	1190	1193	1198	rBV4	889	908	0.04%	0.004%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW042621\
 Data File : VW021139.D
 Acq On : 26 Apr 2021 13:41
 Operator : SY/MD
 Sample : M2123-06DL 40X
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BG7A6DL

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM042121WMA.M
 Title : VOC Analysis

37	4.902	1199	1201	1205	rVV2	856	390	0.02%	0.002%
38	4.950	1214	1216	1217	rBV	641	256	0.01%	0.001%
39	4.979	1224	1225	1227	rBV	396	171	0.01%	0.001%
40	5.050	1230	1247	1279	rBV2	909405	2384175	100.00%	11.624%
41	5.526	1393	1395	1397	rBV2	730	318	0.01%	0.002%
42	5.574	1408	1410	1412	rBV3	632	269	0.01%	0.001%
43	5.622	1412	1425	1451	rBV	823728	1653603	69.36%	8.062%
44	5.918	1508	1517	1530	rVB4	12232	26183	1.10%	0.128%
45	6.075	1552	1566	1595	rBV	530161	1089102	45.68%	5.310%
46	6.326	1641	1644	1646	rBV2	726	468	0.02%	0.002%
47	6.429	1672	1676	1681	rBV4	1203	1198	0.05%	0.006%
48	6.461	1683	1686	1688	rVV3	655	352	0.01%	0.002%
49	6.577	1719	1722	1725	rBV3	982	644	0.03%	0.003%
50	6.841	1801	1804	1805	rBV2	565	252	0.01%	0.001%
51	6.886	1816	1818	1819	rBV	332	119	0.00%	0.001%
52	6.934	1830	1833	1834	rBV	399	220	0.01%	0.001%
53	6.989	1840	1850	1871	rBV	295564	543629	22.80%	2.650%
54	7.320	1941	1953	1972	rBV	1058646	1836618	77.03%	8.954%
55	7.625	2038	2048	2071	rBV2	213164	376617	15.80%	1.836%
56	7.844	2113	2116	2118	rBV3	1241	954	0.04%	0.005%
57	7.882	2126	2128	2130	rVB3	681	212	0.01%	0.001%
58	7.895	2130	2132	2133	rVB2	714	199	0.01%	0.001%
59	7.944	2142	2147	2148	rBV2	950	723	0.03%	0.004%
60	7.963	2151	2153	2156	rBV2	725	474	0.02%	0.002%
61	8.095	2182	2194	2228	rBV	632352	1172468	49.18%	5.716%
62	8.606	2350	2353	2356	rBV3	971	477	0.02%	0.002%
63	8.686	2377	2378	2384	rBV3	722	565	0.02%	0.003%
64	8.812	2415	2417	2419	rBV2	459	258	0.01%	0.001%
65	8.857	2419	2431	2461	rBV	1245685	2029953	85.14%	9.897%
66	9.223	2542	2545	2547	rBV2	837	533	0.02%	0.003%
67	9.278	2560	2562	2563	rBV	932	376	0.02%	0.002%
68	9.413	2601	2604	2606	rBV4	1235	687	0.03%	0.003%
69	9.464	2617	2620	2623	rVB2	845	504	0.02%	0.002%
70	9.490	2625	2628	2630	rBV2	570	382	0.02%	0.002%
71	9.603	2661	2663	2666	rBV2	946	471	0.02%	0.002%
72	9.689	2687	2690	2693	rBV3	605	427	0.02%	0.002%
73	9.757	2709	2711	2712	rBV	600	199	0.01%	0.001%
74	10.014	2788	2791	2793	rBV2	697	347	0.01%	0.002%
75	10.095	2814	2816	2820	rBV2	607	440	0.02%	0.002%
76	10.133	2820	2828	2834	rVB6	3046	4255	0.18%	0.021%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042621\
 Data File : VV021139.D
 Acq On : 26 Apr 2021 13:41
 Operator : SY/MD
 Sample : M2123-06DL 40X
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BG7A6DL

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM042121WMA.M

Title : VOC Analysis

77	10.223	2843	2856	2875	rBV	866066	1358721	56.99%	6.624%
78	10.413	2912	2915	2917	rBV3	1048	547	0.02%	0.003%
79	10.542	2952	2955	2957	rBV	771	616	0.03%	0.003%
80	10.654	2987	2990	2991	rBV	614	335	0.01%	0.002%
81	10.712	3006	3008	3014	rBV3	717	847	0.04%	0.004%
82	10.857	3051	3053	3057	rBV3	897	682	0.03%	0.003%
83	10.924	3067	3074	3083	rBV9	3986	5647	0.24%	0.028%
84	11.033	3105	3108	3109	rBV2	733	437	0.02%	0.002%
85	11.152	3140	3145	3146	rBV3	1549	1137	0.05%	0.006%
86	11.188	3154	3156	3157	rBV	997	396	0.02%	0.002%
87	11.255	3166	3177	3203	rBV	1232678	1886873	79.14%	9.199%
88	11.632	3281	3294	3314	rBV	1172116	1853677	77.75%	9.037%
89	11.821	3350	3353	3354	rBV	917	502	0.02%	0.002%
90	11.879	3368	3371	3374	rVB3	891	423	0.02%	0.002%
91	11.947	3389	3392	3400	rVB5	1264	1257	0.05%	0.006%
92	12.278	3493	3495	3499	rVB2	1109	611	0.03%	0.003%
93	12.365	3520	3522	3525	rVB3	1435	676	0.03%	0.003%
94	12.866	3676	3678	3681	rBV2	618	363	0.02%	0.002%
95	12.889	3681	3685	3688	rBV3	492	502	0.02%	0.002%
96	13.188	3775	3778	3779	rBV2	662	427	0.02%	0.002%
97	13.249	3795	3797	3798	rBV2	487	203	0.01%	0.001%
98	13.278	3804	3806	3812	rBV4	1156	1074	0.05%	0.005%
99	13.676	3927	3930	3932	rBV2	923	733	0.03%	0.004%
100	13.992	4026	4028	4030	rBV	640	334	0.01%	0.002%



Sum of corrected areas: 20511203

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042621\
Data File : VV021139.D
Acq On : 26 Apr 2021 13:41
Operator : SY/MD
Sample : M2123-06DL 40X
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 6 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BG7A6DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM042121WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

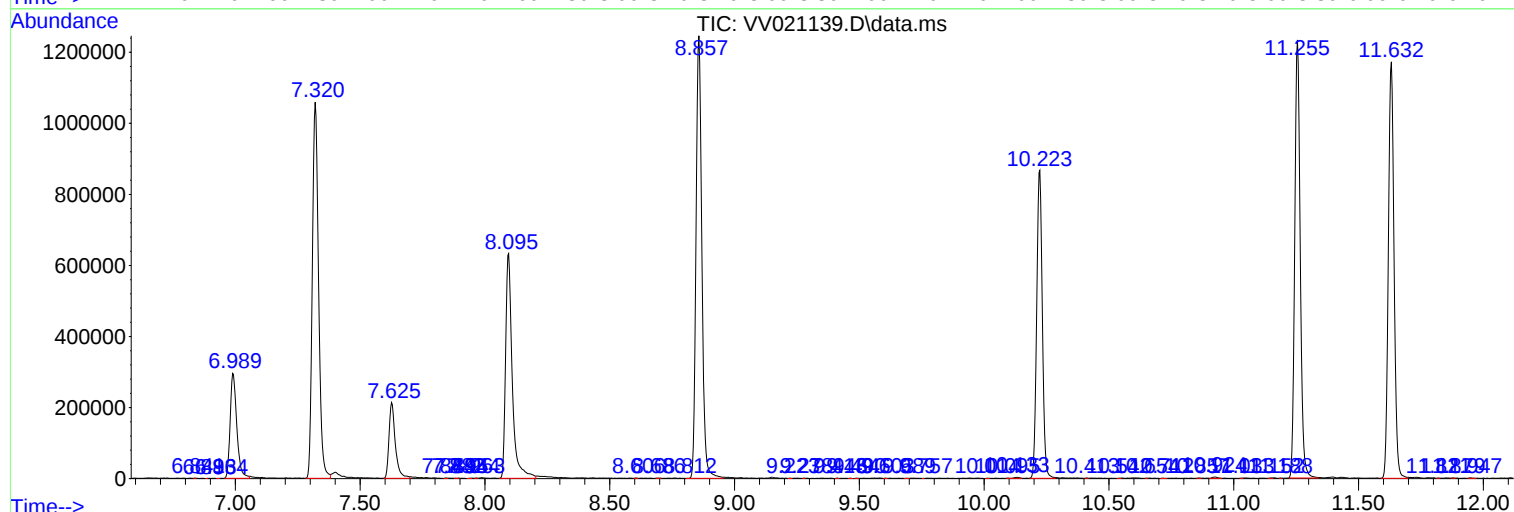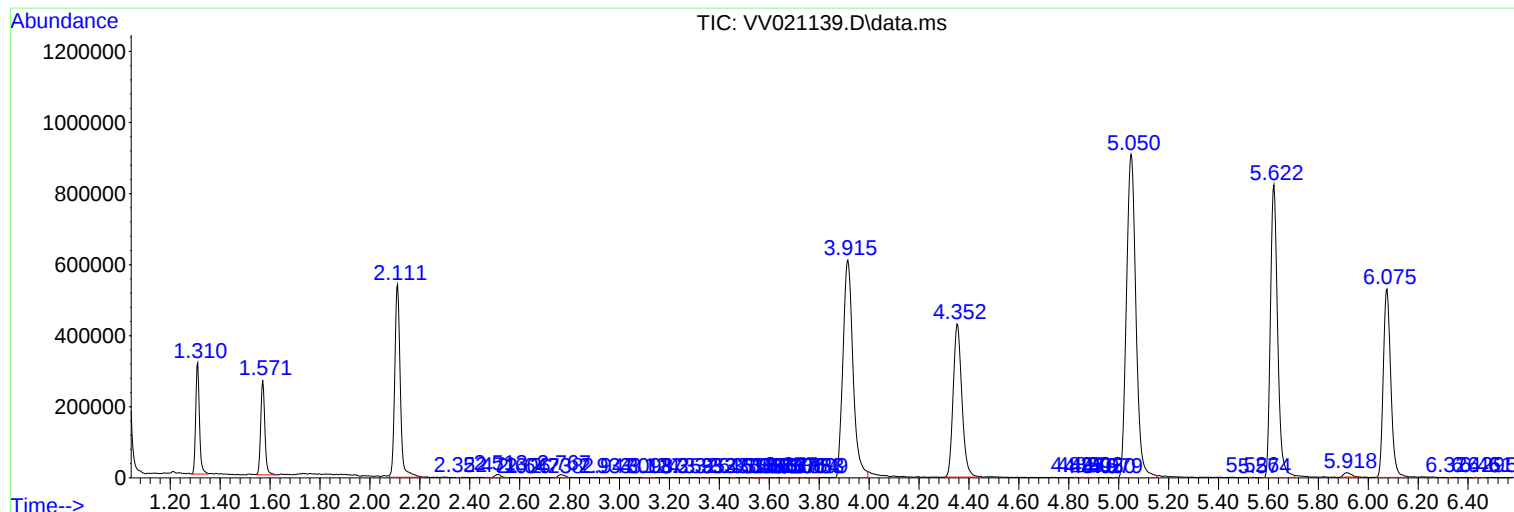

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042621\
Data File : VV021139.D
Acq On : 26 Apr 2021 13:41
Operator : SY/MD
Sample : M2123-06DL 40X
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 6 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BG7A6DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM042121WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042621\
Data File : VV021139.D
Acq On : 26 Apr 2021 13:41
Operator : SY/MD
Sample : M2123-06DL 40X
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 6 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BG7A6DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM042121WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
