

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW042621\
 Data File : VW021143.D
 Acq On : 26 Apr 2021 15:15
 Operator : SY/MD
 Sample : M2326-03
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BG7C0

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM042121WMA.M
 Title : VOC Analysis

Signal : TIC: VW021143.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.217	51	55	65	rVB	72727	64695	3.00%	0.364%
2	1.307	77	83	95	rBV	303786	316140	14.66%	1.780%
3	1.571	159	165	178	rVB	266099	298225	13.83%	1.679%
4	2.111	323	333	350	rBV	551347	802168	37.21%	4.516%
5	2.442	430	436	439	rBV5	1412	1764	0.08%	0.010%
6	2.722	520	523	527	rBV4	809	791	0.04%	0.004%
7	2.760	530	535	538	rBV7	2120	2352	0.11%	0.013%
8	2.912	580	582	583	rBV	405	151	0.01%	0.001%
9	2.940	589	591	592	rBV	451	148	0.01%	0.001%
10	3.011	611	613	615	rBV	1152	736	0.03%	0.004%
11	3.124	644	648	649	rBV2	785	561	0.03%	0.003%
12	3.236	681	683	685	rBV2	428	277	0.01%	0.002%
13	3.249	685	687	691	rVB3	854	493	0.02%	0.003%
14	3.268	691	693	694	rBV2	412	182	0.01%	0.001%
15	3.288	697	699	703	rBV2	248	189	0.01%	0.001%
16	3.307	703	705	707	rBV	444	261	0.01%	0.001%
17	3.336	712	714	716	rBV2	597	393	0.02%	0.002%
18	3.365	720	723	726	rBV2	659	445	0.02%	0.003%
19	3.384	727	729	733	rVB2	572	363	0.02%	0.002%
20	3.426	740	742	743	rBV2	422	223	0.01%	0.001%
21	3.436	743	745	748	rVB	492	144	0.01%	0.001%
22	3.481	756	759	761	rBV2	516	348	0.02%	0.002%
23	3.567	782	786	788	rBV2	463	351	0.02%	0.002%
24	3.584	788	791	793	rVV	507	397	0.02%	0.002%
25	3.609	797	799	801	rBV	396	218	0.01%	0.001%
26	3.703	824	828	832	rVB4	835	786	0.04%	0.004%
27	3.908	880	892	926	rBV	136138	502572	23.31%	2.829%
28	4.352	1014	1030	1063	rBV	384277	963595	44.69%	5.425%
29	4.744	1150	1152	1155	rVB3	760	323	0.01%	0.002%
30	4.764	1156	1158	1159	rBV3	450	166	0.01%	0.001%
31	4.789	1164	1166	1170	rVB2	859	405	0.02%	0.002%
32	4.809	1170	1172	1174	rBV	431	207	0.01%	0.001%
33	4.834	1174	1180	1183	rBV3	1071	957	0.04%	0.005%
34	4.982	1223	1226	1229	rVB4	992	775	0.04%	0.004%
35	5.050	1229	1247	1280	rBV4	828948	2155992	100.00%	12.137%
36	5.349	1338	1340	1344	rVB3	952	533	0.02%	0.003%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW042621\
 Data File : VW021143.D
 Acq On : 26 Apr 2021 15:15
 Operator : SY/MD
 Sample : M2326-03
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BG7C0

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM042121WMA.M
 Title : VOC Analysis

37	5.574	1408	1410	1412	rBV3	721	306	0.01%	0.002%
38	5.622	1412	1425	1449	rBV	769704	1573464	72.98%	8.858%
39	5.911	1507	1515	1531	rVB4	26907	52839	2.45%	0.297%
40	6.075	1552	1566	1592	rBV	480703	981680	45.53%	5.526%
41	6.329	1640	1645	1648	rBV6	1393	1221	0.06%	0.007%
42	6.426	1673	1675	1678	rVB3	466	176	0.01%	0.001%
43	6.455	1682	1684	1686	rBV2	792	430	0.02%	0.002%
44	6.509	1699	1701	1704	rVB2	726	308	0.01%	0.002%
45	6.532	1704	1708	1710	rBV3	850	623	0.03%	0.004%
46	6.603	1728	1730	1732	rBV	414	217	0.01%	0.001%
47	6.648	1740	1744	1746	rBV3	801	742	0.03%	0.004%
48	6.789	1785	1788	1793	rBV5	814	835	0.04%	0.005%
49	6.854	1806	1808	1810	rBV	478	248	0.01%	0.001%
50	6.908	1822	1825	1830	rBV4	1047	977	0.05%	0.006%
51	6.937	1832	1834	1837	rBV2	416	180	0.01%	0.001%
52	6.989	1840	1850	1880	rBV	263550	487949	22.63%	2.747%
53	7.246	1925	1930	1935	rVB5	1114	1234	0.06%	0.007%
54	7.271	1935	1938	1941	rBV5	1054	789	0.04%	0.004%
55	7.320	1941	1953	1972	rBV	943924	1646408	76.36%	9.268%
56	7.577	2030	2033	2035	rVB3	1202	617	0.03%	0.003%
57	7.628	2038	2049	2072	rBV	184445	332263	15.41%	1.870%
58	7.825	2108	2110	2113	rBV2	819	408	0.02%	0.002%
59	8.050	2178	2180	2183	rBV2	543	242	0.01%	0.001%
60	8.095	2183	2194	2234	rBV	547522	1047613	48.59%	5.898%
61	8.493	2315	2318	2322	rBV2	1141	875	0.04%	0.005%
62	8.599	2347	2351	2354	rBV4	1218	1119	0.05%	0.006%
63	8.744	2394	2396	2400	rBV2	655	410	0.02%	0.002%
64	8.857	2418	2431	2456	rBV	1184317	1925952	89.33%	10.842%
65	9.101	2502	2507	2509	rBV2	831	673	0.03%	0.004%
66	9.220	2541	2544	2550	rBV6	792	894	0.04%	0.005%
67	9.259	2555	2556	2558	rBV2	517	257	0.01%	0.001%
68	9.358	2585	2587	2590	rVB2	746	352	0.02%	0.002%
69	9.384	2593	2595	2598	rBV3	682	501	0.02%	0.003%
70	9.439	2610	2612	2613	rBV	466	149	0.01%	0.001%
71	9.484	2622	2626	2629	rVV2	641	573	0.03%	0.003%
72	9.532	2638	2641	2643	rBV2	641	329	0.02%	0.002%
73	9.564	2649	2651	2655	rBV3	820	563	0.03%	0.003%
74	9.664	2680	2682	2685	rBV2	938	442	0.02%	0.002%
75	9.818	2727	2730	2732	rBV	783	505	0.02%	0.003%
76	9.889	2750	2752	2760	rVB3	835	596	0.03%	0.003%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042621\
 Data File : VV021143.D
 Acq On : 26 Apr 2021 15:15
 Operator : SY/MD
 Sample : M2326-03
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BG7C0

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM042121WMA.M
 Title : VOC Analysis

77	10.085	2808	2813	2817	rBV2	955	1091	0.05%	0.006%
78	10.130	2822	2827	2832	rVB5	2807	3008	0.14%	0.017%
79	10.223	2844	2856	2877	rBV	732375	1162476	53.92%	6.544%
80	10.368	2898	2901	2903	rBV2	1252	862	0.04%	0.005%
81	10.529	2948	2951	2953	rBV2	887	510	0.02%	0.003%
82	10.545	2953	2956	2958	rBV	962	589	0.03%	0.003%
83	10.712	3005	3008	3011	rVB	844	487	0.02%	0.003%
84	10.853	3049	3052	3053	rBV2	601	311	0.01%	0.002%
85	10.886	3058	3062	3067	rVB4	1245	1172	0.05%	0.007%
86	10.924	3067	3074	3082	rBV8	3185	4462	0.21%	0.025%
87	11.107	3127	3131	3134	rBV4	907	536	0.02%	0.003%
88	11.255	3165	3177	3199	rBV	1139926	1766556	81.94%	9.945%
89	11.631	3278	3294	3315	rBV	1046231	1629190	75.57%	9.172%
90	12.021	3407	3415	3417	rBV3	1093	1208	0.06%	0.007%
91	12.082	3432	3434	3435	rBV3	538	171	0.01%	0.001%
92	12.111	3441	3443	3447	rBV3	867	573	0.03%	0.003%
93	12.361	3518	3521	3523	rBV4	1297	718	0.03%	0.004%
94	12.496	3561	3563	3566	rBV2	780	493	0.02%	0.003%
95	13.123	3756	3758	3762	rBV3	791	599	0.03%	0.003%
96	13.168	3768	3772	3773	rBV2	803	510	0.02%	0.003%
97	13.178	3773	3775	3781	rVB3	1197	1150	0.05%	0.006%
98	13.210	3781	3785	3786	rBV2	1012	705	0.03%	0.004%
99	13.246	3792	3796	3798	rBV	1010	745	0.03%	0.004%
100	13.844	3979	3982	3988	rBV4	1088	1189	0.06%	0.007%




Sum of corrected areas: 17763596

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042621\
Data File : VV021143.D
Acq On : 26 Apr 2021 15:15
Operator : SY/MD
Sample : M2326-03
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 10 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BG7C0

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM042121WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

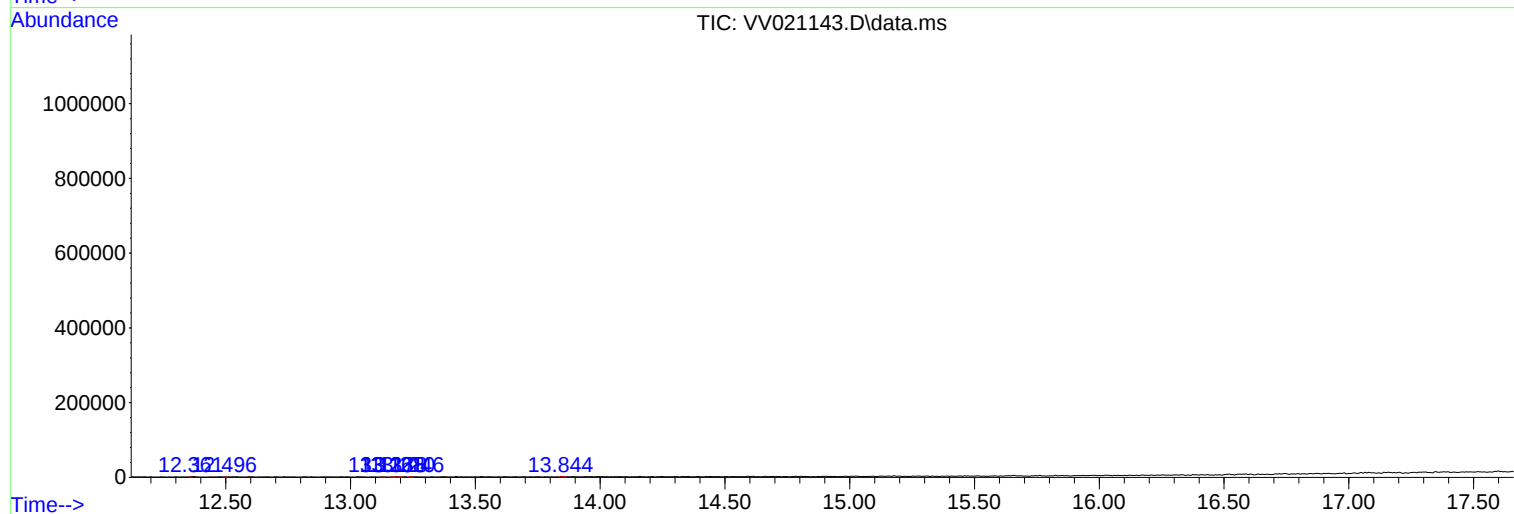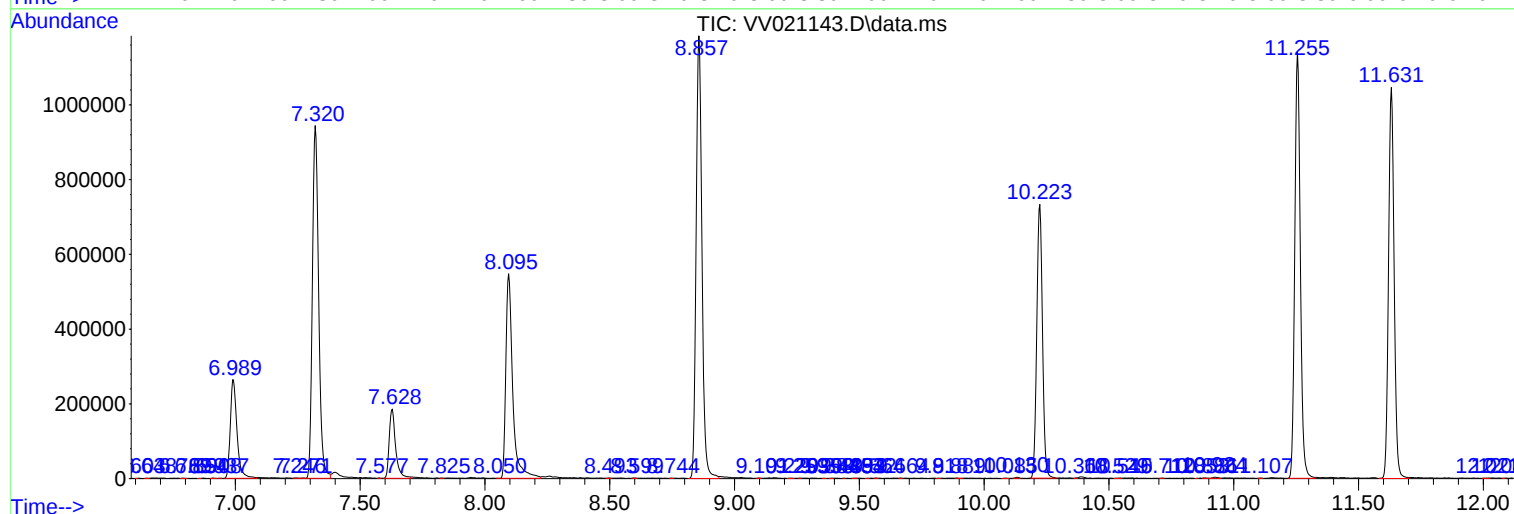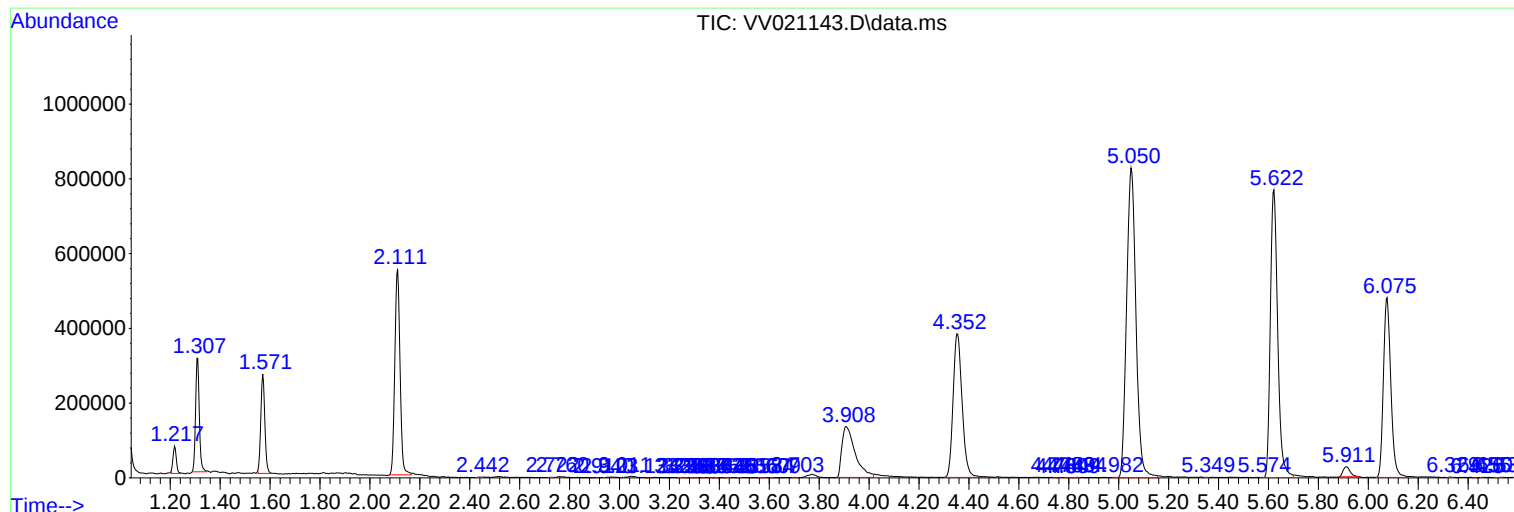

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042621\
Data File : VV021143.D
Acq On : 26 Apr 2021 15:15
Operator : SY/MD
Sample : M2326-03
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 10 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BG7C0

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM042121WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042621\
Data File : VV021143.D
Acq On : 26 Apr 2021 15:15
Operator : SY/MD
Sample : M2326-03
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 10 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BG7C0

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM042121WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
