

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042621\
 Data File : VV021144.D
 Acq On : 26 Apr 2021 15:38
 Operator : SY/MD
 Sample : M2326-04
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BG7C6

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM042121WMA.M
 Title : VOC Analysis

Signal : TIC: VV021144.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.217	50	55	67	rVB	72011	67504	3.15%	0.383%
2	1.310	78	84	101	rVB	293666	307681	14.38%	1.744%
3	1.571	158	165	177	rVB	254986	284294	13.29%	1.612%
4	2.111	324	333	347	rBV	532733	761838	35.60%	4.319%
5	3.050	616	625	634	rBV6	5198	9280	0.43%	0.053%
6	3.137	650	652	654	rBV	596	255	0.01%	0.001%
7	3.214	674	676	679	rBV2	698	401	0.02%	0.002%
8	3.294	699	701	704	rBV	436	287	0.01%	0.002%
9	3.317	704	708	713	rVV3	583	600	0.03%	0.003%
10	3.371	723	725	729	rVB2	593	452	0.02%	0.003%
11	3.416	738	739	740	rBV2	351	103	0.00%	0.001%
12	3.465	751	754	755	rBV2	604	328	0.02%	0.002%
13	3.523	770	772	774	rVB2	441	164	0.01%	0.001%
14	3.561	781	784	785	rBV	380	227	0.01%	0.001%
15	3.584	789	791	792	rBV	256	87	0.00%	0.000%
16	3.613	798	800	802	rBV2	761	497	0.02%	0.003%
17	3.773	835	850	864	rBV7	9218	25186	1.18%	0.143%
18	3.857	874	876	878	rBV2	802	460	0.02%	0.003%
19	3.902	879	890	929	rVV2	126309	457086	21.36%	2.591%
20	4.352	1015	1030	1056	rBV	383039	952003	44.49%	5.397%
21	4.654	1122	1124	1125	rBV	783	369	0.02%	0.002%
22	4.767	1157	1159	1161	rBV2	405	118	0.01%	0.001%
23	4.908	1200	1203	1205	rBV	1016	528	0.02%	0.003%
24	5.050	1230	1247	1273	rBV2	828220	2139868	100.00%	12.132%
25	5.436	1365	1367	1368	rBV	824	331	0.02%	0.002%
26	5.622	1410	1425	1454	rBV	780146	1570592	73.40%	8.905%
27	5.912	1506	1515	1534	rVB3	31021	60362	2.82%	0.342%
28	6.075	1553	1566	1592	rBV	480196	977362	45.67%	5.541%
29	6.294	1632	1634	1636	rVB	1218	553	0.03%	0.003%
30	6.307	1636	1638	1640	rBV2	788	396	0.02%	0.002%
31	6.362	1652	1655	1660	rVB4	1034	954	0.04%	0.005%
32	6.394	1660	1665	1669	rBV4	1061	1372	0.06%	0.008%
33	6.571	1716	1720	1722	rBV3	976	814	0.04%	0.005%
34	6.625	1734	1737	1741	rBV4	545	465	0.02%	0.003%
35	6.757	1776	1778	1781	rVB2	948	409	0.02%	0.002%
36	6.776	1781	1784	1785	rBV	501	284	0.01%	0.002%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042621\
 Data File : VV021144.D
 Acq On : 26 Apr 2021 15:38
 Operator : SY/MD
 Sample : M2326-04
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BG7C6

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM042121WMA.M
 Title : VOC Analysis

37	6.821	1796	1798	1801	rVB	544	283	0.01%	0.002%
38	6.870	1810	1813	1814	rBV	546	263	0.01%	0.001%
39	6.992	1840	1851	1872	rBV	260451	474930	22.19%	2.693%
40	7.320	1941	1953	1971	rBV	943154	1650670	77.14%	9.359%
41	7.625	2038	2048	2073	rBV	188779	337516	15.77%	1.914%
42	7.944	2136	2147	2158	rBV3	6229	13501	0.63%	0.077%
43	8.095	2184	2194	2223	rBV	544671	1000904	46.77%	5.675%
44	8.857	2419	2431	2457	rBV	1199737	1944725	90.88%	11.026%
45	9.204	2537	2539	2540	rBV	482	206	0.01%	0.001%
46	9.233	2546	2548	2553	rVB2	837	498	0.02%	0.003%
47	9.326	2575	2577	2582	rVB2	857	490	0.02%	0.003%
48	9.603	2660	2663	2665	rBV2	1183	636	0.03%	0.004%
49	9.680	2684	2687	2689	rVB2	603	272	0.01%	0.002%
50	9.902	2754	2756	2757	rBV2	526	180	0.01%	0.001%
51	9.989	2780	2783	2784	rBV	1140	485	0.02%	0.003%
52	10.011	2788	2790	2795	rBV3	818	580	0.03%	0.003%
53	10.030	2795	2796	2801	rVV	585	350	0.02%	0.002%
54	10.098	2814	2817	2821	rBV3	749	554	0.03%	0.003%
55	10.127	2821	2826	2827	rBV3	3033	2310	0.11%	0.013%
56	10.223	2844	2856	2878	rVB	733644	1161243	54.27%	6.584%
57	10.525	2949	2950	2953	rBV	731	424	0.02%	0.002%
58	10.818	3038	3041	3043	rBV2	887	541	0.03%	0.003%
59	10.918	3068	3072	3073	rBV3	2757	1785	0.08%	0.010%
60	11.027	3103	3106	3108	rBV2	1021	609	0.03%	0.003%
61	11.255	3165	3177	3200	rBV	1155177	1779278	83.15%	10.088%
62	11.509	3254	3256	3259	rBV4	937	425	0.02%	0.002%
63	11.525	3259	3261	3263	rBV2	1040	563	0.03%	0.003%
64	11.632	3281	3294	3312	rBV	1014175	1633169	76.32%	9.259%
65	11.760	3331	3334	3338	rBV3	1747	1311	0.06%	0.007%
66	12.168	3458	3461	3465	rVB3	1353	1028	0.05%	0.006%
67	12.300	3500	3502	3504	rBV2	582	310	0.01%	0.002%
68	12.413	3534	3537	3539	rBV3	845	492	0.02%	0.003%
69	12.471	3551	3555	3557	rBV2	844	724	0.03%	0.004%
70	12.529	3570	3573	3575	rBV3	678	417	0.02%	0.002%
71	12.558	3579	3582	3585	rBV2	869	741	0.03%	0.004%
72	12.696	3622	3625	3627	rBV	691	529	0.02%	0.003%
73	13.763	3954	3957	3963	rVB3	1949	1659	0.08%	0.009%




Sum of corrected areas: 17638111

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042621\
Data File : VV021144.D
Acq On : 26 Apr 2021 15:38
Operator : SY/MD
Sample : M2326-04
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 11 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampled :
BG7C6

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM042121WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

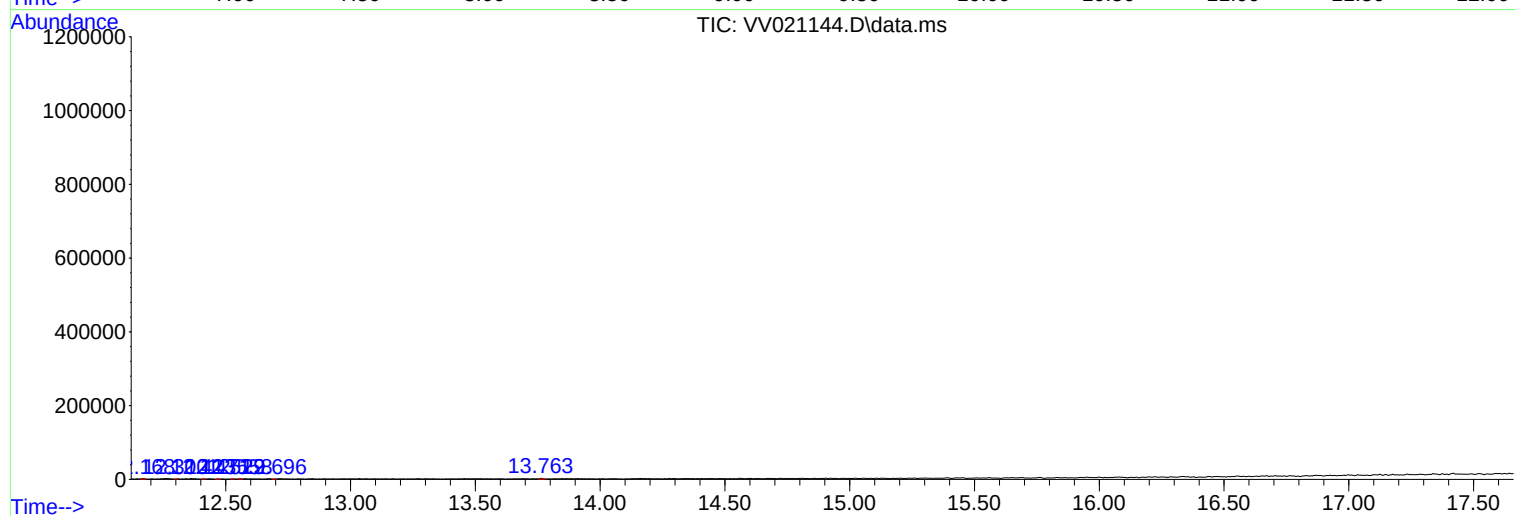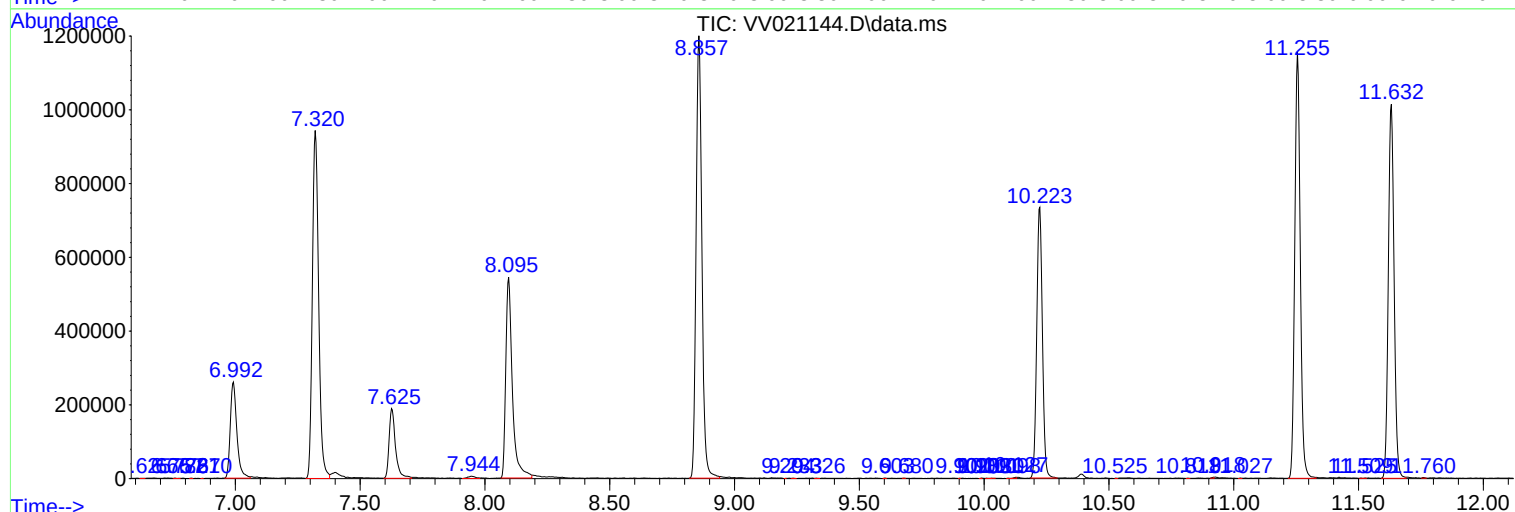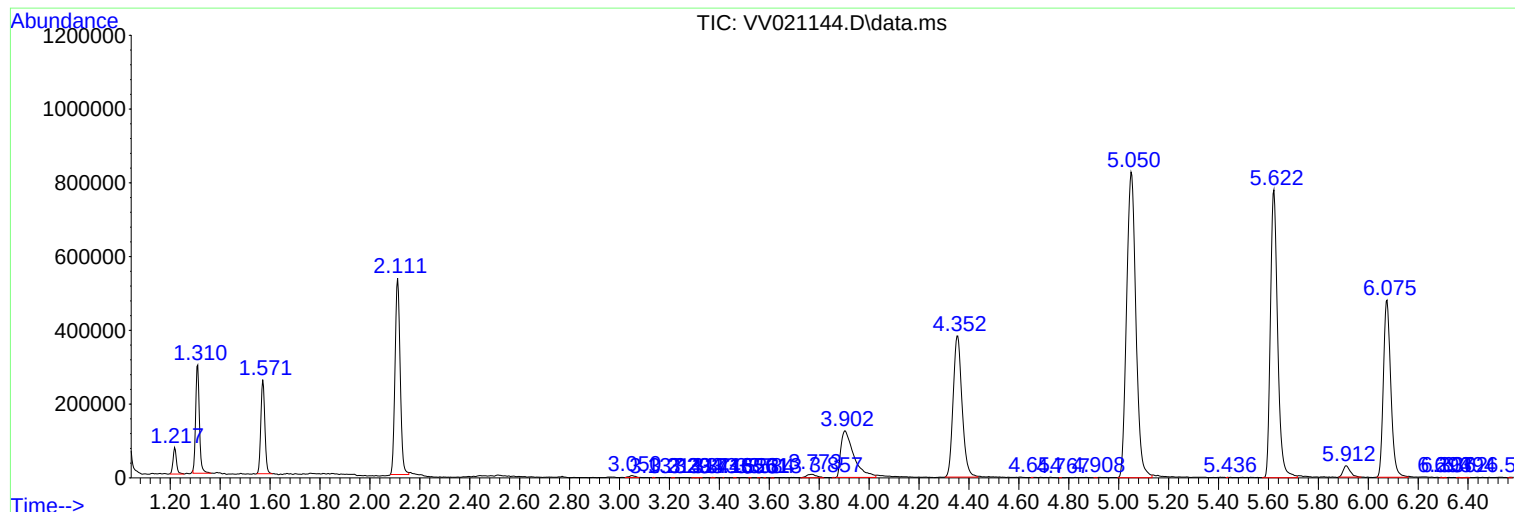

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042621\
Data File : VV021144.D
Acq On : 26 Apr 2021 15:38
Operator : SY/MD
Sample : M2326-04
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 11 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BG7C6

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM042121WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042621\
Data File : VV021144.D
Acq On : 26 Apr 2021 15:38
Operator : SY/MD
Sample : M2326-04
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 11 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BG7C6

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM042121WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
