
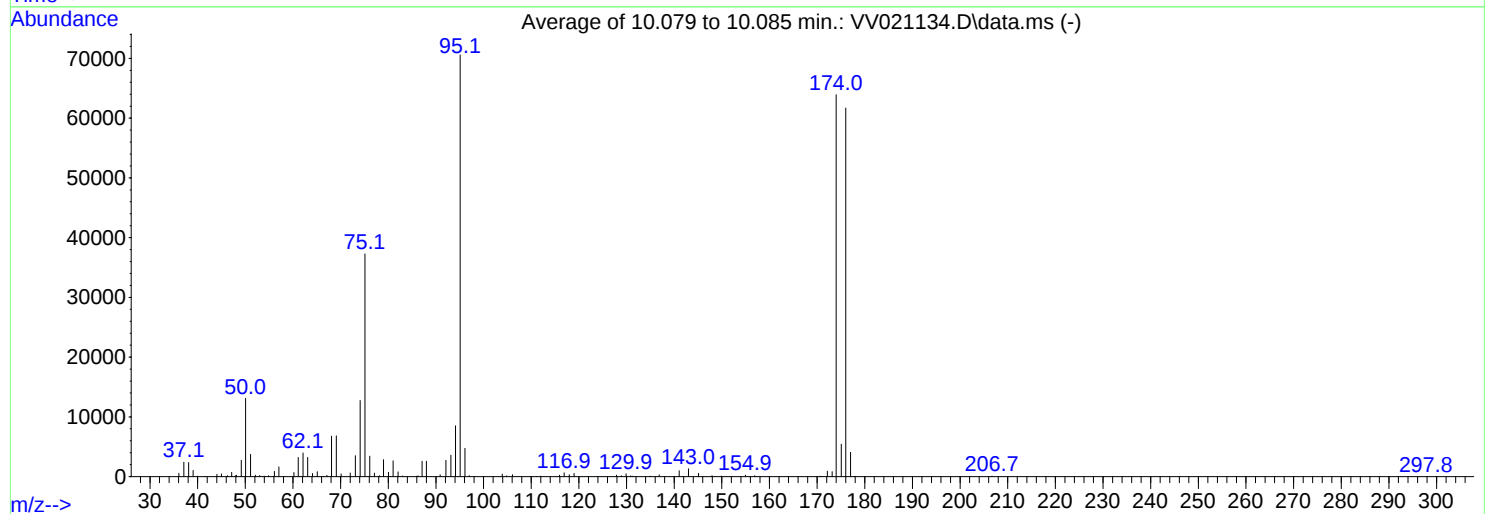


Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042621\
 Data File : VV021134.D
 Acq On : 26 Apr 2021 11:12
 Operator : SY/MD
 Sample : BFB89
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BFB189

Integration File: LSCINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM042121WMA.M
 Title : VOC Analysis
 Last Update : Wed Apr 28 03:28:03 2021

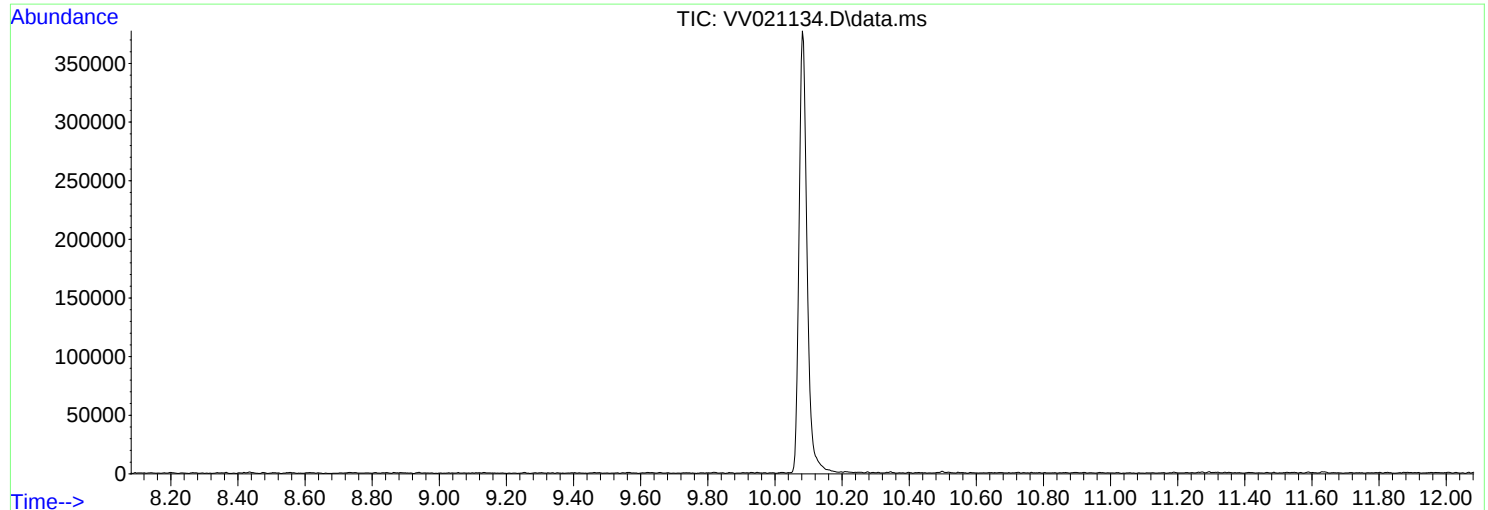

AutoFind: Scans 2811, 2812, 2813; Background Corrected with Scan 2801

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	18.5	13088	PASS
75	95	30	80	52.8	37264	PASS
95	95	100	100	100.0	70595	PASS
96	95	5	9	6.7	4746	PASS
173	174	0.00	2	1.3	825	PASS
174	95	50	120	90.5	63923	PASS
175	174	5	9	8.5	5443	PASS
176	174	95	101	96.5	61688	PASS
177	176	5	9	6.6	4077	PASS

Scan 2801 (10.046 min): VV021134.D\data.ms
BFB89

m/z	Abundance
38.90	105.0
39.90	202.0
44.10	739.0
50.00	110.0

Instrument :
MSVOA_V
ClientSampleId :
BFB189

m/z	Abundance
36.00	511.0
37.10	2449.0
38.10	2522.0
39.10	1105.0
39.90	289.0
41.40	117.0
44.10	1205.0
45.00	456.0
46.20	128.0
47.10	827.0
47.90	475.0
49.10	2462.0
50.10	12253.0
51.10	3810.0
52.00	309.0
52.90	128.0
53.90	157.0
54.90	141.0
56.10	822.0
57.10	1715.0
60.20	658.0
61.10	3367.0
62.10	4068.0
63.10	3191.0
64.10	487.0
65.10	1004.0
67.00	130.0
68.10	6699.0
69.10	6967.0
70.10	444.0
72.00	689.0
73.10	3849.0
74.10	12339.0
75.10	36808.0
76.10	3498.0
77.10	660.0
78.10	296.0
79.00	2960.0
80.10	727.0
81.00	2734.0
82.00	838.0
83.00	180.0
86.30	237.0
87.10	2365.0
88.00	2432.0
90.90	295.0
92.10	2604.0
93.10	3524.0
94.10	8192.0
95.10	69928.0
96.10	4689.0
97.10	196.0
103.90	453.0
104.90	143.0
106.10	290.0
111.10	112.0
115.20	107.0
115.90	259.0
116.90	678.0
118.00	359.0
119.00	615.0
127.80	159.0
129.00	251.0
130.00	573.0
130.80	137.0
131.20	120.0
134.90	144.0
136.80	251.0
141.00	1008.0
141.90	178.0
143.00	1453.0
145.10	613.0
147.90	186.0
149.80	137.0
155.00	301.0
156.90	207.0
170.60	152.0
171.00	130.0
172.10	1024.0
173.20	1040.0
174.00	65872.0
175.00	5478.0
176.00	62712.0
177.00	4223.0
206.70	134.0

Instrument :
MSVOA_V
ClientSampleId :
BFB189

m/z	Abundance
36.10	594.0
37.10	2534.0
38.10	2409.0
39.10	1213.0
39.90	287.0
44.10	1214.0
45.00	446.0
46.20	148.0
47.10	739.0
48.10	398.0
49.20	2806.0
50.10	13815.0
51.10	3887.0
52.10	249.0
53.00	206.0
54.00	120.0
54.90	150.0
56.10	932.0
57.10	1748.0
60.20	752.0
61.10	3322.0
62.10	4144.0
63.10	3262.0
64.10	570.0
65.10	880.0
67.10	211.0
68.10	6922.0
69.10	7049.0
70.10	448.0
72.00	617.0
73.10	3566.0
74.10	13296.0
75.10	38520.0
76.10	3559.0
77.10	585.0
78.20	203.0
79.00	2903.0
80.00	766.0
81.00	2685.0
82.10	846.0
83.00	126.0
85.90	132.0
86.20	137.0
87.10	2616.0
88.00	2685.0
90.90	345.0
92.10	2922.0
93.10	3774.0
94.10	8999.0
95.10	72288.0
96.10	4853.0
97.00	135.0
103.90	449.0
104.80	111.0
106.00	298.0
112.00	100.0
115.90	253.0
116.90	670.0
118.00	324.0
119.00	597.0
127.90	245.0
128.90	148.0
129.90	495.0
130.80	123.0
131.20	120.0
135.00	109.0
136.80	342.0
141.00	972.0
143.00	1380.0
145.10	629.0
148.00	168.0
149.90	100.0
154.90	239.0
156.90	175.0
170.60	105.0
172.20	946.0
173.20	814.0
174.00	65904.0
175.10	5597.0
176.00	63808.0
177.00	4220.0
206.70	135.0
297.80	105.0

Instrument :
MSVOA_V
ClientSampleId :
BFB189

m/z	Abundance
36.10	582.0
37.10	2236.0
38.10	2154.0
39.10	1155.0
39.90	307.0
44.00	1002.0
45.00	487.0
46.30	191.0
47.20	571.0
48.20	333.0
49.20	2904.0
50.10	13526.0
51.10	3487.0
52.20	183.0
53.10	222.0
54.90	203.0
56.10	924.0
57.00	1462.0
60.20	662.0
61.10	2964.0
62.10	3690.0
63.10	3208.0
64.10	584.0
65.10	658.0
66.40	104.0
67.20	295.0
68.10	6706.0
69.10	6510.0
70.10	467.0
72.00	523.0
73.10	3126.0
74.10	12598.0
75.10	36464.0
76.10	3260.0
77.10	505.0
77.90	121.0
79.00	2686.0
80.00	705.0
81.00	2552.0
82.10	729.0
85.90	151.0
87.10	2701.0
88.00	2616.0
90.90	330.0
92.10	2655.0
93.20	3466.0
94.10	8349.0
95.10	69568.0
96.10	4695.0
96.90	129.0
103.90	370.0
104.80	122.0
106.00	381.0
112.00	162.0
116.00	227.0
116.90	620.0
118.00	257.0
119.00	487.0
127.90	317.0
129.80	379.0
130.90	114.0
136.90	283.0
141.10	978.0
143.00	1133.0
145.10	478.0
148.00	101.0
150.00	130.0
154.90	190.0
156.90	131.0
172.10	787.0
173.10	621.0
174.00	59992.0
175.10	5253.0
176.00	58544.0
177.00	3787.0
177.90	147.0

Instrument :
MSVOA_V
ClientSampleId :
BFB189