

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW042623\
 Data File : VW030891.D
 Acq On : 26 Apr 2023 19:59
 Operator : SY/MD
 Sample : 02475-11
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VHBLK001

Quant Time: Apr 27 04:49:18 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM041723WMA.M
 Quant Title : VOC Analysis
 QLast Update : Thu Apr 27 04:45:18 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	5.542	114	219699	50.000	ug/L	0.00
28) Chlorobenzene-d5	8.792	117	217015	50.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.194	152	111617	50.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.281	65	58357	36.234	ug/L	0.00
Spiked Amount 50.000	Range 60 - 135		Recovery =	72.460%		
7) Chloroethane-d5	1.539	69	53364	39.539	ug/L	0.00
Spiked Amount 50.000	Range 70 - 130		Recovery =	79.080%		
11) 1,1-Dichloroethene-d2	2.066	65	31127	40.754	ug/L	0.00
Spiked Amount 50.000	Range 60 - 125		Recovery =	81.500%		
21) 2-Butanone-d5	3.802	46	80384	90.869	ug/L	0.00
Spiked Amount 100.000	Range 40 - 130		Recovery =	90.870%		
24) Chloroform-d	4.259	84	129621	44.410	ug/L	0.00
Spiked Amount 50.000	Range 70 - 125		Recovery =	88.820%		
26) 1,2-Dichloroethane-d4	4.950	65	92931	49.524	ug/L	0.00
Spiked Amount 50.000	Range 70 - 125		Recovery =	99.040%		
32) Benzene-d6	4.969	84	235818	45.961	ug/L	0.00
Spiked Amount 50.000	Range 70 - 125		Recovery =	91.920%		
36) 1,2-Dichloropropane-d6	5.998	67	71649	44.956	ug/L	0.00
Spiked Amount 50.000	Range 70 - 120		Recovery =	89.920%		
41) Toluene-d8	7.252	98	212420	44.095	ug/L	0.00
Spiked Amount 50.000	Range 80 - 120		Recovery =	88.180%		
43) trans-1,3-Dichloroprop...	7.561	79	35801	44.568	ug/L	0.00
Spiked Amount 50.000	Range 60 - 125		Recovery =	89.140%		
47) 2-Hexanone-d5	8.034	63	50581	80.562	ug/L	0.00
Spiked Amount 100.000	Range 45 - 130		Recovery =	80.560%		
56) 1,1,2,2-Tetrachloroeth...	10.159	84	104488	45.181	ug/L	0.00
Spiked Amount 50.000	Range 65 - 120		Recovery =	90.360%		
66) 1,2-Dichlorobenzene-d4	11.567	152	89944	50.698	ug/L	0.00
Spiked Amount 50.000	Range 80 - 120		Recovery =	101.400%		
Target Compounds						Qvalue
44) trans-1,3-Dichloropropene	7.558	75	2171	0.830	ug/L	87


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042623\
Data File : VV030891.D
Acq On : 26 Apr 2023 19:59
Operator : SY/MD
Sample : 02475-11
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 20 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VHBLK001

Quant Time: Apr 27 04:49:18 2023
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM041723WMA.M
Quant Title : VOC Analysis
QLast Update : Thu Apr 27 04:45:18 2023
Response via : Initial Calibration

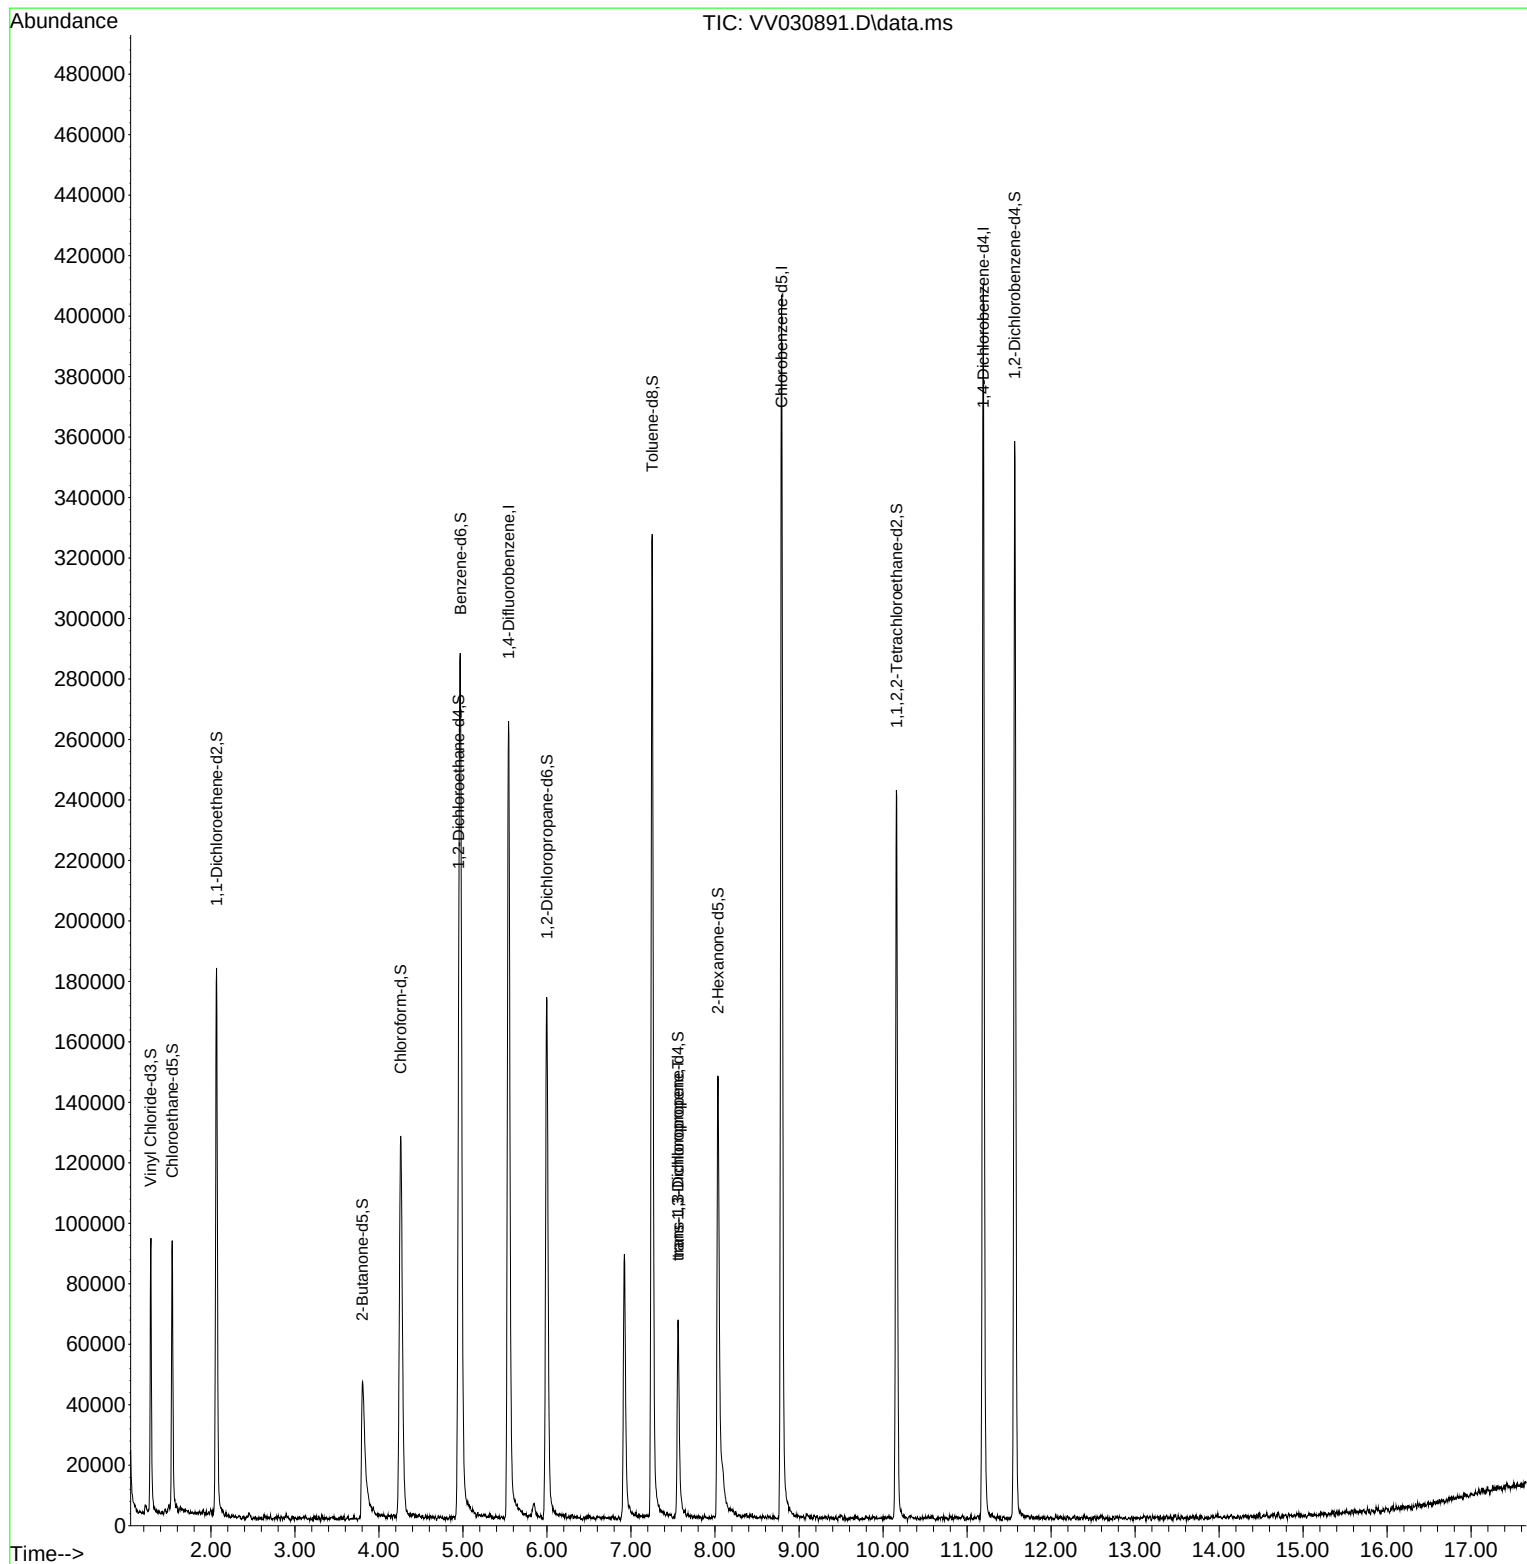

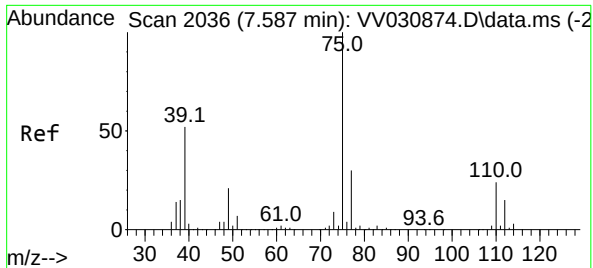

#44
trans-1,3-Dichloropropene
Concen: 0.830 ug/L
RT: 7.558 min Scan# 20
Delta R.T. -0.029 min
Lab File: VV030891.D
Acq: 26 Apr 2023 19:59

Instrument :
MSVOA_V
ClientSampleId :
VHBLK001

Tgt Ion: 75 Resp: 2171
Ion Ratio Lower Upper
75 100
77 38.9 22.1 41.1

