

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW042623\
 Data File : VW030892.D
 Acq On : 26 Apr 2023 20:23
 Operator : SY/MD
 Sample : 02474-21
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VHBLK001

Quant Time: Apr 27 04:49:30 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM041723WMA.M
 Quant Title : VOC Analysis
 QLast Update : Thu Apr 27 04:45:18 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	5.542	114	217482	50.000	ug/L	0.00
28) Chlorobenzene-d5	8.792	117	210379	50.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.194	152	108059	50.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.281	65	55795	34.996	ug/L	0.00
Spiked Amount	50.000	Range	60 - 135	Recovery	=	70.000%
7) Chloroethane-d5	1.539	69	51746	38.731	ug/L	0.00
Spiked Amount	50.000	Range	70 - 130	Recovery	=	77.460%
11) 1,1-Dichloroethene-d2	2.066	65	29394	38.877	ug/L	0.00
Spiked Amount	50.000	Range	60 - 125	Recovery	=	77.760%
21) 2-Butanone-d5	3.809	46	81531	93.105	ug/L	0.00
Spiked Amount	100.000	Range	40 - 130	Recovery	=	93.100%
24) Chloroform-d	4.259	84	128121	44.344	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	88.680%
26) 1,2-Dichloroethane-d4	4.950	65	92255	49.665	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	99.320%
32) Benzene-d6	4.969	84	228913	46.022	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	92.040%
36) 1,2-Dichloropropane-d6	5.998	67	71380	46.199	ug/L	0.00
Spiked Amount	50.000	Range	70 - 120	Recovery	=	92.400%
41) Toluene-d8	7.252	98	208762	44.702	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	89.400%
43) trans-1,3-Dichloroprop...	7.558	79	35635	45.760	ug/L	0.00
Spiked Amount	50.000	Range	60 - 125	Recovery	=	91.520%
47) 2-Hexanone-d5	8.034	63	50315	82.666	ug/L	0.00
Spiked Amount	100.000	Range	45 - 130	Recovery	=	82.670%
56) 1,1,2,2-Tetrachloroeth...	10.159	84	102167	45.571	ug/L	0.00
Spiked Amount	50.000	Range	65 - 120	Recovery	=	91.140%
66) 1,2-Dichlorobenzene-d4	11.567	152	88798	51.700	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	103.400%
Target Compounds						
44) trans-1,3-Dichloropropene	7.558	75	2072	0.817	ug/L	Qvalue 90


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042623\
Data File : VV030892.D
Acq On : 26 Apr 2023 20:23
Operator : SY/MD
Sample : 02474-21
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 21 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VHBLK001

Quant Time: Apr 27 04:49:30 2023
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM041723WMA.M
Quant Title : VOC Analysis
QLast Update : Thu Apr 27 04:45:18 2023
Response via : Initial Calibration

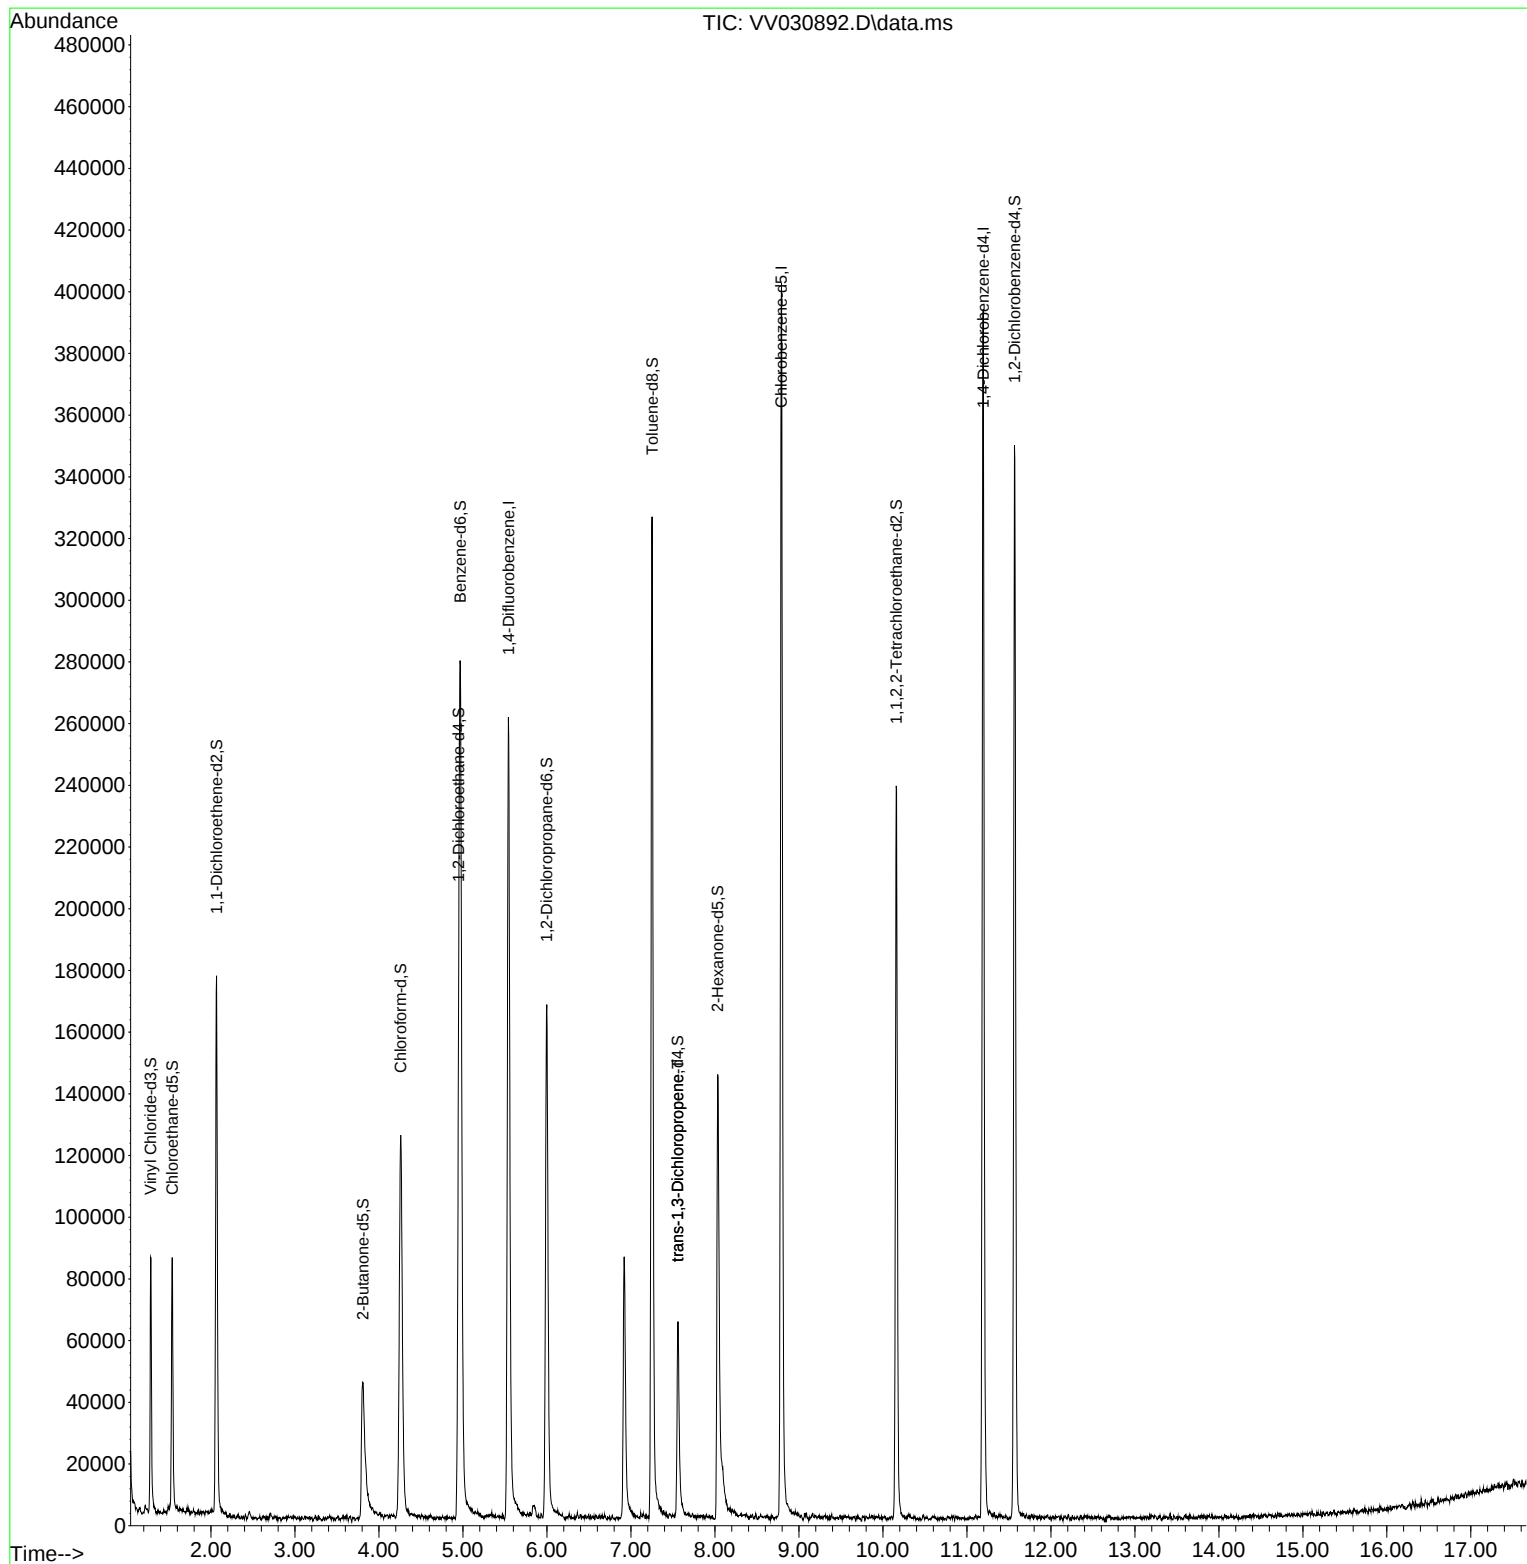

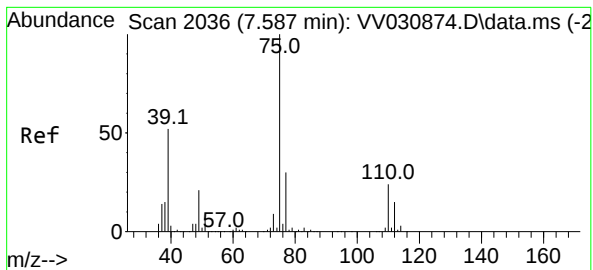

#44
 trans-1,3-Dichloropropene
 Concen: 0.817 ug/L
 RT: 7.558 min Scan# 2036
 Delta R.T. -0.029 min
 Lab File: VV030892.D
 Acq: 26 Apr 2023 20:23

Instrument :
 MSVOA_V
 ClientSampleId :
 VHBLK001

Tgt Ion: 75 Resp: 2072
 Ion Ratio Lower Upper
 75 100
 77 37.3 22.1 41.1

