




Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042623\
 Data File : VV030876.D
 Acq On : 26 Apr 2023 13:31
 Operator : SY/MD
 Sample : VV0426WBL01
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VBLK337

Manual IntegrationsAPPROVED

Quant Time: Apr 27 04:46:04 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM041723WMA.M
 Quant Title : VOC Analysis
 QLast Update : Thu Apr 27 04:45:18 2023
 Response via : Initial Calibration

Reviewed By :Krupa Patel 04/27/2023
 Supervised By :Mahesh Dadoda 04/27/2023

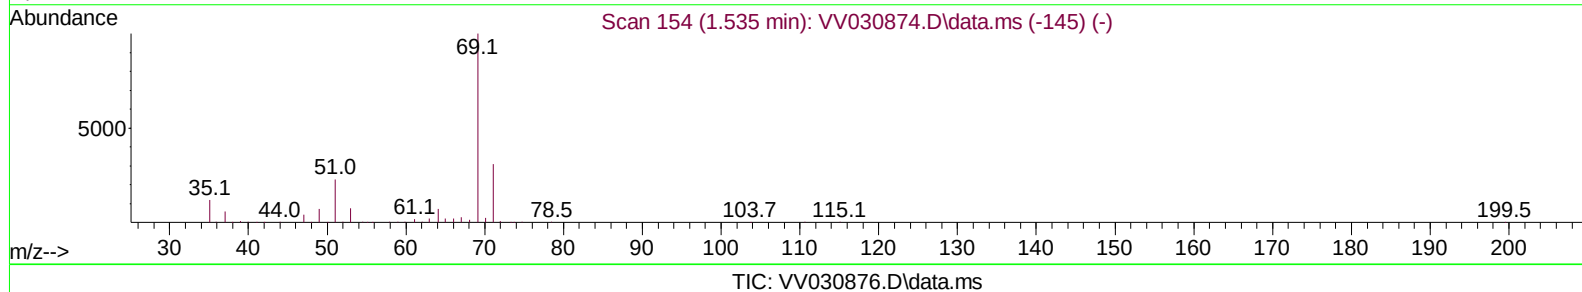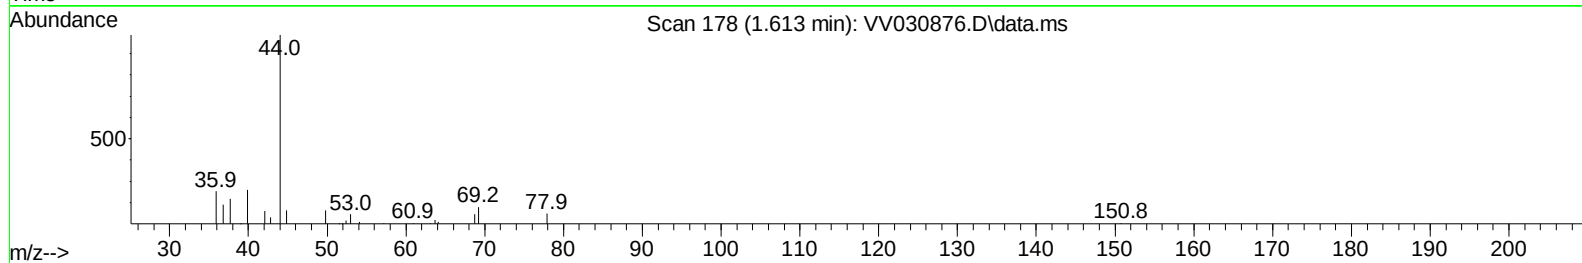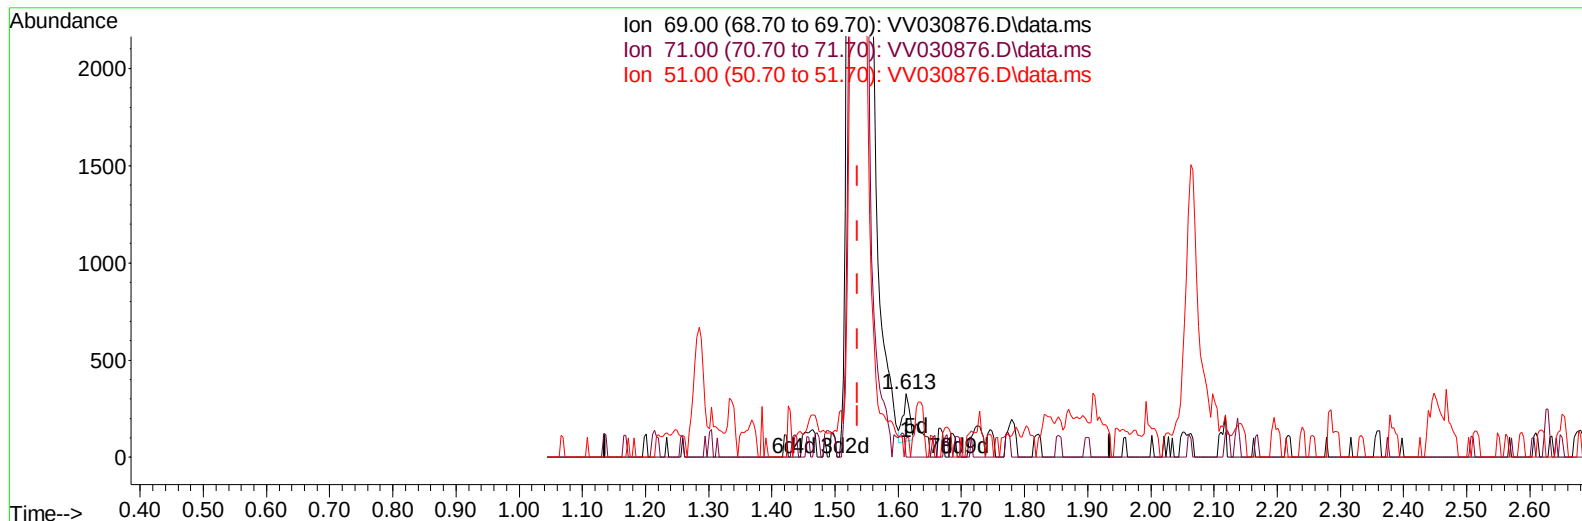

(7) Chloroethane-d5 (S)

1.613min (+ 0.077) 0.13 ug/L

response 178

Ion	Exp%	Act%
69.00	100.00	100.00
71.00	32.00	38.76
51.00	30.70	22.47
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042623\
 Data File : VV030876.D
 Acq On : 26 Apr 2023 13:31
 Operator : SY/MD
 Sample : VV0426WBL01
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VBLK337

Manual IntegrationsAPPROVED

Quant Time: Apr 27 04:46:04 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM041723WMA.M
 Quant Title : VOC Analysis
 QLast Update : Thu Apr 27 04:45:18 2023
 Response via : Initial Calibration

Reviewed By :Krupa Patel 04/27/2023
 Supervised By :Mahesh Dadoda 04/27/2023

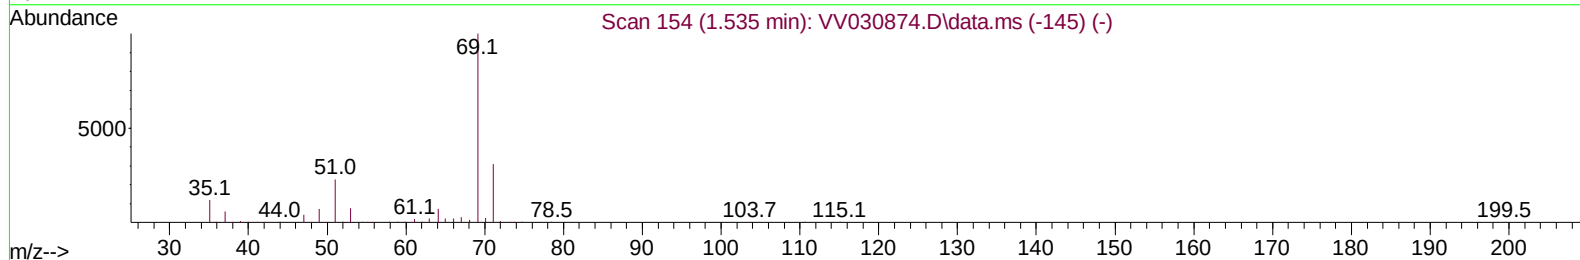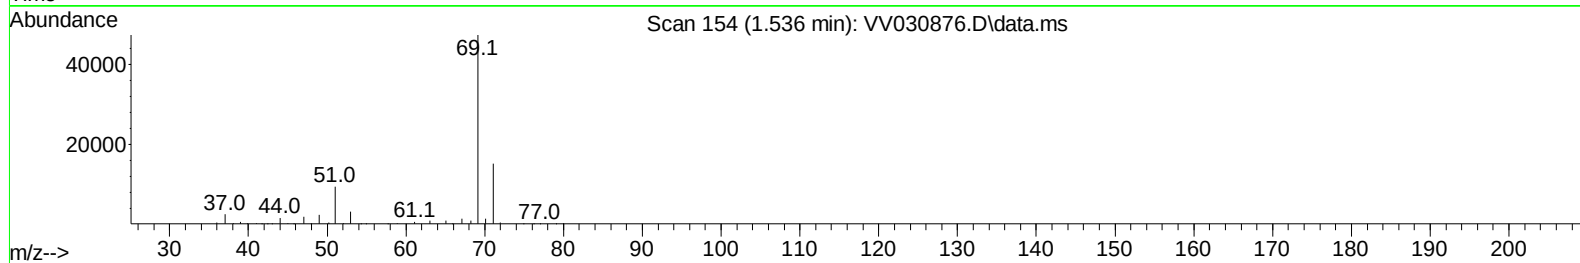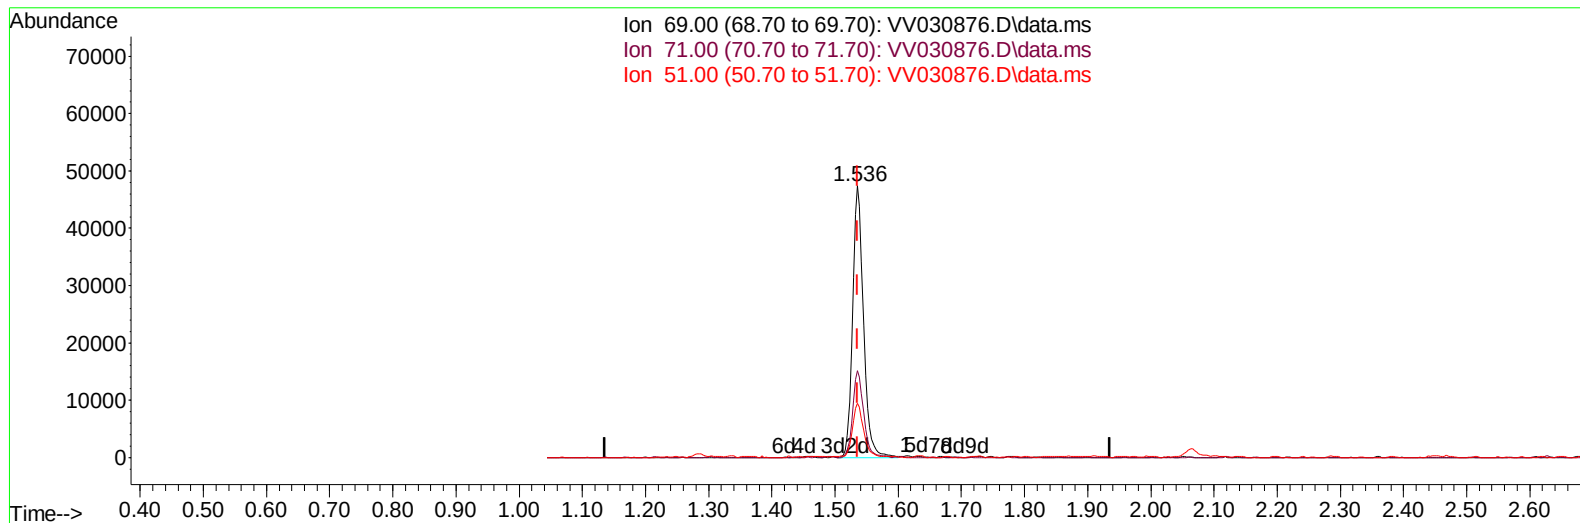

TIC: VV030876.D\data.ms

(7) Chloroethane-d5 (S)

1.536min (+ 0.000) 42.63 ug/L m

response 57235

Ion	Exp%	Act%
69.00	100.00	100.00
71.00	32.00	0.12#
51.00	30.70	0.07#
0.00	0.00	0.00

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042623\
 Data File : VV030876.D
 Acq On : 26 Apr 2023 13:31
 Operator : SY/MD
 Sample : VV0426WBL01
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VBLK337

Manual IntegrationsAPPROVED

Reviewed By :Krupa Patel 04/27/2023
 Supervised By :Mahesh Dadoda 04/27/2023

Quant Time: Apr 27 04:46:04 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM041723WMA.M
 Quant Title : VOC Analysis
 QLast Update : Thu Apr 27 04:45:18 2023
 Response via : Initial Calibration

Compound	R.T.	Q	Ion	Response	Conc	Units	Dev(Min)

Internal Standards							
1) 1,4-Difluorobenzene	5.542	114		218545	50.000	ug/L	0.00
28) Chlorobenzene-d5	8.793	117		208645	50.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.194	152		107372	50.000	ug/L	0.00
System Monitoring Compounds							
4) Vinyl Chloride-d3	1.282	65		65014	40.580	ug/L	0.00
Spiked Amount 50.000	Range 60	- 135		Recovery =	81.160%		
7) Chloroethane-d5	1.536	69		57235m	42.631	ug/L	0.00
Spiked Amount 50.000	Range 70	- 130		Recovery =	85.260%		
11) 1,1-Dichloroethene-d2	2.066	65		33737	44.404	ug/L	0.00
Spiked Amount 50.000	Range 60	- 125		Recovery =	88.800%		
21) 2-Butanone-d5	3.799	46		94360	107.231	ug/L	0.00
Spiked Amount 100.000	Range 40	- 130		Recovery =	107.230%		
24) Chloroform-d	4.259	84		137584	47.387	ug/L	0.00
Spiked Amount 50.000	Range 70	- 125		Recovery =	94.780%		
26) 1,2-Dichloroethane-d4	4.950	65		97448	52.205	ug/L	0.00
Spiked Amount 50.000	Range 70	- 125		Recovery =	104.400%		
32) Benzene-d6	4.970	84		254924	51.678	ug/L	0.00
Spiked Amount 50.000	Range 70	- 125		Recovery =	103.360%		
36) 1,2-Dichloropropane-d6	5.998	67		74475	48.603	ug/L	0.00
Spiked Amount 50.000	Range 70	- 120		Recovery =	97.200%		
41) Toluene-d8	7.249	98		224634	48.501	ug/L	0.00
Spiked Amount 50.000	Range 80	- 120		Recovery =	97.000%		
43) trans-1,3-Dichloroprop...	7.558	79		39159	50.704	ug/L	0.00
Spiked Amount 50.000	Range 60	- 125		Recovery =	101.400%		
47) 2-Hexanone-d5	8.034	63		54707	90.629	ug/L	0.00
Spiked Amount 100.000	Range 45	- 130		Recovery =	90.630%		
56) 1,1,2,2-Tetrachloroeth...	10.159	84		107955	48.553	ug/L	0.00
Spiked Amount 50.000	Range 65	- 120		Recovery =	97.100%		
66) 1,2-Dichlorobenzene-d4	11.567	152		95039	55.688	ug/L	0.00
Spiked Amount 50.000	Range 80	- 120		Recovery =	111.380%		

Target Compounds Qvalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042623\
Data File : VV030876.D
Acq On : 26 Apr 2023 13:31
Operator : SY/MD
Sample : VV0426WBL01
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK337

Manual IntegrationsAPPROVED

Quant Time: Apr 27 04:46:04 2023
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM041723WMA.M
Quant Title : VOC Analysis
QLast Update : Thu Apr 27 04:45:18 2023
Response via : Initial Calibration

Reviewed By :Krupa Patel 04/27/2023
Supervised By :Mahesh Dadoda 04/27/2023

