

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042623\
 Data File : VV030876.D
 Acq On : 26 Apr 2023 13:31
 Operator : SY/MD
 Sample : VV0426WBL01
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VBLK337

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM041723WMA.M
 Title : VOC Analysis

Signal : TIC: VV030876.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.282	69	75	89	rVB	97724	106848	13.27%	1.685%
2	1.536	148	154	165	rVB	87372	106450	13.22%	1.679%
3	2.066	310	319	332	rVB	196036	284391	35.31%	4.486%
4	2.246	370	375	378	rBV7	2565	2950	0.37%	0.047%
5	2.539	461	466	468	rBV5	1703	1160	0.14%	0.018%
6	2.593	479	483	485	rBV5	984	775	0.10%	0.012%
7	2.700	511	516	518	rBV5	3164	3068	0.38%	0.048%
8	2.822	552	554	557	rBV4	1356	652	0.08%	0.010%
9	2.838	557	559	562	rVB3	876	527	0.07%	0.008%
10	2.876	569	571	573	rBV3	1312	649	0.08%	0.010%
11	2.892	573	576	578	rBV4	766	577	0.07%	0.009%
12	2.995	606	608	609	rBV3	1254	486	0.06%	0.008%
13	3.092	634	638	640	rBV5	1383	853	0.11%	0.013%
14	3.118	640	646	647	rBV5	1052	1067	0.13%	0.017%
15	3.217	673	677	678	rBV4	1186	725	0.09%	0.011%
16	3.285	694	698	699	rBV3	795	557	0.07%	0.009%
17	3.394	729	732	733	rBV3	815	525	0.07%	0.008%
18	3.571	784	787	791	rBV4	1094	738	0.09%	0.012%
19	3.648	806	811	812	rBV3	1307	930	0.12%	0.015%
20	3.693	823	825	827	rBV3	1486	662	0.08%	0.010%
21	3.709	827	830	832	rBV4	986	751	0.09%	0.012%
22	3.751	838	843	845	rBV6	1502	1318	0.16%	0.021%
23	3.799	848	858	887	rBV	56145	161405	20.04%	2.546%
24	4.259	987	1001	1024	rBV	131064	335054	41.60%	5.285%
25	4.532	1084	1086	1093	rVB6	1625	1164	0.14%	0.018%
26	4.818	1170	1175	1176	rBV4	1276	848	0.11%	0.013%
27	4.873	1190	1192	1194	rBV3	919	510	0.06%	0.008%
28	4.905	1199	1202	1203	rBV3	1122	515	0.06%	0.008%
29	4.966	1205	1221	1244	rBV2	304758	805469	100.00%	12.705%
30	5.333	1332	1335	1336	rBV3	1110	605	0.08%	0.010%
31	5.542	1388	1400	1425	rVV	261715	544051	67.54%	8.582%
32	5.998	1529	1542	1559	rBV	177808	367764	45.66%	5.801%
33	6.211	1606	1608	1611	rBV4	1761	1045	0.13%	0.016%
34	6.240	1615	1617	1619	rBV3	1090	485	0.06%	0.008%
35	6.388	1660	1663	1666	rBV5	872	634	0.08%	0.010%
36	6.609	1727	1732	1735	rBV7	1269	1165	0.14%	0.018%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042623\
 Data File : VV030876.D
 Acq On : 26 Apr 2023 13:31
 Operator : SY/MD
 Sample : VV0426WBL01
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VBLK337

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM041723WMA.M
 Title : VOC Analysis

37	6.667	1748	1750	1754	rVB3	1189	627	0.08%	0.010%
38	6.709	1759	1763	1764	rBV4	856	499	0.06%	0.008%
39	6.786	1783	1787	1788	rBV4	1048	673	0.08%	0.011%
40	6.921	1819	1829	1850	rBV2	92206	178566	22.17%	2.817%
41	7.175	1906	1908	1911	rBV3	1531	891	0.11%	0.014%
42	7.207	1916	1918	1919	rBV2	1397	533	0.07%	0.008%
43	7.252	1921	1932	1951	rBV	344037	608521	75.55%	9.599%
44	7.561	2019	2028	2050	rBV	66870	122644	15.23%	1.935%
45	7.732	2079	2081	2085	rVB4	1467	1024	0.13%	0.016%
46	7.773	2091	2094	2099	rBV7	2335	2337	0.29%	0.037%
47	8.034	2163	2175	2190	rBV	172274	320230	39.76%	5.051%
48	8.587	2345	2347	2350	rBV4	1316	609	0.08%	0.010%
49	8.696	2377	2381	2383	rBV4	940	679	0.08%	0.011%
50	8.751	2395	2398	2399	rBV3	916	513	0.06%	0.008%
51	8.793	2399	2411	2434	rVV	388921	665033	82.56%	10.490%
52	9.182	2528	2532	2533	rBV4	1728	1322	0.16%	0.021%
53	9.272	2558	2560	2564	rVB5	1444	939	0.12%	0.015%
54	9.352	2582	2585	2586	rBV3	1152	543	0.07%	0.009%
55	9.452	2614	2616	2619	rBV4	899	672	0.08%	0.011%
56	9.606	2660	2664	2668	rBV6	1356	1352	0.17%	0.021%
57	9.641	2671	2675	2677	rVV4	1422	864	0.11%	0.014%
58	9.731	2700	2703	2707	rBV5	1550	1088	0.14%	0.017%
59	9.793	2719	2722	2725	rBV5	1218	833	0.10%	0.013%
60	9.844	2732	2738	2742	rBV9	1134	1364	0.17%	0.022%
61	9.866	2742	2745	2746	rBV3	2331	1345	0.17%	0.021%
62	9.953	2767	2772	2773	rBV4	1236	1067	0.13%	0.017%
63	10.111	2817	2821	2823	rBV4	1093	1013	0.13%	0.016%
64	10.159	2826	2836	2857	rVB	251896	403789	50.13%	6.369%
65	10.349	2892	2895	2898	rBV5	1484	1265	0.16%	0.020%
66	10.391	2906	2908	2910	rBV2	1155	615	0.08%	0.010%
67	10.600	2967	2973	2978	rVB8	1352	2046	0.25%	0.032%
68	10.715	3006	3009	3011	rBV5	864	508	0.06%	0.008%
69	10.754	3019	3021	3022	rBV2	1081	541	0.07%	0.009%
70	10.928	3070	3075	3077	rBV4	1570	1143	0.14%	0.018%
71	11.018	3100	3103	3105	rBV4	993	808	0.10%	0.013%
72	11.130	3130	3138	3144	rBV10	3614	5857	0.73%	0.092%
73	11.194	3147	3158	3176	rVV	399912	638005	79.21%	10.064%
74	11.339	3201	3203	3207	rBV4	1226	799	0.10%	0.013%
75	11.368	3210	3212	3215	rBV4	1401	706	0.09%	0.011%
76	11.567	3262	3274	3292	rBV	374991	603992	74.99%	9.527%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042623\
 Data File : VV030876.D
 Acq On : 26 Apr 2023 13:31
 Operator : SY/MD
 Sample : VV0426WBL01
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VBLK337

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM041723WMA.M
 Title : VOC Analysis

77	11.796	3343	3345	3349	rVB3	1289	758	0.09%	0.012%
78	11.892	3370	3375	3379	rBV7	1571	1622	0.20%	0.026%
79	12.046	3420	3423	3424	rBV3	881	572	0.07%	0.009%
80	12.136	3446	3451	3454	rBV5	1241	1232	0.15%	0.019%
81	12.191	3467	3468	3470	rBV2	1057	517	0.06%	0.008%
82	12.291	3495	3499	3501	rBV4	1134	841	0.10%	0.013%
83	12.445	3543	3547	3548	rBV3	902	612	0.08%	0.010%
84	12.532	3571	3574	3577	rBV4	1069	552	0.07%	0.009%
85	12.554	3577	3581	3583	rBV4	913	703	0.09%	0.011%
86	12.808	3658	3660	3663	rBV3	1551	957	0.12%	0.015%
87	12.828	3663	3666	3667	rBV3	1091	544	0.07%	0.009%
88	12.956	3704	3706	3709	rVB4	833	516	0.06%	0.008%
89	12.992	3714	3717	3720	rBV5	1364	880	0.11%	0.014%
90	13.400	3842	3844	3847	rVB3	1003	549	0.07%	0.009%
91	13.452	3853	3860	3861	rBV6	6342	6744	0.84%	0.106%
92	13.735	3946	3948	3951	rVB4	1542	952	0.12%	0.015%
93	13.763	3951	3957	3959	rBV5	1975	1988	0.25%	0.031%
94	13.844	3980	3982	3983	rBV2	1147	573	0.07%	0.009%
95	13.963	4016	4019	4020	rBV2	997	534	0.07%	0.008%
96	14.040	4040	4043	4046	rBV4	1675	1169	0.15%	0.018%
97	14.098	4059	4061	4064	rBV3	1135	735	0.09%	0.012%
98	14.265	4109	4113	4115	rBV4	1515	1089	0.14%	0.017%
99	14.323	4128	4131	4133	rVV3	1888	1107	0.14%	0.017%
100	14.390	4151	4152	4155	rBV3	1287	567	0.07%	0.009%




Sum of corrected areas: 6339541

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042623\
Data File : VV030876.D
Acq On : 26 Apr 2023 13:31
Operator : SY/MD
Sample : VV0426WBL01
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK337

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM041723WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

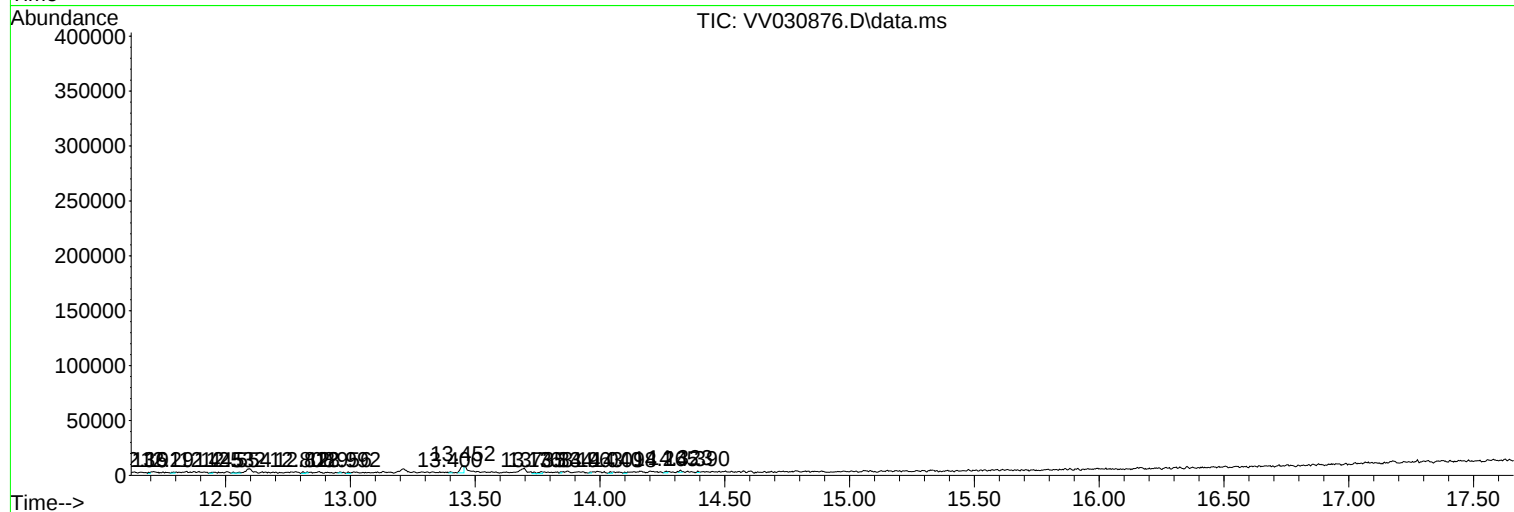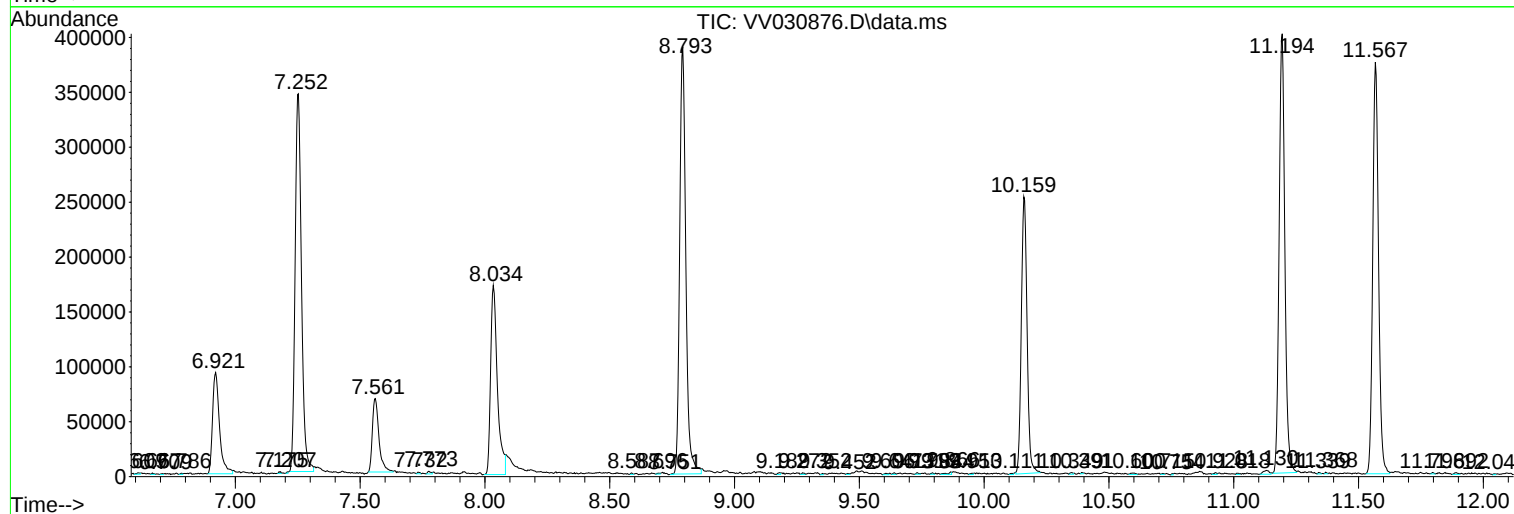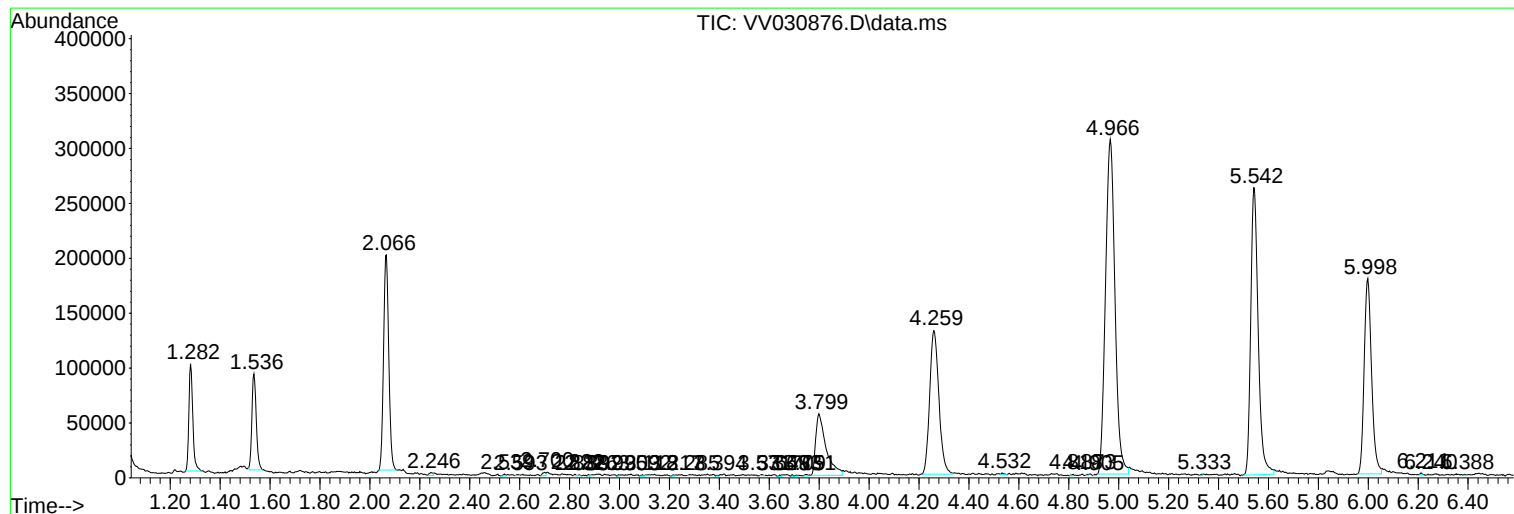

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042623\
Data File : VV030876.D
Acq On : 26 Apr 2023 13:31
Operator : SY/MD
Sample : VV0426WBL01
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK337

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM041723WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042623\
Data File : VV030876.D
Acq On : 26 Apr 2023 13:31
Operator : SY/MD
Sample : VV0426WBL01
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK337

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM041723WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------