

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042623\
 Data File : VV030877.D
 Acq On : 26 Apr 2023 14:02
 Operator : SY/MD
 Sample : 02474-05 10X
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0AS7

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM041723WMA.M
 Title : VOC Analysis

Signal : TIC: VV030877.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.282	69	75	88	rVB	96205	104425	12.28%	1.380%
2	1.536	148	154	165	rVB	93156	111484	13.11%	1.473%
3	2.063	310	318	334	rVB	202194	292228	34.36%	3.862%
4	2.227	366	369	372	rBV5	1507	1058	0.12%	0.014%
5	2.442	434	436	437	rBV2	1398	623	0.07%	0.008%
6	2.584	478	480	483	rBV3	992	667	0.08%	0.009%
7	2.645	496	499	501	rBV4	1159	710	0.08%	0.009%
8	2.658	501	503	505	rVV3	973	587	0.07%	0.008%
9	2.812	548	551	552	rBV3	1195	690	0.08%	0.009%
10	2.902	577	579	582	rBV3	905	706	0.08%	0.009%
11	2.999	607	609	614	rVV5	1148	708	0.08%	0.009%
12	3.024	614	617	620	rVB5	1121	710	0.08%	0.009%
13	3.175	662	664	666	rBV3	738	438	0.05%	0.006%
14	3.320	705	709	713	rBV5	1348	1449	0.17%	0.019%
15	3.388	726	730	734	rBV6	1543	1662	0.20%	0.022%
16	3.481	757	759	762	rBV4	1138	649	0.08%	0.009%
17	3.523	769	772	778	rBV7	1061	878	0.10%	0.012%
18	3.552	779	781	783	rBV3	1038	490	0.06%	0.006%
19	3.600	792	796	798	rBV3	1578	1170	0.14%	0.015%
20	3.645	807	810	814	rVB6	1367	823	0.10%	0.011%
21	3.671	814	818	821	rVB4	1096	668	0.08%	0.009%
22	3.687	821	823	826	rBV3	1068	654	0.08%	0.009%
23	3.799	849	858	881	rBV	54883	163784	19.26%	2.165%
24	4.098	949	951	954	rVB4	1265	686	0.08%	0.009%
25	4.256	986	1000	1023	rBV	138998	351127	41.29%	4.641%
26	4.693	1134	1136	1139	rBV3	1159	499	0.06%	0.007%
27	4.834	1178	1180	1182	rBV2	1086	548	0.06%	0.007%
28	4.963	1204	1220	1243	rBV2	319827	850489	100.00%	11.240%
29	5.407	1356	1358	1360	rVB3	1588	767	0.09%	0.010%
30	5.423	1360	1363	1364	rBV2	1508	727	0.09%	0.010%
31	5.542	1385	1400	1421	rBV	300859	629460	74.01%	8.319%
32	5.841	1480	1493	1513	rBV	352694	704631	82.85%	9.313%
33	5.995	1530	1541	1564	rVB	188733	389318	45.78%	5.145%
34	6.413	1669	1671	1675	rBV5	1032	680	0.08%	0.009%
35	6.719	1764	1766	1769	rVB4	1444	709	0.08%	0.009%
36	6.735	1769	1771	1775	rVB5	1059	815	0.10%	0.011%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW042623\
 Data File : VW030877.D
 Acq On : 26 Apr 2023 14:02
 Operator : SY/MD
 Sample : 02474-05 10X
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0AS7

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM041723WMA.M
 Title : VOC Analysis

37	6.757	1775	1778	1779	rBV3	824	497	0.06%	0.007%
38	6.828	1795	1800	1806	rBV7	1556	1971	0.23%	0.026%
39	6.918	1815	1828	1850	rBV2	101437	200398	23.56%	2.649%
40	7.079	1875	1878	1880	rBV4	1522	868	0.10%	0.011%
41	7.146	1897	1899	1900	rBV2	1184	488	0.06%	0.006%
42	7.249	1919	1931	1954	rBV	369320	658588	77.44%	8.704%
43	7.558	2018	2027	2043	rBV	73403	133628	15.71%	1.766%
44	7.828	2109	2111	2113	rBV3	901	480	0.06%	0.006%
45	7.886	2127	2129	2131	rBV3	1169	496	0.06%	0.007%
46	7.921	2137	2140	2144	rBV5	1230	933	0.11%	0.012%
47	7.963	2150	2153	2154	rBV3	1085	653	0.08%	0.009%
48	8.034	2166	2175	2205	rBV	163179	337329	39.66%	4.458%
49	8.455	2304	2306	2309	rBV2	1087	726	0.09%	0.010%
50	8.641	2361	2364	2365	rBV3	1007	635	0.07%	0.008%
51	8.680	2374	2376	2380	rBV5	1281	1004	0.12%	0.013%
52	8.789	2399	2410	2435	rBV	460124	765524	90.01%	10.117%
53	9.034	2482	2486	2489	rBV5	1311	827	0.10%	0.011%
54	9.117	2507	2512	2517	rBV7	1599	1696	0.20%	0.022%
55	9.236	2547	2549	2551	rBV3	1097	491	0.06%	0.006%
56	9.317	2572	2574	2579	rVV6	1201	984	0.12%	0.013%
57	9.346	2579	2583	2585	rBV4	1256	875	0.10%	0.012%
58	9.760	2707	2712	2718	rBV8	1379	1880	0.22%	0.025%
59	9.950	2769	2771	2776	rVB4	1397	1053	0.12%	0.014%
60	9.973	2776	2778	2782	rVB6	1989	1175	0.14%	0.016%
61	9.992	2782	2784	2785	rBV	1124	488	0.06%	0.006%
62	10.040	2796	2799	2800	rBV3	954	450	0.05%	0.006%
63	10.075	2806	2810	2813	rBV4	865	701	0.08%	0.009%
64	10.159	2824	2836	2853	rBV	254650	415787	48.89%	5.495%
65	10.477	2933	2935	2939	rVB6	1158	713	0.08%	0.009%
66	10.564	2959	2962	2965	rBV4	1407	1071	0.13%	0.014%
67	10.606	2972	2975	2977	rBV4	1416	811	0.10%	0.011%
68	10.754	3018	3021	3024	rBV5	1255	1030	0.12%	0.014%
69	10.911	3068	3070	3073	rVB3	819	454	0.05%	0.006%
70	10.940	3077	3079	3081	rVV3	1025	470	0.06%	0.006%
71	11.005	3096	3099	3103	rBV6	1307	1160	0.14%	0.015%
72	11.191	3146	3157	3177	rBV	470745	751304	88.34%	9.930%
73	11.339	3199	3203	3206	rBV6	1048	1074	0.13%	0.014%
74	11.448	3234	3237	3239	rBV4	971	589	0.07%	0.008%
75	11.567	3263	3274	3293	rBV	406509	636078	74.79%	8.407%
76	11.770	3335	3337	3341	rBV5	1250	1004	0.12%	0.013%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042623\
 Data File : VV030877.D
 Acq On : 26 Apr 2023 14:02
 Operator : SY/MD
 Sample : 02474-05 10X
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0AS7

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM041723WMA.M
 Title : VOC Analysis

77	11.853	3361	3363	3368	rBV6	1389	1068	0.13%	0.014%
78	11.882	3368	3372	3374	rVV5	1085	882	0.10%	0.012%
79	11.947	3387	3392	3394	rBV6	1153	1063	0.12%	0.014%
80	11.972	3398	3400	3404	rBV4	1033	506	0.06%	0.007%
81	12.005	3408	3410	3412	rBV3	883	454	0.05%	0.006%
82	12.027	3415	3417	3419	rBV3	1058	513	0.06%	0.007%
83	12.117	3442	3445	3449	rVB7	1106	942	0.11%	0.012%
84	12.149	3451	3455	3458	rBV5	1041	704	0.08%	0.009%
85	12.236	3479	3482	3484	rVB4	873	514	0.06%	0.007%
86	12.400	3530	3533	3534	rBV3	748	457	0.05%	0.006%
87	12.500	3562	3564	3567	rBV4	815	497	0.06%	0.007%
88	12.577	3586	3588	3590	rBV2	937	571	0.07%	0.008%
89	12.654	3607	3612	3613	rBV4	1005	964	0.11%	0.013%
90	12.831	3661	3667	3669	rBV4	1383	1317	0.15%	0.017%
91	12.937	3697	3700	3705	rVB5	1324	1013	0.12%	0.013%
92	12.966	3705	3709	3713	rBV7	2068	2192	0.26%	0.029%
93	13.255	3794	3799	3802	rVB5	1895	1842	0.22%	0.024%
94	13.271	3802	3804	3805	rBV	1160	449	0.05%	0.006%
95	13.368	3833	3834	3840	rVB6	1259	853	0.10%	0.011%
96	13.394	3840	3842	3845	rBV4	1227	929	0.11%	0.012%
97	13.603	3903	3907	3910	rBV5	1004	999	0.12%	0.013%
98	13.943	4008	4013	4014	rBV4	1120	780	0.09%	0.010%
99	14.529	4190	4195	4199	rBV8	1448	1788	0.21%	0.024%
100	14.979	4332	4335	4337	rBV4	1407	943	0.11%	0.012%




Sum of corrected areas: 7566340

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042623\
Data File : VV030877.D
Acq On : 26 Apr 2023 14:02
Operator : SY/MD
Sample : 02474-05 10X
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 5 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0AS7

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM041723WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

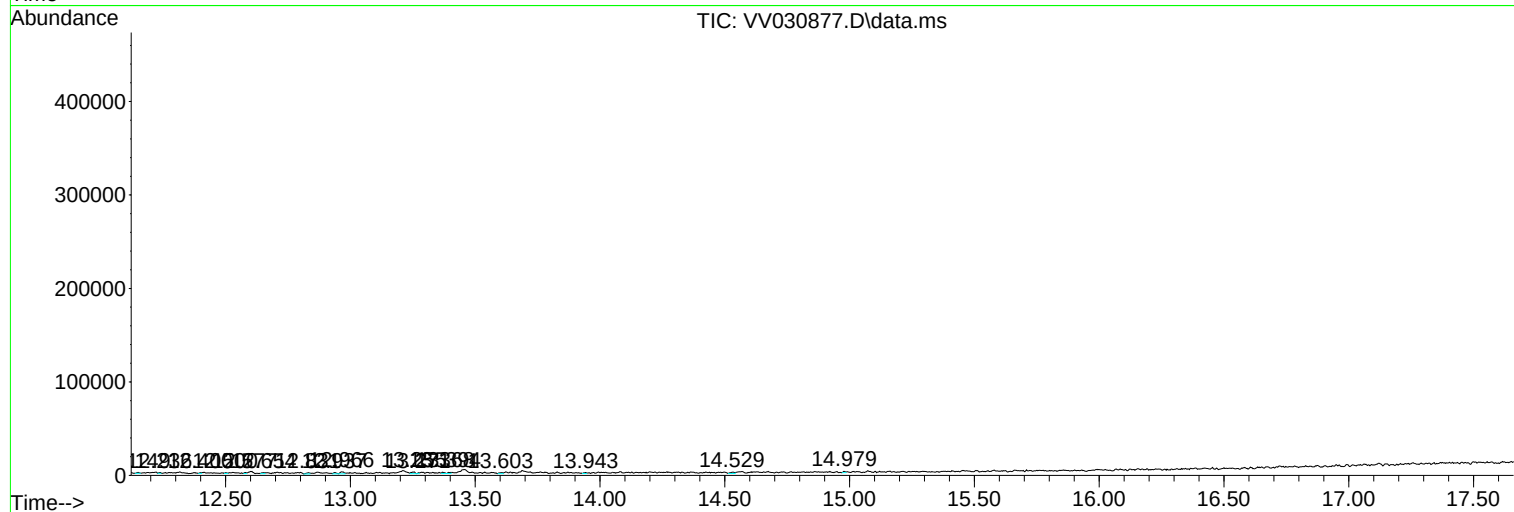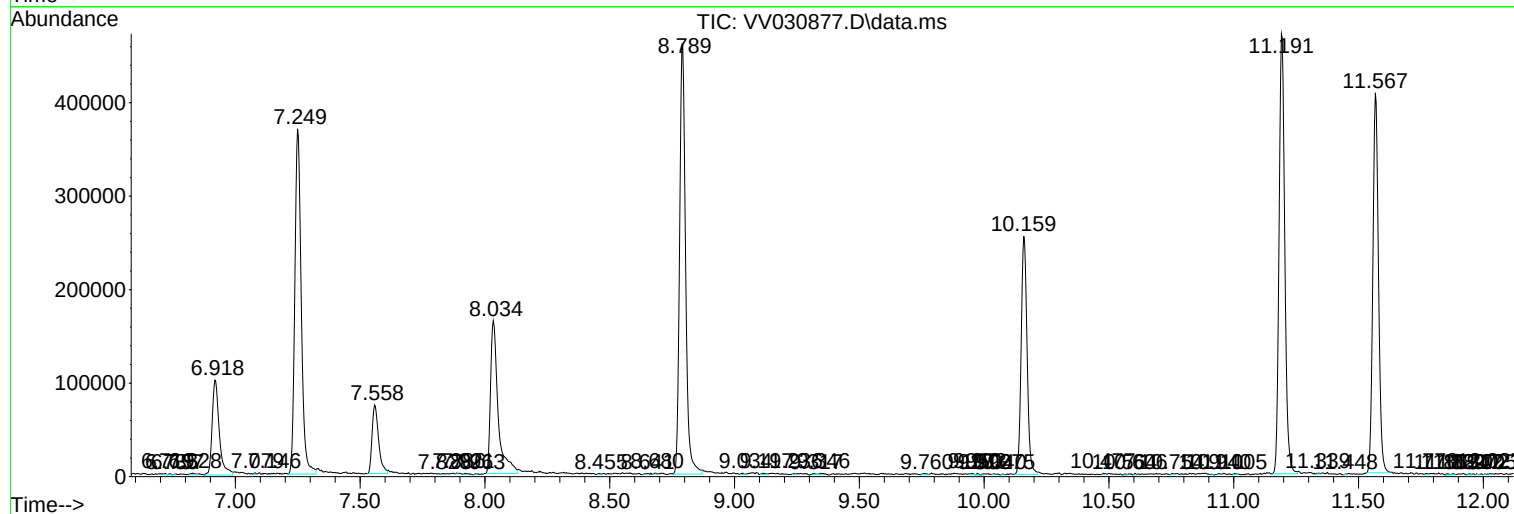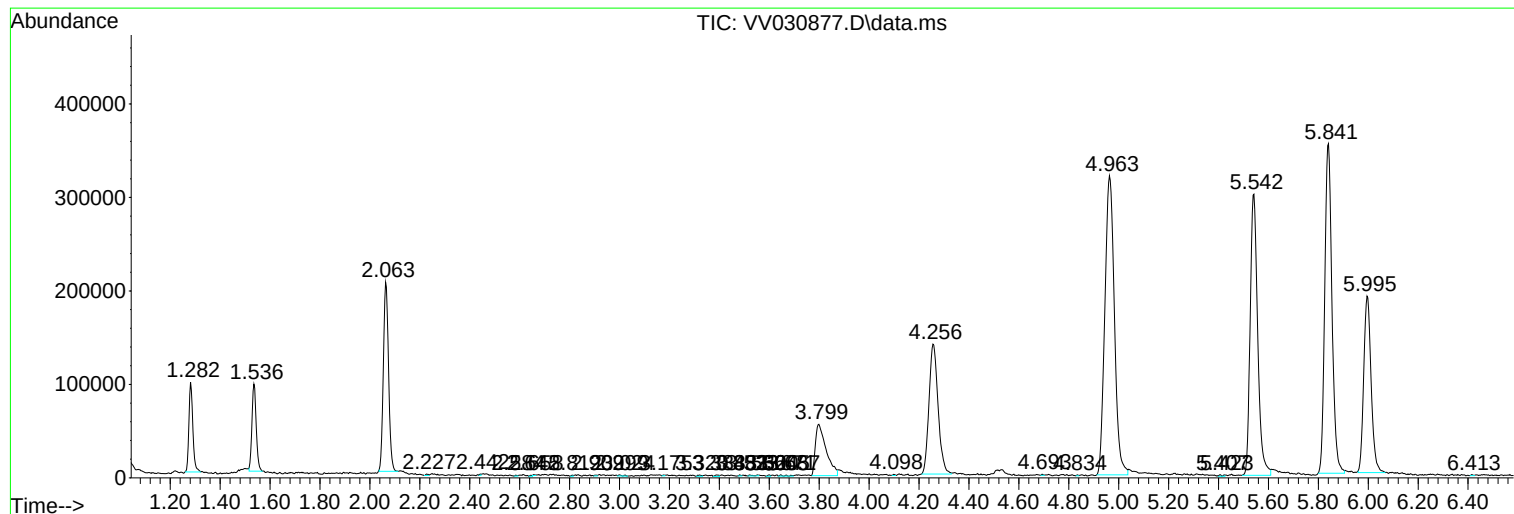

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042623\
Data File : VV030877.D
Acq On : 26 Apr 2023 14:02
Operator : SY/MD
Sample : 02474-05 10X
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 5 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0AS7

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM041723WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042623\
Data File : VV030877.D
Acq On : 26 Apr 2023 14:02
Operator : SY/MD
Sample : 02474-05 10X
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 5 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0AS7

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM041723WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------