

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042623\
 Data File : VV030878.D
 Acq On : 26 Apr 2023 14:26
 Operator : SY/MD
 Sample : 02475-08 50X
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0AX0

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM041723WMA.M

Title : VOC Analysis

Signal : TIC: VV030878.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.282	69	75	92	rVB	90865	98235	12.35%	1.546%
2	1.536	148	154	167	rVB	87501	106659	13.40%	1.678%
3	2.063	310	318	333	rBV	184523	268722	33.77%	4.229%
4	2.458	431	441	450	rBV4	9090	15396	1.93%	0.242%
5	2.860	564	566	569	rVB3	1065	533	0.07%	0.008%
6	2.880	569	572	574	rBV4	1218	747	0.09%	0.012%
7	2.918	579	584	585	rBV4	1082	713	0.09%	0.011%
8	2.973	599	601	603	rBV3	1002	705	0.09%	0.011%
9	3.060	625	628	629	rBV3	931	459	0.06%	0.007%
10	3.114	640	645	647	rBV7	1523	1236	0.16%	0.019%
11	3.143	652	654	657	rBV4	968	523	0.07%	0.008%
12	3.175	662	664	669	rVB4	1310	850	0.11%	0.013%
13	3.198	669	671	673	rBV3	1001	527	0.07%	0.008%
14	3.294	699	701	704	rBV3	1183	572	0.07%	0.009%
15	3.323	707	710	715	rVB5	1575	1438	0.18%	0.023%
16	3.372	721	725	728	rBV6	1085	936	0.12%	0.015%
17	3.478	755	758	760	rBV4	1169	716	0.09%	0.011%
18	3.503	763	766	769	rBV5	1168	581	0.07%	0.009%
19	3.568	782	786	788	rBV4	806	564	0.07%	0.009%
20	3.613	798	800	802	rBV2	1062	593	0.07%	0.009%
21	3.667	814	817	819	rBV4	884	576	0.07%	0.009%
22	3.699	825	827	832	rVB4	1161	849	0.11%	0.013%
23	3.725	832	835	836	rBV2	1235	642	0.08%	0.010%
24	3.761	845	846	849	rBV3	674	465	0.06%	0.007%
25	3.799	849	858	885	rVV2	53821	155431	19.53%	2.446%
26	4.259	986	1001	1024	rBV	133831	336662	42.31%	5.298%
27	4.812	1171	1173	1179	rVB5	1508	955	0.12%	0.015%
28	4.863	1187	1189	1190	rBV	1051	518	0.07%	0.008%
29	4.966	1204	1221	1247	rBV2	300569	795725	100.00%	12.522%
30	5.375	1346	1348	1349	rBV2	1177	442	0.06%	0.007%
31	5.465	1373	1376	1379	rBV4	1619	1033	0.13%	0.016%
32	5.542	1387	1400	1427	rBV	264917	560191	70.40%	8.815%
33	5.995	1530	1541	1566	rBV	177647	364823	45.85%	5.741%
34	6.195	1601	1603	1607	rBV5	1326	582	0.07%	0.009%
35	6.220	1609	1611	1614	rBV3	1180	668	0.08%	0.011%
36	6.503	1695	1699	1701	rVB4	1667	1264	0.16%	0.020%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW042623\
 Data File : VW030878.D
 Acq On : 26 Apr 2023 14:26
 Operator : SY/MD
 Sample : 02475-08 50X
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0AX0

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM041723WMA.M
 Title : VOC Analysis

37	6.516	1701	1703	1705	rBV3	1372	846	0.11%	0.013%
38	6.577	1719	1722	1724	rBV4	1391	942	0.12%	0.015%
39	6.648	1742	1744	1747	rVB4	1938	980	0.12%	0.015%
40	6.796	1786	1790	1793	rBV5	1407	1263	0.16%	0.020%
41	6.921	1817	1829	1849	rBV	93184	180240	22.65%	2.836%
42	7.079	1875	1878	1880	rBV4	1449	688	0.09%	0.011%
43	7.252	1920	1932	1952	rBV	341521	608954	76.53%	9.583%
44	7.561	2018	2028	2044	rBV2	69082	126314	15.87%	1.988%
45	7.738	2078	2083	2087	rBV6	1364	1522	0.19%	0.024%
46	7.863	2120	2122	2124	rBV2	926	580	0.07%	0.009%
47	8.034	2165	2175	2209	rBV	166747	346258	43.51%	5.449%
48	8.667	2370	2372	2373	rBV	1308	516	0.06%	0.008%
49	8.793	2400	2411	2432	rBV	407690	684480	86.02%	10.771%
50	9.165	2522	2527	2530	rBV5	1880	2200	0.28%	0.035%
51	9.339	2578	2581	2582	rBV3	898	600	0.08%	0.009%
52	9.362	2586	2588	2591	rBV3	1112	727	0.09%	0.011%
53	9.410	2601	2603	2606	rBV4	691	481	0.06%	0.008%
54	9.564	2649	2651	2654	rBV4	1191	684	0.09%	0.011%
55	9.667	2680	2683	2685	rBV3	1181	832	0.10%	0.013%
56	9.796	2718	2723	2726	rBV5	1451	1436	0.18%	0.023%
57	9.956	2771	2773	2774	rBV2	971	436	0.05%	0.007%
58	10.101	2815	2818	2821	rBV4	1031	551	0.07%	0.009%
59	10.162	2825	2837	2856	rVV	249031	402564	50.59%	6.335%
60	10.275	2868	2872	2873	rBV4	1432	1068	0.13%	0.017%
61	10.323	2885	2887	2889	rBV3	1584	775	0.10%	0.012%
62	10.336	2889	2891	2892	rBV2	1094	554	0.07%	0.009%
63	10.384	2902	2906	2907	rBV5	755	603	0.08%	0.009%
64	10.571	2962	2964	2967	rBV3	986	603	0.08%	0.009%
65	10.596	2970	2972	2973	rBV3	1344	535	0.07%	0.008%
66	10.667	2992	2994	2998	rBV4	825	595	0.07%	0.009%
67	10.741	3014	3017	3020	rVB3	1243	780	0.10%	0.012%
68	10.789	3030	3032	3034	rVB3	1330	458	0.06%	0.007%
69	10.998	3093	3097	3101	rBV5	1460	1526	0.19%	0.024%
70	11.194	3147	3158	3175	rBV	409815	650267	81.72%	10.233%
71	11.368	3210	3212	3215	rBV4	1231	649	0.08%	0.010%
72	11.567	3263	3274	3290	rBV	367862	587112	73.78%	9.239%
73	11.786	3340	3342	3344	rBV3	1385	601	0.08%	0.009%
74	11.821	3351	3353	3356	rVB3	1075	586	0.07%	0.009%
75	11.847	3356	3361	3363	rBV5	1692	1639	0.21%	0.026%
76	11.886	3371	3373	3379	rVB7	1099	743	0.09%	0.012%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW042623\
 Data File : VW030878.D
 Acq On : 26 Apr 2023 14:26
 Operator : SY/MD
 Sample : 02475-08 50X
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 COAX0

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM041723WMA.M
 Title : VOC Analysis

77	11.911	3379	3381	3383	rBV3	955	588	0.07%	0.009%
78	11.937	3387	3389	3390	rBV2	1335	576	0.07%	0.009%
79	11.972	3398	3400	3404	rBV5	1147	707	0.09%	0.011%
80	12.030	3415	3418	3421	rBV3	745	660	0.08%	0.010%
81	12.159	3455	3458	3460	rBV4	1324	1012	0.13%	0.016%
82	12.320	3506	3508	3512	rBV4	1231	844	0.11%	0.013%
83	12.419	3535	3539	3540	rBV3	1746	1086	0.14%	0.017%
84	12.506	3563	3566	3571	rVB6	870	620	0.08%	0.010%
85	12.590	3585	3592	3596	rBV8	1244	1827	0.23%	0.029%
86	12.657	3611	3613	3616	rVB4	1196	553	0.07%	0.009%
87	12.728	3633	3635	3639	rVB5	822	514	0.06%	0.008%
88	12.783	3649	3652	3654	rBV4	1268	958	0.12%	0.015%
89	13.098	3748	3750	3751	rVV	1221	438	0.06%	0.007%
90	13.127	3757	3759	3762	rBV3	722	468	0.06%	0.007%
91	13.275	3801	3805	3807	rBV4	1135	830	0.10%	0.013%
92	13.596	3902	3905	3908	rBV4	974	856	0.11%	0.013%
93	13.632	3914	3916	3918	rBV3	1073	613	0.08%	0.010%
94	13.831	3973	3978	3979	rBV5	1757	1157	0.15%	0.018%
95	14.037	4041	4042	4045	rBV3	1190	599	0.08%	0.009%
96	14.201	4091	4093	4098	rBV5	1288	814	0.10%	0.013%
97	14.416	4158	4160	4164	rVB5	1436	833	0.10%	0.013%
98	14.551	4200	4202	4203	rBV2	1321	445	0.06%	0.007%
99	14.664	4233	4237	4240	rBV6	1364	1229	0.15%	0.019%
100	15.458	4481	4484	4487	rBV4	2383	1807	0.23%	0.028%




Sum of corrected areas: 6354753

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042623\
Data File : VV030878.D
Acq On : 26 Apr 2023 14:26
Operator : SY/MD
Sample : 02475-08 50X
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 6 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
COAX0

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM041723WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

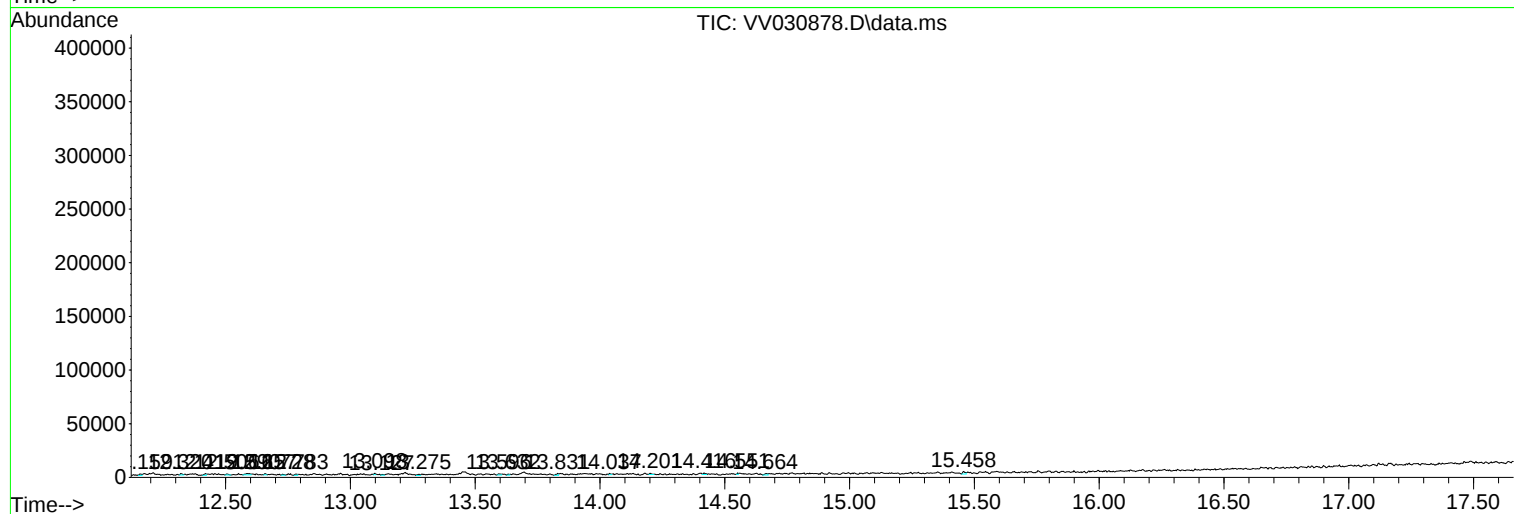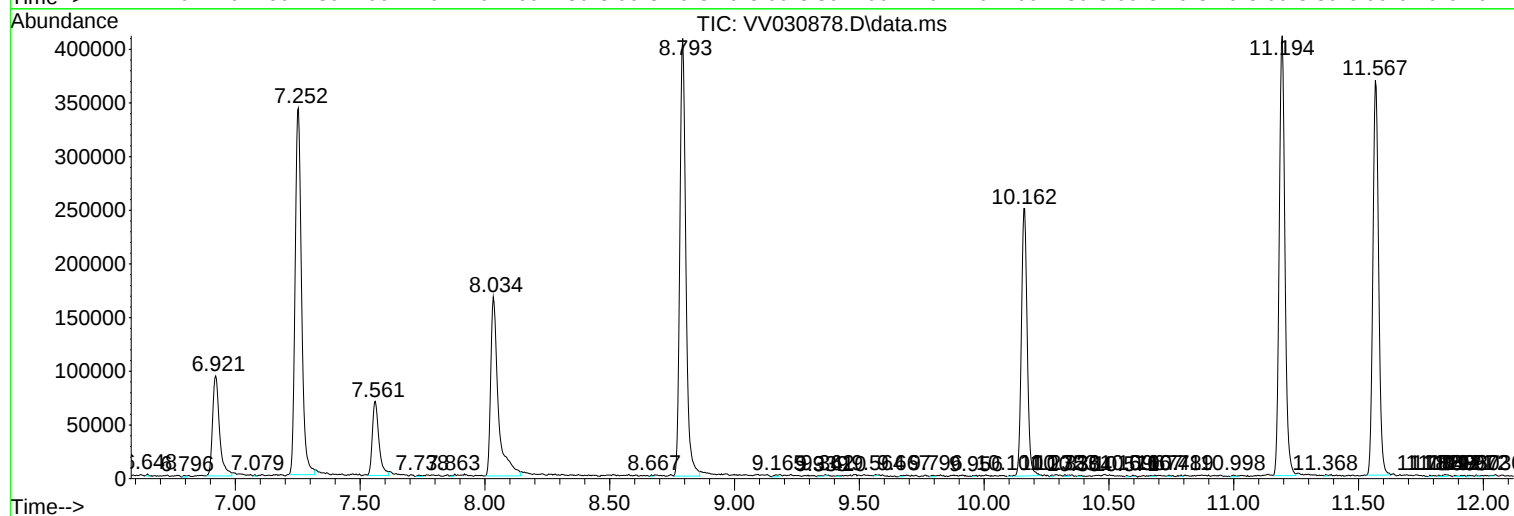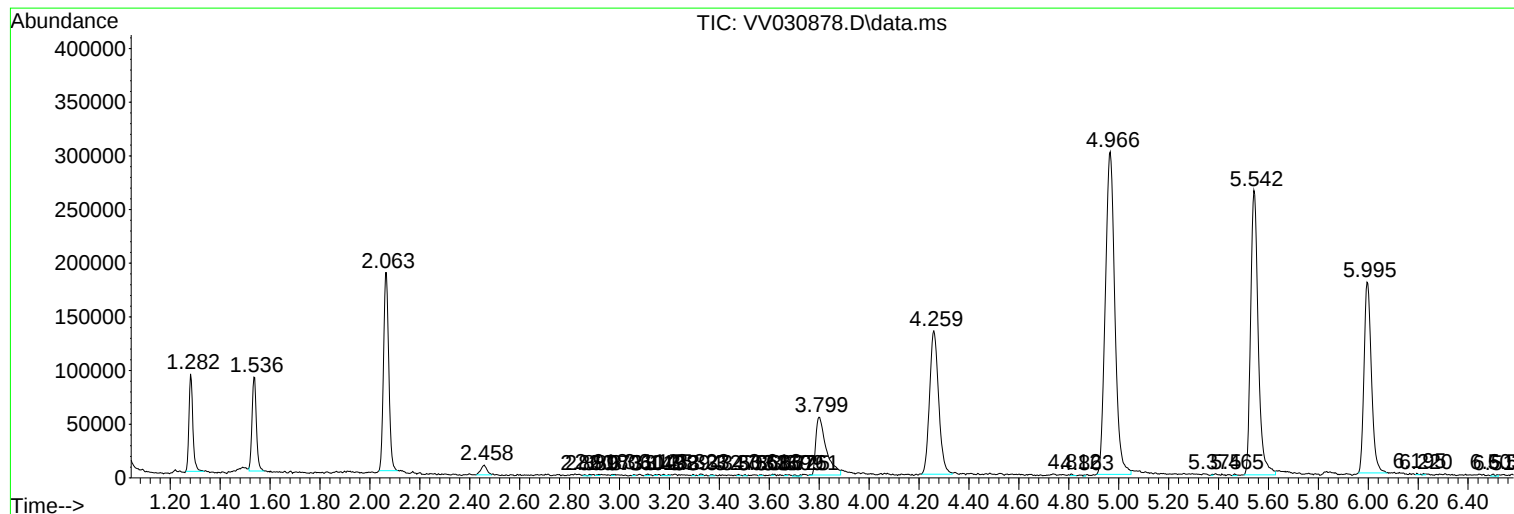

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042623\
Data File : VV030878.D
Acq On : 26 Apr 2023 14:26
Operator : SY/MD
Sample : 02475-08 50X
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 6 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0AX0

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM041723WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042623\
Data File : VV030878.D
Acq On : 26 Apr 2023 14:26
Operator : SY/MD
Sample : 02475-08 50X
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 6 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0AX0

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM041723WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------