

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042623\
 Data File : VV030879.D
 Acq On : 26 Apr 2023 14:50
 Operator : SY/MD
 Sample : 02475-10 50X
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0AX3

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM041723WMA.M
 Title : VOC Analysis

Signal : TIC: VV030879.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.282	69	75	88	rVB	88625	96102	12.31%	1.507%
2	1.536	148	154	170	rVB	85670	107819	13.82%	1.690%
3	2.066	310	319	333	rVB	184190	267666	34.30%	4.196%
4	2.246	371	375	380	rBV6	1328	1058	0.14%	0.017%
5	2.278	383	385	389	rVB4	1362	509	0.07%	0.008%
6	2.323	396	399	404	rBV6	1338	1213	0.16%	0.019%
7	2.458	432	441	448	rVV3	7648	12484	1.60%	0.196%
8	2.561	469	473	475	rVB4	991	625	0.08%	0.010%
9	2.593	479	483	485	rBV4	1021	831	0.11%	0.013%
10	2.626	490	493	497	rVB5	1414	963	0.12%	0.015%
11	2.664	504	505	509	rVV4	1337	677	0.09%	0.011%
12	2.928	582	587	588	rVV3	1174	960	0.12%	0.015%
13	3.188	663	668	671	rVB6	891	720	0.09%	0.011%
14	3.211	671	675	678	rBV5	1343	1052	0.13%	0.016%
15	3.288	696	699	702	rBV3	1303	811	0.10%	0.013%
16	3.336	709	714	716	rBV6	884	613	0.08%	0.010%
17	3.368	720	724	728	rBV6	1322	1432	0.18%	0.022%
18	3.445	746	748	752	rBV5	975	515	0.07%	0.008%
19	3.500	763	765	767	rBV3	1208	572	0.07%	0.009%
20	3.519	767	771	775	rVV6	923	751	0.10%	0.012%
21	3.616	798	801	802	rBV3	1325	628	0.08%	0.010%
22	3.732	834	837	839	rBV4	1039	757	0.10%	0.012%
23	3.799	849	858	888	rBV	53981	162399	20.81%	2.546%
24	4.259	984	1001	1022	rBV	132657	334655	42.88%	5.246%
25	4.661	1124	1126	1131	rBV4	1233	756	0.10%	0.012%
26	4.712	1140	1142	1145	rVB2	1338	530	0.07%	0.008%
27	4.732	1145	1148	1150	rBV4	1511	979	0.13%	0.015%
28	4.966	1205	1221	1243	rBV2	295753	780412	100.00%	12.234%
29	5.542	1388	1400	1428	rBV	264223	555823	71.22%	8.714%
30	5.844	1484	1494	1513	rVB2	57355	115326	14.78%	1.808%
31	5.998	1528	1542	1564	rBV	176610	373691	47.88%	5.858%
32	6.516	1699	1703	1706	rBV6	1262	859	0.11%	0.013%
33	6.551	1713	1714	1719	rBV5	830	734	0.09%	0.012%
34	6.805	1788	1793	1797	rBV6	1491	1370	0.18%	0.021%
35	6.921	1819	1829	1844	rBV	92618	170261	21.82%	2.669%
36	7.104	1884	1886	1892	rVB5	1331	1048	0.13%	0.016%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042623\
 Data File : VV030879.D
 Acq On : 26 Apr 2023 14:50
 Operator : SY/MD
 Sample : 02475-10 50X
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0AX3

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM041723WMA.M
 Title : VOC Analysis

37	7.252	1918	1932	1957	rBV	336745	613300	78.59%	9.615%
38	7.561	2019	2028	2048	rBV	66226	119640	15.33%	1.876%
39	7.748	2084	2086	2092	rBV6	1416	1099	0.14%	0.017%
40	7.957	2149	2151	2157	rVB5	1424	1011	0.13%	0.016%
41	8.034	2165	2175	2190	rBV	161852	311952	39.97%	4.890%
42	8.600	2347	2351	2354	rBV5	980	859	0.11%	0.013%
43	8.793	2400	2411	2430	rBV	403391	673044	86.24%	10.551%
44	9.227	2542	2546	2548	rBV4	1066	626	0.08%	0.010%
45	9.307	2569	2571	2572	rBV2	1038	527	0.07%	0.008%
46	9.323	2574	2576	2580	rVB5	1795	1132	0.15%	0.018%
47	9.355	2580	2586	2587	rBV5	964	833	0.11%	0.013%
48	9.471	2618	2622	2625	rBV5	1057	769	0.10%	0.012%
49	9.628	2667	2671	2673	rBV5	1702	1310	0.17%	0.021%
50	9.722	2697	2700	2702	rBV3	1021	661	0.08%	0.010%
51	9.815	2727	2729	2734	rBV4	1108	831	0.11%	0.013%
52	9.876	2745	2748	2759	rVB4	1625	2019	0.26%	0.032%
53	9.960	2770	2774	2777	rBV5	1425	979	0.13%	0.015%
54	9.982	2777	2781	2782	rBV4	863	593	0.08%	0.009%
55	10.030	2794	2796	2798	rBV2	1136	525	0.07%	0.008%
56	10.046	2799	2801	2805	rVB5	1260	723	0.09%	0.011%
57	10.159	2826	2836	2850	rBV	247006	391890	50.22%	6.144%
58	10.310	2881	2883	2887	rVB5	1319	541	0.07%	0.008%
59	10.358	2895	2898	2900	rBV4	1265	624	0.08%	0.010%
60	10.461	2927	2930	2932	rBV4	1112	823	0.11%	0.013%
61	10.645	2982	2987	2989	rBV6	896	750	0.10%	0.012%
62	10.812	3036	3039	3042	rBV3	1224	982	0.13%	0.015%
63	10.857	3048	3053	3054	rBV5	1840	1462	0.19%	0.023%
64	10.927	3073	3075	3081	rVB6	1073	890	0.11%	0.014%
65	11.194	3147	3158	3176	rBV	401741	635569	81.44%	9.964%
66	11.394	3218	3220	3224	rVB5	1768	1016	0.13%	0.016%
67	11.455	3236	3239	3241	rBV3	936	590	0.08%	0.009%
68	11.516	3257	3258	3260	rBV2	922	515	0.07%	0.008%
69	11.567	3262	3274	3292	rVV	363623	583527	74.77%	9.148%
70	11.825	3349	3354	3355	rBV4	1049	911	0.12%	0.014%
71	12.001	3405	3409	3412	rBV5	1353	1100	0.14%	0.017%
72	12.017	3412	3414	3417	rVB4	1368	644	0.08%	0.010%
73	12.117	3440	3445	3447	rBV5	1538	1158	0.15%	0.018%
74	12.130	3447	3449	3452	rVB4	1124	617	0.08%	0.010%
75	12.432	3541	3543	3546	rVB3	1441	759	0.10%	0.012%
76	12.596	3589	3594	3597	rBV6	1480	1496	0.19%	0.023%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042623\
 Data File : VV030879.D
 Acq On : 26 Apr 2023 14:50
 Operator : SY/MD
 Sample : 02475-10 50X
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0AX3

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM041723WMA.M
 Title : VOC Analysis

77	12.667	3612	3616	3619	rBV6	1489	1366	0.18%	0.021%
78	12.734	3634	3637	3640	rVB6	1155	570	0.07%	0.009%
79	12.808	3654	3660	3663	rBV7	1230	1159	0.15%	0.018%
80	12.927	3693	3697	3700	rBV6	1202	1139	0.15%	0.018%
81	12.966	3702	3709	3713	rBV9	1873	1940	0.25%	0.030%
82	13.024	3724	3727	3731	rVB5	1028	647	0.08%	0.010%
83	13.056	3731	3737	3739	rBV6	1649	1462	0.19%	0.023%
84	13.255	3796	3799	3803	rBV6	766	516	0.07%	0.008%
85	13.304	3811	3814	3818	rVB3	1665	1122	0.14%	0.018%
86	13.329	3818	3822	3826	rBV5	1181	964	0.12%	0.015%
87	13.458	3858	3862	3866	rVB7	2520	2483	0.32%	0.039%
88	13.622	3909	3913	3915	rBV4	753	508	0.07%	0.008%
89	13.673	3927	3929	3931	rBV3	1005	646	0.08%	0.010%
90	13.751	3949	3953	3955	rBV5	1006	869	0.11%	0.014%
91	13.783	3961	3963	3966	rBV4	857	628	0.08%	0.010%
92	13.837	3976	3980	3983	rBV6	1574	1054	0.14%	0.017%
93	13.895	3995	3998	3999	rBV2	838	498	0.06%	0.008%
94	14.130	4068	4071	4073	rBV3	1398	792	0.10%	0.012%
95	14.226	4099	4101	4104	rBV5	825	549	0.07%	0.009%
96	14.619	4219	4223	4224	rBV2	1467	835	0.11%	0.013%
97	14.815	4282	4284	4287	rBV4	1227	610	0.08%	0.010%
98	15.059	4358	4360	4362	rBV3	1321	857	0.11%	0.013%
99	15.271	4425	4426	4428	rBV3	1374	632	0.08%	0.010%
100	15.387	4461	4462	4467	rBV5	1694	1078	0.14%	0.017%




Sum of corrected areas: 6378822

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042623\
Data File : VV030879.D
Acq On : 26 Apr 2023 14:50
Operator : SY/MD
Sample : 02475-10 50X
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 7 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0AX3

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM041723WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

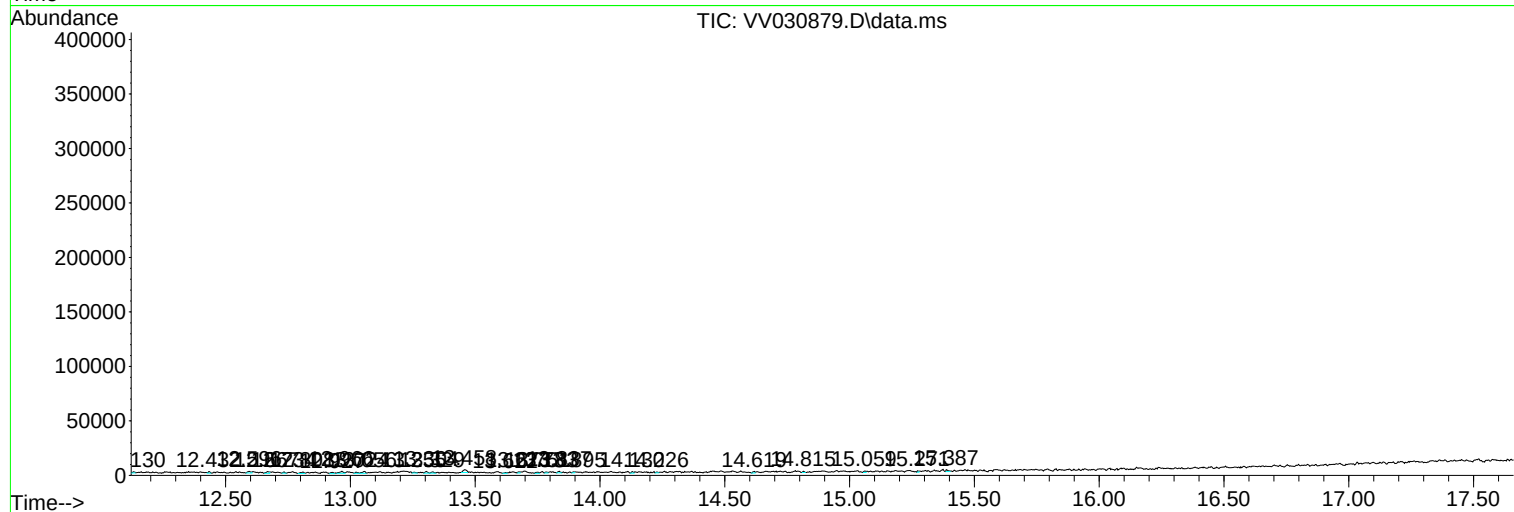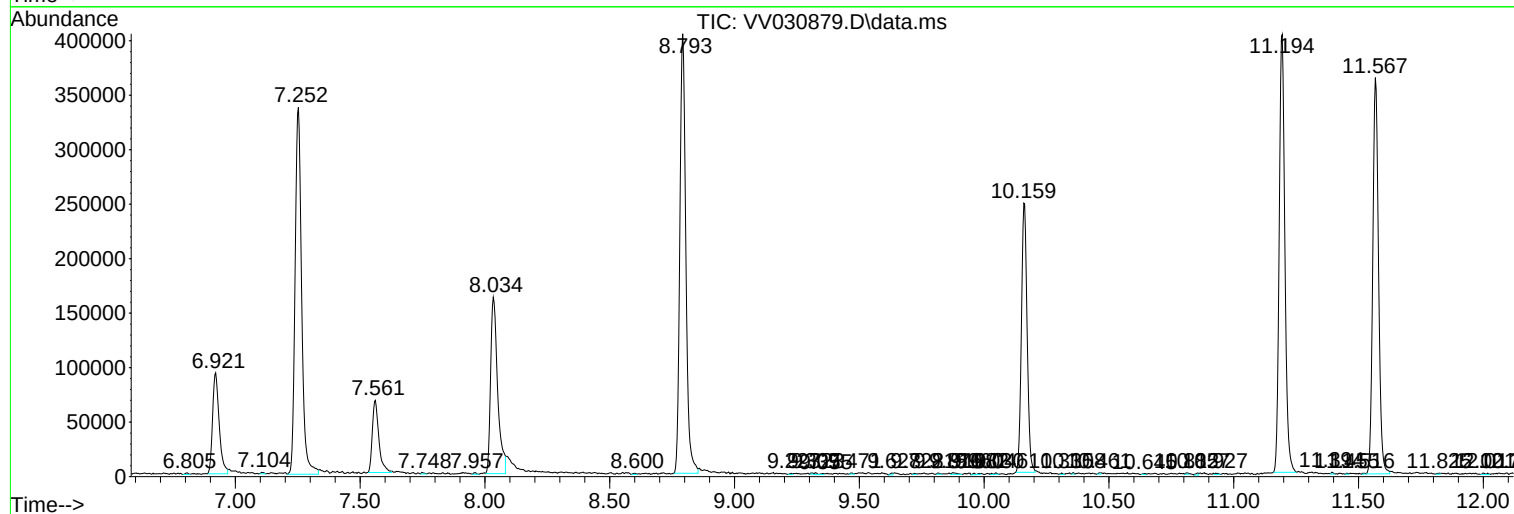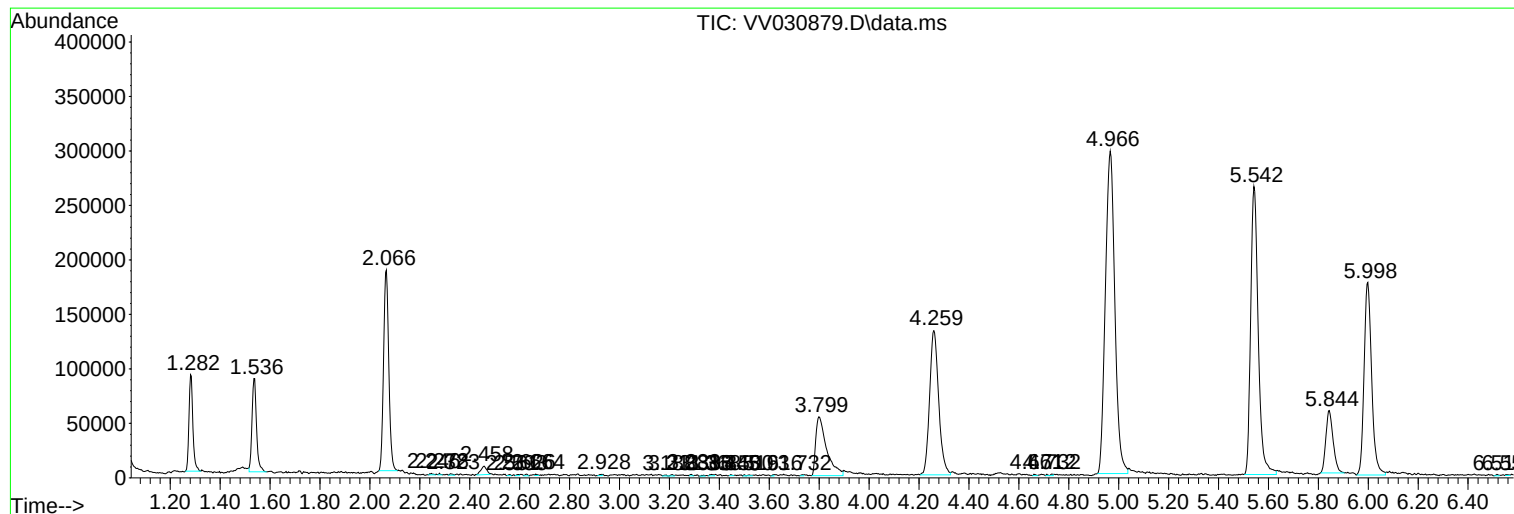

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042623\
Data File : VV030879.D
Acq On : 26 Apr 2023 14:50
Operator : SY/MD
Sample : 02475-10 50X
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 7 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0AX3

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM041723WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042623\
Data File : VV030879.D
Acq On : 26 Apr 2023 14:50
Operator : SY/MD
Sample : 02475-10 50X
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 7 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0AX3

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM041723WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------