

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042623\
 Data File : VV030881.D
 Acq On : 26 Apr 2023 15:36
 Operator : SY/MD
 Sample : 02475-02
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0AW4

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM041723WMA.M
 Title : VOC Analysis

Signal : TIC: VV030881.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.281	69	75	86	rBV	82970	91442	4.23%	1.086%
2	1.536	148	154	167	rVB	78007	95176	4.40%	1.130%
3	2.066	310	319	332	rBV	179348	266620	12.33%	3.166%
4	2.188	354	357	361	rBV5	884	844	0.04%	0.010%
5	2.445	434	437	439	rBV4	1186	816	0.04%	0.010%
6	2.523	459	461	466	rBV6	1514	1034	0.05%	0.012%
7	2.552	467	470	471	rBV4	1410	811	0.04%	0.010%
8	2.622	490	492	494	rBV3	1105	525	0.02%	0.006%
9	2.667	502	506	509	rVB5	1040	806	0.04%	0.010%
10	2.767	533	537	539	rBV5	1695	1266	0.06%	0.015%
11	3.021	613	616	620	rBV5	1228	922	0.04%	0.011%
12	3.040	620	622	627	rVB4	1017	850	0.04%	0.010%
13	3.095	637	639	641	rBV3	1092	671	0.03%	0.008%
14	3.201	670	672	678	rVB6	1067	954	0.04%	0.011%
15	3.314	704	707	711	rVB6	1259	1043	0.05%	0.012%
16	3.336	711	714	718	rBV5	1456	1229	0.06%	0.015%
17	3.407	732	736	737	rBV5	1028	647	0.03%	0.008%
18	3.558	781	783	789	rVB6	1597	969	0.04%	0.012%
19	3.629	800	805	810	rVV8	1389	1361	0.06%	0.016%
20	3.751	840	843	844	rBV2	1633	806	0.04%	0.010%
21	3.822	849	865	892	rVV4	86554	308071	14.24%	3.659%
22	4.182	975	977	981	rBV6	906	560	0.03%	0.007%
23	4.262	988	1002	1026	rVB	124814	313188	14.48%	3.720%
24	4.732	1146	1148	1151	rBV3	1264	915	0.04%	0.011%
25	4.789	1163	1166	1167	rBV2	790	528	0.02%	0.006%
26	4.966	1204	1221	1248	rBV2	282691	758513	35.07%	9.008%
27	5.275	1313	1317	1320	rVB4	1643	1362	0.06%	0.016%
28	5.297	1320	1324	1328	rBV6	1546	1494	0.07%	0.018%
29	5.317	1328	1330	1332	rBV2	1825	1025	0.05%	0.012%
30	5.445	1368	1370	1374	rBV4	1055	632	0.03%	0.008%
31	5.542	1388	1400	1426	rBV	258455	537315	24.84%	6.381%
32	5.841	1479	1493	1521	rBV	1105041	2162863	100.00%	25.687%
33	5.998	1532	1542	1559	rVB	170524	340126	15.73%	4.039%
34	6.522	1701	1705	1706	rBV4	1072	548	0.03%	0.007%
35	6.571	1718	1720	1725	rBV7	897	636	0.03%	0.008%
36	6.709	1760	1763	1768	rBV6	2462	2377	0.11%	0.028%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW042623\
 Data File : VW030881.D
 Acq On : 26 Apr 2023 15:36
 Operator : SY/MD
 Sample : 02475-02
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0AW4

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM041723WMA.M
 Title : VOC Analysis

37	6.921	1818	1829	1843	rBV	89730	166530	7.70%	1.978%
38	7.252	1920	1932	1958	rBV	317942	581862	26.90%	6.910%
39	7.468	1997	1999	2002	rBV4	1785	1186	0.05%	0.014%
40	7.561	2018	2028	2042	rBV	65582	117408	5.43%	1.394%
41	7.982	2156	2159	2162	rBV3	1209	982	0.05%	0.012%
42	8.034	2166	2175	2207	rVV	160425	326105	15.08%	3.873%
43	8.426	2294	2297	2300	rBV4	1402	1106	0.05%	0.013%
44	8.506	2319	2322	2326	rVB4	1331	900	0.04%	0.011%
45	8.744	2392	2396	2399	rBV6	1151	1092	0.05%	0.013%
46	8.792	2400	2411	2432	rVV	395008	656709	30.36%	7.799%
47	9.040	2483	2488	2489	rBV3	1447	1074	0.05%	0.013%
48	9.188	2529	2534	2535	rVV4	1022	776	0.04%	0.009%
49	9.243	2547	2551	2552	rBV4	1265	904	0.04%	0.011%
50	9.342	2579	2582	2584	rBV3	1496	1009	0.05%	0.012%
51	9.381	2591	2594	2596	rBV4	766	535	0.02%	0.006%
52	9.397	2596	2599	2602	rVV5	977	787	0.04%	0.009%
53	9.654	2677	2679	2681	rBV3	1158	738	0.03%	0.009%
54	9.747	2703	2708	2709	rBV4	1143	736	0.03%	0.009%
55	9.870	2743	2746	2748	rBV4	1413	916	0.04%	0.011%
56	9.989	2781	2783	2786	rBV3	794	707	0.03%	0.008%
57	10.021	2789	2793	2796	rVB4	840	525	0.02%	0.006%
58	10.043	2796	2800	2802	rBV5	1368	1056	0.05%	0.013%
59	10.162	2822	2837	2855	rBV	235555	390050	18.03%	4.632%
60	10.336	2882	2891	2900	rVB2	18017	29986	1.39%	0.356%
61	10.429	2914	2920	2923	rBV6	1864	1662	0.08%	0.020%
62	10.612	2971	2977	2982	rBV9	1158	1501	0.07%	0.018%
63	10.712	3005	3008	3009	rBV3	804	514	0.02%	0.006%
64	10.741	3015	3017	3020	rBV4	1183	715	0.03%	0.008%
65	10.902	3065	3067	3070	rVB4	1087	724	0.03%	0.009%
66	10.937	3075	3078	3080	rBV4	1374	789	0.04%	0.009%
67	11.059	3113	3116	3118	rBV4	1353	869	0.04%	0.010%
68	11.194	3147	3158	3176	rBV	399526	626533	28.97%	7.441%
69	11.304	3188	3192	3196	rBV6	1625	1632	0.08%	0.019%
70	11.464	3240	3242	3246	rVB5	787	570	0.03%	0.007%
71	11.497	3248	3252	3253	rBV4	1003	790	0.04%	0.009%
72	11.567	3264	3274	3296	rVB	350858	563554	26.06%	6.693%
73	11.763	3332	3335	3336	rBV3	1016	691	0.03%	0.008%
74	11.879	3369	3371	3376	rVB4	1331	1096	0.05%	0.013%
75	12.204	3463	3472	3480	rBV6	4941	8537	0.39%	0.101%
76	12.259	3485	3489	3492	rVB5	1558	1128	0.05%	0.013%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042623\
 Data File : VV030881.D
 Acq On : 26 Apr 2023 15:36
 Operator : SY/MD
 Sample : 02475-02
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0AW4

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM041723WMA.M
 Title : VOC Analysis

77	12.278	3492	3495	3496	rBV2	1463	801	0.04%	0.010%
78	12.455	3549	3550	3555	rVB4	1198	758	0.04%	0.009%
79	12.484	3555	3559	3561	rBV4	1441	1247	0.06%	0.015%
80	12.564	3579	3584	3585	rBV4	1309	810	0.04%	0.010%
81	12.754	3640	3643	3646	rVB5	1353	618	0.03%	0.007%
82	12.789	3651	3654	3657	rBV3	1300	1228	0.06%	0.015%
83	12.966	3707	3709	3711	rBV4	1026	548	0.03%	0.007%
84	13.095	3744	3749	3751	rBV5	1250	1135	0.05%	0.013%
85	13.217	3781	3787	3793	rVB8	2185	2857	0.13%	0.034%
86	13.249	3793	3797	3802	rBV6	1353	1533	0.07%	0.018%
87	13.313	3814	3817	3820	rBV5	1307	794	0.04%	0.009%
88	13.355	3826	3830	3832	rBV5	1373	1078	0.05%	0.013%
89	13.561	3887	3894	3896	rBV5	1529	1589	0.07%	0.019%
90	13.603	3904	3907	3914	rBV8	1461	1541	0.07%	0.018%
91	13.635	3914	3917	3918	rBV3	1551	909	0.04%	0.011%
92	13.670	3925	3928	3929	rBV3	1299	711	0.03%	0.008%
93	13.795	3964	3967	3968	rBV2	1126	596	0.03%	0.007%
94	13.879	3989	3993	4000	rBV8	1377	1736	0.08%	0.021%
95	13.914	4002	4004	4007	rVB4	1350	686	0.03%	0.008%
96	13.937	4007	4011	4014	rBV5	2184	1644	0.08%	0.020%
97	14.062	4047	4050	4052	rBV3	913	604	0.03%	0.007%
98	14.207	4090	4095	4096	rBV4	1665	1480	0.07%	0.018%
99	14.339	4134	4136	4140	rBV5	1292	728	0.03%	0.009%
100	14.541	4197	4199	4200	rBV2	1235	580	0.03%	0.007%




Sum of corrected areas: 8420140

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042623\
Data File : VV030881.D
Acq On : 26 Apr 2023 15:36
Operator : SY/MD
Sample : 02475-02
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 9 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0AW4

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM041723WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

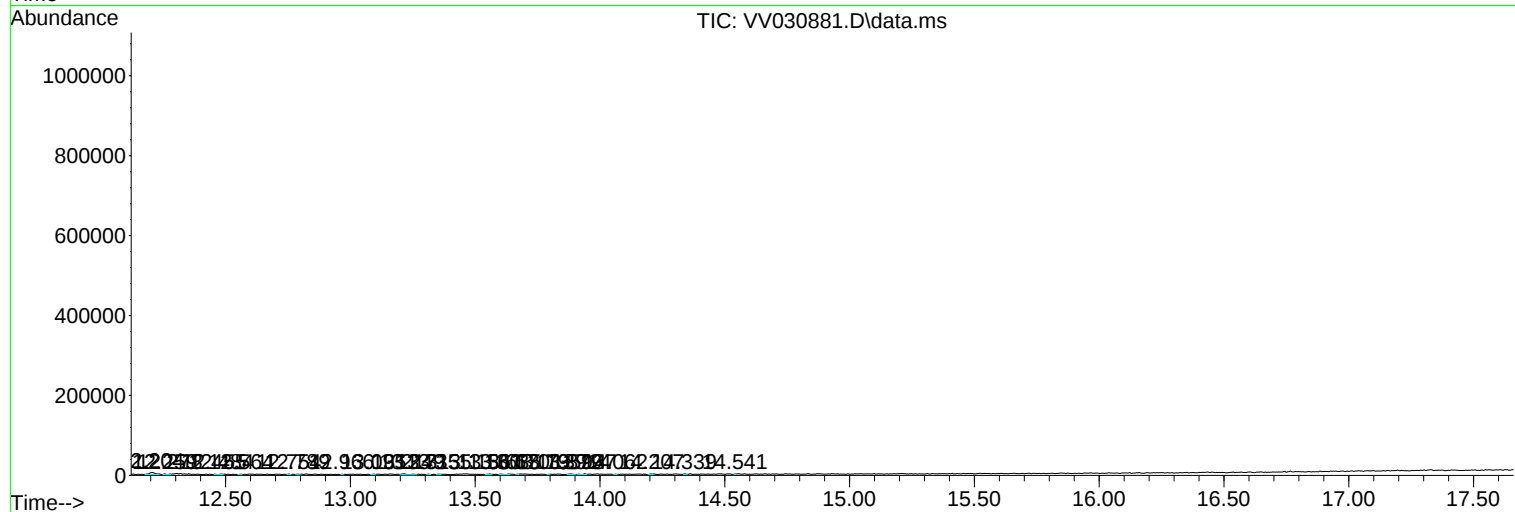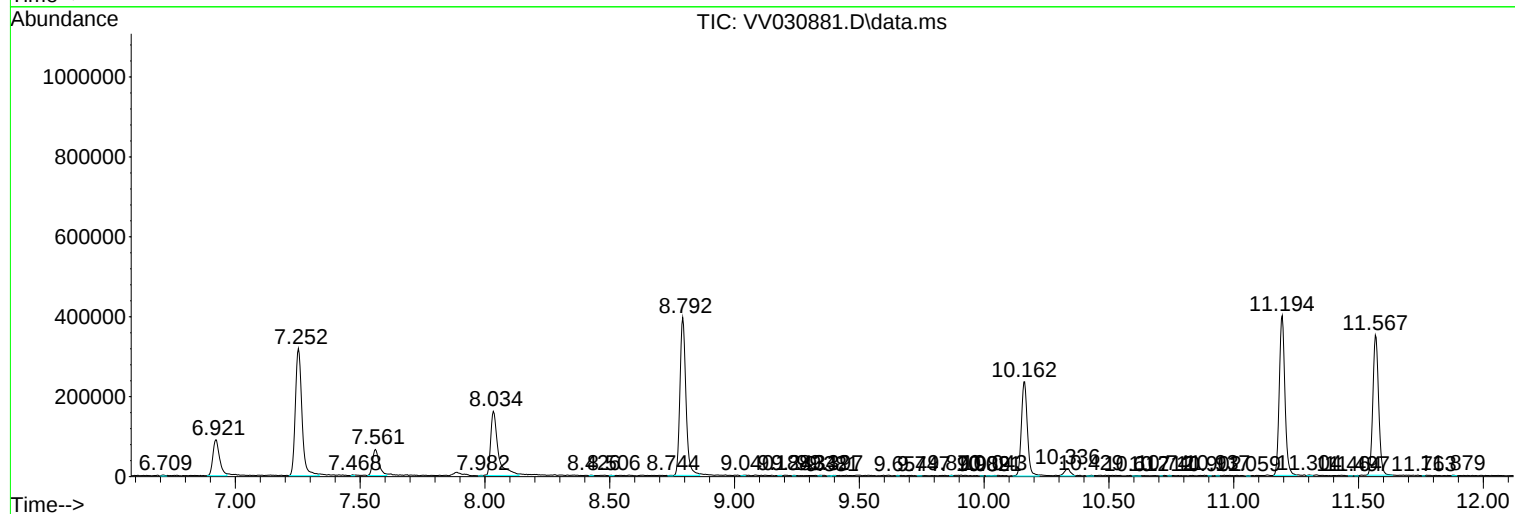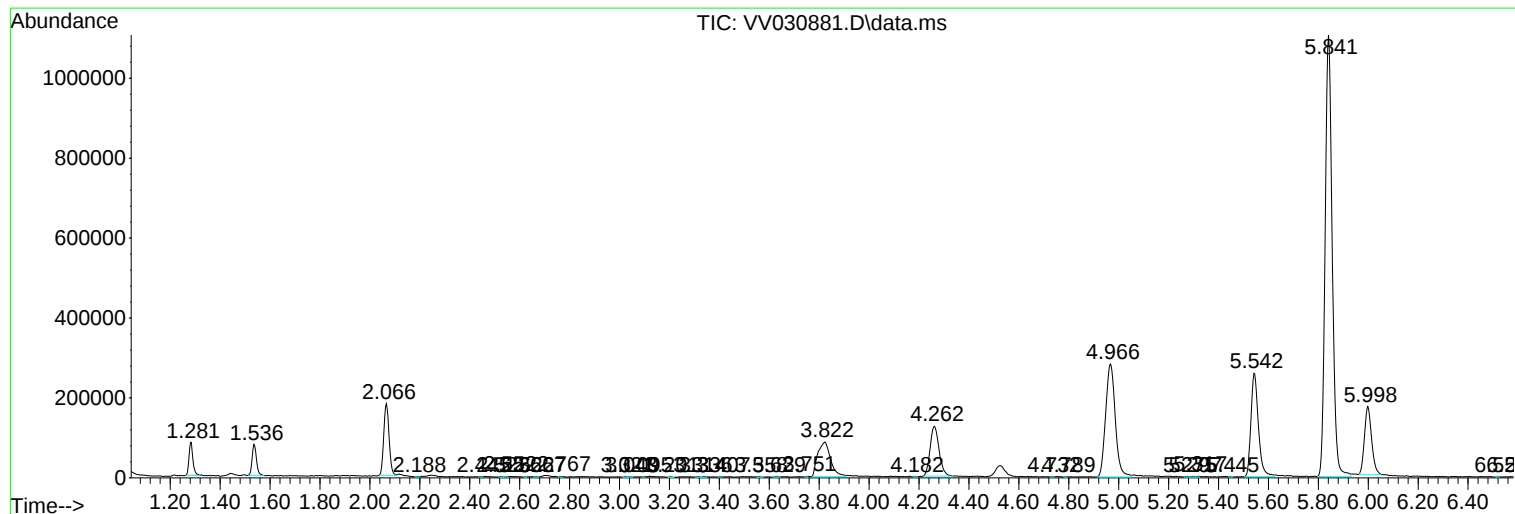

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042623\
Data File : VV030881.D
Acq On : 26 Apr 2023 15:36
Operator : SY/MD
Sample : 02475-02
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 9 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0AW4

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM041723WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042623\
Data File : VV030881.D
Acq On : 26 Apr 2023 15:36
Operator : SY/MD
Sample : 02475-02
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 9 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0AW4

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM041723WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc