

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042623\
 Data File : VV030882.D
 Acq On : 26 Apr 2023 16:00
 Operator : SY/MD
 Sample : 02475-09
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0AX2

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM041723WMA.M
 Title : VOC Analysis

Signal : TIC: VV030882.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.281	69	75	88	rVB	91910	98456	12.68%	1.621%
2	1.535	148	154	167	rVB	91239	109701	14.13%	1.806%
3	2.066	310	319	334	rBV	187971	275710	35.50%	4.539%
4	2.510	454	457	458	rBV3	1156	558	0.07%	0.009%
5	2.616	487	490	494	rBV6	1831	1428	0.18%	0.024%
6	2.651	498	501	505	rVB5	1597	1363	0.18%	0.022%
7	2.686	505	512	514	rBV8	1764	1938	0.25%	0.032%
8	2.764	533	536	537	rBV3	944	543	0.07%	0.009%
9	2.850	561	563	568	rVB6	1561	788	0.10%	0.013%
10	3.204	670	673	674	rBV3	1381	693	0.09%	0.011%
11	3.268	691	693	697	rBV4	950	575	0.07%	0.009%
12	3.317	704	708	710	rVB4	940	584	0.08%	0.010%
13	3.429	739	743	744	rVV5	1129	751	0.10%	0.012%
14	3.452	748	750	752	rBV3	764	497	0.06%	0.008%
15	3.494	760	763	764	rBV2	1390	767	0.10%	0.013%
16	3.629	803	805	807	rBV3	1022	618	0.08%	0.010%
17	3.754	841	844	847	rVB5	1428	950	0.12%	0.016%
18	3.799	848	858	886	rBV	55565	165709	21.34%	2.728%
19	4.262	985	1002	1026	rBV2	129306	338803	43.63%	5.578%
20	4.484	1069	1071	1074	rBV3	1746	920	0.12%	0.015%
21	4.686	1132	1134	1138	rBV4	1366	734	0.09%	0.012%
22	4.712	1138	1142	1143	rBV2	1201	549	0.07%	0.009%
23	4.728	1144	1147	1148	rVV2	1647	931	0.12%	0.015%
24	4.744	1150	1152	1156	rVV4	1441	801	0.10%	0.013%
25	4.966	1205	1221	1244	rBV2	287228	776619	100.00%	12.785%
26	5.442	1366	1369	1371	rBV4	1215	688	0.09%	0.011%
27	5.542	1386	1400	1420	rBV	227297	481137	61.95%	7.921%
28	5.998	1529	1542	1562	rBV	174014	362594	46.69%	5.969%
29	6.448	1678	1682	1685	rBV5	1157	867	0.11%	0.014%
30	6.487	1691	1694	1695	rBV2	1035	564	0.07%	0.009%
31	6.677	1750	1753	1757	rBV5	1117	852	0.11%	0.014%
32	6.735	1769	1771	1774	rBV3	1166	822	0.11%	0.014%
33	6.921	1817	1829	1848	rBV	91791	172970	22.27%	2.848%
34	7.252	1918	1932	1960	rBV	330165	600703	77.35%	9.889%
35	7.480	2000	2003	2004	rBV2	1580	733	0.09%	0.012%
36	7.561	2018	2028	2045	rBV	67626	121025	15.58%	1.992%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW042623\
 Data File : VW030882.D
 Acq On : 26 Apr 2023 16:00
 Operator : SY/MD
 Sample : 02475-09
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0AX2

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM041723WMA.M
 Title : VOC Analysis

37	7.796	2099	2101	2105	rBV4	1265	761	0.10%	0.013%
38	7.834	2110	2113	2115	rBV4	773	548	0.07%	0.009%
39	7.886	2122	2129	2137	rVB6	4903	7998	1.03%	0.132%
40	7.956	2150	2151	2155	rBV4	997	784	0.10%	0.013%
41	8.034	2165	2175	2211	rBV	162827	339390	43.70%	5.587%
42	8.792	2399	2411	2435	rBV	356797	593874	76.47%	9.777%
43	9.062	2493	2495	2498	rVV4	901	575	0.07%	0.009%
44	9.265	2553	2558	2561	rBV7	1508	1609	0.21%	0.026%
45	9.477	2622	2624	2628	rBV3	1561	811	0.10%	0.013%
46	9.580	2653	2656	2658	rBV4	1487	1172	0.15%	0.019%
47	9.612	2664	2666	2669	rBV3	814	605	0.08%	0.010%
48	9.641	2673	2675	2677	rBV3	991	527	0.07%	0.009%
49	9.718	2696	2699	2702	rBV5	1179	841	0.11%	0.014%
50	9.776	2715	2717	2722	rVB5	1377	1096	0.14%	0.018%
51	9.805	2722	2726	2728	rVB4	1061	674	0.09%	0.011%
52	9.824	2728	2732	2734	rBV5	984	669	0.09%	0.011%
53	9.969	2774	2777	2780	rBV3	1402	672	0.09%	0.011%
54	10.024	2786	2794	2798	rBV9	1166	1847	0.24%	0.030%
55	10.114	2820	2822	2825	rBV4	1091	627	0.08%	0.010%
56	10.159	2825	2836	2860	rVB	244798	402319	51.80%	6.623%
57	10.249	2860	2864	2865	rBV3	1370	1069	0.14%	0.018%
58	10.291	2872	2877	2880	rBV6	1339	1063	0.14%	0.017%
59	10.336	2880	2891	2903	rBV	8912	18436	2.37%	0.304%
60	10.410	2911	2914	2917	rBV5	1340	640	0.08%	0.011%
61	10.439	2922	2923	2926	rVB3	1139	558	0.07%	0.009%
62	10.686	2997	3000	3001	rBV2	1142	596	0.08%	0.010%
63	10.763	3021	3024	3029	rBV6	1278	1306	0.17%	0.022%
64	10.853	3049	3052	3054	rBV3	1579	1087	0.14%	0.018%
65	11.104	3127	3130	3133	rBV5	677	505	0.07%	0.008%
66	11.194	3146	3158	3179	rBV	353059	565168	72.77%	9.304%
67	11.387	3215	3218	3220	rBV4	1243	816	0.11%	0.013%
68	11.467	3237	3243	3244	rBV5	1137	816	0.11%	0.013%
69	11.477	3244	3246	3249	rVB3	1241	658	0.08%	0.011%
70	11.567	3263	3274	3293	rBV	358766	572193	73.68%	9.420%
71	11.738	3325	3327	3329	rBV3	1202	750	0.10%	0.012%
72	11.786	3337	3342	3345	rBV6	2018	1687	0.22%	0.028%
73	11.892	3374	3375	3381	rBV5	983	1055	0.14%	0.017%
74	12.040	3418	3421	3424	rBV3	1089	753	0.10%	0.012%
75	12.120	3444	3446	3453	rBV7	1037	1203	0.15%	0.020%
76	12.184	3462	3466	3468	rBV4	1756	1227	0.16%	0.020%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042623\
 Data File : VV030882.D
 Acq On : 26 Apr 2023 16:00
 Operator : SY/MD
 Sample : 02475-09
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0AX2

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM041723WMA.M
 Title : VOC Analysis

77	12.313	3502	3506	3509	rBV6	1451	795	0.10%	0.013%
78	12.477	3549	3557	3559	rBV9	1485	1651	0.21%	0.027%
79	12.551	3578	3580	3585	rVB4	2073	1192	0.15%	0.020%
80	12.583	3587	3590	3592	rBV4	943	558	0.07%	0.009%
81	12.596	3592	3594	3597	rBV4	1574	1054	0.14%	0.017%
82	12.631	3602	3605	3607	rBV3	1108	593	0.08%	0.010%
83	12.644	3607	3609	3613	rVB4	1428	913	0.12%	0.015%
84	12.683	3617	3621	3622	rBV3	1008	695	0.09%	0.011%
85	12.709	3627	3629	3632	rBV3	1124	687	0.09%	0.011%
86	12.773	3645	3649	3651	rBV3	1260	1086	0.14%	0.018%
87	12.834	3665	3668	3671	rBV3	829	704	0.09%	0.012%
88	13.120	3749	3757	3763	rBV10	1471	2256	0.29%	0.037%
89	13.297	3810	3812	3817	rVB6	1105	608	0.08%	0.010%
90	13.419	3846	3850	3853	rBV6	1400	1196	0.15%	0.020%
91	13.615	3908	3911	3913	rBV4	1290	635	0.08%	0.010%
92	13.741	3948	3950	3953	rVB3	1561	664	0.09%	0.011%
93	13.856	3985	3986	3991	rVB5	1244	779	0.10%	0.013%
94	13.882	3991	3994	3995	rBV3	1365	639	0.08%	0.011%
95	14.210	4092	4096	4099	rBV4	1516	1193	0.15%	0.020%
96	14.361	4139	4143	4146	rBV6	1115	786	0.10%	0.013%
97	14.448	4167	4170	4171	rBV4	1465	782	0.10%	0.013%
98	14.789	4274	4276	4279	rBV3	1387	866	0.11%	0.014%
99	14.946	4323	4325	4327	rBV3	1428	599	0.08%	0.010%
100	15.172	4393	4395	4396	rBV2	1427	494	0.06%	0.008%




Sum of corrected areas: 6074351

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042623\
Data File : VV030882.D
Acq On : 26 Apr 2023 16:00
Operator : SY/MD
Sample : 02475-09
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 10 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0AX2

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM041723WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

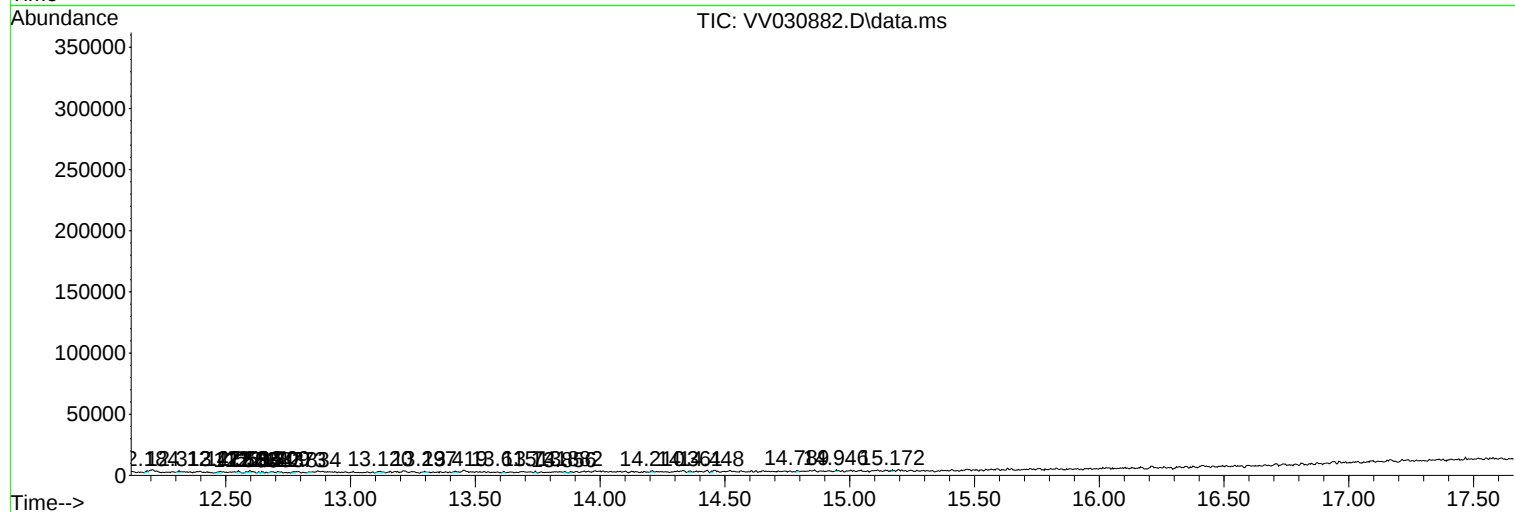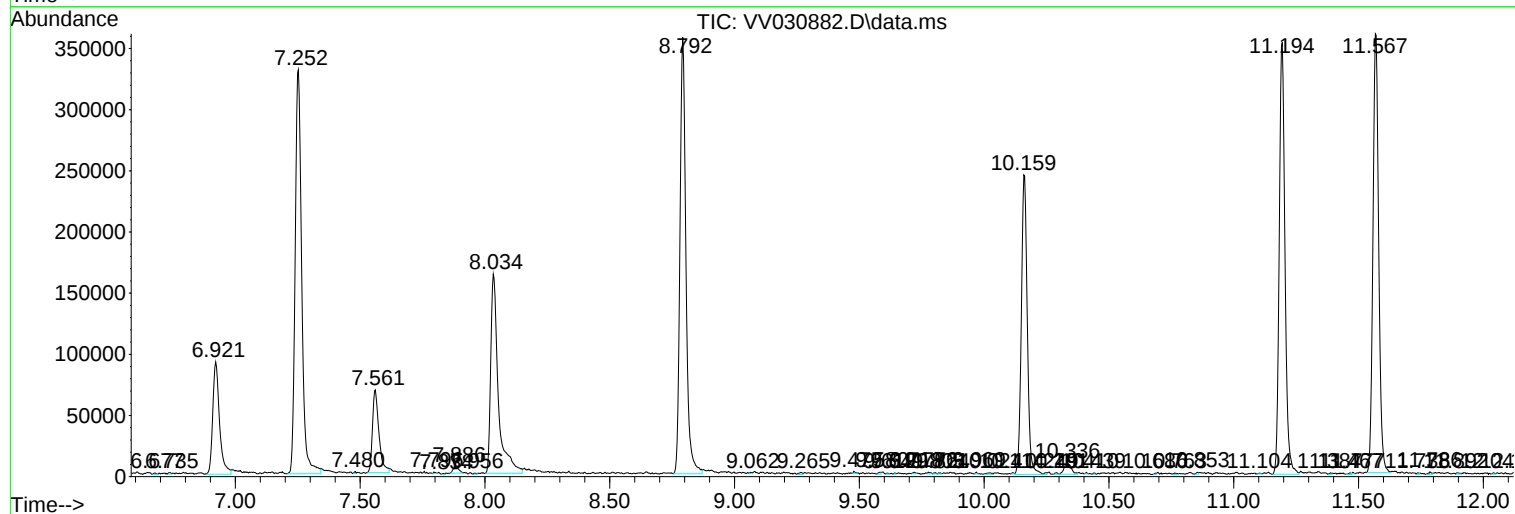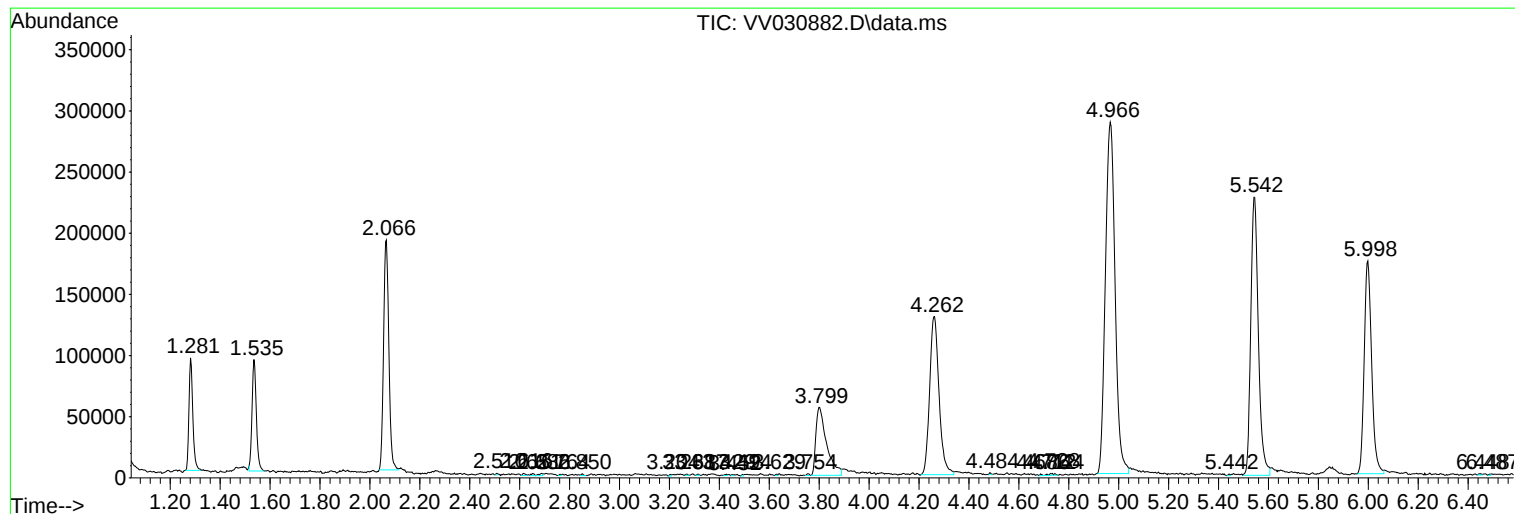

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042623\
Data File : VV030882.D
Acq On : 26 Apr 2023 16:00
Operator : SY/MD
Sample : 02475-09
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 10 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0AX2

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM041723WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042623\
Data File : VV030882.D
Acq On : 26 Apr 2023 16:00
Operator : SY/MD
Sample : 02475-09
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 10 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0AX2

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM041723WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc