

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042623\
 Data File : VV030883.D
 Acq On : 26 Apr 2023 16:24
 Operator : SY/MD
 Sample : VIBLK206
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VIBLK206

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM041723WMA.M
 Title : VOC Analysis

Signal : TIC: VV030883.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.281	69	75	92	rVB	78647	87882	11.69%	1.496%
2	1.535	148	154	169	rVB	82881	96401	12.82%	1.641%
3	2.066	310	319	334	rVB	164132	236628	31.47%	4.029%
4	2.288	385	388	390	rBV4	1343	1012	0.13%	0.017%
5	2.362	408	411	415	rBV4	1178	868	0.12%	0.015%
6	2.400	421	423	426	rBV4	1610	1090	0.14%	0.019%
7	2.561	468	473	475	rBV5	1852	1141	0.15%	0.019%
8	2.635	492	496	498	rVB4	1198	638	0.08%	0.011%
9	2.654	498	502	505	rBV6	1770	1371	0.18%	0.023%
10	2.889	573	575	578	rBV3	1022	688	0.09%	0.012%
11	2.915	580	583	586	rBV3	882	715	0.10%	0.012%
12	2.960	595	597	600	rVB4	1462	784	0.10%	0.013%
13	3.169	657	662	666	rVB7	1251	1305	0.17%	0.022%
14	3.281	693	697	699	rVB5	1041	683	0.09%	0.012%
15	3.368	719	724	726	rBV4	1009	805	0.11%	0.014%
16	3.596	792	795	803	rVB9	1324	1413	0.19%	0.024%
17	3.641	805	809	812	rBV6	1086	936	0.12%	0.016%
18	3.802	848	859	884	rBV	52970	155463	20.68%	2.647%
19	4.259	988	1001	1020	rBV	130122	307140	40.85%	5.230%
20	4.612	1107	1111	1114	rBV5	1672	1325	0.18%	0.023%
21	4.712	1139	1142	1146	rBV3	1193	716	0.10%	0.012%
22	4.751	1151	1154	1158	rBV6	1017	897	0.12%	0.015%
23	4.821	1174	1176	1181	rVB4	1311	675	0.09%	0.011%
24	4.966	1204	1221	1246	rVV2	282872	751825	100.00%	12.801%
25	5.255	1309	1311	1315	rBV4	718	696	0.09%	0.012%
26	5.349	1336	1340	1345	rBV6	1906	1394	0.19%	0.024%
27	5.497	1382	1386	1387	rBV3	1450	1069	0.14%	0.018%
28	5.542	1388	1400	1424	rVV	238902	498305	66.28%	8.485%
29	5.767	1467	1470	1471	rBV4	1740	893	0.12%	0.015%
30	5.998	1528	1542	1560	rBV	169247	352350	46.87%	5.999%
31	6.326	1641	1644	1648	rBV5	1028	703	0.09%	0.012%
32	6.484	1689	1693	1695	rBV4	1939	1622	0.22%	0.028%
33	6.526	1703	1706	1709	rBV5	1265	1060	0.14%	0.018%
34	6.580	1721	1723	1726	rBV3	809	631	0.08%	0.011%
35	6.628	1735	1738	1740	rBV4	1027	707	0.09%	0.012%
36	6.744	1772	1774	1776	rBV4	1795	954	0.13%	0.016%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW042623\
 Data File : VW030883.D
 Acq On : 26 Apr 2023 16:24
 Operator : SY/MD
 Sample : VIBLK206
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VIBLK206

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM041723WMA.M
 Title : VOC Analysis

37	6.815	1790	1796	1799	rBV7	1685	1602	0.21%	0.027%
38	6.860	1808	1810	1813	rBV4	1139	779	0.10%	0.013%
39	6.921	1819	1829	1849	rBV	85867	161072	21.42%	2.743%
40	7.079	1874	1878	1880	rBV4	1237	1092	0.15%	0.019%
41	7.252	1921	1932	1951	rVV	304693	542104	72.11%	9.230%
42	7.513	2009	2013	2017	rBV7	1069	1089	0.14%	0.019%
43	7.561	2019	2028	2043	rBV	64849	115227	15.33%	1.962%
44	7.734	2081	2082	2087	rBV5	917	716	0.10%	0.012%
45	7.802	2099	2103	2105	rBV3	1250	797	0.11%	0.014%
46	7.882	2126	2128	2133	rVB5	2034	1408	0.19%	0.024%
47	8.033	2163	2175	2208	rBV	162166	343794	45.73%	5.854%
48	8.394	2282	2287	2288	rBV5	1432	1069	0.14%	0.018%
49	8.641	2361	2364	2369	rVB7	1168	838	0.11%	0.014%
50	8.683	2374	2377	2381	rVB6	1291	901	0.12%	0.015%
51	8.792	2398	2411	2432	rBV	366451	622779	82.84%	10.604%
52	9.088	2501	2503	2507	rVB4	1646	993	0.13%	0.017%
53	9.133	2514	2517	2518	rBV3	1311	892	0.12%	0.015%
54	9.207	2537	2540	2542	rBV3	1260	846	0.11%	0.014%
55	9.316	2570	2574	2576	rBV3	1625	1136	0.15%	0.019%
56	9.477	2622	2624	2627	rBV3	1057	802	0.11%	0.014%
57	9.535	2638	2642	2643	rBV4	1472	824	0.11%	0.014%
58	9.580	2653	2656	2658	rVB5	1363	820	0.11%	0.014%
59	9.644	2671	2676	2677	rBV4	1184	993	0.13%	0.017%
60	9.763	2708	2713	2715	rBV4	1023	820	0.11%	0.014%
61	9.795	2718	2723	2724	rBV5	850	755	0.10%	0.013%
62	9.992	2781	2784	2788	rVB5	975	650	0.09%	0.011%
63	10.024	2791	2794	2797	rBV3	1371	1197	0.16%	0.020%
64	10.159	2826	2836	2851	rBV	244243	390237	51.91%	6.645%
65	10.538	2952	2954	2957	rVB3	1726	890	0.12%	0.015%
66	10.564	2960	2962	2966	rVB5	1199	640	0.09%	0.011%
67	10.631	2976	2983	2986	rBV9	779	833	0.11%	0.014%
68	10.699	3001	3004	3006	rBV4	1439	793	0.11%	0.014%
69	10.828	3042	3044	3048	rBV5	1056	943	0.13%	0.016%
70	10.853	3048	3052	3055	rVB5	1168	833	0.11%	0.014%
71	10.879	3055	3060	3064	rVB6	1552	1606	0.21%	0.027%
72	11.004	3097	3099	3104	rVB6	1632	1058	0.14%	0.018%
73	11.030	3104	3107	3111	rBV5	1811	1663	0.22%	0.028%
74	11.088	3123	3125	3127	rVB3	1298	638	0.08%	0.011%
75	11.143	3139	3142	3145	rBV5	1185	725	0.10%	0.012%
76	11.194	3147	3158	3179	rVV	366645	586038	77.95%	9.979%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042623\
 Data File : VV030883.D
 Acq On : 26 Apr 2023 16:24
 Operator : SY/MD
 Sample : VIBLK206
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VIBLK206

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM041723WMA.M
 Title : VOC Analysis

77	11.567	3263	3274	3291	rBV	338203	542600	72.17%	9.239%
78	11.705	3311	3317	3318	rBV5	1394	1211	0.16%	0.021%
79	12.213	3470	3475	3477	rBV5	2181	2001	0.27%	0.034%
80	12.319	3503	3508	3512	rVB6	1565	1606	0.21%	0.027%
81	12.657	3610	3613	3616	rVB5	1393	813	0.11%	0.014%
82	12.680	3616	3620	3625	rBV7	1930	1951	0.26%	0.033%
83	12.754	3640	3643	3646	rBV4	1272	955	0.13%	0.016%
84	12.840	3664	3670	3672	rVV4	1181	983	0.13%	0.017%
85	13.024	3726	3727	3730	rBV3	1100	683	0.09%	0.012%
86	13.117	3752	3756	3760	rBV7	1348	1408	0.19%	0.024%
87	13.194	3777	3780	3781	rBV3	1461	754	0.10%	0.013%
88	13.300	3811	3813	3818	rVV4	818	695	0.09%	0.012%
89	13.348	3823	3828	3830	rVV6	1163	910	0.12%	0.015%
90	13.516	3876	3880	3881	rBV4	1380	854	0.11%	0.015%
91	13.612	3905	3910	3912	rBV6	1264	1166	0.16%	0.020%
92	13.699	3933	3937	3942	rVB8	2112	2075	0.28%	0.035%
93	13.779	3960	3962	3964	rBV2	1009	668	0.09%	0.011%
94	13.799	3966	3968	3972	rBV4	1272	865	0.12%	0.015%
95	13.943	4010	4013	4017	rBV5	1610	1407	0.19%	0.024%
96	14.181	4083	4087	4088	rBV3	1091	691	0.09%	0.012%
97	14.223	4096	4100	4101	rBV3	1051	880	0.12%	0.015%
98	14.461	4171	4174	4175	rBV3	1327	650	0.09%	0.011%
99	14.856	4295	4297	4301	rVB5	1358	835	0.11%	0.014%
100	14.917	4314	4316	4318	rBV3	1213	665	0.09%	0.011%




Sum of corrected areas: 5873003

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042623\
Data File : VV030883.D
Acq On : 26 Apr 2023 16:24
Operator : SY/MD
Sample : VIBLK206
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 11 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VIBLK206

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM041723WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

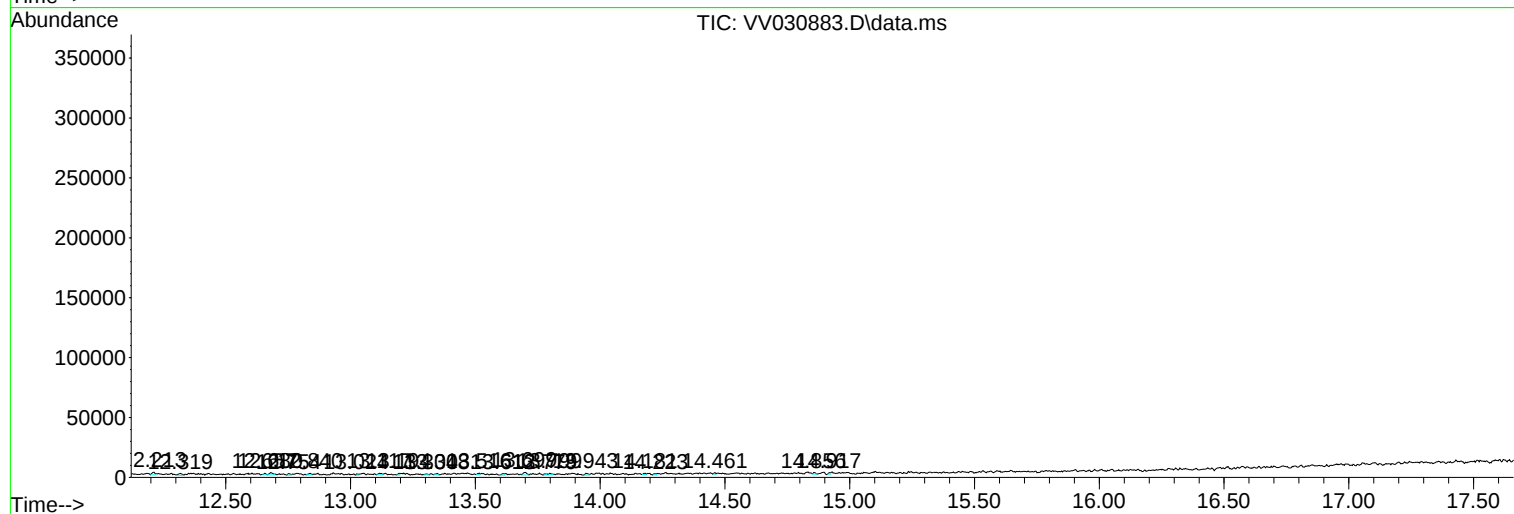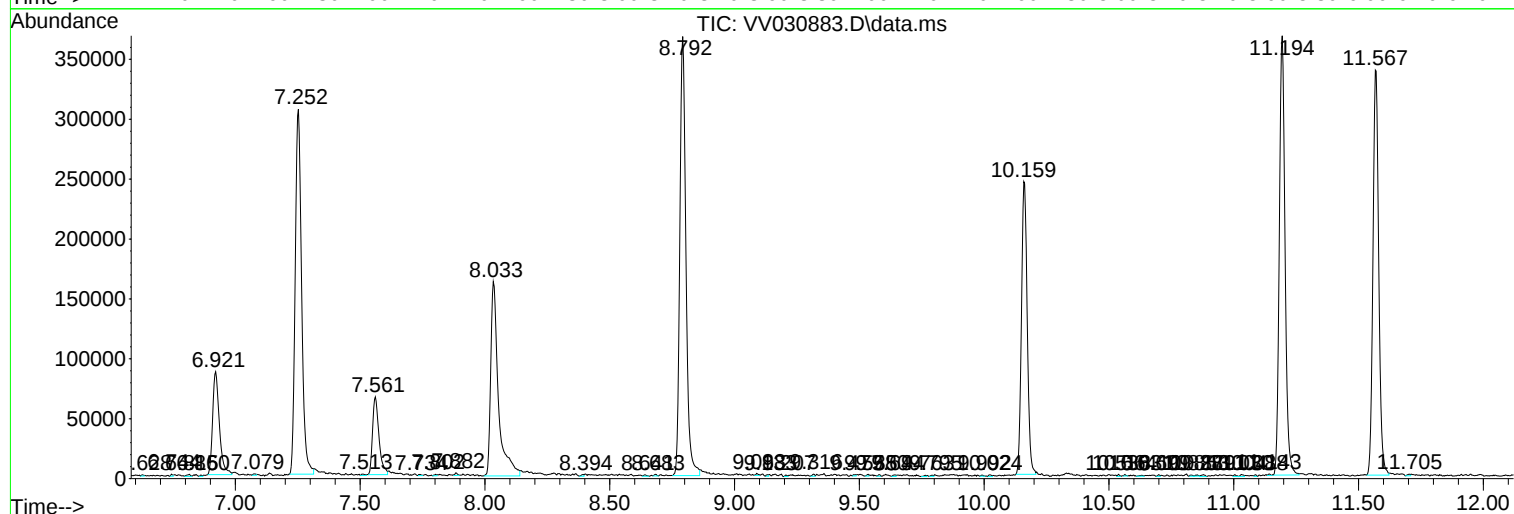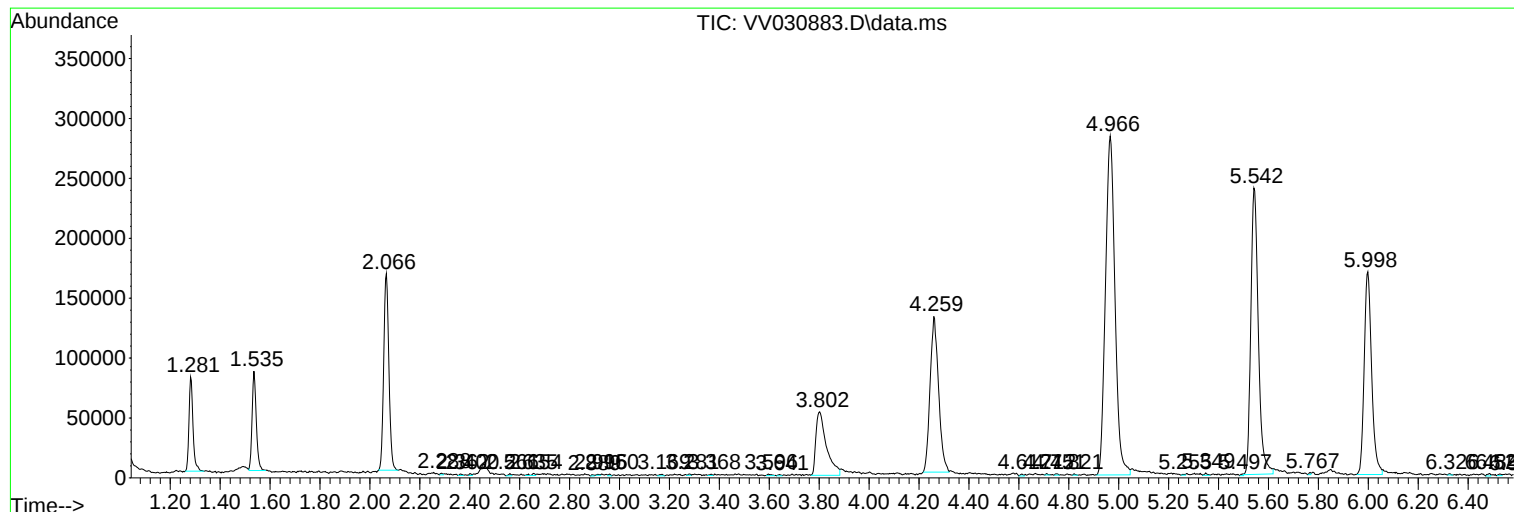

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042623\
Data File : VV030883.D
Acq On : 26 Apr 2023 16:24
Operator : SY/MD
Sample : VIBLK206
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 11 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VIBLK206

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM041723WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042623\
Data File : VV030883.D
Acq On : 26 Apr 2023 16:24
Operator : SY/MD
Sample : VIBLK206
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 11 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VIBLK206

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM041723WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------