

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042623\
 Data File : VV030884.D
 Acq On : 26 Apr 2023 16:48
 Operator : SY/MD
 Sample : 02475-03
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0AW5

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM041723WMA.M
 Title : VOC Analysis

Signal : TIC: VV030884.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.282	69	75	85	rBV	93947	101109	12.66%	1.621%
2	1.536	148	154	166	rVB	84629	101490	12.71%	1.627%
3	2.066	310	319	332	rVB	189938	276981	34.68%	4.441%
4	2.442	433	436	439	rBV3	1301	1126	0.14%	0.018%
5	2.638	493	497	499	rBV5	1380	1256	0.16%	0.020%
6	2.790	542	544	546	rBV2	948	505	0.06%	0.008%
7	2.835	556	558	559	rBV2	1300	525	0.07%	0.008%
8	2.873	565	570	575	rBV8	1167	1109	0.14%	0.018%
9	3.069	630	631	634	rVB3	1430	608	0.08%	0.010%
10	3.224	676	679	681	rBV4	1026	580	0.07%	0.009%
11	3.429	741	743	746	rBV3	1098	608	0.08%	0.010%
12	3.442	746	747	750	rVV2	1213	474	0.06%	0.008%
13	3.465	750	754	757	rVB5	1674	1055	0.13%	0.017%
14	3.494	760	763	767	rVB3	1307	914	0.11%	0.015%
15	3.629	803	805	808	rBV4	1291	745	0.09%	0.012%
16	3.683	818	822	824	rBV5	944	654	0.08%	0.010%
17	3.799	849	858	885	rVV	53799	155525	19.47%	2.494%
18	4.259	987	1001	1021	rBV2	132278	338537	42.39%	5.428%
19	4.664	1125	1127	1130	rVB3	1315	565	0.07%	0.009%
20	4.687	1132	1134	1137	rBV4	1358	1018	0.13%	0.016%
21	4.783	1162	1164	1170	rVB6	1397	950	0.12%	0.015%
22	4.818	1170	1175	1178	rBV7	860	835	0.10%	0.013%
23	4.876	1190	1193	1195	rBV4	940	593	0.07%	0.010%
24	4.966	1203	1221	1243	rBV2	297813	798634	100.00%	12.805%
25	5.542	1388	1400	1425	rBV	249700	518885	64.97%	8.319%
26	5.998	1530	1542	1563	rBV	175754	362096	45.34%	5.806%
27	6.233	1612	1615	1617	rBV4	1181	751	0.09%	0.012%
28	6.429	1673	1676	1677	rBV3	1412	1005	0.13%	0.016%
29	6.532	1706	1708	1714	rVB5	2030	1464	0.18%	0.023%
30	6.558	1714	1716	1717	rBV	896	472	0.06%	0.008%
31	6.619	1732	1735	1738	rBV6	1793	1101	0.14%	0.018%
32	6.696	1755	1759	1762	rBV4	1893	1435	0.18%	0.023%
33	6.757	1776	1778	1781	rVV4	1222	742	0.09%	0.012%
34	6.818	1794	1797	1799	rBV4	1426	749	0.09%	0.012%
35	6.876	1811	1815	1817	rBV6	1135	1019	0.13%	0.016%
36	6.921	1818	1829	1843	rBV2	93910	173144	21.68%	2.776%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW042623\
 Data File : VW030884.D
 Acq On : 26 Apr 2023 16:48
 Operator : SY/MD
 Sample : 02475-03
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0AW5

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM041723WMA.M
 Title : VOC Analysis

37	7.252	1919	1932	1958	rBV	336064	616378	77.18%	9.882%
38	7.449	1991	1993	1996	rBV3	1666	1137	0.14%	0.018%
39	7.561	2018	2028	2043	rBV2	67601	124105	15.54%	1.990%
40	7.818	2106	2108	2114	rBV6	1503	1361	0.17%	0.022%
41	7.876	2121	2126	2129	rBV7	3082	3775	0.47%	0.061%
42	8.034	2165	2175	2205	rBV	163325	345681	43.28%	5.542%
43	8.526	2326	2328	2330	rBV3	1505	789	0.10%	0.013%
44	8.719	2385	2388	2392	rBV4	1381	633	0.08%	0.010%
45	8.793	2400	2411	2432	rBV	379485	636710	79.72%	10.208%
46	9.358	2583	2587	2588	rBV4	825	513	0.06%	0.008%
47	9.368	2588	2590	2592	rVV3	1389	578	0.07%	0.009%
48	9.484	2623	2626	2628	rBV3	1037	700	0.09%	0.011%
49	9.564	2650	2651	2654	rBV3	1196	508	0.06%	0.008%
50	9.612	2662	2666	2669	rVB6	982	677	0.08%	0.011%
51	9.741	2703	2706	2709	rBV4	1245	922	0.12%	0.015%
52	9.767	2709	2714	2717	rVB7	1334	1061	0.13%	0.017%
53	9.815	2727	2729	2731	rVB3	1489	557	0.07%	0.009%
54	9.841	2735	2737	2740	rBV3	1378	1017	0.13%	0.016%
55	9.963	2771	2775	2776	rBV4	916	610	0.08%	0.010%
56	10.056	2801	2804	2806	rBV3	1320	784	0.10%	0.013%
57	10.085	2811	2813	2815	rVB3	1240	513	0.06%	0.008%
58	10.098	2815	2817	2819	rBV3	1227	737	0.09%	0.012%
59	10.159	2825	2836	2850	rBV	252113	403202	50.49%	6.465%
60	10.259	2863	2867	2868	rBV4	1145	981	0.12%	0.016%
61	10.336	2884	2891	2897	rVB4	6011	8391	1.05%	0.135%
62	10.429	2917	2920	2922	rBV5	1255	660	0.08%	0.011%
63	10.471	2930	2933	2934	rBV2	1256	614	0.08%	0.010%
64	10.484	2934	2937	2938	rBV3	940	519	0.06%	0.008%
65	10.645	2983	2987	2990	rBV6	2177	2201	0.28%	0.035%
66	10.780	3026	3029	3032	rBV5	1275	982	0.12%	0.016%
67	10.805	3035	3037	3040	rVB4	1165	663	0.08%	0.011%
68	10.854	3047	3052	3054	rBV5	1425	1208	0.15%	0.019%
69	11.021	3100	3104	3107	rBV5	1467	1158	0.14%	0.019%
70	11.194	3146	3158	3177	rBV	384122	610181	76.40%	9.783%
71	11.339	3200	3203	3207	rBV6	1325	1008	0.13%	0.016%
72	11.567	3263	3274	3295	rVB	363967	588760	73.72%	9.440%
73	11.828	3354	3355	3359	rVB3	1124	596	0.07%	0.010%
74	11.966	3394	3398	3402	rBV6	1459	1427	0.18%	0.023%
75	12.024	3413	3416	3418	rBV4	1110	687	0.09%	0.011%
76	12.204	3466	3472	3474	rBV7	2484	2772	0.35%	0.044%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042623\
 Data File : VV030884.D
 Acq On : 26 Apr 2023 16:48
 Operator : SY/MD
 Sample : 02475-03
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0AW5

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM041723WMA.M
 Title : VOC Analysis

77	12.368	3520	3523	3526	rVB3	1372	782	0.10%	0.013%
78	12.423	3538	3540	3542	rBV3	1389	804	0.10%	0.013%
79	12.493	3559	3562	3563	rBV3	1014	596	0.07%	0.010%
80	12.571	3584	3586	3588	rBV3	872	500	0.06%	0.008%
81	12.593	3590	3593	3598	rVB5	2159	1788	0.22%	0.029%
82	12.625	3598	3603	3607	rBV7	1245	1431	0.18%	0.023%
83	12.670	3614	3617	3618	rBV3	1164	497	0.06%	0.008%
84	12.683	3618	3621	3626	rVB5	1826	1519	0.19%	0.024%
85	12.718	3628	3632	3633	rVV2	1094	759	0.10%	0.012%
86	12.744	3637	3640	3642	rBV3	1340	780	0.10%	0.013%
87	12.757	3642	3644	3646	rVB3	1444	631	0.08%	0.010%
88	12.808	3657	3660	3665	rVB6	1624	1267	0.16%	0.020%
89	13.088	3745	3747	3748	rBV2	954	480	0.06%	0.008%
90	13.181	3774	3776	3780	rBV4	1297	1039	0.13%	0.017%
91	13.329	3820	3822	3825	rVB4	1268	486	0.06%	0.008%
92	13.394	3839	3842	3844	rBV4	1164	719	0.09%	0.012%
93	13.439	3854	3856	3858	rBV3	1093	573	0.07%	0.009%
94	13.599	3903	3906	3908	rBV4	828	511	0.06%	0.008%
95	13.715	3940	3942	3945	rVB4	1360	652	0.08%	0.010%
96	13.735	3945	3948	3950	rBV4	1404	890	0.11%	0.014%
97	14.198	4088	4092	4095	rBV5	1426	1391	0.17%	0.022%
98	14.709	4249	4251	4253	rBV3	1440	701	0.09%	0.011%
99	15.188	4397	4400	4404	rVB4	1872	1264	0.16%	0.020%
100	15.210	4404	4407	4413	rBV6	1792	2043	0.26%	0.033%




Sum of corrected areas: 6237118

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042623\
Data File : VV030884.D
Acq On : 26 Apr 2023 16:48
Operator : SY/MD
Sample : 02475-03
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 12 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0AW5

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM041723WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

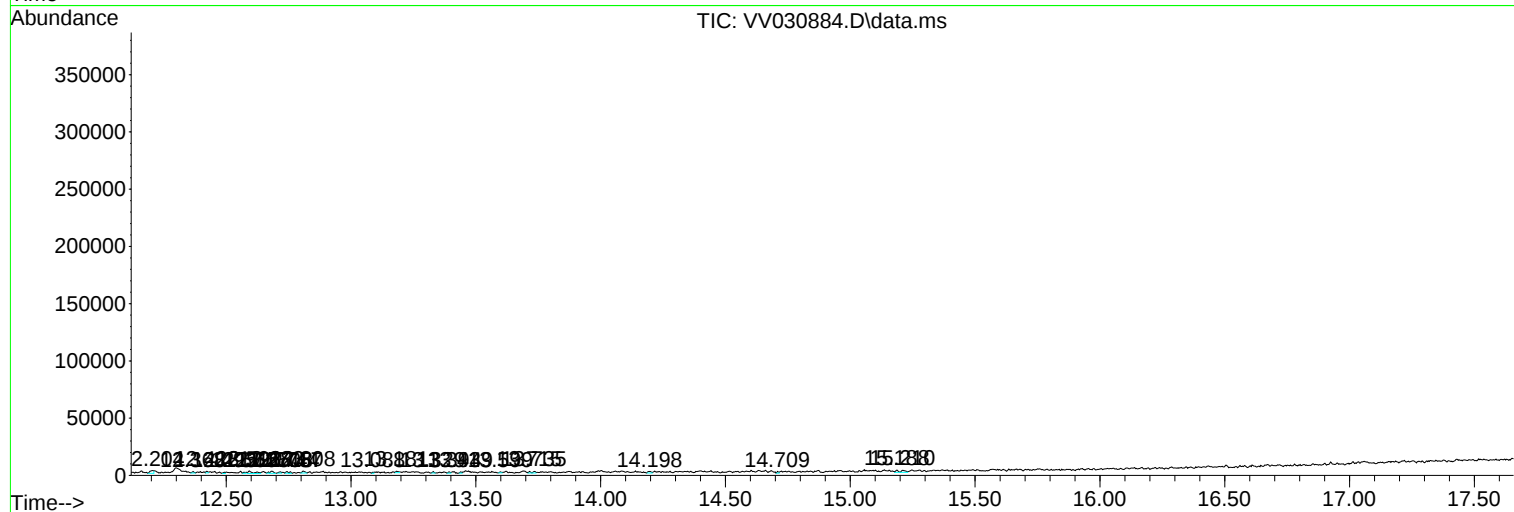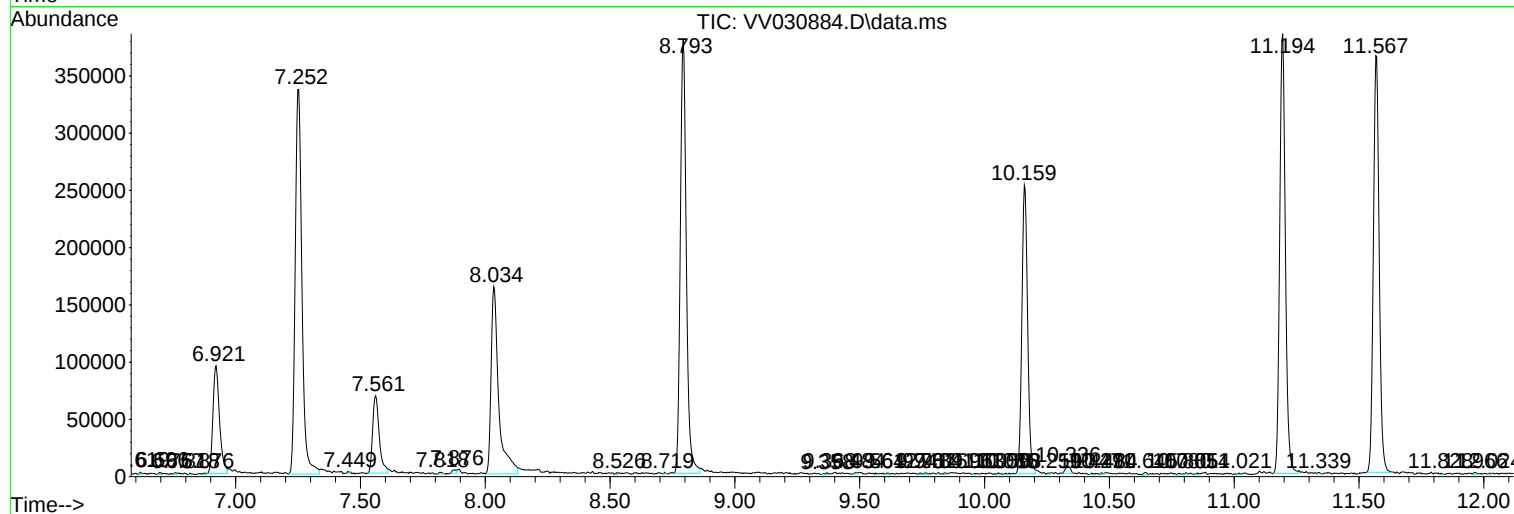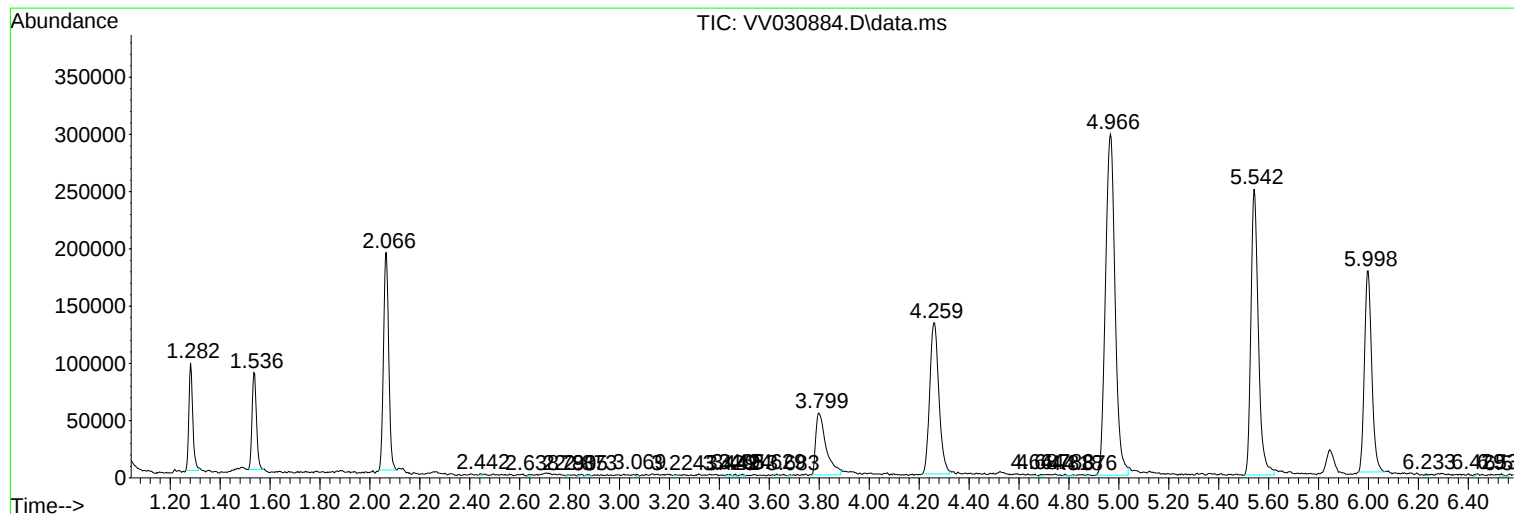

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042623\
Data File : VV030884.D
Acq On : 26 Apr 2023 16:48
Operator : SY/MD
Sample : 02475-03
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 12 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0AW5

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM041723WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042623\
Data File : VV030884.D
Acq On : 26 Apr 2023 16:48
Operator : SY/MD
Sample : 02475-03
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 12 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0AW5

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM041723WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------