

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042623\
 Data File : VV030885.D
 Acq On : 26 Apr 2023 17:12
 Operator : SY/MD
 Sample : 02475-02DL 4X
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0AW4DL

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM041723WMA.M
 Title : VOC Analysis

Signal : TIC: VV030885.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.282	69	75	86	rBV	81825	89960	12.20%	1.407%
2	1.536	148	154	168	rVB	82899	98255	13.32%	1.537%
3	2.066	310	319	333	rVB	171477	252649	34.26%	3.952%
4	2.581	476	479	481	rBV4	1361	1050	0.14%	0.016%
5	2.635	494	496	497	rBV	1036	416	0.06%	0.007%
6	2.783	539	542	544	rBV3	937	757	0.10%	0.012%
7	2.822	552	554	555	rBV2	1004	417	0.06%	0.007%
8	2.854	562	564	570	rVB6	1380	1012	0.14%	0.016%
9	2.876	570	571	574	rBV4	867	546	0.07%	0.009%
10	2.928	585	587	590	rBV4	921	637	0.09%	0.010%
11	2.960	593	597	601	rBV6	1226	1293	0.18%	0.020%
12	3.111	641	644	646	rBV2	1509	1152	0.16%	0.018%
13	3.182	663	666	669	rBV4	1250	769	0.10%	0.012%
14	3.310	704	706	709	rBV4	640	365	0.05%	0.006%
15	3.481	755	759	763	rBV6	1199	1086	0.15%	0.017%
16	3.516	768	770	772	rBV2	1064	568	0.08%	0.009%
17	3.600	793	796	800	rVB6	1597	955	0.13%	0.015%
18	3.622	800	803	807	rBV3	1346	1348	0.18%	0.021%
19	3.735	832	838	840	rBV6	1786	1913	0.26%	0.030%
20	3.799	848	858	882	rBV3	52348	177234	24.03%	2.772%
21	4.259	988	1001	1026	rVB	122520	307273	41.66%	4.806%
22	4.783	1162	1164	1165	rBV2	1232	481	0.07%	0.008%
23	4.822	1170	1176	1178	rBV5	1123	1148	0.16%	0.018%
24	4.857	1185	1187	1189	rVB3	1066	426	0.06%	0.007%
25	4.896	1197	1199	1203	rBV4	980	680	0.09%	0.011%
26	4.966	1205	1221	1245	rVV3	279045	737505	100.00%	11.536%
27	5.342	1335	1338	1340	rBV4	1588	1076	0.15%	0.017%
28	5.474	1378	1379	1381	rBV2	814	395	0.05%	0.006%
29	5.542	1387	1400	1420	rBV	256864	537623	72.90%	8.409%
30	5.841	1482	1493	1513	rBV	218730	435635	59.07%	6.814%
31	5.998	1531	1542	1558	rVB2	164359	327571	44.42%	5.124%
32	6.352	1650	1652	1653	rBV2	928	380	0.05%	0.006%
33	6.416	1670	1672	1674	rVB3	1179	482	0.07%	0.008%
34	6.436	1674	1678	1680	rBV5	901	710	0.10%	0.011%
35	6.674	1749	1752	1754	rBV4	739	602	0.08%	0.009%
36	6.799	1788	1791	1794	rBV6	1047	691	0.09%	0.011%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW042623\
 Data File : VW030885.D
 Acq On : 26 Apr 2023 17:12
 Operator : SY/MD
 Sample : 02475-02DL 4X
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0AW4DL

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM041723WMA.M
 Title : VOC Analysis

37	6.921	1819	1829	1847	rBV2	85382	162870	22.08%	2.548%
38	7.149	1898	1900	1901	rBV2	1322	724	0.10%	0.011%
39	7.252	1919	1932	1953	rBV	308244	562023	76.21%	8.791%
40	7.471	1999	2000	2001	rBV	1621	546	0.07%	0.009%
41	7.500	2006	2009	2011	rBV4	1626	865	0.12%	0.014%
42	7.561	2017	2028	2050	rBV	66116	122392	16.60%	1.914%
43	8.034	2166	2175	2191	rBV	151711	282825	38.35%	4.424%
44	8.606	2351	2353	2354	rBV	778	354	0.05%	0.006%
45	8.715	2385	2387	2390	rBV4	1000	584	0.08%	0.009%
46	8.735	2391	2393	2396	rVV3	1166	481	0.07%	0.008%
47	8.792	2400	2411	2436	rVV	398053	662497	89.83%	10.363%
48	9.001	2474	2476	2479	rBV5	1920	1032	0.14%	0.016%
49	9.053	2490	2492	2496	rVB6	1188	670	0.09%	0.010%
50	9.072	2496	2498	2499	rBV2	1011	444	0.06%	0.007%
51	9.442	2612	2613	2618	rBV3	1050	691	0.09%	0.011%
52	9.641	2672	2675	2676	rBV3	935	491	0.07%	0.008%
53	9.664	2680	2682	2683	rBV	1206	497	0.07%	0.008%
54	9.702	2691	2694	2697	rBV4	709	590	0.08%	0.009%
55	9.760	2703	2712	2715	rBV8	1889	2535	0.34%	0.040%
56	9.947	2767	2770	2772	rVB3	966	495	0.07%	0.008%
57	10.082	2809	2812	2817	rBV6	1111	806	0.11%	0.013%
58	10.159	2824	2836	2853	rBV	233188	381730	51.76%	5.971%
59	10.281	2872	2874	2877	rVB3	1170	625	0.08%	0.010%
60	10.307	2880	2882	2884	rBV3	1202	656	0.09%	0.010%
61	10.326	2884	2888	2889	rBV4	3824	2490	0.34%	0.039%
62	10.381	2903	2905	2907	rBV2	1218	643	0.09%	0.010%
63	10.394	2907	2909	2911	rVB2	1094	481	0.07%	0.008%
64	10.426	2917	2919	2923	rBV4	673	508	0.07%	0.008%
65	10.445	2923	2925	2928	rBV4	941	715	0.10%	0.011%
66	10.651	2981	2989	2991	rBV7	1657	1856	0.25%	0.029%
67	10.673	2994	2996	2999	rBV3	1489	1034	0.14%	0.016%
68	10.693	2999	3002	3004	rBV4	1036	610	0.08%	0.010%
69	10.899	3063	3066	3069	rVB3	796	538	0.07%	0.008%
70	10.944	3078	3080	3083	rBV4	984	708	0.10%	0.011%
71	11.024	3102	3105	3109	rBV5	1515	1022	0.14%	0.016%
72	11.046	3109	3112	3113	rBV2	1233	716	0.10%	0.011%
73	11.098	3126	3128	3129	rBV2	986	451	0.06%	0.007%
74	11.194	3145	3158	3176	rBV	391655	636065	86.25%	9.949%
75	11.365	3209	3211	3215	rVB5	1574	854	0.12%	0.013%
76	11.387	3215	3218	3220	rVB4	1565	617	0.08%	0.010%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042623\
 Data File : VV030885.D
 Acq On : 26 Apr 2023 17:12
 Operator : SY/MD
 Sample : 02475-02DL 4X
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0AW4DL

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM041723WMA.M
 Title : VOC Analysis

77	11.419	3226	3228	3232	rVB3	1628	789	0.11%	0.012%
78	11.567	3263	3274	3290	rBV	341607	551280	74.75%	8.623%
79	12.014	3411	3413	3417	rVB5	1477	680	0.09%	0.011%
80	12.046	3417	3423	3424	rBV5	1618	1630	0.22%	0.025%
81	12.095	3436	3438	3442	rBV5	829	657	0.09%	0.010%
82	12.207	3471	3473	3474	rBV2	1171	382	0.05%	0.006%
83	12.255	3485	3488	3489	rBV3	1620	860	0.12%	0.013%
84	12.294	3497	3500	3502	rVB4	1485	882	0.12%	0.014%
85	12.310	3502	3505	3514	rVB8	1937	2654	0.36%	0.042%
86	12.349	3514	3517	3518	rBV3	944	574	0.08%	0.009%
87	12.384	3526	3528	3531	rVB4	1268	739	0.10%	0.012%
88	12.506	3564	3566	3569	rBV3	1264	856	0.12%	0.013%
89	12.635	3602	3606	3608	rBV4	939	821	0.11%	0.013%
90	12.706	3627	3628	3632	rVB5	1090	457	0.06%	0.007%
91	13.233	3790	3792	3795	rVB3	1678	732	0.10%	0.011%
92	13.275	3801	3805	3810	rBV7	1184	1147	0.16%	0.018%
93	13.352	3828	3829	3832	rBV3	744	373	0.05%	0.006%
94	13.403	3842	3845	3849	rVB4	1723	963	0.13%	0.015%
95	13.664	3921	3926	3927	rBV4	1086	877	0.12%	0.014%
96	13.770	3955	3959	3963	rBV6	1030	893	0.12%	0.014%
97	13.824	3975	3976	3978	rBV2	991	518	0.07%	0.008%
98	14.213	4095	4097	4099	rVB3	1187	461	0.06%	0.007%
99	14.230	4099	4102	4106	rBV5	1002	835	0.11%	0.013%
100	14.676	4239	4241	4246	rBV4	1603	1291	0.18%	0.020%




Sum of corrected areas: 6393142

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042623\
Data File : VV030885.D
Acq On : 26 Apr 2023 17:12
Operator : SY/MD
Sample : 02475-02DL 4X
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 13 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0AW4DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM041723WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

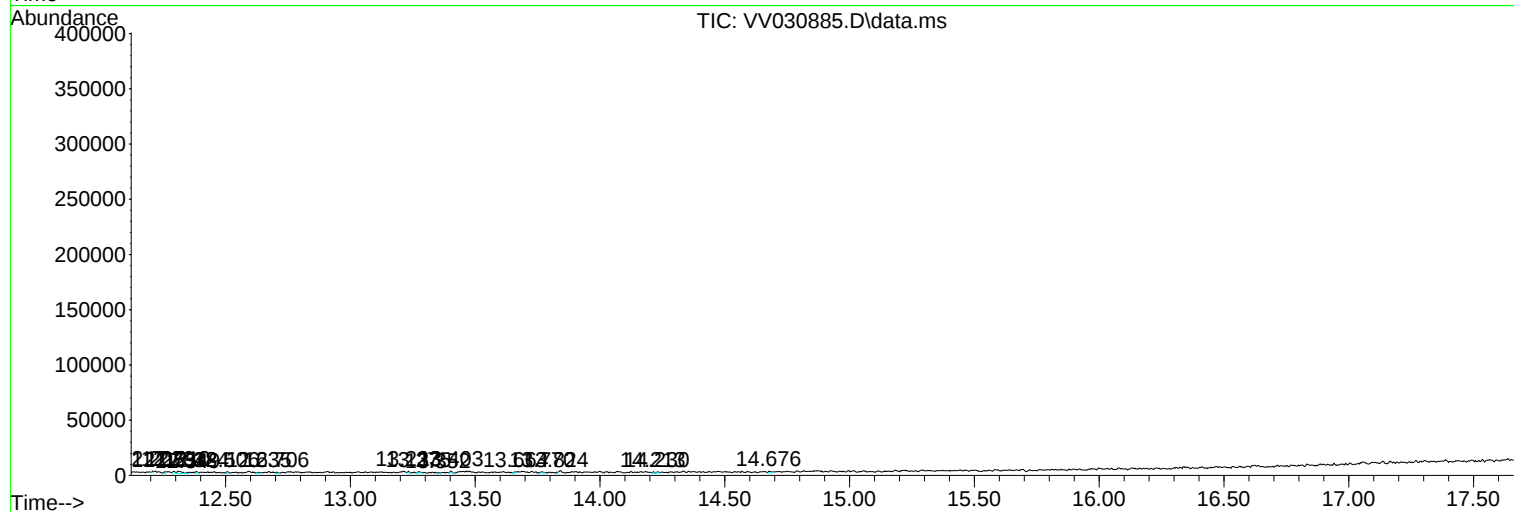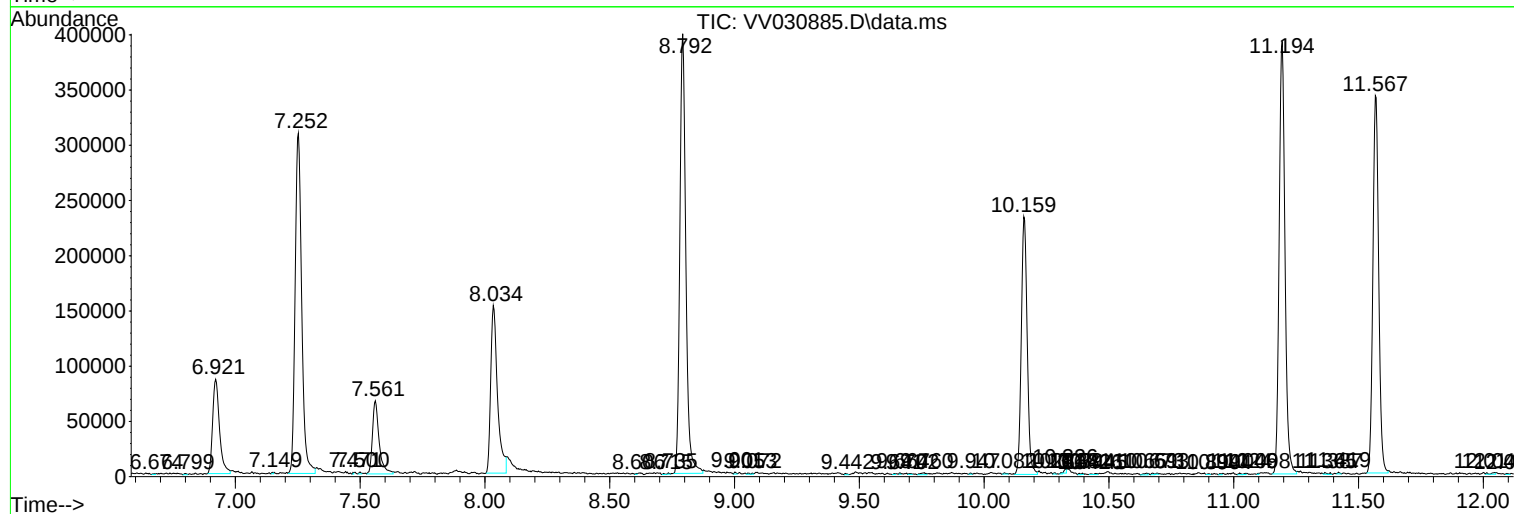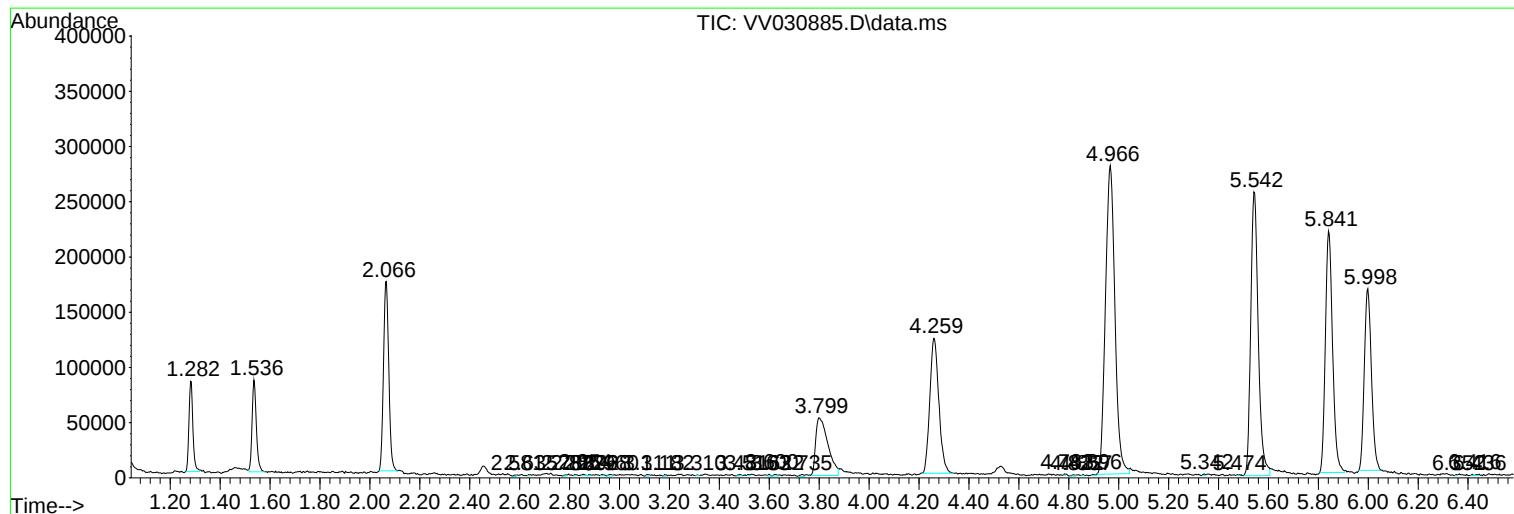

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042623\
Data File : VV030885.D
Acq On : 26 Apr 2023 17:12
Operator : SY/MD
Sample : 02475-02DL 4X
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 13 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0AW4DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM041723WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042623\
Data File : VV030885.D
Acq On : 26 Apr 2023 17:12
Operator : SY/MD
Sample : 02475-02DL 4X
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 13 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0AW4DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM041723WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------