

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042623\
 Data File : VV030886.D
 Acq On : 26 Apr 2023 17:36
 Operator : SY/MD
 Sample : 02475-04 5X
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0AW6

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM041723WMA.M

Title : VOC Analysis

Signal : TIC: VV030886.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.285	69	76	91	rVB	89170	99055	10.74%	1.377%
2	1.539	148	155	171	rVB	85526	105175	11.40%	1.462%
3	2.066	310	319	334	rVB	184996	277076	30.04%	3.851%
4	2.539	464	466	470	rBV4	1431	884	0.10%	0.012%
5	2.809	547	550	552	rVB4	1720	877	0.10%	0.012%
6	2.847	558	562	566	rVB5	1568	1161	0.13%	0.016%
7	3.098	639	640	642	rBV2	754	415	0.04%	0.006%
8	3.214	674	676	679	rBV4	643	410	0.04%	0.006%
9	3.275	693	695	698	rVB4	1304	602	0.07%	0.008%
10	3.481	758	759	763	rVB4	1283	597	0.06%	0.008%
11	3.571	782	787	791	rBV8	1357	1295	0.14%	0.018%
12	3.625	800	804	805	rBV3	881	712	0.08%	0.010%
13	3.658	811	814	816	rBV3	875	599	0.06%	0.008%
14	3.719	831	833	837	rBV4	1505	1259	0.14%	0.017%
15	3.815	849	863	889	rBV3	68573	243658	26.42%	3.387%
16	4.117	954	957	959	rBV4	1418	899	0.10%	0.012%
17	4.259	988	1001	1022	rBV	126270	316987	34.36%	4.406%
18	4.490	1070	1073	1074	rBV3	1747	1019	0.11%	0.014%
19	4.670	1127	1129	1132	rBV3	895	444	0.05%	0.006%
20	4.863	1187	1189	1193	rVB4	1302	542	0.06%	0.008%
21	4.966	1205	1221	1244	rBV2	290465	781073	84.68%	10.856%
22	5.542	1388	1400	1425	rBV	259846	550933	59.73%	7.657%
23	5.841	1481	1493	1516	rBV	467072	922417	100.00%	12.821%
24	5.998	1531	1542	1561	rVB	175855	352991	38.27%	4.906%
25	6.211	1606	1608	1610	rBV3	1169	563	0.06%	0.008%
26	6.291	1631	1633	1635	rBV3	1264	790	0.09%	0.011%
27	6.432	1675	1677	1678	rBV2	1109	356	0.04%	0.005%
28	6.548	1711	1713	1715	rBV3	1398	499	0.05%	0.007%
29	6.696	1756	1759	1762	rBV5	1195	852	0.09%	0.012%
30	6.744	1772	1774	1779	rVB6	1695	1228	0.13%	0.017%
31	6.767	1779	1781	1784	rBV4	1261	908	0.10%	0.013%
32	6.921	1819	1829	1846	rBV	90352	171796	18.62%	2.388%
33	7.156	1900	1902	1905	rBV5	1478	698	0.08%	0.010%
34	7.252	1920	1932	1950	rBV	335644	589531	63.91%	8.194%
35	7.561	2019	2028	2046	rBV	65244	118738	12.87%	1.650%
36	7.876	2123	2126	2127	rBV3	2629	1541	0.17%	0.021%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW042623\
 Data File : VW030886.D
 Acq On : 26 Apr 2023 17:36
 Operator : SY/MD
 Sample : 02475-04 5X
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0AW6

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM041723WMA.M
 Title : VOC Analysis

37	8.034	2164	2175	2191	rBV	162590	311414	33.76%	4.328%
38	8.252	2241	2243	2244	rBV2	1839	814	0.09%	0.011%
39	8.493	2316	2318	2319	rBV2	896	332	0.04%	0.005%
40	8.503	2319	2321	2324	rVB4	1518	658	0.07%	0.009%
41	8.792	2401	2411	2436	rBV	406193	658771	71.42%	9.156%
42	9.188	2530	2534	2538	rBV6	1451	1609	0.17%	0.022%
43	9.246	2550	2552	2557	rVB5	2020	1494	0.16%	0.021%
44	9.345	2578	2583	2584	rBV6	2248	1608	0.17%	0.022%
45	9.368	2588	2590	2594	rVV4	748	533	0.06%	0.007%
46	9.548	2641	2646	2650	rBV7	1389	1468	0.16%	0.020%
47	9.570	2650	2653	2654	rBV3	1519	830	0.09%	0.012%
48	9.860	2739	2743	2745	rBV5	1472	1128	0.12%	0.016%
49	10.011	2788	2790	2792	rBV3	817	430	0.05%	0.006%
50	10.111	2819	2821	2822	rBV2	773	388	0.04%	0.005%
51	10.159	2825	2836	2856	rVV	248851	403546	43.75%	5.609%
52	10.442	2922	2924	2926	rBV2	679	383	0.04%	0.005%
53	10.596	2970	2972	2973	rBV2	1494	526	0.06%	0.007%
54	10.622	2977	2980	2982	rBV4	710	475	0.05%	0.007%
55	10.763	3020	3024	3025	rBV3	1299	829	0.09%	0.012%
56	10.792	3030	3033	3038	rVB7	1291	1255	0.14%	0.017%
57	10.850	3047	3051	3055	rBV5	1367	1540	0.17%	0.021%
58	10.902	3065	3067	3071	rBV4	1080	698	0.08%	0.010%
59	10.995	3093	3096	3100	rBV6	912	798	0.09%	0.011%
60	11.024	3102	3105	3108	rBV4	966	902	0.10%	0.013%
61	11.095	3124	3127	3128	rBV3	935	507	0.05%	0.007%
62	11.120	3133	3135	3136	rBV2	1044	414	0.04%	0.006%
63	11.194	3146	3158	3175	rBV	406077	641932	69.59%	8.922%
64	11.413	3224	3226	3229	rVB3	919	388	0.04%	0.005%
65	11.429	3229	3231	3234	rBV4	812	561	0.06%	0.008%
66	11.567	3263	3274	3295	rBV	361321	581512	63.04%	8.082%
67	11.667	3303	3305	3309	rBV5	1604	736	0.08%	0.010%
68	12.030	3415	3418	3419	rBV3	1208	816	0.09%	0.011%
69	12.053	3423	3425	3427	rBV3	913	443	0.05%	0.006%
70	12.194	3466	3469	3470	rBV3	1314	693	0.08%	0.010%
71	12.233	3479	3481	3488	rVB6	1013	987	0.11%	0.014%
72	12.300	3500	3502	3504	rBV3	1110	527	0.06%	0.007%
73	12.429	3540	3542	3545	rVB3	819	367	0.04%	0.005%
74	12.445	3545	3547	3549	rBV3	674	417	0.05%	0.006%
75	12.509	3565	3567	3570	rBV4	1040	755	0.08%	0.010%
76	12.577	3586	3588	3590	rBV3	1034	544	0.06%	0.008%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042623\
 Data File : VV030886.D
 Acq On : 26 Apr 2023 17:36
 Operator : SY/MD
 Sample : 02475-04 5X
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0AW6

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM041723WMA.M
 Title : VOC Analysis

77	12.660	3607	3614	3618	rVB8	1869	2189	0.24%	0.030%
78	12.686	3618	3622	3623	rBV3	1437	1154	0.13%	0.016%
79	12.773	3645	3649	3652	rBV5	1283	1161	0.13%	0.016%
80	12.802	3657	3658	3661	rBV3	957	515	0.06%	0.007%
81	12.937	3697	3700	3701	rBV2	963	513	0.06%	0.007%
82	12.966	3706	3709	3711	rBV4	1492	858	0.09%	0.012%
83	13.201	3778	3782	3784	rBV5	1583	1147	0.12%	0.016%
84	13.336	3820	3824	3825	rBV4	1889	1298	0.14%	0.018%
85	13.500	3873	3875	3881	rBV5	1391	1270	0.14%	0.018%
86	13.541	3885	3888	3891	rVV4	1052	716	0.08%	0.010%
87	13.622	3910	3913	3916	rBV4	940	671	0.07%	0.009%
88	13.651	3919	3922	3927	rBV6	1607	1603	0.17%	0.022%
89	13.792	3964	3966	3969	rBV4	1469	1001	0.11%	0.014%
90	13.911	4001	4003	4006	rBV4	1002	689	0.07%	0.010%
91	13.966	4018	4020	4023	rVB4	919	404	0.04%	0.006%
92	14.069	4049	4052	4055	rVB4	1572	745	0.08%	0.010%
93	14.104	4061	4063	4066	rBV4	1145	520	0.06%	0.007%
94	14.133	4070	4072	4074	rBV3	1094	590	0.06%	0.008%
95	14.297	4121	4123	4125	rVB3	1628	645	0.07%	0.009%
96	14.522	4190	4193	4195	rBV4	1476	784	0.08%	0.011%
97	14.635	4225	4228	4231	rBV4	1098	796	0.09%	0.011%
98	14.705	4248	4250	4252	rBV4	932	458	0.05%	0.006%
99	15.065	4359	4362	4365	rBV5	2535	1521	0.16%	0.021%
100	15.184	4397	4399	4403	rVB5	1999	977	0.11%	0.014%




Sum of corrected areas: 7194833

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042623\
Data File : VV030886.D
Acq On : 26 Apr 2023 17:36
Operator : SY/MD
Sample : 02475-04 5X
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 14 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0AW6

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM041723WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

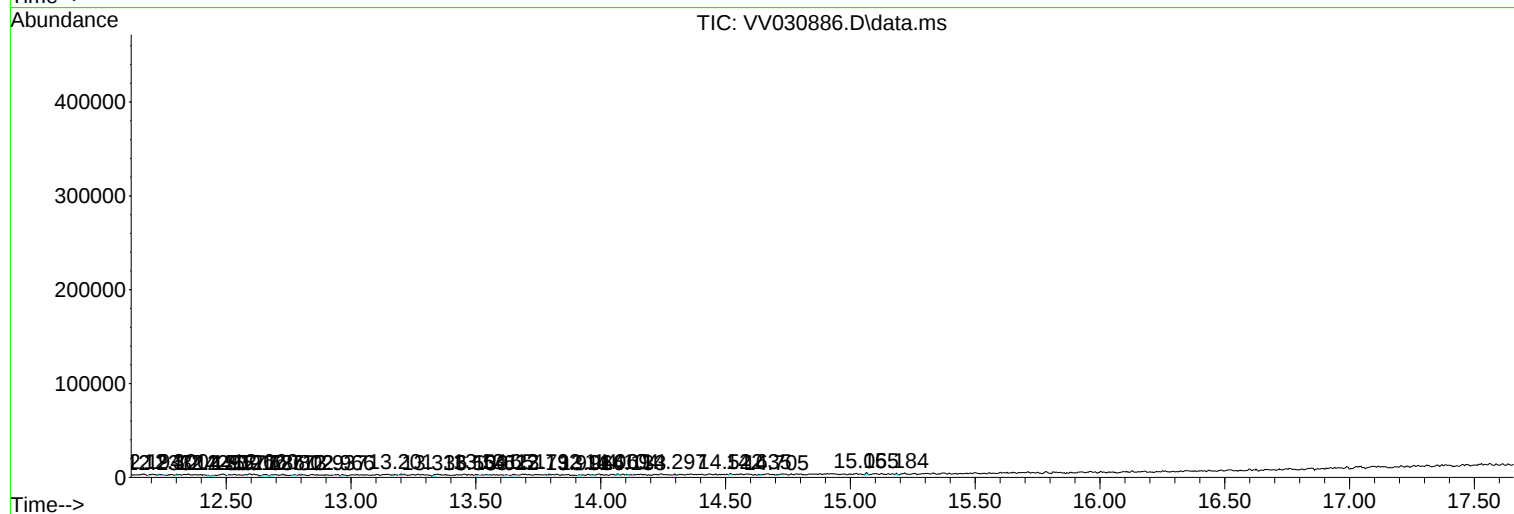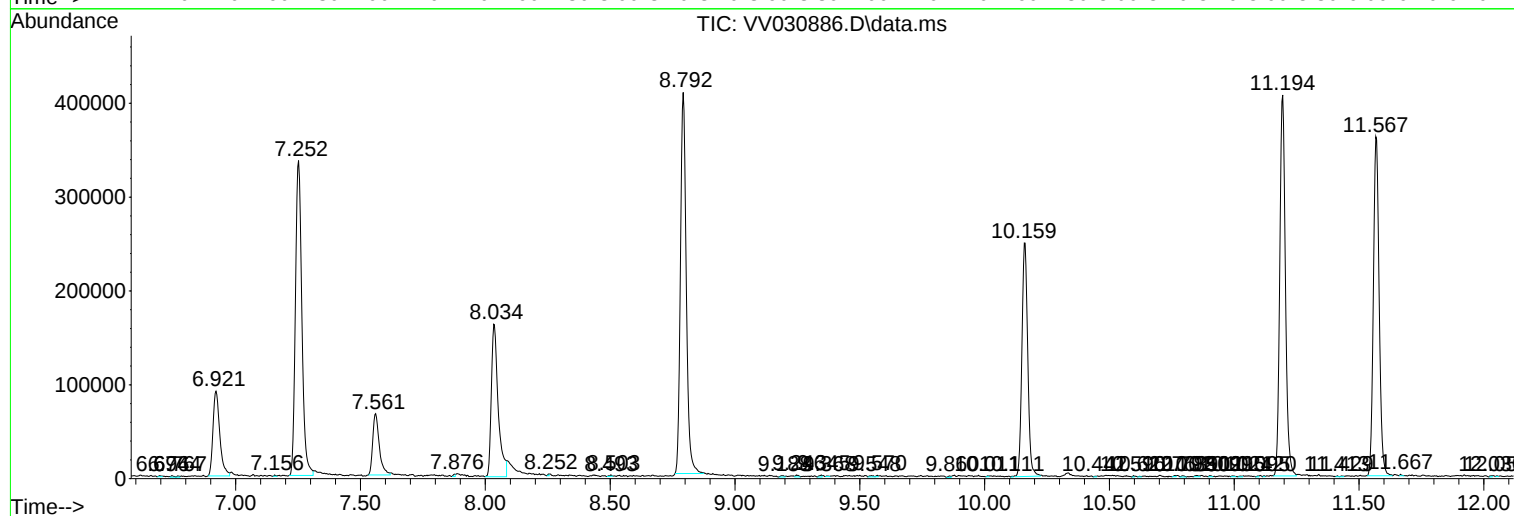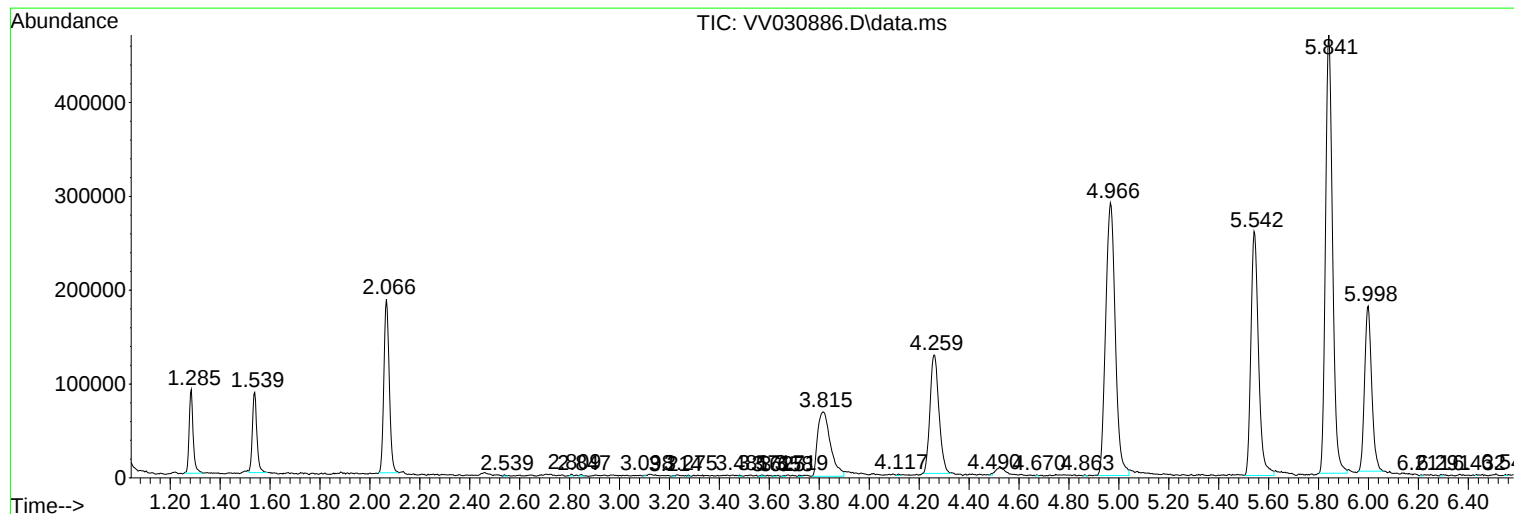

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042623\
Data File : VV030886.D
Acq On : 26 Apr 2023 17:36
Operator : SY/MD
Sample : 02475-04 5X
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 14 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0AW6

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM041723WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042623\
Data File : VV030886.D
Acq On : 26 Apr 2023 17:36
Operator : SY/MD
Sample : 02475-04 5X
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 14 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0AW6

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM041723WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------