

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042623\
 Data File : VV030887.D
 Acq On : 26 Apr 2023 18:00
 Operator : SY/MD
 Sample : 02475-10 5X
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0AX3

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM041723WMA.M
 Title : VOC Analysis

Signal : TIC: VV030887.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.281	69	75	91	rBV	84219	94526	8.09%	1.306%
2	1.535	148	154	167	rVB	83084	101262	8.67%	1.400%
3	2.066	310	319	333	rBV	185459	260913	22.34%	3.606%
4	2.288	385	388	391	rBV4	1386	923	0.08%	0.013%
5	2.436	432	434	436	rBV3	1602	961	0.08%	0.013%
6	2.516	456	459	460	rBV3	1053	587	0.05%	0.008%
7	2.555	467	471	472	rBV3	1168	856	0.07%	0.012%
8	2.590	479	482	486	rBV6	1798	1222	0.10%	0.017%
9	2.613	486	489	493	rVB5	1766	1388	0.12%	0.019%
10	2.632	493	495	500	rBV6	1119	827	0.07%	0.011%
11	2.661	500	504	506	rBV4	1277	905	0.08%	0.013%
12	2.838	556	559	562	rBV5	1027	741	0.06%	0.010%
13	2.886	572	574	577	rBV4	1014	533	0.05%	0.007%
14	2.918	583	584	588	rVB4	1370	594	0.05%	0.008%
15	2.937	588	590	592	rVB3	1325	500	0.04%	0.007%
16	2.950	592	594	601	rBV6	1326	1467	0.13%	0.020%
17	3.153	656	657	660	rVB3	1663	607	0.05%	0.008%
18	3.179	660	665	668	rBV5	1215	1330	0.11%	0.018%
19	3.307	703	705	709	rVB5	1645	922	0.08%	0.013%
20	3.342	711	716	718	rBV5	1426	1352	0.12%	0.019%
21	3.474	754	757	758	rBV3	1421	694	0.06%	0.010%
22	3.555	778	782	783	rBV5	950	569	0.05%	0.008%
23	3.600	794	796	799	rBV3	853	570	0.05%	0.008%
24	3.651	807	812	813	rBV5	1244	881	0.08%	0.012%
25	3.805	850	860	884	rBV2	49462	155106	13.28%	2.144%
26	4.076	942	944	945	rBV2	1102	513	0.04%	0.007%
27	4.259	982	1001	1023	rBV	127250	332179	28.44%	4.591%
28	4.706	1136	1140	1141	rBV4	879	507	0.04%	0.007%
29	4.738	1147	1150	1151	rBV3	981	619	0.05%	0.009%
30	4.844	1180	1183	1186	rBV4	1130	737	0.06%	0.010%
31	4.966	1205	1221	1250	rBV2	283869	762510	65.28%	10.538%
32	5.487	1381	1383	1386	rBV4	1222	665	0.06%	0.009%
33	5.542	1387	1400	1426	rBV	249992	527074	45.13%	7.285%
34	5.841	1480	1493	1519	rBV	588574	1167973	100.00%	16.142%
35	5.998	1532	1542	1561	rVB	170704	345574	29.59%	4.776%
36	6.281	1628	1630	1633	rBV4	1294	601	0.05%	0.008%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW042623\
 Data File : VW030887.D
 Acq On : 26 Apr 2023 18:00
 Operator : SY/MD
 Sample : 02475-10 5X
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0AX3

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM041723WMA.M
 Title : VOC Analysis

37	6.403	1665	1668	1669	rBV3	1722	653	0.06%	0.009%
38	6.603	1727	1730	1733	rBV5	1387	1279	0.11%	0.018%
39	6.883	1814	1817	1819	rBV3	763	630	0.05%	0.009%
40	6.921	1819	1829	1849	rVV	91343	174271	14.92%	2.409%
41	7.252	1921	1932	1949	rBV	326775	578395	49.52%	7.994%
42	7.561	2019	2028	2046	rBV	64789	113755	9.74%	1.572%
43	8.037	2167	2176	2210	rBV	144443	302581	25.91%	4.182%
44	8.548	2330	2335	2337	rBV6	1540	1632	0.14%	0.023%
45	8.792	2397	2411	2428	rBV	389750	658951	56.42%	9.107%
46	9.188	2532	2534	2538	rBV5	1555	1177	0.10%	0.016%
47	9.268	2557	2559	2568	rVB8	1977	2120	0.18%	0.029%
48	9.304	2568	2570	2573	rBV3	1854	1291	0.11%	0.018%
49	9.390	2595	2597	2603	rVB5	1504	1295	0.11%	0.018%
50	9.445	2612	2614	2618	rBV5	1257	836	0.07%	0.012%
51	9.468	2618	2621	2624	rBV4	1313	1009	0.09%	0.014%
52	9.548	2643	2646	2651	rBV5	943	851	0.07%	0.012%
53	9.641	2673	2675	2676	rBV3	1160	489	0.04%	0.007%
54	9.686	2685	2689	2691	rBV4	874	834	0.07%	0.012%
55	9.738	2702	2705	2710	rBV6	1732	1201	0.10%	0.017%
56	9.847	2737	2739	2742	rVB3	1072	625	0.05%	0.009%
57	9.908	2755	2758	2760	rBV3	1234	623	0.05%	0.009%
58	10.017	2789	2792	2797	rVV6	920	823	0.07%	0.011%
59	10.159	2825	2836	2854	rBV	238783	384675	32.94%	5.316%
60	10.265	2866	2869	2872	rVB5	1738	1018	0.09%	0.014%
61	10.310	2880	2883	2884	rBV3	1103	577	0.05%	0.008%
62	10.336	2884	2891	2901	rVV7	4976	8578	0.73%	0.119%
63	10.419	2915	2917	2923	rBV6	1091	880	0.08%	0.012%
64	10.487	2934	2938	2939	rBV5	1010	787	0.07%	0.011%
65	10.522	2947	2949	2953	rBV5	1236	680	0.06%	0.009%
66	10.683	2995	2999	3000	rBV3	1145	756	0.06%	0.010%
67	10.805	3034	3037	3039	rBV3	1049	684	0.06%	0.009%
68	10.892	3062	3064	3066	rBV4	1635	634	0.05%	0.009%
69	11.079	3120	3122	3125	rVB4	1563	856	0.07%	0.012%
70	11.117	3131	3134	3135	rBV3	1019	695	0.06%	0.010%
71	11.194	3145	3158	3174	rBV	392433	624400	53.46%	8.630%
72	11.439	3231	3234	3235	rBV3	1064	557	0.05%	0.008%
73	11.519	3257	3259	3262	rVV4	1046	558	0.05%	0.008%
74	11.567	3263	3274	3292	rVV	353658	574416	49.18%	7.939%
75	11.818	3350	3352	3355	rBV3	1413	745	0.06%	0.010%
76	11.937	3384	3389	3392	rBV5	1964	1974	0.17%	0.027%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042623\
 Data File : VV030887.D
 Acq On : 26 Apr 2023 18:00
 Operator : SY/MD
 Sample : 02475-10 5X
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0AX3

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM041723WMA.M
 Title : VOC Analysis

77	12.056	3424	3426	3429	rBV4	1277	886	0.08%	0.012%
78	12.197	3465	3470	3473	rVV8	1742	1465	0.13%	0.020%
79	12.230	3478	3480	3483	rVB4	1329	693	0.06%	0.010%
80	12.246	3483	3485	3487	rBV2	1171	500	0.04%	0.007%
81	12.474	3554	3556	3558	rBV3	1419	729	0.06%	0.010%
82	12.548	3576	3579	3581	rBV4	1137	538	0.05%	0.007%
83	12.586	3589	3591	3593	rBV2	1030	643	0.06%	0.009%
84	12.696	3623	3625	3628	rBV4	1107	615	0.05%	0.008%
85	12.715	3629	3631	3635	rVV5	1234	862	0.07%	0.012%
86	12.792	3652	3655	3658	rBV4	739	779	0.07%	0.011%
87	12.857	3672	3675	3676	rBV2	1441	843	0.07%	0.012%
88	12.889	3683	3685	3687	rVB3	1594	600	0.05%	0.008%
89	13.136	3758	3762	3763	rBV4	1006	674	0.06%	0.009%
90	13.406	3843	3846	3848	rBV4	796	590	0.05%	0.008%
91	13.583	3899	3901	3905	rVB3	877	539	0.05%	0.007%
92	13.615	3908	3911	3914	rBV6	810	602	0.05%	0.008%
93	13.683	3929	3932	3935	rBV4	1682	1212	0.10%	0.017%
94	13.712	3939	3941	3944	rVB3	1278	780	0.07%	0.011%
95	13.747	3950	3952	3955	rBV2	976	542	0.05%	0.007%
96	13.792	3964	3966	3969	rBV3	899	610	0.05%	0.008%
97	13.895	3996	3998	4000	rBV3	1244	673	0.06%	0.009%
98	14.008	4030	4033	4034	rBV3	924	585	0.05%	0.008%
99	14.127	4067	4070	4071	rBV3	953	531	0.05%	0.007%
100	14.709	4249	4251	4254	rVB3	2211	1076	0.09%	0.015%




Sum of corrected areas: 7235546

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042623\
Data File : VV030887.D
Acq On : 26 Apr 2023 18:00
Operator : SY/MD
Sample : 02475-10 5X
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 15 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0AX3

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM041723WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

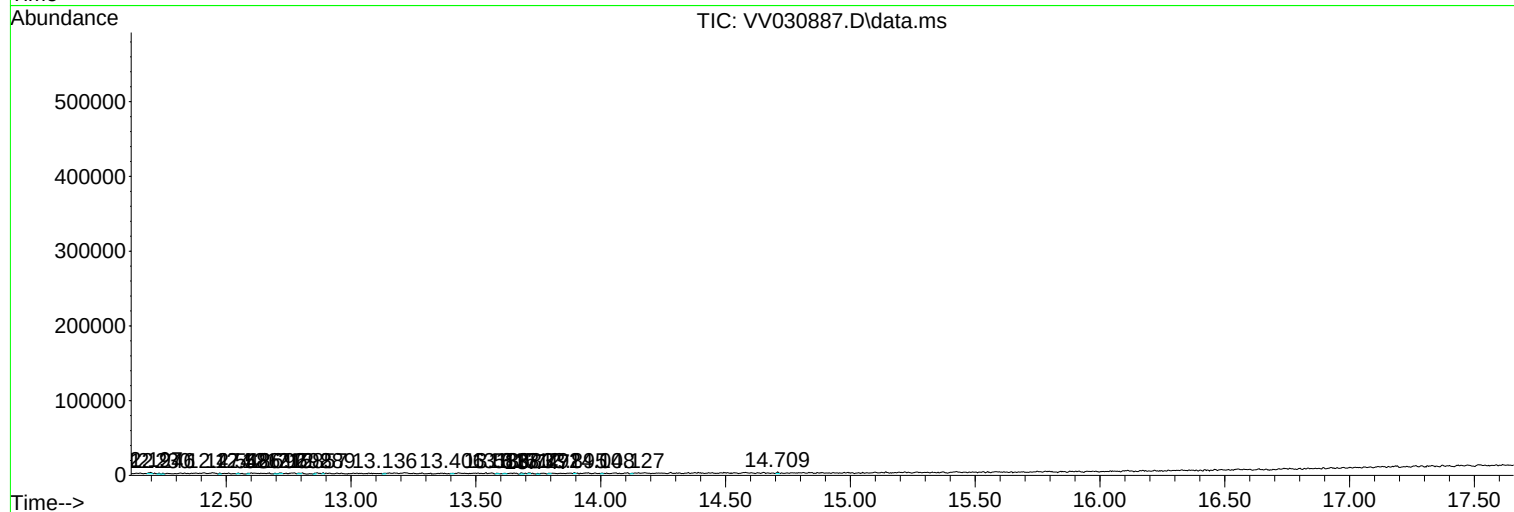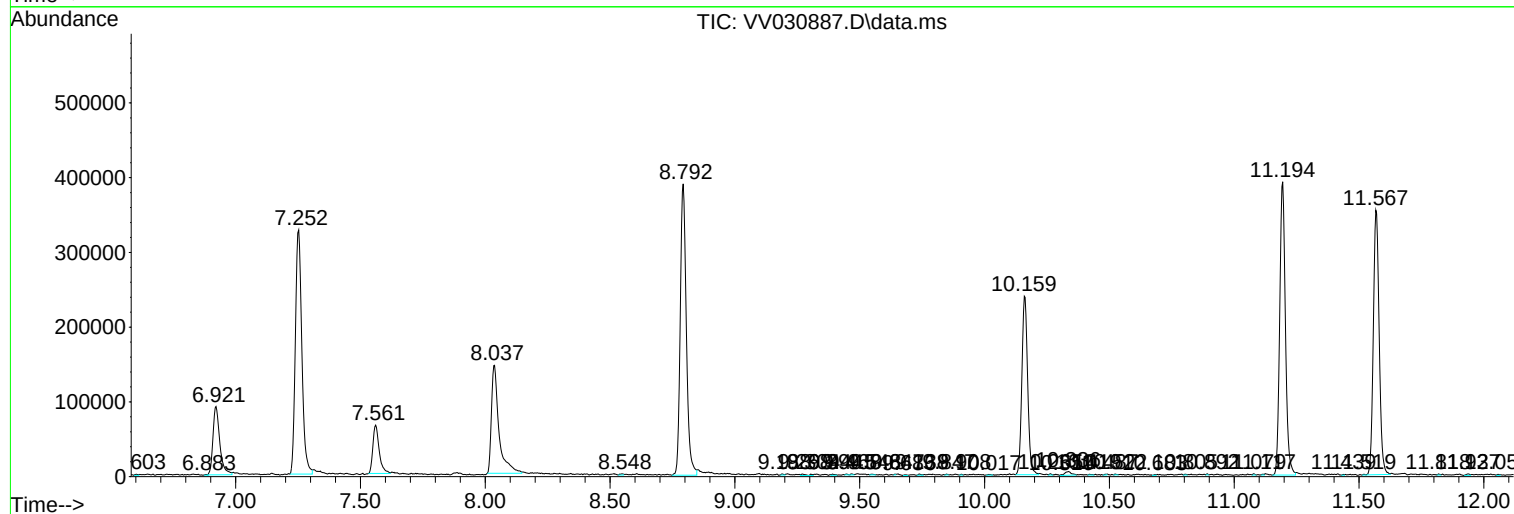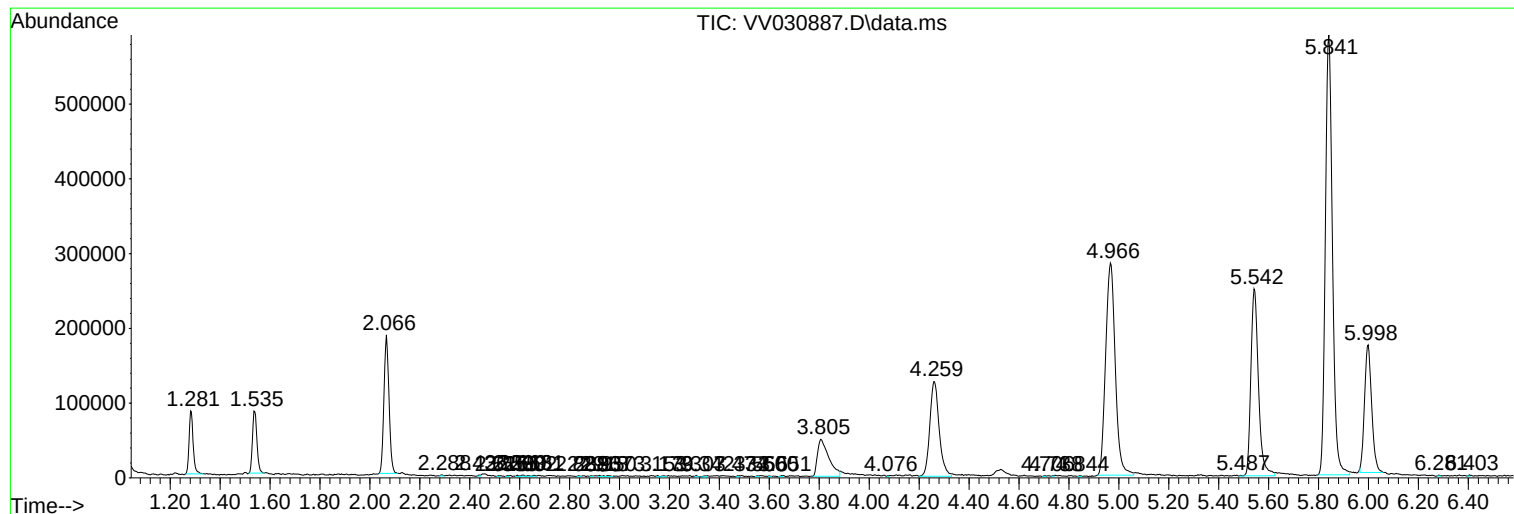

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042623\
Data File : VV030887.D
Acq On : 26 Apr 2023 18:00
Operator : SY/MD
Sample : 02475-10 5X
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 15 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0AX3

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM041723WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042623\
Data File : VV030887.D
Acq On : 26 Apr 2023 18:00
Operator : SY/MD
Sample : 02475-10 5X
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 15 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0AX3

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM041723WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
