

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042623\
 Data File : VV030890.D
 Acq On : 26 Apr 2023 19:36
 Operator : SY/MD
 Sample : VIBLK207
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VIBLK207

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM041723WMA.M
 Title : VOC Analysis

Signal : TIC: VV030890.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.282	70	75	86	rVB	58939	62136	9.24%	1.255%
2	1.539	149	155	169	rVB	65571	82081	12.21%	1.657%
3	2.066	310	319	333	rBV	122041	175911	26.16%	3.552%
4	2.545	465	468	472	rVB6	1950	1383	0.21%	0.028%
5	2.565	472	474	476	rBV3	1662	856	0.13%	0.017%
6	2.629	491	494	500	rBV6	1058	1363	0.20%	0.028%
7	2.709	515	519	521	rBV3	1591	1157	0.17%	0.023%
8	2.838	553	559	561	rBV6	1720	1250	0.19%	0.025%
9	2.876	568	571	579	rBV7	1620	2185	0.32%	0.044%
10	3.050	623	625	629	rVB4	1739	1012	0.15%	0.020%
11	3.082	629	635	637	rBV7	1511	1693	0.25%	0.034%
12	3.105	637	642	643	rBV4	947	684	0.10%	0.014%
13	3.130	648	650	654	rVV5	1621	1128	0.17%	0.023%
14	3.159	657	659	663	rVB3	861	670	0.10%	0.014%
15	3.298	700	702	706	rVB3	1113	521	0.08%	0.011%
16	3.355	718	720	727	rBV7	1172	1087	0.16%	0.022%
17	3.420	737	740	743	rBV6	886	629	0.09%	0.013%
18	3.507	764	767	771	rVB5	1258	914	0.14%	0.018%
19	3.687	817	823	825	rBV5	824	702	0.10%	0.014%
20	3.741	838	840	843	rVB3	1223	643	0.10%	0.013%
21	3.767	846	848	850	rBV2	942	545	0.08%	0.011%
22	3.809	851	861	888	rBV	46549	145054	21.57%	2.929%
23	4.259	987	1001	1027	rBV	110568	277615	41.29%	5.606%
24	4.487	1069	1072	1073	rBV3	1338	696	0.10%	0.014%
25	4.793	1164	1167	1170	rBV4	987	706	0.10%	0.014%
26	4.966	1202	1221	1251	rBV2	239851	672420	100.00%	13.577%
27	5.272	1314	1316	1318	rBV3	1410	613	0.09%	0.012%
28	5.371	1345	1347	1350	rBV4	1428	714	0.11%	0.014%
29	5.542	1388	1400	1422	rBV	195165	405240	60.27%	8.182%
30	5.998	1531	1542	1559	rBV	147553	299472	44.54%	6.047%
31	6.365	1654	1656	1660	rBV4	1003	696	0.10%	0.014%
32	6.513	1700	1702	1703	rBV	1210	568	0.08%	0.011%
33	6.568	1717	1719	1721	rBV3	1181	513	0.08%	0.010%
34	6.664	1747	1749	1751	rVB3	1767	641	0.10%	0.013%
35	6.693	1751	1758	1765	rBV3	2034	2977	0.44%	0.060%
36	6.738	1769	1772	1776	rBV4	965	737	0.11%	0.015%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042623\
 Data File : VV030890.D
 Acq On : 26 Apr 2023 19:36
 Operator : SY/MD
 Sample : VIBLK207
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VIBLK207

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM041723WMA.M
 Title : VOC Analysis

37	6.786	1785	1787	1789	rBV3	1022	637	0.09%	0.013%
38	6.921	1818	1829	1848	rBV	75633	149513	22.24%	3.019%
39	7.140	1895	1897	1900	rBV3	919	610	0.09%	0.012%
40	7.156	1900	1902	1906	rVB4	1797	923	0.14%	0.019%
41	7.252	1920	1932	1951	rBV	240314	427998	63.65%	8.642%
42	7.561	2019	2028	2046	rBV	57610	104862	15.59%	2.117%
43	7.815	2105	2107	2111	rVB5	1299	734	0.11%	0.015%
44	7.847	2114	2117	2120	rBV4	1258	754	0.11%	0.015%
45	7.892	2129	2131	2134	rBV3	1253	673	0.10%	0.014%
46	7.960	2150	2152	2155	rBV4	1643	1119	0.17%	0.023%
47	8.034	2164	2175	2209	rBV	149597	331626	49.32%	6.696%
48	8.423	2295	2296	2301	rVB5	1484	778	0.12%	0.016%
49	8.593	2347	2349	2352	rBV3	984	534	0.08%	0.011%
50	8.793	2399	2411	2435	rBV	289033	496561	73.85%	10.026%
51	9.018	2477	2481	2487	rVB10	1254	1357	0.20%	0.027%
52	9.169	2523	2528	2531	rBV6	1155	1037	0.15%	0.021%
53	9.191	2533	2535	2538	rBV4	1114	573	0.09%	0.012%
54	9.304	2567	2570	2572	rBV4	1103	751	0.11%	0.015%
55	9.342	2578	2582	2585	rBV4	1219	940	0.14%	0.019%
56	9.577	2652	2655	2659	rBV3	662	625	0.09%	0.013%
57	9.635	2669	2673	2675	rBV4	922	848	0.13%	0.017%
58	9.709	2692	2696	2701	rBV6	1213	1108	0.16%	0.022%
59	9.748	2705	2708	2709	rBV3	931	613	0.09%	0.012%
60	9.895	2752	2754	2759	rVB5	1242	959	0.14%	0.019%
61	10.021	2790	2793	2795	rBV4	1391	739	0.11%	0.015%
62	10.111	2817	2821	2822	rBV3	938	646	0.10%	0.013%
63	10.159	2822	2836	2858	rVV	230280	377661	56.16%	7.626%
64	10.426	2917	2919	2922	rBV4	832	648	0.10%	0.013%
65	10.458	2927	2929	2933	rBV4	1448	935	0.14%	0.019%
66	10.484	2935	2937	2939	rBV3	906	533	0.08%	0.011%
67	10.519	2944	2948	2950	rBV4	1198	806	0.12%	0.016%
68	10.619	2975	2979	2980	rBV3	987	655	0.10%	0.013%
69	10.728	3011	3013	3017	rVB5	1213	851	0.13%	0.017%
70	10.809	3031	3038	3039	rBV6	1238	1362	0.20%	0.028%
71	10.850	3049	3051	3054	rBV4	1174	891	0.13%	0.018%
72	10.940	3074	3079	3082	rBV6	1219	1082	0.16%	0.022%
73	10.960	3082	3085	3088	rBV5	1271	902	0.13%	0.018%
74	11.037	3105	3109	3112	rVB6	1032	844	0.13%	0.017%
75	11.063	3113	3117	3119	rVB3	1189	836	0.12%	0.017%
76	11.075	3119	3121	3125	rBV5	1396	775	0.12%	0.016%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042623\
 Data File : VV030890.D
 Acq On : 26 Apr 2023 19:36
 Operator : SY/MD
 Sample : VIBLK207
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VIBLK207

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM041723WMA.M
 Title : VOC Analysis

77	11.098	3125	3128	3130	rBV4	1274	700	0.10%	0.014%
78	11.194	3146	3158	3178	rBV	273629	444432	66.09%	8.974%
79	11.419	3222	3228	3231	rBV7	1750	1595	0.24%	0.032%
80	11.458	3238	3240	3242	rBV3	1426	835	0.12%	0.017%
81	11.567	3263	3274	3291	rVV	264340	422737	62.87%	8.536%
82	11.773	3336	3338	3340	rBV3	1430	714	0.11%	0.014%
83	12.091	3434	3437	3439	rBV4	1310	929	0.14%	0.019%
84	12.136	3449	3451	3455	rBV5	1172	813	0.12%	0.016%
85	12.667	3608	3616	3620	rBV8	1400	1884	0.28%	0.038%
86	12.731	3632	3636	3637	rVV2	885	581	0.09%	0.012%
87	12.805	3656	3659	3661	rBV3	985	598	0.09%	0.012%
88	13.024	3725	3727	3730	rVB4	1338	706	0.10%	0.014%
89	13.050	3730	3735	3737	rBV5	1209	959	0.14%	0.019%
90	13.159	3766	3769	3779	rVB7	1368	1988	0.30%	0.040%
91	13.278	3803	3806	3807	rBV3	1059	692	0.10%	0.014%
92	13.468	3857	3865	3868	rBV6	1204	1496	0.22%	0.030%
93	13.564	3893	3895	3898	rBV3	1151	623	0.09%	0.013%
94	13.635	3911	3917	3919	rBV7	1092	857	0.13%	0.017%
95	13.760	3954	3956	3959	rBV4	1609	982	0.15%	0.020%
96	13.776	3959	3961	3967	rVB6	1387	987	0.15%	0.020%
97	14.220	4097	4099	4103	rVB4	1183	716	0.11%	0.014%
98	14.329	4129	4133	4134	rBV3	910	730	0.11%	0.015%
99	14.397	4151	4154	4158	rBV4	1413	1367	0.20%	0.028%
100	15.053	4355	4358	4361	rBV4	1223	1102	0.16%	0.022%




Sum of corrected areas: 4952534

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042623\
Data File : VV030890.D
Acq On : 26 Apr 2023 19:36
Operator : SY/MD
Sample : VIBLK207
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 19 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VIBLK207

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM041723WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

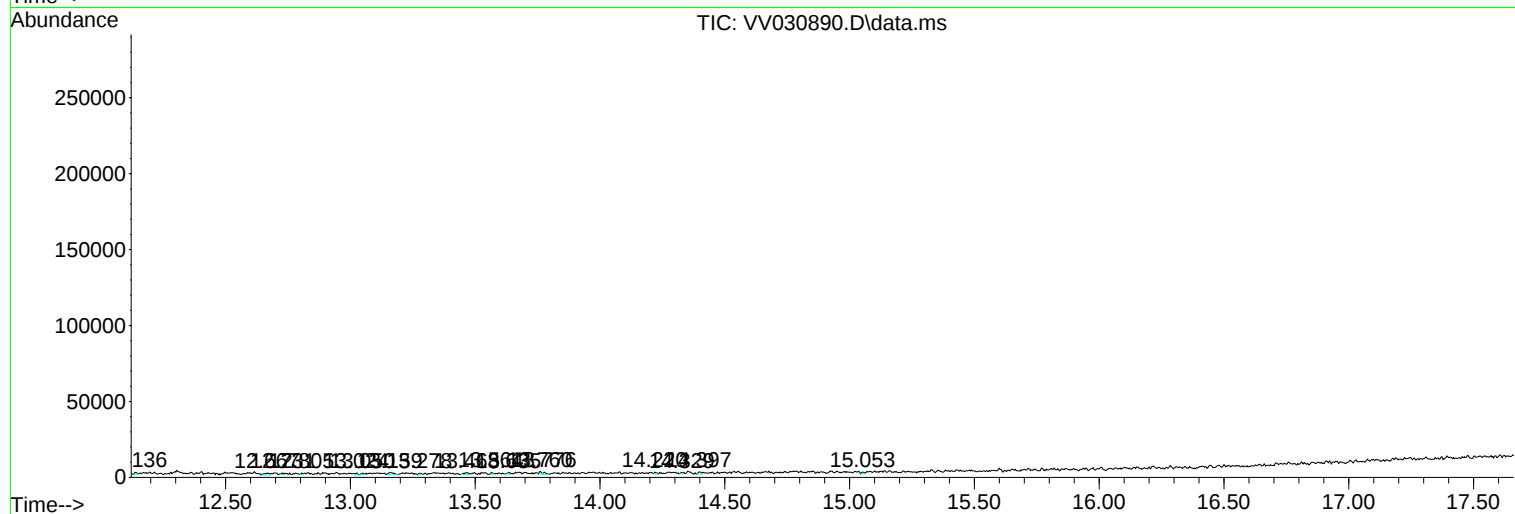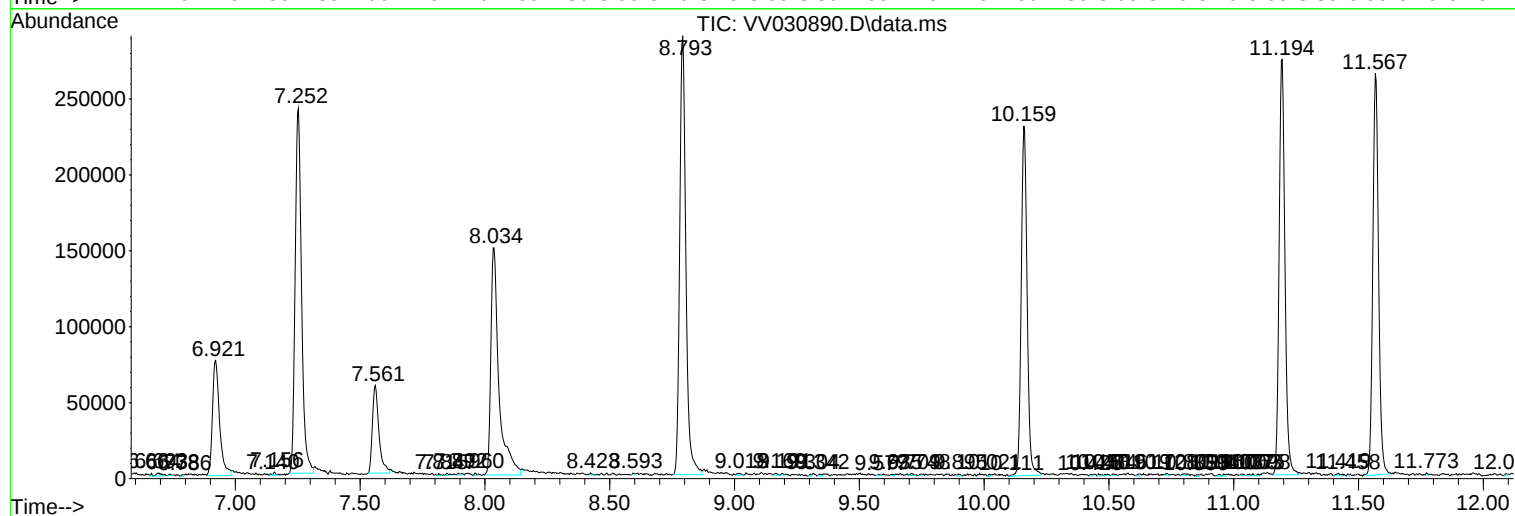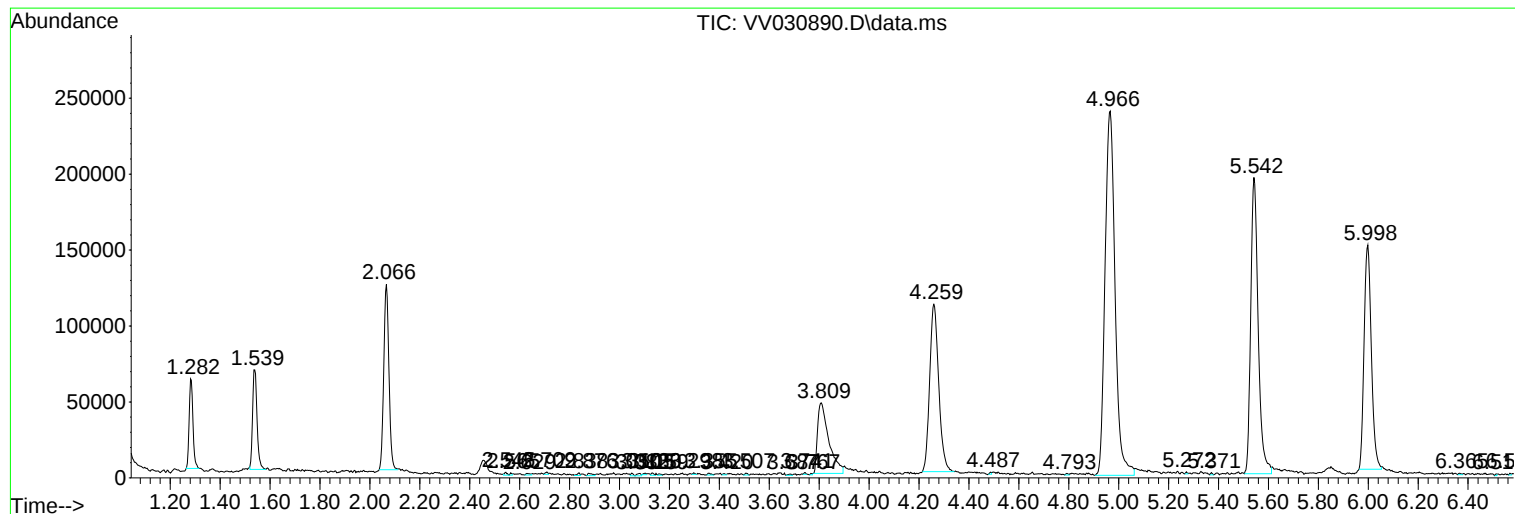

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042623\
Data File : VV030890.D
Acq On : 26 Apr 2023 19:36
Operator : SY/MD
Sample : VIBLK207
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 19 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VIBLK207

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM041723WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042623\
Data File : VV030890.D
Acq On : 26 Apr 2023 19:36
Operator : SY/MD
Sample : VIBLK207
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 19 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VIBLK207

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM041723WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------